

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003347.D
 Acq On : 01 Dec 2015 22:04
 Operator : UM/IZ
 Sample : G4545-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA785

Quant Time: Dec 02 01:18:29 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 02 01:07:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	70672	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	326302	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	192944	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	403392	20.00	ng/ul	0.00
78) Chrysene-d12	21.32	240	360551	20.00	ng/ul	0.00
86) Perylene-d12	23.58	264	330150	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	1374	0.97	ng/uL	0.00
5) Phenol-d5	6.89	99	32182	5.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	78462	25.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	96146	20.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	71865	15.18	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	61273	27.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	68017	29.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	133087	28.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	8480	1.62	ng/ul	0.00
44) Dimethylphthalate-d6	13.79	166	552928	38.12	ng/ul	0.00
47) Acenaphthylene-d8	14.07	160	616663	34.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.57	143	14717	5.66	ng/ul	0.00
58) Fluorene-d10	15.37	176	460978	36.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	68771	33.32	ng/ul	0.00
71) Anthracene-d10	17.22	188	684891	38.21	ng/ul	0.00
79) Pyrene-d10	19.52	212	701170	39.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	580040	36.41	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
46) 2,6-Dinitrotoluene	13.79	165	3074	1.12	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003347.D
Acq On : 01 Dec 2015 22:04
Operator : UM/IZ
Sample : G4545-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA785

Quant Time: Dec 02 01:18:29 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 02 01:07:29 2015
Response via : Initial Calibration

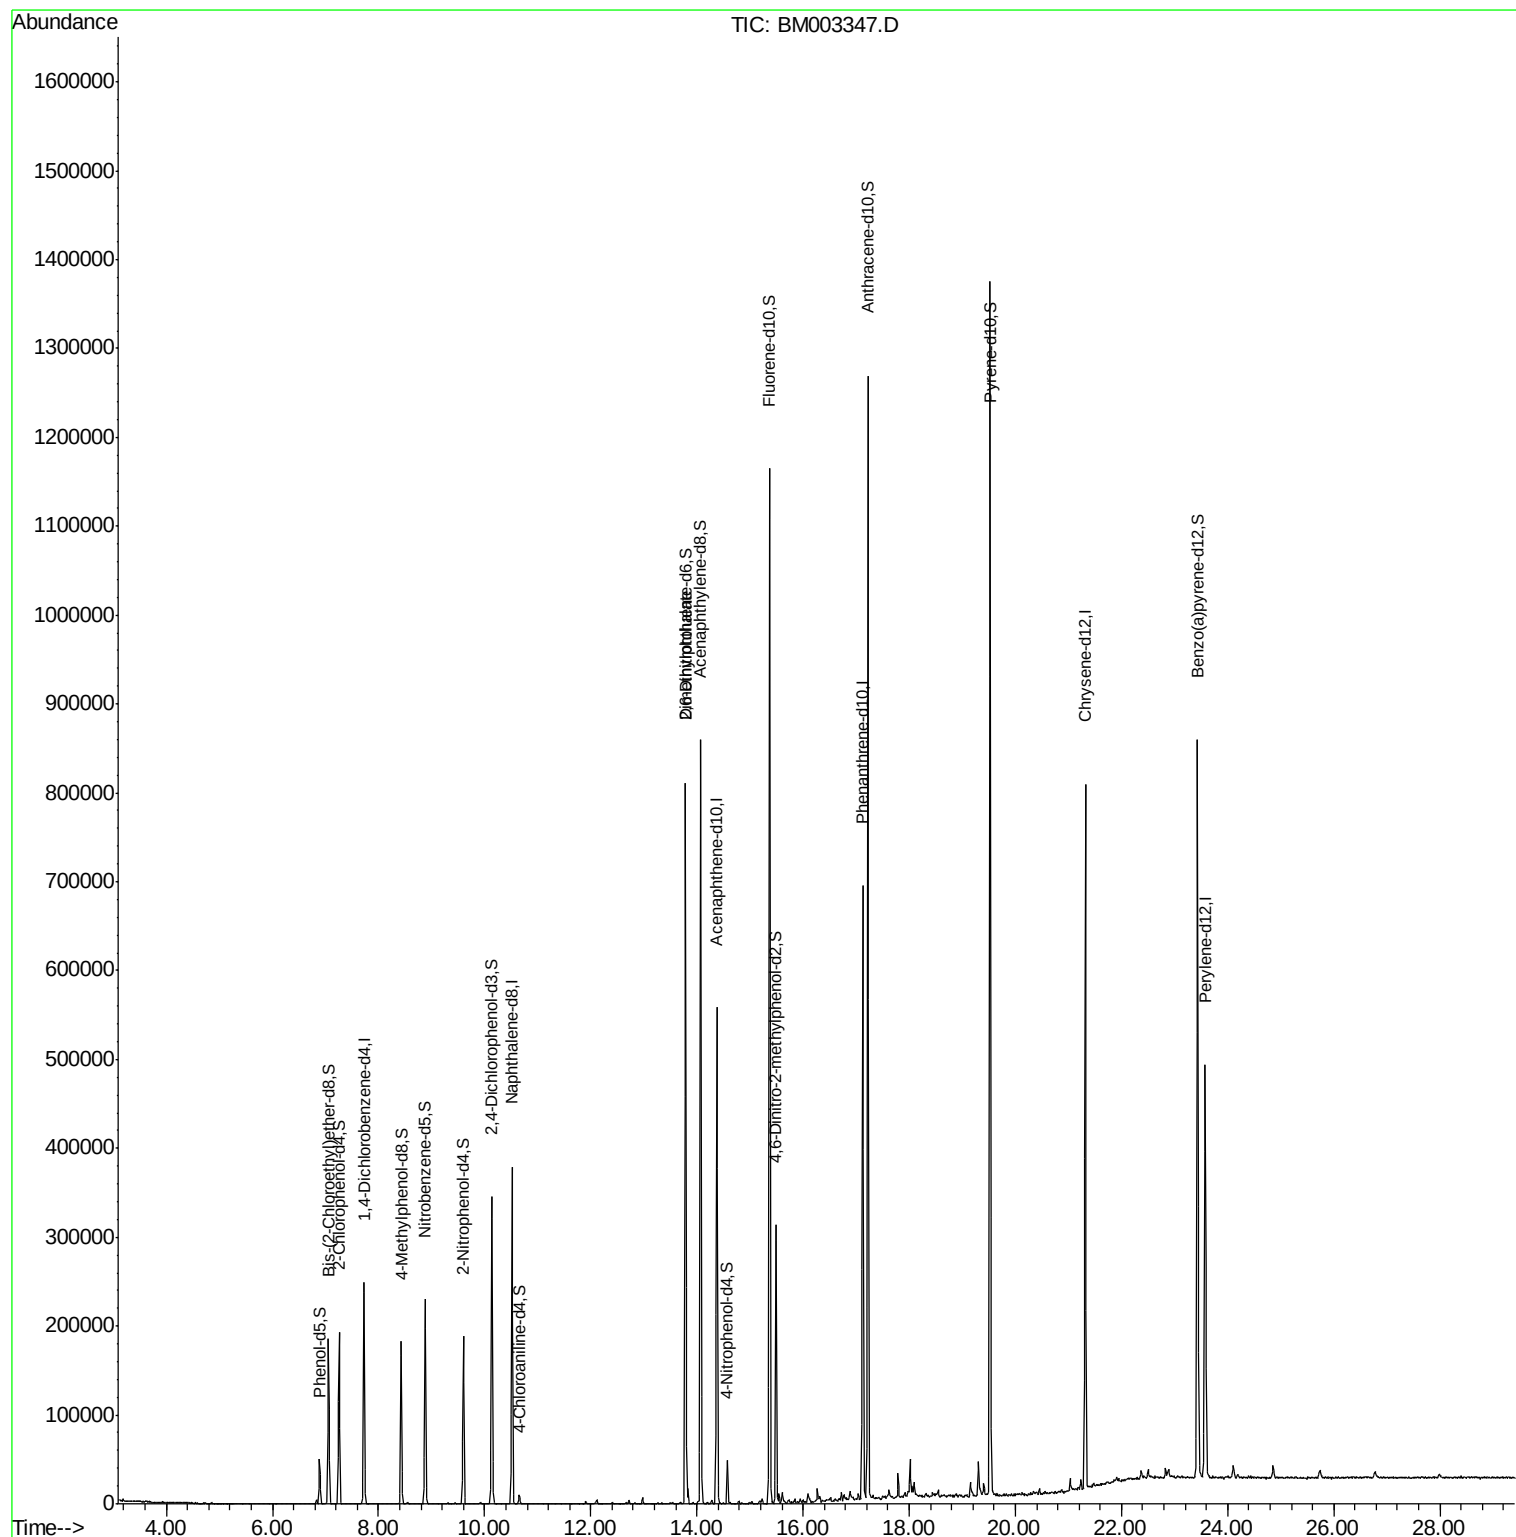

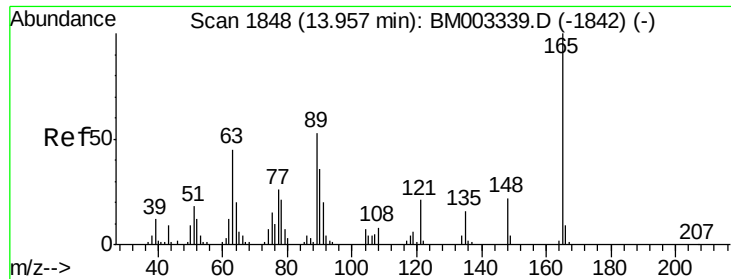

#46
 2,6-Dinitrotoluene
 Concen: 1.12 ng/ul
 RT: 13.79 min Scan# 1819
 Delta R.T. -0.17 min
 Lab File: BM003347.D
 Acq: 01 Dec 2015 22:04

Instrument :
 BNA_M
 ClientSampleId :
 CA785

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	42.0	63.0#
121	43.1	16.6	24.8#

