

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003343.D
 Acq On : 01 Dec 2015 19:40
 Operator : UM/IZ
 Sample : PB86966BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	13	17	23	rVB	19455	24034	1.18%	0.118%
2	3.746	108	112	115	rBV	2484	2710	0.13%	0.013%
3	6.887	640	646	655	rBV	308732	474752	23.29%	2.323%
4	7.057	669	675	685	rVB	269694	407836	20.00%	1.995%
5	7.257	702	709	717	rBV	335570	518047	25.41%	2.534%
6	7.728	782	789	796	rBV	259931	406343	19.93%	1.988%
7	8.428	902	908	920	rBV	431592	663244	32.53%	3.245%
8	8.881	979	985	994	rVB	312830	490196	24.04%	2.398%
9	9.604	1101	1108	1115	rBB	255692	414425	20.33%	2.027%
10	10.133	1192	1198	1207	rBV	414597	675580	33.14%	3.305%
11	10.516	1255	1263	1272	rBV	393523	651320	31.95%	3.186%
12	10.651	1279	1286	1298	rBV	460464	752140	36.89%	3.680%
13	12.110	1530	1534	1539	rVB2	5418	8542	0.42%	0.042%
14	13.786	1812	1819	1827	rBV	858744	1177399	57.75%	5.760%
15	14.068	1860	1867	1880	rBV	947331	1366709	67.04%	6.686%
16	14.380	1913	1920	1927	rBV2	612715	937906	46.00%	4.589%
17	14.568	1947	1952	1969	rBV	343063	487551	23.91%	2.385%
18	15.368	2082	2088	2097	rBV	1214141	1766155	86.63%	8.641%
19	15.486	2103	2108	2118	rBV	282164	380373	18.66%	1.861%
20	15.610	2125	2129	2133	rBV	9757	12666	0.62%	0.062%
21	16.909	2347	2350	2356	rVB	2067	2778	0.14%	0.014%
22	17.121	2380	2386	2393	rBV2	794192	1105692	54.23%	5.409%
23	17.221	2397	2403	2418	rVB2	1305136	1872068	91.82%	9.159%
24	19.156	2726	2732	2737	rBV	10389	13132	0.64%	0.064%
25	19.409	2771	2775	2780	rBV	8465	10577	0.52%	0.052%
26	19.527	2787	2795	2808	rBV	1491056	2038764	100.00%	9.974%
27	21.321	3095	3100	3108	rBV	875253	1083133	53.13%	5.299%
28	22.838	3354	3358	3362	rBV	9168	13717	0.67%	0.067%
29	23.438	3452	3460	3470	rBV	961570	1711068	83.93%	8.371%
30	23.580	3477	3484	3495	rBV	517761	971428	47.65%	4.753%


Sum of corrected areas: 20440285

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003343.D
Acq On : 01 Dec 2015 19:40
Operator : UM/IZ
Sample : PB86966BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

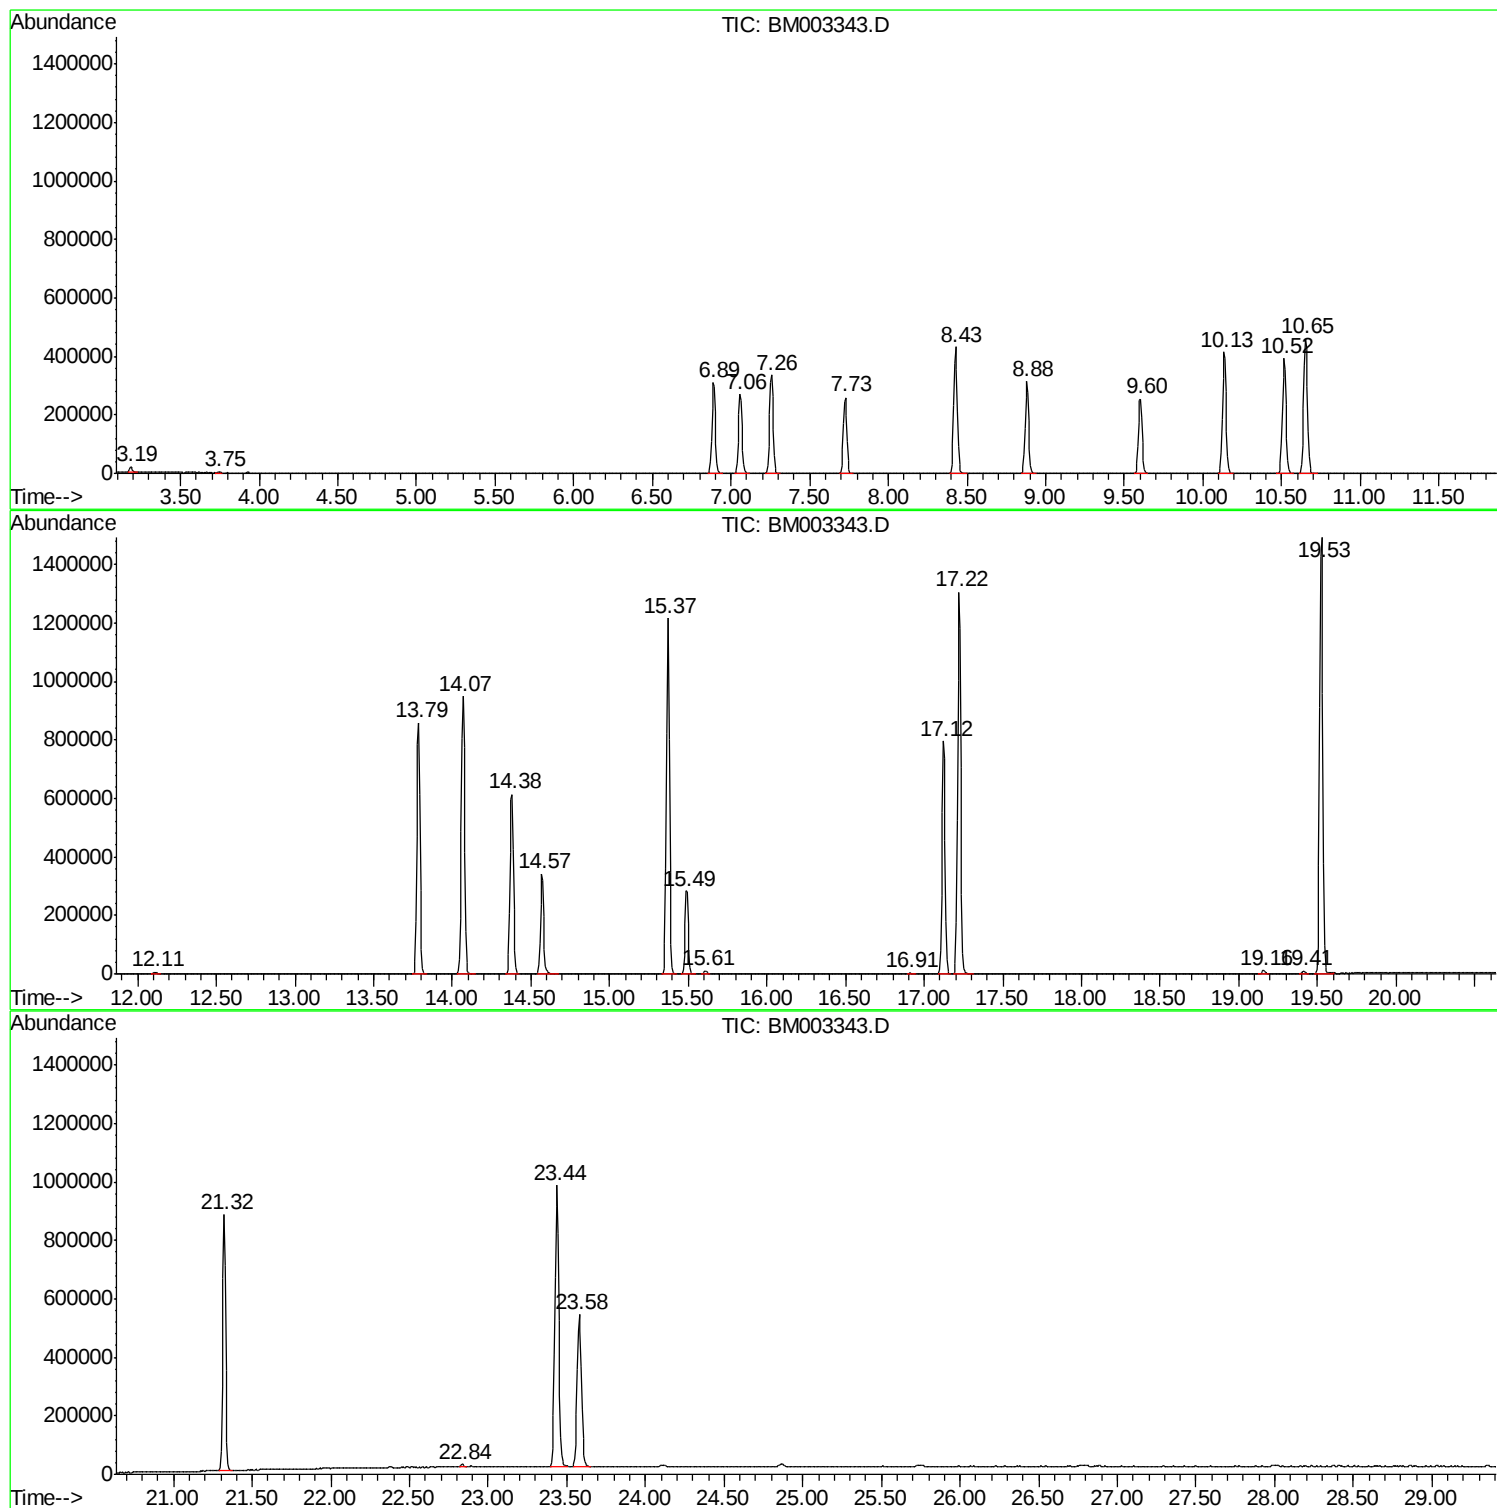

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003343.D
Acq On : 01 Dec 2015 19:40
Operator : UM/IZ
Sample : PB86966BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003343.D
Acq On : 01 Dec 2015 19:40
Operator : UM/IZ
Sample : PB86966BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc