

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003344.D
 Acq On : 01 Dec 2015 20:16
 Operator : UM/IZ
 Sample : PB86966TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	13	17	21	rBV	19045	23141	0.89%	0.102%
2	3.746	109	112	115	rBV	2385	2612	0.10%	0.012%
3	6.886	640	646	658	rVB	317339	496022	19.08%	2.190%
4	7.057	668	675	685	rVB	276246	424320	16.32%	1.873%
5	7.257	703	709	717	rVB	352596	538482	20.71%	2.377%
6	7.728	783	789	795	rBV	216006	337238	12.97%	1.489%
7	8.428	901	908	918	rVB	456298	697510	26.83%	3.079%
8	8.880	978	985	993	rVB	323849	508408	19.56%	2.244%
9	9.604	1101	1108	1115	rVB	268076	429378	16.52%	1.895%
10	10.133	1191	1198	1212	rVB	432953	708869	27.27%	3.129%
11	10.516	1254	1263	1272	rBV	335879	545542	20.99%	2.408%
12	10.651	1279	1286	1297	rBV	482723	795711	30.61%	3.513%
13	12.110	1528	1534	1541	rBB2	5879	9047	0.35%	0.040%
14	13.786	1812	1819	1827	rVB	947784	1271432	48.91%	5.613%
15	14.068	1860	1867	1877	rBV	1019927	1459107	56.13%	6.441%
16	14.374	1912	1919	1927	rBV2	517514	796557	30.64%	3.516%
17	14.568	1947	1952	1970	rVB	405268	585290	22.51%	2.584%
18	15.374	2082	2089	2099	rVB	1289873	1911409	73.53%	8.438%
19	15.492	2103	2109	2115	rBV	325554	446266	17.17%	1.970%
20	15.609	2124	2129	2134	rVB	11498	14461	0.56%	0.064%
21	17.121	2380	2386	2393	rBV2	726331	1002588	38.57%	4.426%
22	17.221	2397	2403	2420	rVB2	1512697	2137434	82.22%	9.435%
23	19.156	2727	2732	2737	rVB2	12647	16316	0.63%	0.072%
24	19.409	2770	2775	2779	rBV	11513	14251	0.55%	0.063%
25	19.527	2788	2795	2806	rBV	1857489	2599568	100.00%	11.475%
26	21.321	3094	3100	3109	rBV	1007762	1255873	48.31%	5.544%
27	22.833	3353	3357	3362	rBV2	13865	23476	0.90%	0.104%
28	22.885	3363	3366	3372	rVB2	9677	11621	0.45%	0.051%
29	23.438	3452	3460	3473	rBV	1283915	2444110	94.02%	10.789%
30	23.580	3476	3484	3496	rVB	601327	1096294	42.17%	4.839%
31	24.109	3571	3574	3579	rVB3	15394	23691	0.91%	0.105%
32	24.868	3698	3703	3709	rVB3	13455	27343	1.05%	0.121%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003344.D
Acq On : 01 Dec 2015 20:16
Operator : UM/IZ
Sample : PB86966TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB03

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION


Sum of corrected areas: 22653367

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003344.D
Acq On : 01 Dec 2015 20:16
Operator : UM/IZ
Sample : PB86966TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB03

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

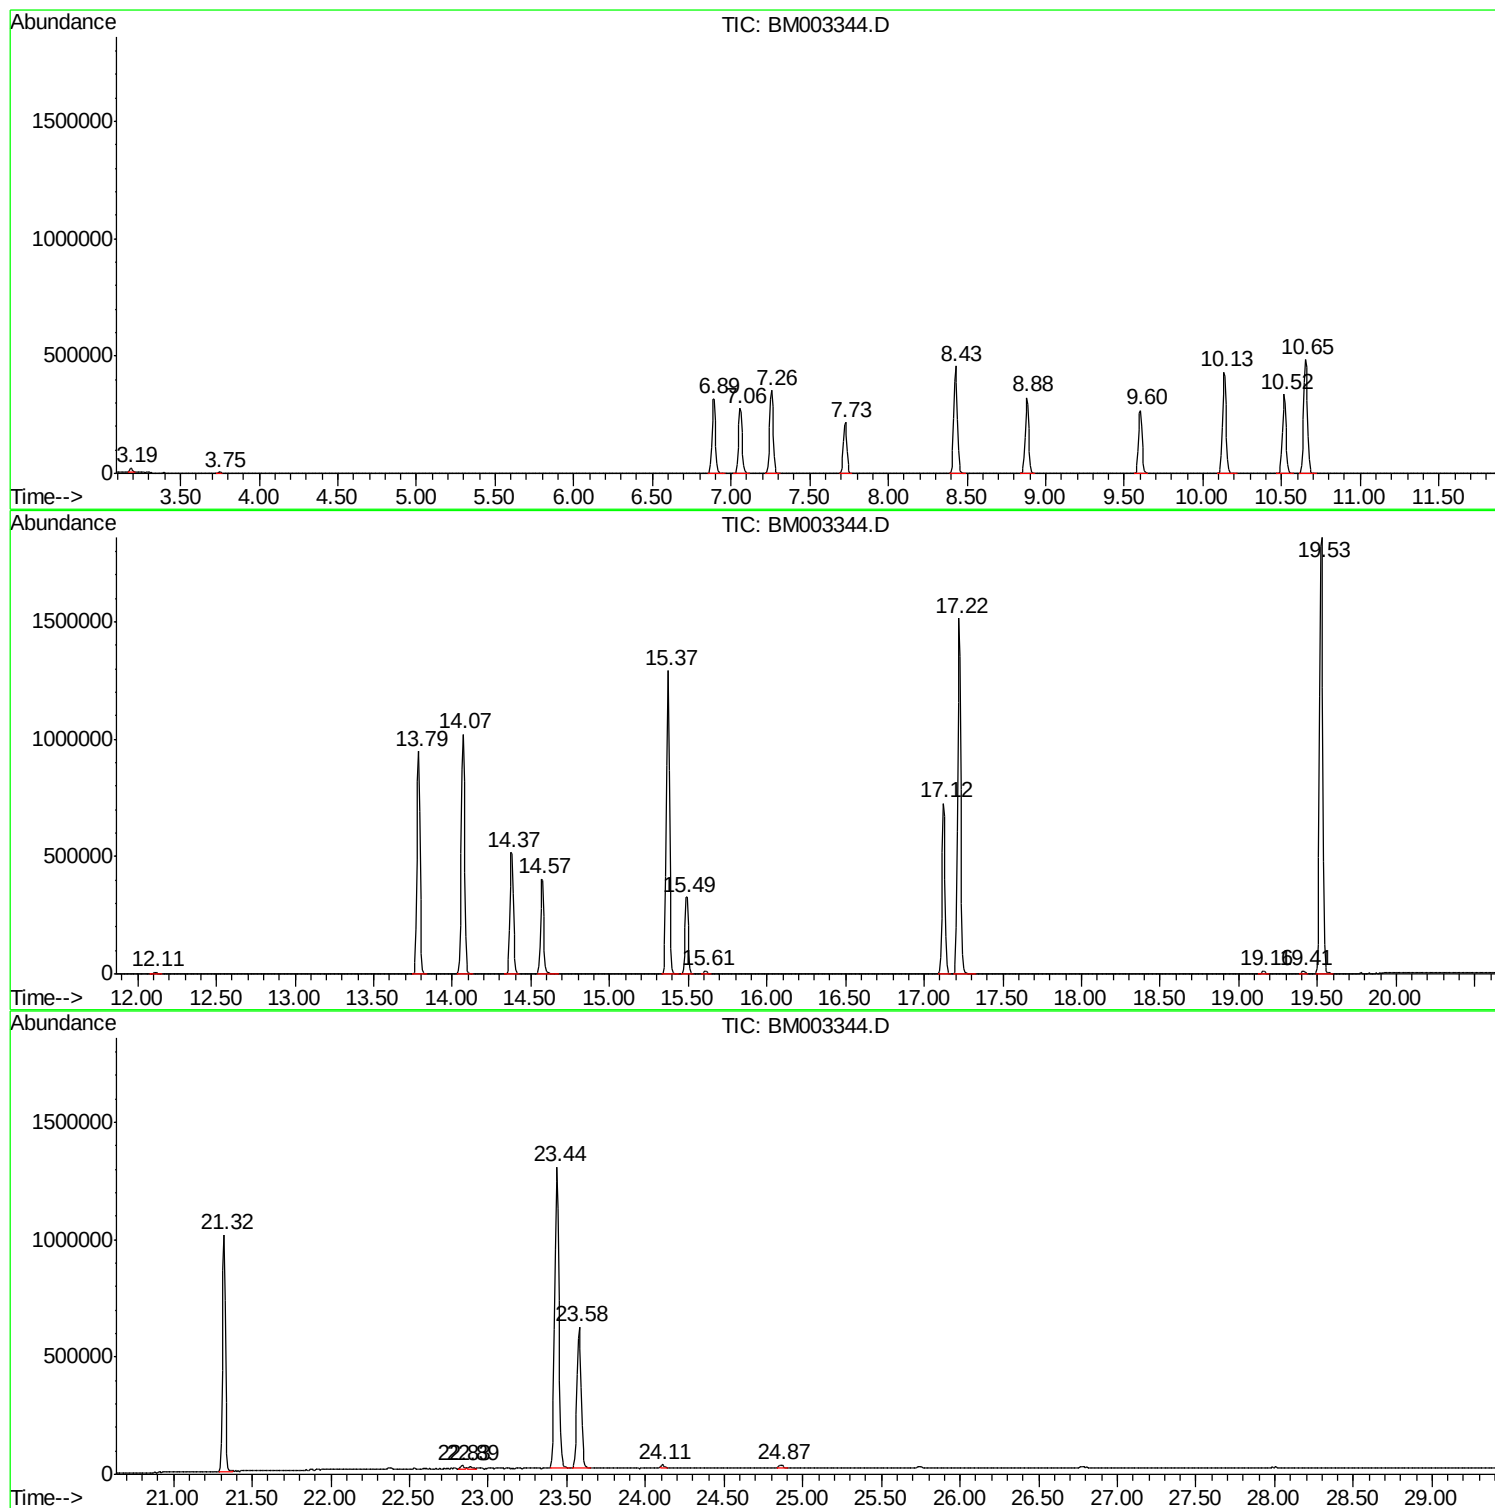

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003344.D
Acq On : 01 Dec 2015 20:16
Operator : UM/IZ
Sample : PB86966TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB03

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003344.D
Acq On : 01 Dec 2015 20:16
Operator : UM/IZ
Sample : PB86966TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB03

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc