

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003345.D
 Acq On : 01 Dec 2015 20:52
 Operator : UM/IZ
 Sample : G4545-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA761

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	21	rVB3	1578	1769	0.11%	0.012%
2	6.886	641	646	655	rBB2	28921	45701	2.89%	0.301%
3	7.057	669	675	683	rBB	123769	182023	11.50%	1.201%
4	7.257	703	709	716	rBB	121043	182273	11.52%	1.202%
5	7.728	782	789	796	rBB	264072	414285	26.18%	2.733%
6	8.428	902	908	915	rBB	113001	170922	10.80%	1.128%
7	8.880	979	985	993	rBB	144717	226801	14.33%	1.496%
8	9.304	1053	1057	1060	rBB	2540	3394	0.21%	0.022%
9	9.604	1102	1108	1114	rBB	120251	187208	11.83%	1.235%
10	10.133	1192	1198	1208	rBB	221697	357971	22.62%	2.362%
11	10.516	1256	1263	1268	rBV	402536	668433	42.24%	4.410%
12	10.569	1268	1272	1279	rVB	73536	116226	7.34%	0.767%
13	10.657	1282	1287	1289	rBV	3052	4819	0.30%	0.032%
14	12.110	1530	1534	1537	rBB	2807	3622	0.23%	0.024%
15	12.186	1542	1547	1552	rBB	17885	26270	1.66%	0.173%
16	12.404	1580	1584	1588	rBB	5258	7491	0.47%	0.049%
17	12.721	1634	1638	1642	rBB	5981	7191	0.45%	0.047%
18	12.974	1677	1681	1685	rBB	10239	13383	0.85%	0.088%
19	13.204	1716	1720	1724	rBB	2029	2523	0.16%	0.017%
20	13.786	1812	1819	1823	rBV	606807	851636	53.82%	5.618%
21	13.827	1823	1826	1832	rVB	70175	92721	5.86%	0.612%
22	14.068	1860	1867	1875	rVV	624634	888934	56.17%	5.864%
23	14.280	1898	1903	1907	rBB	6089	7628	0.48%	0.050%
24	14.374	1912	1919	1926	rBV2	614658	949880	60.03%	6.266%
25	14.439	1926	1930	1935	rVV	5677	7868	0.50%	0.052%
26	14.510	1937	1942	1946	rBV	3307	4603	0.29%	0.030%
27	14.568	1948	1952	1963	rBB	30846	48373	3.06%	0.319%
28	14.780	1983	1988	1991	rVB	5251	7686	0.49%	0.051%
29	15.180	2051	2056	2057	rBV	4321	5301	0.33%	0.035%
30	15.198	2057	2059	2062	rVV	6645	6919	0.44%	0.046%
31	15.227	2062	2064	2068	rVB	9637	11063	0.70%	0.073%
32	15.368	2082	2088	2094	rBV	875637	1261686	79.73%	8.324%
33	15.421	2094	2097	2103	rVV	10412	14129	0.89%	0.093%
34	15.486	2103	2108	2116	rVV	219076	289657	18.30%	1.911%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003345.D
 Acq On : 01 Dec 2015 20:52
 Operator : UM/IZ
 Sample : G4545-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA761

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.609	2125	2129	2132	rVV	7895	11217	0.71%	0.074%
36	15.639	2132	2134	2139	rVB	3870	4488	0.28%	0.030%
37	15.727	2145	2149	2154	rBB4	4335	8348	0.53%	0.055%
38	15.851	2164	2170	2174	rVV4	4694	7039	0.44%	0.046%
39	15.945	2182	2186	2189	rVB	2650	2633	0.17%	0.017%
40	16.098	2204	2212	2220	rVV3	21067	39643	2.51%	0.262%
41	16.168	2220	2224	2228	rVB3	1417	1846	0.12%	0.012%
42	16.268	2237	2241	2244	rBV	13318	16166	1.02%	0.107%
43	16.298	2244	2246	2248	rVV	5199	6000	0.38%	0.040%
44	16.321	2248	2250	2253	rVB2	4525	4637	0.29%	0.031%
45	16.362	2253	2257	2260	rVB	1687	1939	0.12%	0.013%
46	16.427	2262	2268	2273	rBV4	1928	4044	0.26%	0.027%
47	16.515	2278	2283	2287	rVB2	3763	6666	0.42%	0.044%
48	16.674	2304	2310	2312	rBV2	1556	2527	0.16%	0.017%
49	16.774	2317	2327	2331	rBV	43446	62055	3.92%	0.409%
50	16.839	2336	2338	2342	rVV2	2584	3661	0.23%	0.024%
51	16.886	2342	2346	2351	rVV2	17845	25831	1.63%	0.170%
52	16.939	2351	2355	2359	rVV2	7641	12802	0.81%	0.084%
53	17.045	2368	2373	2377	rVB2	7999	11445	0.72%	0.076%
54	17.121	2380	2386	2391	rBV2	790383	1113021	70.33%	7.343%
55	17.162	2391	2393	2397	rVV	29427	38382	2.43%	0.253%
56	17.221	2397	2403	2414	rVV2	1007821	1402266	88.61%	9.251%
57	17.315	2416	2419	2422	rVB3	4872	4701	0.30%	0.031%
58	17.356	2422	2426	2432	rBV2	3602	6251	0.40%	0.041%
59	17.415	2432	2436	2445	rVB4	3705	8382	0.53%	0.055%
60	17.498	2445	2450	2451	rBV2	3052	4242	0.27%	0.028%
61	17.527	2451	2455	2462	rVB	9436	15826	1.00%	0.104%
62	17.621	2467	2471	2475	rBV	14331	17536	1.11%	0.116%
63	17.709	2482	2486	2488	rBV2	2479	2831	0.18%	0.019%
64	17.798	2495	2501	2504	rBV4	5141	7109	0.45%	0.047%
65	17.915	2513	2521	2526	rBV5	5654	12500	0.79%	0.082%
66	17.986	2528	2533	2535	rBV2	10346	16142	1.02%	0.106%
67	18.015	2535	2538	2541	rVV	20231	24785	1.57%	0.164%
68	18.050	2541	2544	2546	rVV	4537	6575	0.42%	0.043%
69	18.092	2547	2551	2556	rVB	21554	25508	1.61%	0.168%
70	18.192	2560	2568	2572	rBV3	4045	7410	0.47%	0.049%
71	18.256	2577	2579	2582	rVV2	2359	2153	0.14%	0.014%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003345.D
 Acq On : 01 Dec 2015 20:52
 Operator : UM/IZ
 Sample : G4545-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA761

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

72	18.321	2584	2590	2594	rBV4	5415	9245	0.58%	0.061%
73	18.545	2617	2628	2632	rBV4	22689	32513	2.05%	0.214%
74	18.603	2636	2638	2641	rVV3	1754	2026	0.13%	0.013%
75	18.780	2665	2668	2670	rBV2	2155	2246	0.14%	0.015%
76	18.874	2680	2684	2690	rBV3	4400	7600	0.48%	0.050%
77	18.956	2693	2698	2701	rVB2	2481	3418	0.22%	0.023%
78	19.062	2712	2716	2724	rVB	4759	7009	0.44%	0.046%
79	19.156	2728	2732	2734	rVV	10340	12403	0.78%	0.082%
80	19.186	2734	2737	2743	rVB	15211	19321	1.22%	0.127%
81	19.303	2753	2757	2766	rBV3	13520	20149	1.27%	0.133%
82	19.409	2770	2775	2782	rVB2	7693	13023	0.82%	0.086%
83	19.521	2788	2794	2807	rBV	1154565	1582459	100.00%	10.440%
84	20.068	2885	2887	2891	rBV2	1298	1839	0.12%	0.012%
85	20.303	2924	2927	2931	rBV2	9538	9954	0.63%	0.066%
86	20.456	2947	2953	2959	rBV4	3943	8995	0.57%	0.059%
87	20.550	2966	2969	2970	rBV3	1606	1875	0.12%	0.012%
88	20.874	3021	3024	3026	rBV4	1905	2024	0.13%	0.013%
89	21.027	3047	3050	3059	rBV3	18021	32373	2.05%	0.214%
90	21.091	3059	3061	3066	rVB2	3555	5087	0.32%	0.034%
91	21.233	3082	3085	3090	rBV2	6634	8469	0.54%	0.056%
92	21.321	3094	3100	3106	rBV	875452	1116279	70.54%	7.364%
93	21.556	3138	3140	3142	rBV2	3162	2340	0.15%	0.015%
94	22.374	3275	3279	3283	rBV	11047	15294	0.97%	0.101%
95	22.885	3362	3366	3372	rVB3	15900	24391	1.54%	0.161%
96	23.432	3452	3459	3471	rVB	594055	1113090	70.34%	7.343%
97	23.580	3476	3484	3493	rVB	515268	983160	62.13%	6.486%
98	24.109	3570	3574	3580	rVB	21044	35292	2.23%	0.233%
99	24.862	3697	3702	3708	rVB2	17880	36841	2.33%	0.243%
100	25.738	3846	3851	3860	rVB5	12903	30401	1.92%	0.201%


Sum of corrected areas: 15158112

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003345.D
Acq On : 01 Dec 2015 20:52
Operator : UM/IZ
Sample : G4545-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
CA761

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

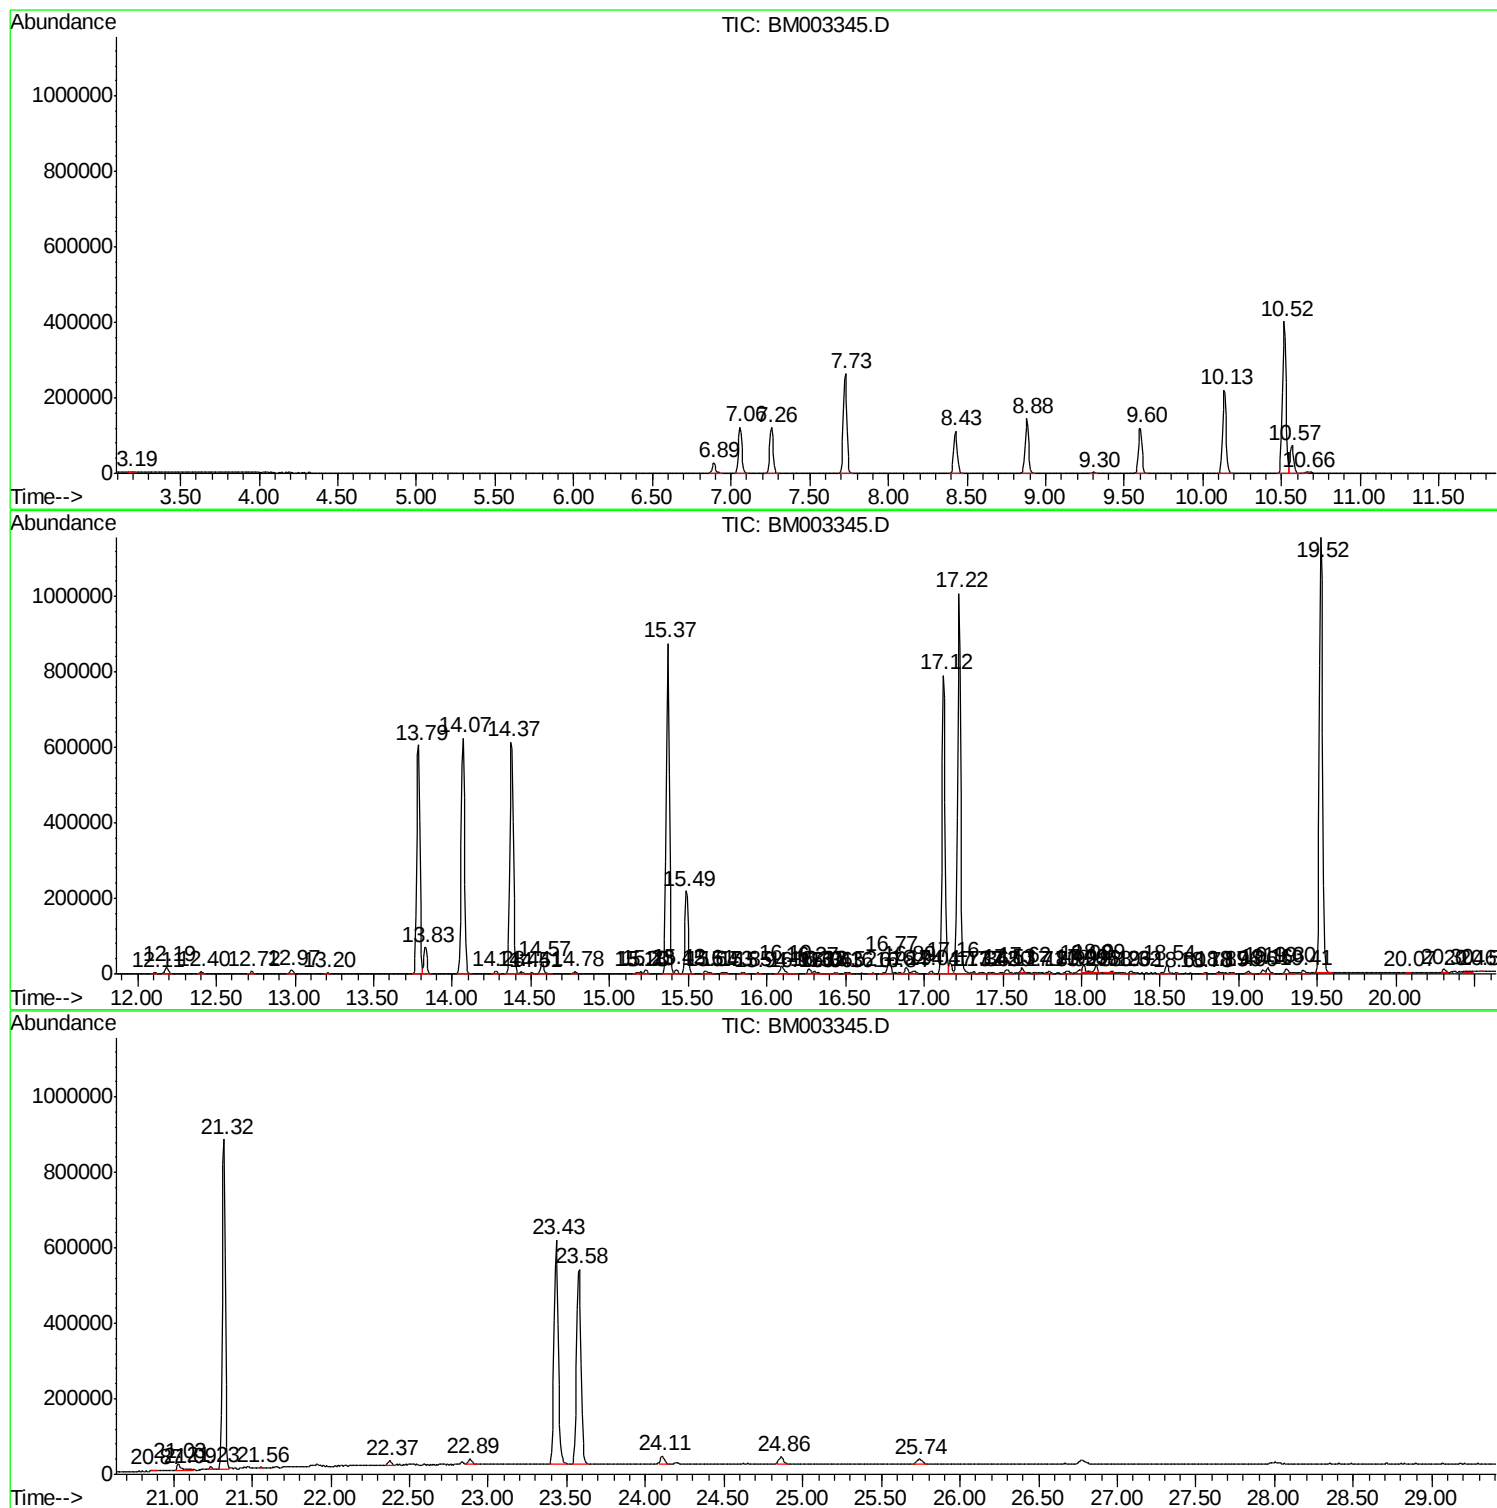

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003345.D
Acq On : 01 Dec 2015 20:52
Operator : UM/IZ
Sample : G4545-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA761

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003345.D
Acq On : 01 Dec 2015 20:52
Operator : UM/IZ
Sample : G4545-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA761

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc