

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003346.D
 Acq On : 01 Dec 2015 21:28
 Operator : UM/IZ
 Sample : G4545-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA782

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	22	rVB2	2513	3612	0.18%	0.019%
2	6.886	641	646	655	rBB	52481	82387	4.10%	0.444%
3	7.057	669	675	684	rBB	182584	274038	13.63%	1.477%
4	7.257	703	709	717	rBB	191030	289428	14.39%	1.560%
5	7.728	782	789	795	rBB	271817	425163	21.15%	2.292%
6	8.428	902	908	916	rBB	181996	275423	13.70%	1.485%
7	8.880	979	985	993	rBB	221158	342117	17.02%	1.844%
8	9.304	1053	1057	1060	rBB	2478	3533	0.18%	0.019%
9	9.604	1101	1108	1114	rBB	180384	288807	14.36%	1.557%
10	10.133	1192	1198	1209	rBB	318344	510490	25.39%	2.752%
11	10.516	1256	1263	1270	rBV	419699	690093	34.32%	3.720%
12	10.569	1270	1272	1277	rVB	5321	6304	0.31%	0.034%
13	10.651	1281	1286	1294	rBB	14587	22952	1.14%	0.124%
14	10.869	1319	1323	1327	rBB	5898	8575	0.43%	0.046%
15	11.904	1495	1499	1503	rBB	5015	6910	0.34%	0.037%
16	12.110	1530	1534	1538	rBB2	4031	5869	0.29%	0.032%
17	12.186	1543	1547	1550	rBB	2573	3361	0.17%	0.018%
18	12.404	1580	1584	1588	rBB	3896	5685	0.28%	0.031%
19	12.721	1634	1638	1642	rBB	4723	5467	0.27%	0.029%
20	12.974	1678	1681	1685	rBB	7781	10048	0.50%	0.054%
21	13.786	1812	1819	1823	rBV	784261	1084925	53.96%	5.849%
22	13.827	1823	1826	1832	rVB	56216	73628	3.66%	0.397%
23	14.068	1860	1867	1877	rVB	833224	1188428	59.11%	6.407%
24	14.280	1899	1903	1907	rBB	8173	10102	0.50%	0.054%
25	14.374	1913	1919	1926	rBV2	647941	992189	49.35%	5.349%
26	14.439	1926	1930	1935	rVB	58605	79518	3.95%	0.429%
27	14.504	1936	1941	1946	rBB	10196	13145	0.65%	0.071%
28	14.568	1947	1952	1963	rBB	60112	89053	4.43%	0.480%
29	14.774	1982	1987	1992	rVB	33178	44969	2.24%	0.242%
30	15.174	2052	2055	2057	rBV	3979	4670	0.23%	0.025%
31	15.198	2057	2059	2061	rVV	3606	4199	0.21%	0.023%
32	15.233	2061	2065	2068	rVB	13763	16785	0.83%	0.090%
33	15.368	2082	2088	2094	rBV	1125059	1638301	81.48%	8.833%
34	15.427	2094	2098	2103	rVV2	41019	53563	2.66%	0.289%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003346.D
 Acq On : 01 Dec 2015 21:28
 Operator : UM/IZ
 Sample : G4545-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA782

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.486	2103	2108	2117	rVV	300822	408744	20.33%	2.204%
36	15.609	2124	2129	2132	rBV	12076	17189	0.85%	0.093%
37	15.639	2132	2134	2138	rVB3	4361	4898	0.24%	0.026%
38	15.721	2145	2148	2153	rBB4	5310	9215	0.46%	0.050%
39	15.792	2155	2160	2162	rBV2	2327	2868	0.14%	0.015%
40	15.856	2167	2171	2176	rVV5	4182	8650	0.43%	0.047%
41	15.945	2178	2186	2191	rBV	3775	6119	0.30%	0.033%
42	16.092	2207	2211	2219	rVV3	28014	52188	2.60%	0.281%
43	16.162	2219	2223	2227	rVB4	2957	4213	0.21%	0.023%
44	16.268	2235	2241	2244	rVV2	14030	18871	0.94%	0.102%
45	16.298	2244	2246	2253	rVV2	7843	14989	0.75%	0.081%
46	16.356	2253	2256	2260	rVB3	2664	4163	0.21%	0.022%
47	16.433	2265	2269	2270	rBV2	3457	3452	0.17%	0.019%
48	16.515	2277	2283	2287	rBV4	5023	8508	0.42%	0.046%
49	16.551	2287	2289	2292	rVB2	2231	2516	0.13%	0.014%
50	16.598	2292	2297	2303	rBV5	3631	8310	0.41%	0.045%
51	16.662	2303	2308	2311	rBV	1832	2795	0.14%	0.015%
52	16.698	2311	2314	2317	rVB3	2658	2337	0.12%	0.013%
53	16.774	2321	2327	2332	rBV	79601	107600	5.35%	0.580%
54	16.886	2342	2346	2351	rBV2	22342	27768	1.38%	0.150%
55	16.939	2351	2355	2361	rVB	13924	20320	1.01%	0.110%
56	17.045	2367	2373	2379	rVB2	7578	10482	0.52%	0.057%
57	17.121	2380	2386	2391	rVV2	809443	1171563	58.27%	6.316%
58	17.162	2391	2393	2397	rVV	63694	79315	3.94%	0.428%
59	17.221	2397	2403	2414	rVV2	1279050	1845955	91.81%	9.952%
60	17.315	2416	2419	2424	rVB3	3983	4563	0.23%	0.025%
61	17.368	2424	2428	2432	rBV3	2834	4710	0.23%	0.025%
62	17.415	2433	2436	2443	rVB4	3515	7385	0.37%	0.040%
63	17.498	2443	2450	2451	rBV4	3951	6331	0.31%	0.034%
64	17.527	2451	2455	2461	rVB	22303	32109	1.60%	0.173%
65	17.621	2467	2471	2477	rBV2	16800	20896	1.04%	0.113%
66	17.703	2482	2485	2491	rVV	1854	2887	0.14%	0.016%
67	17.798	2497	2501	2507	rVB4	4363	5998	0.30%	0.032%
68	17.915	2513	2521	2525	rBV4	8664	16848	0.84%	0.091%
69	17.980	2528	2532	2534	rBV2	9056	11762	0.58%	0.063%
70	18.015	2534	2538	2542	rVB	30442	33630	1.67%	0.181%
71	18.092	2548	2551	2555	rVB	12233	13971	0.69%	0.075%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003346.D
 Acq On : 01 Dec 2015 21:28
 Operator : UM/IZ
 Sample : G4545-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA782

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

72	18.192	2561	2568	2573	rBV3	8038	13912	0.69%	0.075%
73	18.233	2573	2575	2578	rVB3	2500	2459	0.12%	0.013%
74	18.321	2586	2590	2593	rBV3	5167	6832	0.34%	0.037%
75	18.374	2597	2599	2602	rBV	2378	2776	0.14%	0.015%
76	18.545	2623	2628	2632	rVV3	20760	28931	1.44%	0.156%
77	18.615	2635	2640	2642	rBV3	1626	2684	0.13%	0.014%
78	18.756	2660	2664	2666	rBV2	1530	2098	0.10%	0.011%
79	18.786	2666	2669	2672	rVV4	2067	2915	0.14%	0.016%
80	18.880	2680	2685	2693	rBV4	5089	11255	0.56%	0.061%
81	18.950	2693	2697	2700	rBV3	1750	2867	0.14%	0.015%
82	19.062	2713	2716	2721	rVB	5245	6557	0.33%	0.035%
83	19.156	2728	2732	2734	rBV	14363	17473	0.87%	0.094%
84	19.186	2734	2737	2742	rVB	21402	24410	1.21%	0.132%
85	19.303	2752	2757	2766	rBV3	20608	30819	1.53%	0.166%
86	19.409	2772	2775	2782	rVB	10625	15447	0.77%	0.083%
87	19.521	2788	2794	2808	rVV	1409948	2010644	100.00%	10.840%
88	20.386	2939	2941	2943	rBV2	2332	2387	0.12%	0.013%
89	20.556	2967	2970	2971	rBV2	2324	2844	0.14%	0.015%
90	20.680	2988	2991	2994	rBV4	1868	2246	0.11%	0.012%
91	20.709	2994	2996	3000	rBV4	1658	2467	0.12%	0.013%
92	20.874	3022	3024	3028	rVB4	3436	4071	0.20%	0.022%
93	21.033	3047	3051	3060	rBV2	23249	39006	1.94%	0.210%
94	21.238	3082	3086	3090	rBV	17231	21235	1.06%	0.114%
95	21.321	3094	3100	3109	rBV	911557	1136921	56.55%	6.129%
96	22.374	3276	3279	3283	rVB3	8481	12954	0.64%	0.070%
97	22.838	3355	3358	3362	rVB2	9080	11964	0.60%	0.065%
98	23.432	3452	3459	3468	rBV	835356	1558450	77.51%	8.402%
99	23.580	3476	3484	3495	rVB2	515775	989758	49.23%	5.336%
100	24.109	3571	3574	3583	rVB5	13030	24278	1.21%	0.131%


Sum of corrected areas: 18548515

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003346.D
Acq On : 01 Dec 2015 21:28
Operator : UM/IZ
Sample : G4545-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA782

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

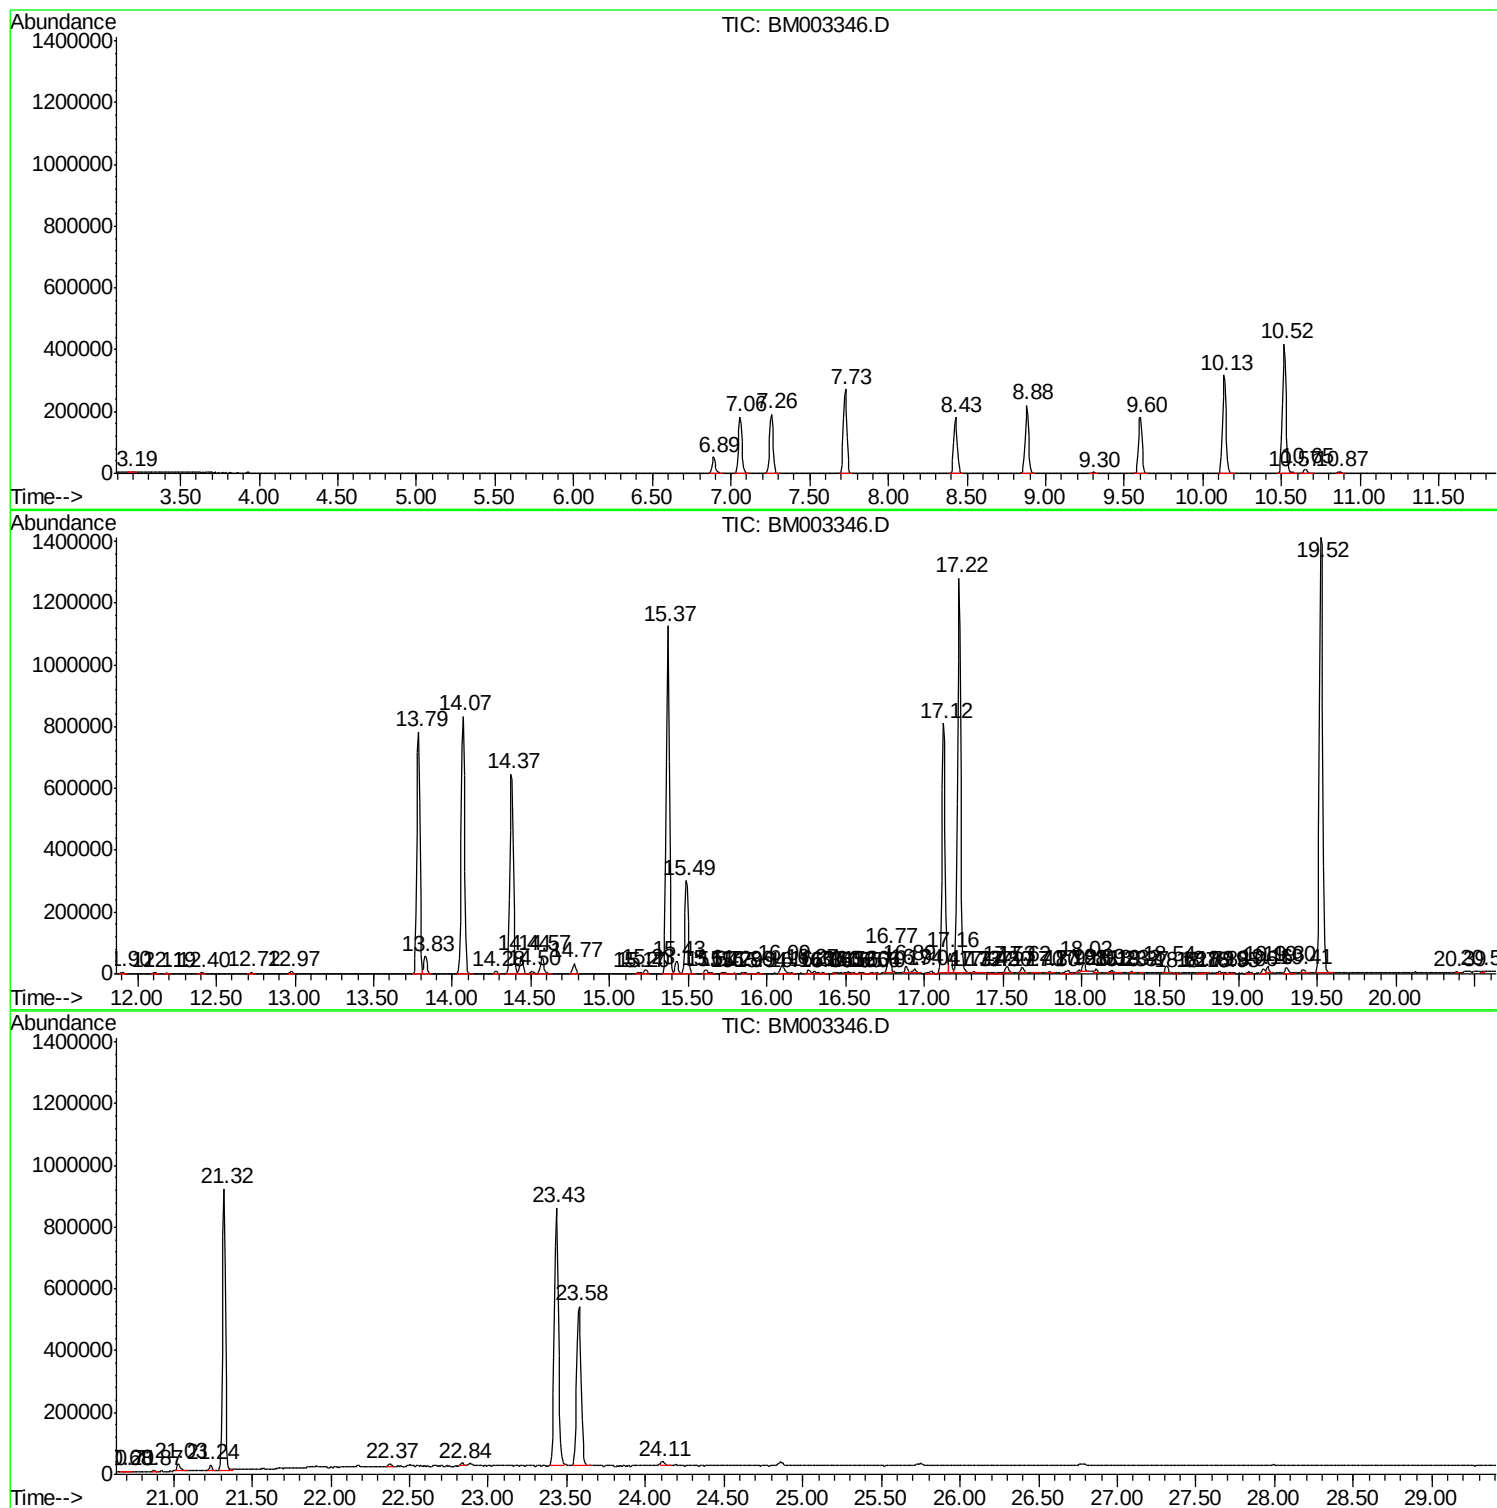

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003346.D
Acq On : 01 Dec 2015 21:28
Operator : UM/IZ
Sample : G4545-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA782

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003346.D
Acq On : 01 Dec 2015 21:28
Operator : UM/IZ
Sample : G4545-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA782

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc