

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003347.D
 Acq On : 01 Dec 2015 22:04
 Operator : UM/IZ
 Sample : G4545-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA785

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	21	rVB	2314	2380	0.13%	0.014%
2	4.845	295	299	302	rVB	1336	2070	0.11%	0.012%
3	6.834	633	637	640	rBB	4535	5065	0.27%	0.029%
4	6.886	641	646	654	rBB	50646	76669	4.04%	0.441%
5	7.057	669	675	683	rBB	185885	281981	14.86%	1.624%
6	7.257	703	709	716	rBB	193760	295938	15.60%	1.704%
7	7.728	782	789	795	rBB	249490	386933	20.40%	2.228%
8	8.428	902	908	916	rBB	183098	281600	14.84%	1.621%
9	8.880	978	985	993	rBB	230463	360307	18.99%	2.074%
10	9.304	1053	1057	1060	rBB	2229	2869	0.15%	0.017%
11	9.604	1101	1108	1114	rBB	188737	304559	16.05%	1.754%
12	9.916	1158	1161	1165	rBB2	2153	2550	0.13%	0.015%
13	10.133	1192	1198	1208	rBV	345978	557180	29.37%	3.208%
14	10.516	1256	1263	1270	rBV	379572	624768	32.93%	3.597%
15	10.651	1280	1286	1292	rBB	10450	16027	0.84%	0.092%
16	11.904	1496	1499	1502	rBB2	2547	3034	0.16%	0.017%
17	12.110	1530	1534	1538	rBB	4522	6365	0.34%	0.037%
18	12.721	1635	1638	1642	rBB	4225	4853	0.26%	0.028%
19	12.974	1676	1681	1685	rBB	7483	9532	0.50%	0.055%
20	13.539	1774	1777	1781	rBB2	2035	2678	0.14%	0.015%
21	13.692	1800	1803	1806	rBB2	1396	2066	0.11%	0.012%
22	13.745	1809	1812	1813	rBV	2017	1992	0.10%	0.011%
23	13.786	1813	1819	1824	rVV	811590	1111906	58.61%	6.402%
24	13.827	1824	1826	1831	rVB	17701	21564	1.14%	0.124%
25	14.010	1854	1857	1859	rBV	2992	3666	0.19%	0.021%
26	14.068	1861	1867	1881	rVB	859482	1249299	65.85%	7.193%
27	14.280	1898	1903	1907	rBV2	4478	6530	0.34%	0.038%
28	14.374	1913	1919	1927	rBV2	558740	878112	46.28%	5.056%
29	14.439	1927	1930	1933	rVB	1799	2068	0.11%	0.012%
30	14.568	1947	1952	1958	rBV	48907	75691	3.99%	0.436%
31	14.786	1985	1989	1992	rBB	2738	4526	0.24%	0.026%
32	15.039	2028	2032	2034	rBB	2352	3022	0.16%	0.017%
33	15.174	2052	2055	2057	rBV	3217	3846	0.20%	0.022%
34	15.192	2057	2058	2061	rVV	3180	3641	0.19%	0.021%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003347.D
 Acq On : 01 Dec 2015 22:04
 Operator : UM/IZ
 Sample : G4545-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA785

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.227	2061	2064	2068	rVB	6098	8452	0.45%	0.049%
36	15.368	2082	2088	2095	rBV	1163730	1682064	88.66%	9.685%
37	15.421	2095	2097	2100	rVB	2324	2533	0.13%	0.015%
38	15.486	2102	2108	2116	rBV	314215	425320	22.42%	2.449%
39	15.551	2116	2119	2123	rVB2	10481	14647	0.77%	0.084%
40	15.609	2123	2129	2139	rBV3	11655	21556	1.14%	0.124%
41	15.721	2142	2148	2156	rVB4	4113	9763	0.51%	0.056%
42	15.845	2167	2169	2172	rVB2	5126	5278	0.28%	0.030%
43	15.945	2183	2186	2191	rVB4	4288	5298	0.28%	0.031%
44	15.998	2191	2195	2199	rBV4	3439	5961	0.31%	0.034%
45	16.092	2207	2211	2214	rBV3	9976	16015	0.84%	0.092%
46	16.209	2229	2231	2234	rBV3	1796	2029	0.11%	0.012%
47	16.245	2234	2237	2238	rVV2	2563	2986	0.16%	0.017%
48	16.268	2238	2241	2245	rVV	14507	20053	1.06%	0.115%
49	16.321	2248	2250	2254	rVB2	6705	7274	0.38%	0.042%
50	16.362	2254	2257	2263	rBV6	3077	6068	0.32%	0.035%
51	16.445	2266	2271	2275	rBV4	2116	4615	0.24%	0.027%
52	16.521	2281	2284	2287	rVB3	3514	4727	0.25%	0.027%
53	16.592	2292	2296	2298	rBV4	2430	3877	0.20%	0.022%
54	16.609	2298	2299	2304	rVB4	3190	3458	0.18%	0.020%
55	16.721	2313	2318	2322	rVB3	9368	13033	0.69%	0.075%
56	16.774	2324	2327	2330	rBV2	6328	7972	0.42%	0.046%
57	16.809	2330	2333	2335	rVB3	2541	2614	0.14%	0.015%
58	16.886	2339	2346	2353	rBV9	10516	19973	1.05%	0.115%
59	16.986	2359	2363	2365	rBV4	1699	2743	0.14%	0.016%
60	17.045	2367	2373	2376	rVV2	6898	10828	0.57%	0.062%
61	17.121	2380	2386	2392	rVV2	690529	996969	52.55%	5.740%
62	17.168	2392	2394	2396	rVV	4033	4237	0.22%	0.024%
63	17.221	2396	2403	2413	rVV2	1264066	1777737	93.70%	10.235%
64	17.321	2416	2420	2423	rVB5	4080	5016	0.26%	0.029%
65	17.474	2444	2446	2448	rBV3	2873	3482	0.18%	0.020%
66	17.539	2455	2457	2461	rVB4	2607	2880	0.15%	0.017%
67	17.603	2464	2468	2469	rVV2	5442	7273	0.38%	0.042%
68	17.621	2469	2471	2479	rVB2	8017	10626	0.56%	0.061%
69	17.792	2497	2500	2506	rVB2	27529	33852	1.78%	0.195%
70	17.915	2516	2521	2525	rVB6	5095	8114	0.43%	0.047%
71	17.986	2529	2533	2535	rBV3	6571	9553	0.50%	0.055%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
 Data File : BM003347.D
 Acq On : 01 Dec 2015 22:04
 Operator : UM/IZ
 Sample : G4545-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CA785

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

72	18.015	2535	2538	2542	rVV	40626	52531	2.77%	0.302%
73	18.056	2542	2545	2548	rVV2	11431	15158	0.80%	0.087%
74	18.092	2548	2551	2555	rVB	14369	17441	0.92%	0.100%
75	18.321	2584	2590	2592	rBV4	5127	8889	0.47%	0.051%
76	18.445	2609	2611	2614	rBV4	4100	2846	0.15%	0.016%
77	18.545	2625	2628	2631	rVB3	5825	6169	0.33%	0.036%
78	18.762	2663	2665	2668	rBV3	2149	2494	0.13%	0.014%
79	18.939	2693	2695	2696	rBV2	2955	2770	0.15%	0.016%
80	19.156	2727	2732	2735	rBV	16609	23604	1.24%	0.136%
81	19.303	2753	2757	2767	rBV2	38383	57954	3.05%	0.334%
82	19.409	2771	2775	2779	rVB	12575	15989	0.84%	0.092%
83	19.521	2788	2794	2802	rBV	1364854	1897194	100.00%	10.923%
84	19.609	2807	2809	2813	rVB5	3601	3393	0.18%	0.020%
85	19.639	2813	2814	2816	rBV2	2679	2090	0.11%	0.012%
86	20.050	2881	2884	2885	rBV3	2361	2694	0.14%	0.016%
87	20.127	2895	2897	2900	rVV3	2989	2849	0.15%	0.016%
88	20.344	2930	2934	2936	rBV3	4124	5396	0.28%	0.031%
89	20.450	2950	2952	2957	rVB5	6607	7441	0.39%	0.043%
90	21.033	3047	3051	3059	rVB8	13486	21712	1.14%	0.125%
91	21.238	3082	3086	3089	rVB	10479	11649	0.61%	0.067%
92	21.321	3094	3100	3106	rBV	792320	986865	52.02%	5.682%
93	21.474	3123	3126	3131	rBV5	4382	7420	0.39%	0.043%
94	22.833	3355	3357	3361	rVB3	8447	9124	0.48%	0.053%
95	23.432	3451	3459	3475	rBV	829858	1550325	81.72%	8.926%
96	23.580	3476	3484	3495	rVB2	463597	890361	46.93%	5.126%


Sum of corrected areas: 17368521

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003347.D
Acq On : 01 Dec 2015 22:04
Operator : UM/IZ
Sample : G4545-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA785

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

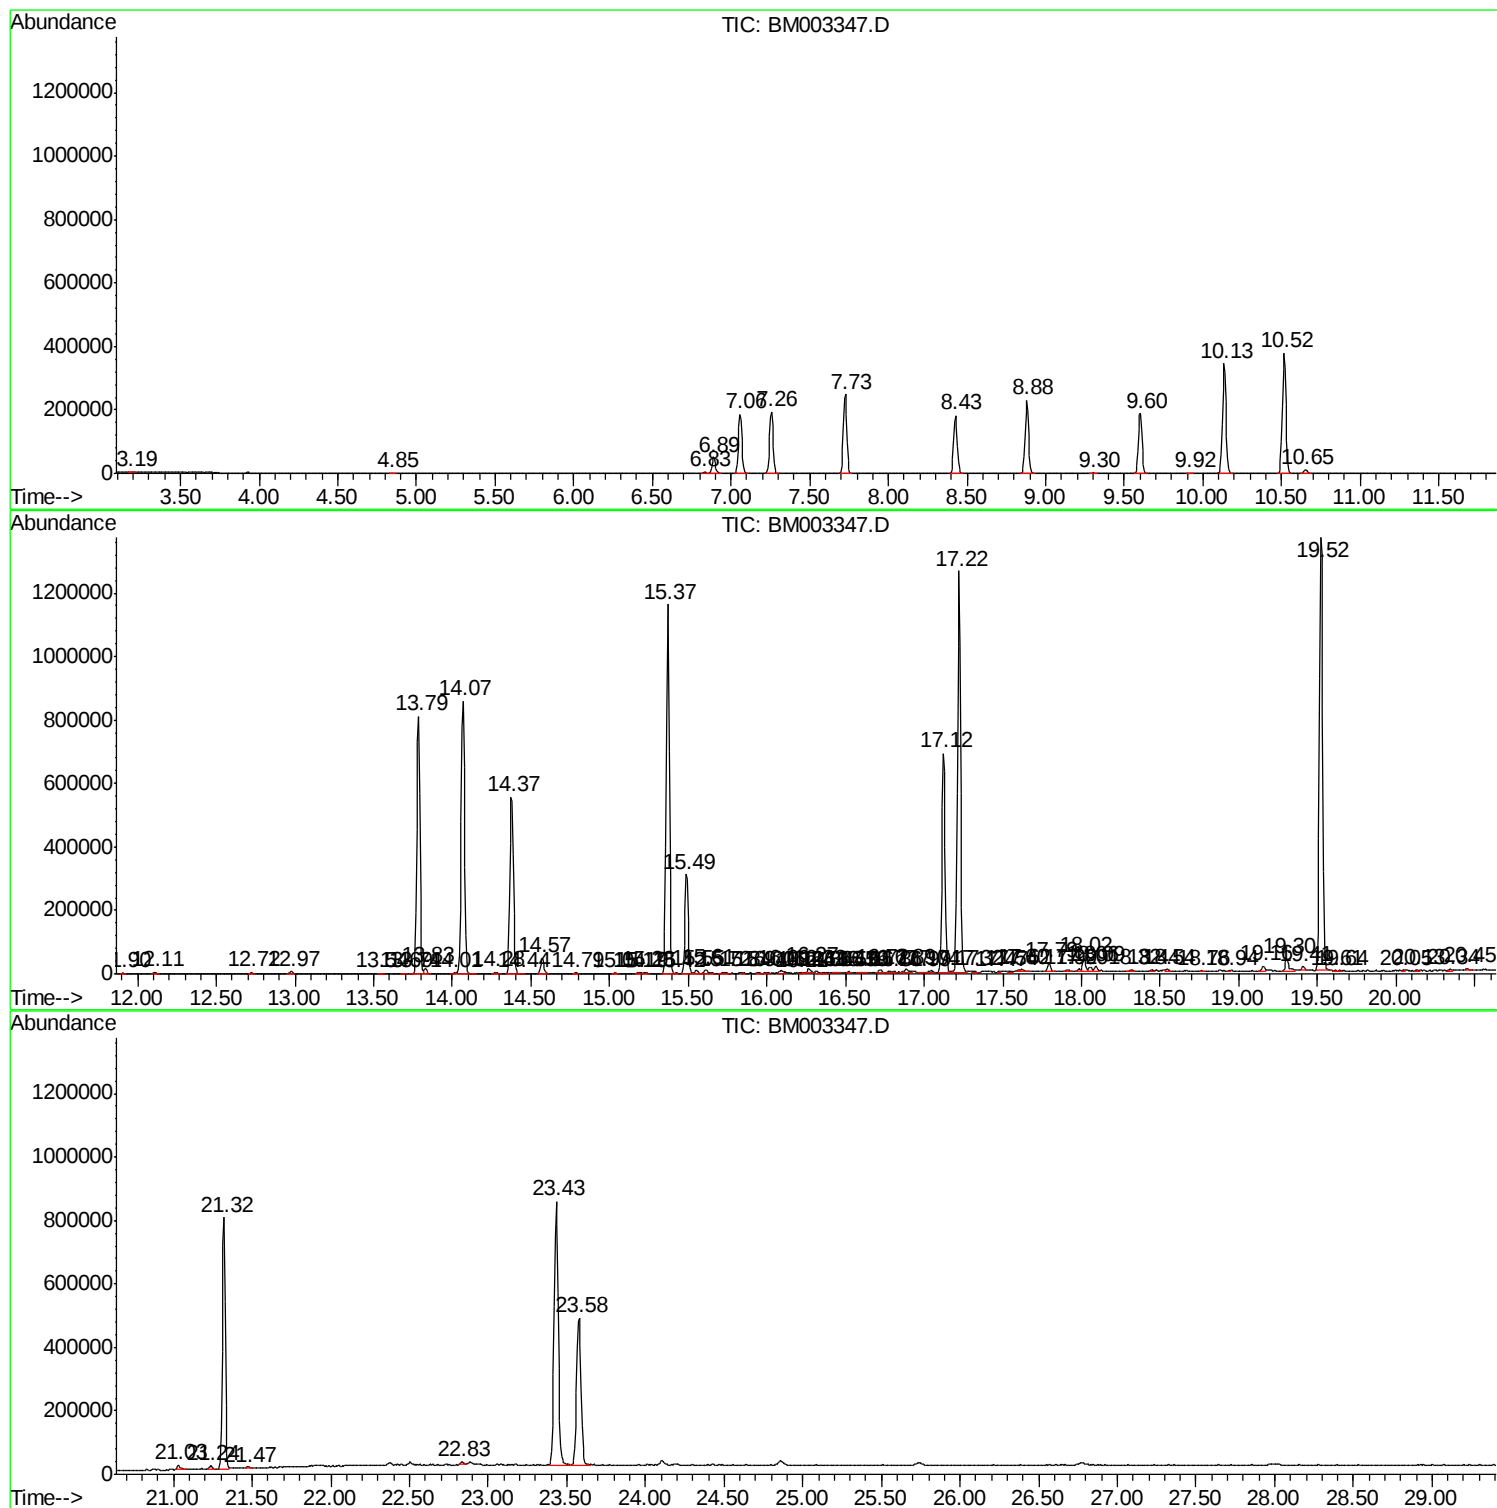

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003347.D
Acq On : 01 Dec 2015 22:04
Operator : UM/IZ
Sample : G4545-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA785

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120115\
Data File : BM003347.D
Acq On : 01 Dec 2015 22:04
Operator : UM/IZ
Sample : G4545-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CA785

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc