


Data Path : Z:\HPCHEM1\BNA M\DATA\BM120115\
Data File : BM003336.D
Acq On : 01 Dec 2015 15:28
Operator : UM/IZ
Sample : DFTPP52
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP52

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION
Last Update : Wed Dec 02 01:07:29 2015

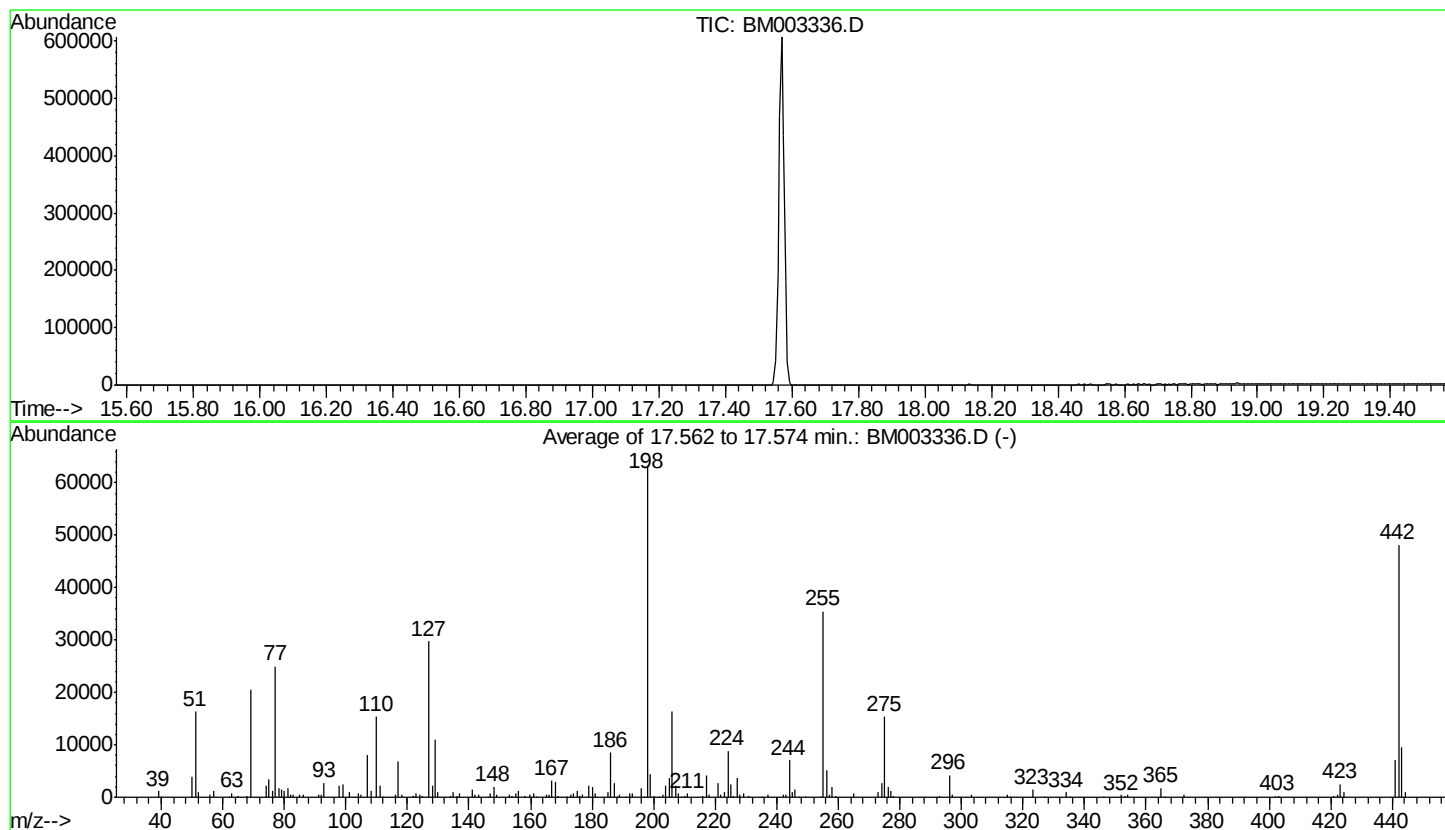

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	16311	PASS
68	69	0.00	2	1.7	345	PASS
69	198	0.00	100	32.4	20532	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	29744	PASS
197	198	0.00	2	0.2	111	PASS
198	198	100	100	100.0	63285	PASS
199	198	5	9	6.8	4316	PASS
275	198	10	60	24.3	15349	PASS
365	198	1	100	2.9	1826	PASS
441	443	0.01	100	76.2	7202	PASS
442	198	50	100	76.2	48250	PASS
443	442	15	24	19.6	9452	PASS

Scan 2456 (17.533 min): BM003336.D
DFTPP52

m/z	Abundance
44.00	344.0
207.10	578.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

m/z	Abundance
39.00	1234.0
40.00	315.0
44.00	326.0
50.00	4222.0
51.10	17608.0
52.00	877.0
56.00	523.0
57.00	1232.0
63.10	834.0
65.00	368.0
68.00	361.0
69.00	21848.0
74.00	2283.0
75.00	3735.0
76.00	1265.0
77.10	26288.0
78.00	2094.0
79.00	1634.0
80.00	1370.0
81.00	1954.0
81.90	463.0
83.00	468.0
85.00	396.0
85.90	529.0
91.00	451.0
92.00	603.0
93.00	3028.0
98.00	2420.0
99.00	2852.0
101.00	1036.0
104.00	730.0
105.00	609.0
107.00	8513.0
108.00	1321.0
110.00	15740.0
111.00	2505.0
116.00	420.0
117.00	6898.0
118.00	586.0
121.90	511.0
122.90	807.0
124.00	398.0
125.00	339.0
127.00	29616.0
128.00	2368.0
129.00	11093.0
130.00	1027.0
133.90	320.0
135.00	909.0
136.00	379.0
137.00	825.0
141.00	1398.0
142.00	498.0
143.00	386.0
147.10	703.0
148.00	1875.0
149.00	521.0
153.00	449.0
154.00	367.0
155.00	918.0
156.00	1259.0
158.00	302.0
159.90	371.0
161.00	730.0
165.00	531.0
166.00	444.0
167.00	3074.0
168.00	3490.0
169.00	373.0
173.00	308.0
174.00	637.0
175.00	1075.0
175.90	373.0
177.00	460.0
179.00	2033.0
180.00	2083.0
181.00	795.0
185.00	1045.0
186.00	7887.0
187.10	2376.0
189.00	445.0
192.00	745.0
193.00	869.0
196.00	1651.0
196.90	335.0
198.00	59128.0
199.00	4208.0
200.00	339.0
202.90	410.0
204.00	1947.0
205.00	3509.0
206.10	15345.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

207.10	2733.0
208.00	634.0
209.00	364.0
211.00	562.0
216.00	310.0
217.00	3916.0
218.00	482.0
221.10	2526.0
221.90	547.0
223.00	889.0
224.10	7954.0
225.00	2245.0
226.00	357.0
227.00	3449.0
228.00	547.0
229.00	673.0
237.10	568.0
241.90	366.0
243.00	318.0
244.10	6090.0
245.00	881.0
246.00	1403.0
255.10	30976.0
256.10	4765.0
257.00	563.0
258.00	1649.0
259.00	365.0
265.00	599.0
273.10	898.0
274.00	2276.0
275.10	13062.0
276.00	1762.0
277.00	1181.0
278.00	308.0
293.00	331.0
296.10	3413.0
297.00	539.0
303.00	442.0
315.10	397.0
323.10	1035.0
334.10	810.0
352.00	316.0
354.10	365.0
365.00	1338.0
372.10	434.0
403.10	311.0
422.00	308.0
423.10	1974.0
424.10	882.0
441.10	4911.0
442.10	33720.0
443.10	6862.0
444.10	640.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

m/z	Abundance
39.00	1416.0
50.10	4942.0
51.10	19200.0
52.00	1024.0
56.00	632.0
57.00	1470.0
62.00	313.0
63.00	913.0
65.10	458.0
68.00	374.0
69.00	24368.0
74.10	2601.0
75.00	4142.0
76.10	1496.0
77.10	29608.0
78.10	2063.0
79.00	1968.0
80.00	1393.0
81.00	2187.0
82.00	507.0
83.00	533.0
85.00	493.0
86.00	532.0
91.00	464.0
92.00	541.0
93.00	3275.0
98.00	2880.0
99.00	2849.0
101.00	1225.0
102.90	337.0
103.90	682.0
105.00	712.0
107.00	9619.0
108.00	1521.0
110.00	18200.0
111.00	2600.0
111.90	390.0
116.00	453.0
117.00	8301.0
118.00	657.0
122.10	610.0
123.00	875.0
124.00	488.0
125.00	404.0
127.00	35280.0
128.00	2765.0
129.00	13194.0
130.00	1078.0
133.90	353.0
135.00	1053.0
136.00	344.0
137.00	779.0
141.00	1852.0
142.00	496.0
143.00	507.0
146.00	339.0
147.00	992.0
148.00	2463.0
149.00	470.0
153.00	612.0
154.00	416.0
155.00	986.0
156.00	1368.0
158.00	310.0
159.90	546.0
161.00	935.0
161.90	306.0
165.00	655.0
166.00	533.0
167.00	3606.0
168.00	3249.0
169.00	387.0
172.00	318.0
173.00	503.0
174.00	832.0
175.10	1366.0
176.00	426.0
177.00	682.0
179.00	2590.0
180.00	2387.0
181.00	1021.0
185.00	1228.0
186.10	10281.0
187.00	3127.0
188.00	394.0
189.00	580.0
191.00	394.0
192.00	883.0
193.10	948.0
196.00	2037.0
198.00	76416.0
199.00	5123.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

200.00	388.0
201.60	319.0
203.00	526.0
204.10	2647.0
205.00	4447.0
206.10	19328.0
207.10	3360.0
208.00	804.0
210.10	409.0
211.10	759.0
216.00	411.0
217.00	5133.0
218.00	692.0
221.10	3049.0
221.90	723.0
223.00	1117.0
224.10	10598.0
225.00	2710.0
226.00	367.0
227.00	4473.0
228.00	666.0
229.00	1009.0
231.00	330.0
235.00	332.0
237.00	690.0
242.00	531.0
243.10	655.0
244.10	8687.0
245.10	1278.0
246.10	1794.0
247.00	314.0
249.00	301.0
254.10	338.0
255.10	42992.0
256.00	6216.0
257.00	618.0
258.00	2297.0
259.10	343.0
265.00	946.0
273.10	1292.0
274.10	3378.0
275.10	18464.0
276.10	2432.0
277.00	1643.0
278.10	351.0
293.00	400.0
296.10	4997.0
297.10	675.0
303.10	562.0
315.10	569.0
315.90	302.0
323.10	1745.0
327.00	335.0
334.10	1053.0
335.10	303.0
346.10	339.0
352.10	504.0
353.00	368.0
354.00	466.0
365.00	2211.0
366.00	325.0
372.10	720.0
403.00	369.0
421.10	446.0
422.00	424.0
423.10	2896.0
424.10	1213.0
441.10	8716.0
442.20	57744.0
443.10	11305.0
444.00	1086.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

m/z	Abundance
39.00	975.0
44.00	329.0
50.00	2930.0
51.10	12127.0
52.00	692.0
55.90	369.0
57.00	814.0
63.00	617.0
68.00	301.0
69.00	15381.0
74.00	1748.0
75.00	2663.0
76.00	961.0
77.10	19216.0
78.10	1310.0
79.00	1080.0
80.00	998.0
81.00	1277.0
81.90	362.0
83.10	320.0
85.00	396.0
86.00	444.0
91.00	310.0
92.10	329.0
93.00	2107.0
98.00	1692.0
99.00	1861.0
101.00	770.0
104.00	490.0
105.00	436.0
107.00	6373.0
108.00	982.0
110.00	11970.0
111.00	1774.0
116.00	302.0
117.00	5414.0
118.00	387.0
122.00	388.0
122.90	584.0
124.00	324.0
127.00	24336.0
128.00	1817.0
129.00	8964.0
130.00	711.0
135.00	743.0
136.90	496.0
141.00	1017.0
141.90	424.0
142.90	316.0
147.00	563.0
148.00	1578.0
148.90	431.0
152.90	412.0
155.00	634.0
156.00	954.0
160.00	391.0
161.10	534.0
165.00	465.0
165.90	338.0
167.00	2815.0
168.00	2002.0
169.00	301.0
173.00	317.0
174.00	491.0
175.00	1059.0
177.00	491.0
179.00	1880.0
180.00	1654.0
180.90	693.0
185.00	843.0
186.00	7343.0
187.00	2252.0
188.90	441.0
192.00	602.0
192.90	754.0
196.00	1437.0
198.00	54312.0
199.00	3619.0
202.90	342.0
204.00	2184.0
205.10	3424.0
206.10	14522.0
207.10	2597.0
208.00	516.0
211.00	561.0
216.00	311.0
217.00	3773.0
218.00	435.0
221.10	2377.0
223.00	823.0
224.10	7930.0
225.10	2174.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

227.00	3200.0
228.00	350.0
229.10	674.0
231.00	300.0
237.00	373.0
242.00	419.0
243.00	414.0
244.10	6174.0
245.10	768.0
246.00	1179.0
255.00	32688.0
256.10	4453.0
257.00	470.0
258.10	1834.0
265.10	788.0
273.00	799.0
274.00	2389.0
275.10	14522.0
276.10	1804.0
277.00	1176.0
278.00	315.0
296.00	4354.0
297.00	479.0
303.00	500.0
315.00	388.0
323.10	1350.0
334.10	849.0
352.10	364.0
353.00	310.0
354.10	419.0
365.00	1929.0
372.10	668.0
402.00	365.0
403.10	402.0
421.10	401.0
422.00	409.0
423.10	2478.0
424.10	988.0
441.10	7979.0
442.10	53288.0
443.10	10189.0
444.10	868.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52