

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120116\
 Data File : BM008135.D
 Acq On : 01 Dec 2016 13:43
 Operator : UM/SJ
 Sample : PB94884BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM112916.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.251	110	113	119	rVB	38306	55079	1.63%	0.143%
2	6.875	724	729	748	rBV	583226	1048334	31.10%	2.731%
3	7.039	751	757	769	rBV	531643	832858	24.71%	2.169%
4	7.233	784	790	800	rBV	678235	1120503	33.24%	2.919%
5	7.698	862	869	879	rBV	579201	991270	29.41%	2.582%
6	8.404	983	989	1008	rBV	799778	1379812	40.94%	3.594%
7	8.857	1059	1066	1078	rBV	613108	1104506	32.77%	2.877%
8	9.569	1180	1187	1200	rBV	526828	938723	27.85%	2.445%
9	10.104	1272	1278	1293	rBV	716171	1345949	39.93%	3.506%
10	10.469	1333	1340	1351	rBV	798992	1391911	41.29%	3.626%
11	10.621	1360	1366	1390	rBV	630018	1353260	40.15%	3.525%
12	13.751	1892	1898	1912	rBV	1397428	2089499	61.99%	5.443%
13	14.027	1937	1945	1958	rBV	1631081	2426944	72.00%	6.322%
14	14.333	1991	1997	2008	rBV	1269640	1852421	54.96%	4.825%
15	14.568	2032	2037	2060	rBV	245870	739502	21.94%	1.926%
16	15.333	2157	2167	2181	rBV	2054524	3053328	90.58%	7.953%
17	15.480	2186	2192	2205	rVV	473505	786531	23.33%	2.049%
18	15.574	2205	2208	2213	rVB2	26671	37315	1.11%	0.097%
19	17.086	2459	2465	2475	rBV	1457570	2040572	60.54%	5.315%
20	17.186	2475	2482	2500	rVV	2131117	3142651	93.23%	8.186%
21	19.486	2867	2873	2885	rBV	2378848	3370730	100.00%	8.780%
22	21.280	3173	3178	3189	rBV	1525336	2223070	65.95%	5.790%
23	23.374	3528	3534	3543	rBV2	1637992	3058522	90.74%	7.967%
24	23.521	3553	3559	3570	rBV	1019933	2008583	59.59%	5.232%


Sum of corrected areas: 38391873

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120116\
Data File : BM008135.D
Acq On : 01 Dec 2016 13:43
Operator : UM/SJ
Sample : PB94884BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK84

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM112916.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

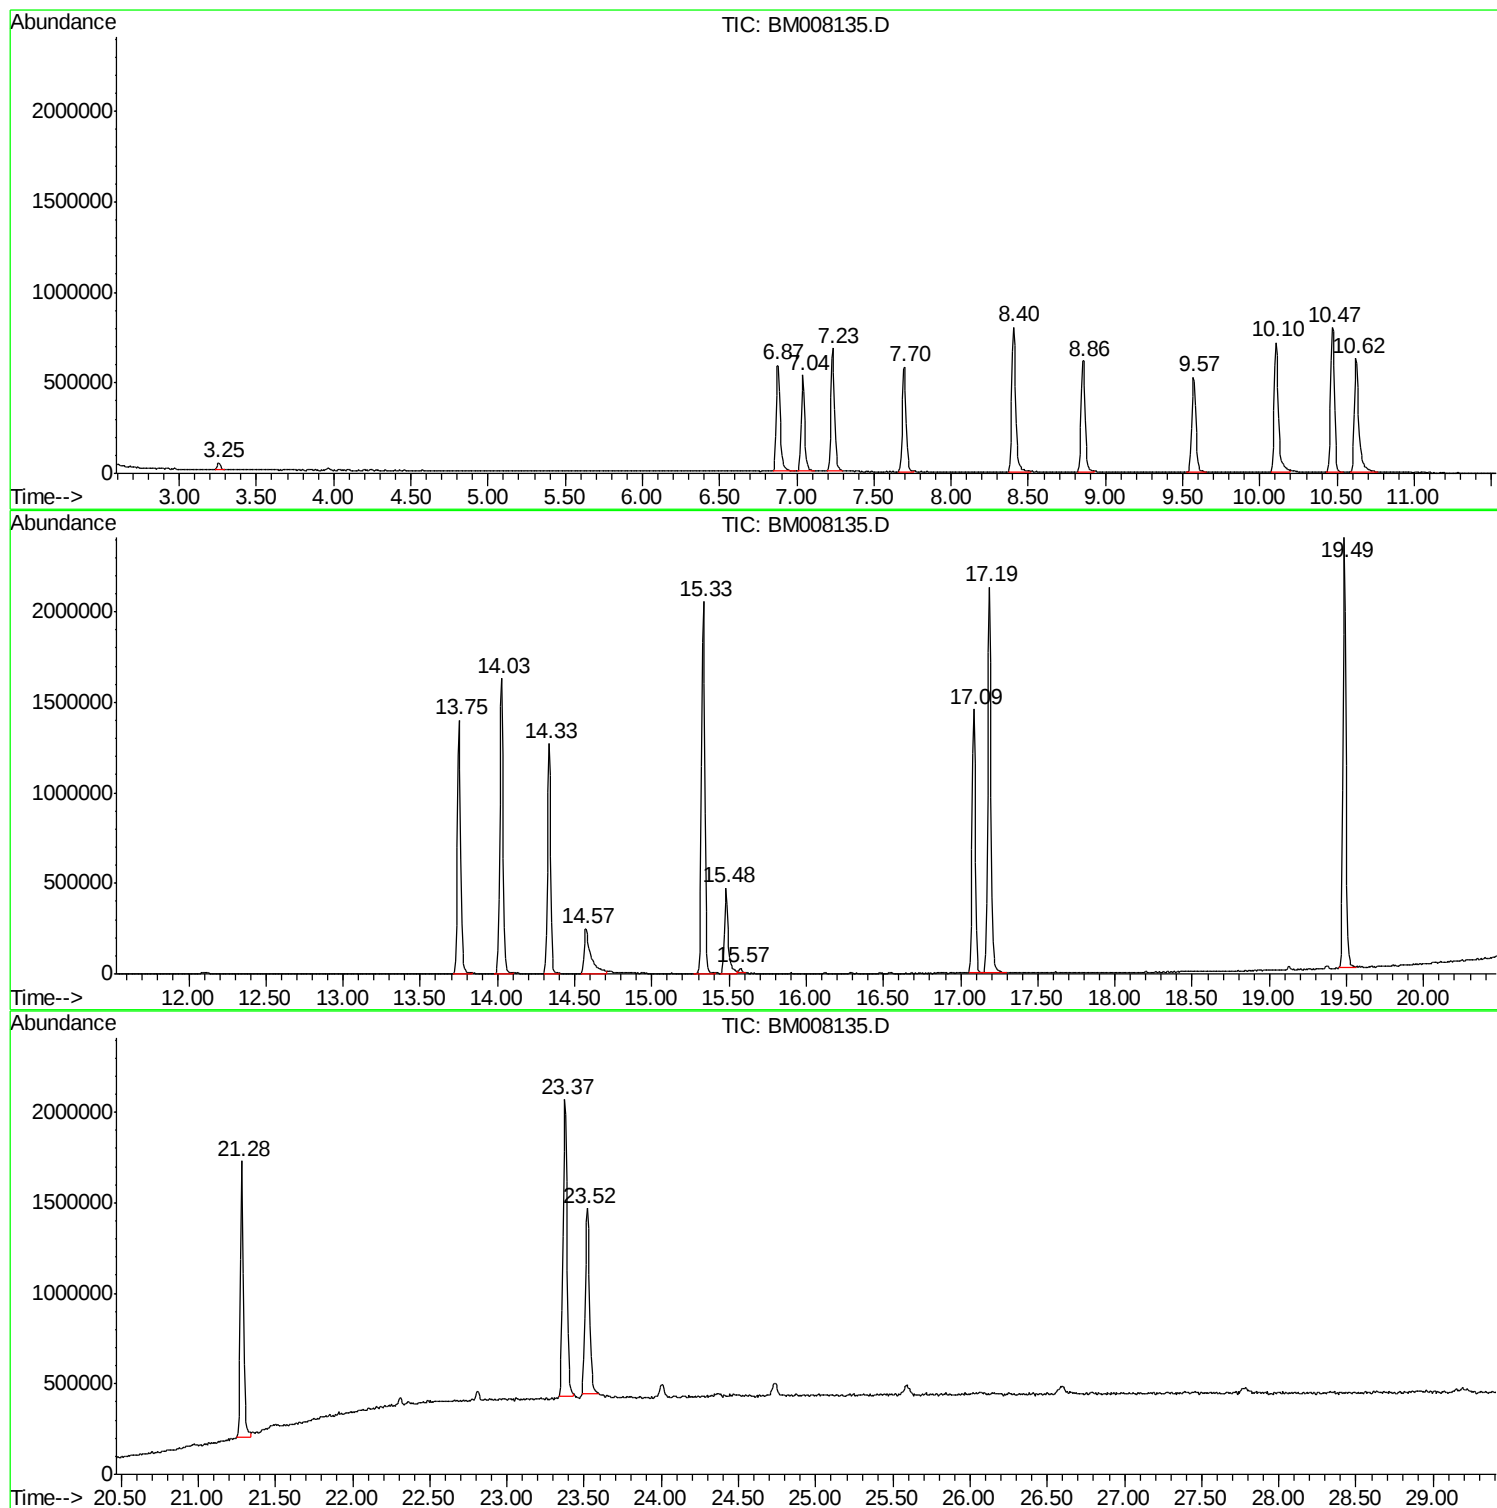

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120116\
Data File : BM008135.D
Acq On : 01 Dec 2016 13:43
Operator : UM/SJ
Sample : PB94884BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK84

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM112916.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120116\
Data File : BM008135.D
Acq On : 01 Dec 2016 13:43
Operator : UM/SJ
Sample : PB94884BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK84

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM112916.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc