

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120122\
 Data File : BM037813.D
 Acq On : 01 Dec 2022 17:01
 Operator : CG/JU
 Sample : SSTD01097
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048

Quant Time: Dec 02 00:17:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 02 00:13:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.098	152	212139	20.000	ng/u1	0.00
20) Naphthalene-d8	10.922	136	970070	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.727	164	637645	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.462	188	1390015	20.000	ng/u1	0.00
79) Chrysene-d12	21.633	240	1409808	20.000	ng/u1	0.00
88) Perylene-d12	24.121	264	1421917	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	17047	3.333	ng/uL	0.00
4) Pyridine-d5	3.869	84	126906	7.622	ng/u1	0.00
7) Phenol-d5	7.245	99	173690	8.207	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	106333	7.532	ng/u1	0.00
11) 2-Chlorophenol-d4	7.622	132	139535	9.488	ng/u1	0.00
15) 4-Methylphenol-d8	8.804	113	140115	8.320	ng/u1	0.00
21) Nitrobenzene-d5	9.269	128	74237	9.762	ng/u1	0.00
24) 2-Nitrophenol-d4	9.992	143	75045	10.015	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.533	165	143434	10.460	ng/u1	0.00
31) 4-Chloroaniline-d4	11.057	131	219764	9.658	ng/u1	0.00
46) Dimethylphthalate-d6	14.127	166	441587	9.777	ng/u1	0.00
49) Acenaphthylene-d8	14.421	160	537867	10.089	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	79852	8.026	ng/u1	0.00
60) Fluorene-d10	15.710	176	400272	10.119	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.821	200	59069	7.900	ng/u1	0.00
73) Anthracene-d10	17.557	188	638140	9.817	ng/u1	0.00
81) Pyrene-d10	19.839	212	738727	10.311	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.956	264	713995	9.755	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.463	88	18909	3.362	ng/uL#	78
5) Pyridine	3.887	79	127170	7.511	ng/u1	99
6) Benzaldehyde	7.228	77	91119	8.203	ng/u1	98
8) Phenol	7.275	94	178806	8.060	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.510	93	148485	8.256	ng/u1	99
12) 2-Chlorophenol	7.657	128	149354	9.297	ng/u1	96
13) 2-Methylphenol	8.539	108	145380	8.590	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.628	45	284977	8.772	ng/u1	99
16) Acetophenone	8.928	105	229212	8.268	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.910	70	118676	7.303	ng/u1	99
18) 4-Methylphenol	8.869	108	152645	8.164	ng/u1	98
19) Hexachloroethane	9.192	117	57364	8.256	ng/u1	98
22) Nitrobenzene	9.310	77	158739	7.655	ng/u1	99
23) Isophorone	9.839	82	343299	8.214	ng/u1	99
25) 2-Nitrophenol	10.028	139	82359	9.717	ng/u1	98
26) 2,4-Dimethylphenol	10.081	107	159588	8.574	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.322	93	208776	8.708	ng/u1	99
29) 2,4-Dichlorophenol	10.557	162	145716	10.387	ng/u1	99
30) Naphthalene	10.969	128	525008	9.898	ng/u1	100
32) 4-Chloroaniline	11.075	127	224507	9.467	ng/u1	98
33) Hexachlorobutadiene	11.251	225	91761	12.460	ng/u1	98
34) Caprolactam	11.845	113	48825	8.356	ng/u1	94
35) 4-Chloro-3-methylphenol	12.186	107	151068	8.424	ng/u1	99
36) 2-Methylnaphthalene	12.563	142	361574	9.813	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120122\
 Data File : BM037813.D
 Acq On : 01 Dec 2022 17:01
 Operator : CG/JU
 Sample : SSTD01097
 Misc :
 ALS Vial : 3 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048


Quant Time: Dec 02 00:17:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 02 00:13:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.786	142	363040	9.794	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.927	216	183255	11.704	ng/ul	98
40) Hexachlorocyclopentadiene	12.910	237	93834	9.624	ng/ul	100
41) 2,4,6-Trichlorophenol	13.163	196	115869	10.277	ng/ul	96
42) 2,4,5-Trichlorophenol	13.233	196	122055	10.118	ng/ul	96
43) 1,1'-Biphenyl	13.563	154	470237	9.711	ng/ul	98
44) 2-Chloronaphthalene	13.610	162	364622	9.688	ng/ul	99
45) 2-Nitroaniline	13.810	65	100607	7.051	ng/ul	97
47) Dimethylphthalate	14.174	163	460262	9.587	ng/ul	99
48) 2,6-Dinitrotoluene	14.298	165	90734	9.787	ng/ul	98
50) Acenaphthylene	14.451	152	597943	9.923	ng/ul	98
51) 3-Nitroaniline	14.627	138	95250	8.467	ng/ul	99
52) Acenaphthene	14.786	153	414559	9.619	ng/ul	99
53) 2,4-Dinitrophenol	14.827	184	40917	7.523	ng/ul	94
55) 4-Nitrophenol	14.921	109	51897	5.821	ng/ul	97
56) Dibenzofuran	15.121	168	560071	9.957	ng/ul	100
57) 2,4-Dinitrotoluene	15.074	165	126255	9.281	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.339	232	110023	11.116	ng/ul	96
59) Diethylphthalate	15.527	149	468560	9.043	ng/ul	100
61) Fluorene	15.768	166	474584	9.740	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.757	204	226971	10.678	ng/ul	97
63) 4-Nitroaniline	15.780	138	101181	9.464	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.839	198	61763	7.783	ng/ul#	97
67) N-Nitrosodiphenylamine	15.968	169	397750	9.209	ng/ul	99
68) 4-Bromophenyl-phenylether	16.651	248	143062	12.796	ng/ul	96
69) Hexachlorobenzene	16.768	284	167356	11.655	ng/ul	98
70) Atrazine	16.915	200	145676	9.937	ng/ul	99
71) Pentachlorophenol	17.109	266	94932	9.985	ng/ul	97
72) Phenanthrene	17.504	178	762332	9.362	ng/ul	99
74) Anthracene	17.592	178	783365	9.476	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.533	216	187577	11.280	ng/uL	97
76) Pentachlorobenzene	15.039	250	203218	11.490	ng/uL	100
77) Carbazole	17.862	167	722560	9.194	ng/ul	99
78) Di-n-butylphthalate	18.415	149	899113	7.903	ng/ul	100
80) Fluoranthene	19.509	202	906879	9.909	ng/ul	98
82) Pyrene	19.868	202	943447	9.760	ng/ul	98
83) Butylbenzylphthalate	20.756	149	395247	8.777	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.544	252	308312	10.889	ng/ul	100
85) Benzo(a)anthracene	21.615	228	925398	9.812	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.527	149	617104	9.070	ng/ul	100
87) Chrysene	21.668	228	859124	9.680	ng/ul	99
89) Di-n-octyl phthalate	22.474	149	1056748	8.700	ng/ul	100
90) Benzo(b)fluoranthene	23.356	252	922751	9.546	ng/ul	99
91) Benzo(k)fluoranthene	23.403	252	883278	9.370	ng/ul	99
93) Benzo(a)pyrene	24.003	252	797774	9.496	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.715	276	895114	9.287	ng/ul	98
95) Dibenzo(a,h)anthracene	26.732	278	815260	9.421	ng/ul	99
96) Benzo(g,h,i)perylene	27.515	276	771237	9.189	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 02 00:17:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 02 00:13:28 2022
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 3.362 ng/uL
RT: 3.463 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion: 88 Resp: 18909
Ion Ratio Lower Upper
88 100
43 89.2 51.3 76.9#
58 113.7 79.0 118.6

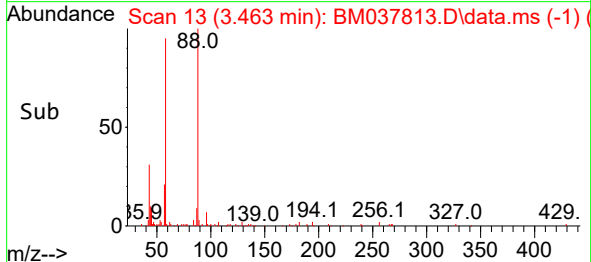

#5
Pyridine
Concen: 7.511 ng/uL
RT: 3.887 min Scan# 85
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion: 79 Resp: 127170
Ion Ratio Lower Upper
79 100
52 95.4 75.2 112.8
51 41.7 33.9 50.9









#6
Benzaldehyde
Concen: 8.203 ng/ul
RT: 7.228 min Scan# 611
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion: 77 Resp: 91119
Ion Ratio Lower Upper
77 100
105 98.0 81.2 121.8
106 99.3 79.0 118.6

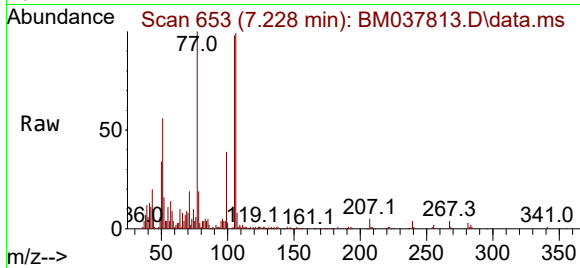

#8
Phenol
Concen: 8.060 ng/ul
RT: 7.275 min Scan# 661
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion: 94 Resp: 178806
Ion Ratio Lower Upper
94 100
65 27.5 21.1 31.7
66 31.6 25.2 37.8




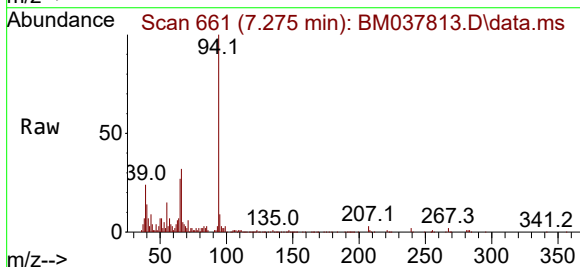




#10
Bis(2-Chloroethyl)ether
Concen: 8.256 ng/ul
RT: 7.510 min Scan# 701
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion: 93 Resp: 148485
Ion Ratio Lower Upper
93 100
63 82.4 65.7 98.5
95 35.3 26.8 40.2



#12
2-Chlorophenol
Concen: 9.297 ng/ul
RT: 7.657 min Scan# 726
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:128 Resp: 149354
Ion Ratio Lower Upper
128 100
64 48.2 37.3 55.9
130 31.0 27.1 40.7









#13
2-Methylphenol
Concen: 8.590 ng/ul
RT: 8.539 min Scan# 81
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:108 Resp: 145380
Ion Ratio Lower Upper
108 100
107 85.1 70.1 105.1

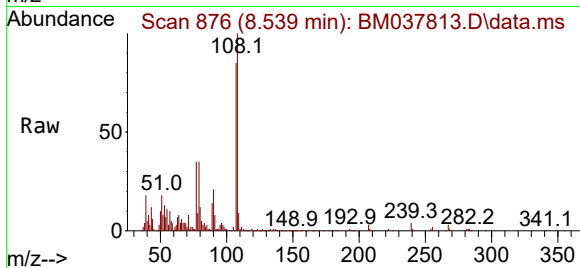

#14
2,2'-oxybis(1-Chloropropane)
Concen: 8.772 ng/ul
RT: 8.628 min Scan# 891
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion: 45 Resp: 284977
Ion Ratio Lower Upper
45 100
77 11.0 8.2 12.4
79 8.5 6.7 10.1




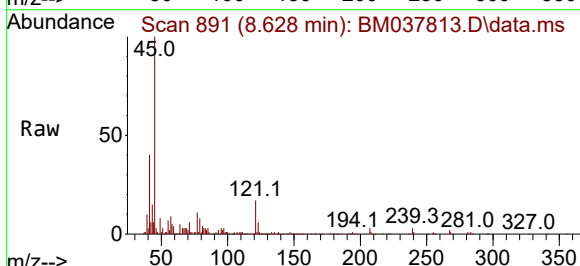




#16
Acetophenone
Concen: 8.268 ng/ul
RT: 8.928 min Scan# 942
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:105 Resp: 229212
Ion Ratio Lower Upper
105 100
77 73.8 59.0 88.4
51 29.5 24.4 36.6



#17
N-Nitroso-di-n-propylamine
Concen: 7.303 ng/ul
RT: 8.910 min Scan# 939
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion: 70 Resp: 118676
Ion Ratio Lower Upper
70 100
42 70.4 55.8 83.6
101 9.2 8.0 12.0
130 21.9 18.6 27.8









#18
4-Methylphenol
Concen: 8.164 ng/ul
RT: 8.869 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:108 Resp: 152645
Ion Ratio Lower Upper
108 100
107 109.3 89.3 133.9



#19
Hexachloroethane
Concen: 8.256 ng/ul
RT: 9.192 min Scan# 987
Delta R.T. 0.005 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:117 Resp: 57364
Ion Ratio Lower Upper
117 100
201 101.2 82.3 123.5
199 64.9 49.8 74.6


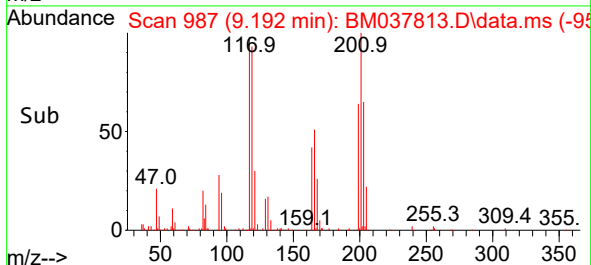
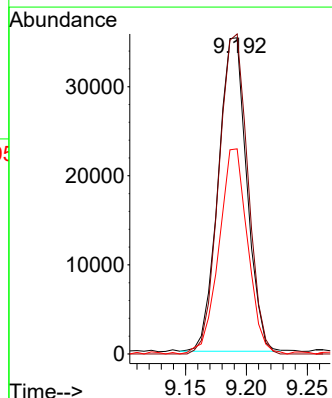



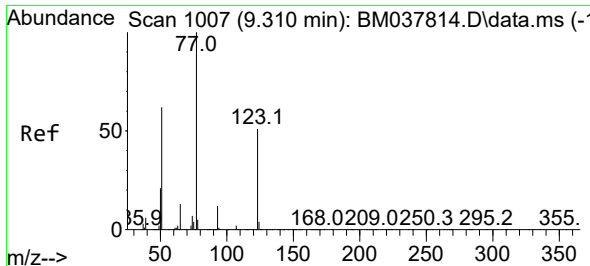

#22
Nitrobenzene
Concen: 7.655 ng/ul
RT: 9.310 min Scan# 1007
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion: 77 Resp: 158739
Ion Ratio Lower Upper
77 100
123 52.3 41.4 62.0
65 13.9 10.9 16.3

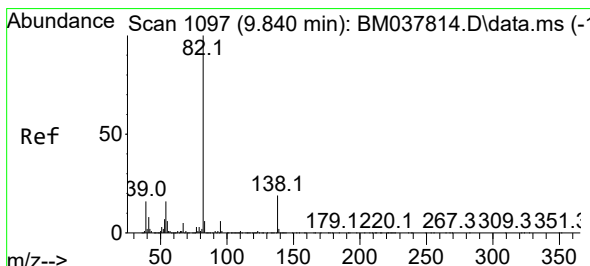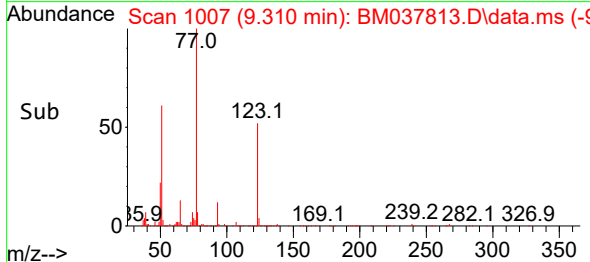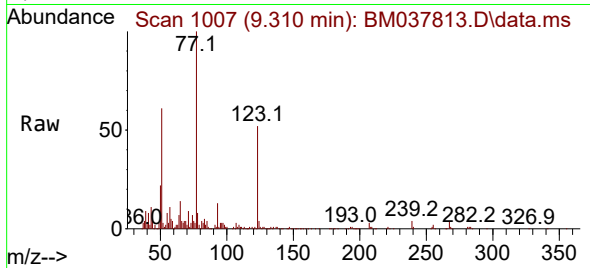

#23
Isophorone
Concen: 8.214 ng/ul
RT: 9.839 min Scan# 1097
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion: 82 Resp: 343299
Ion Ratio Lower Upper
82 100
95 7.5 5.5 8.3
138 19.2 15.3 22.9


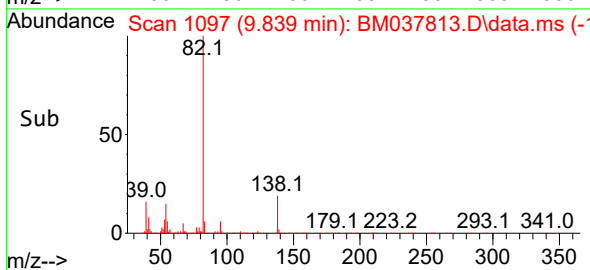

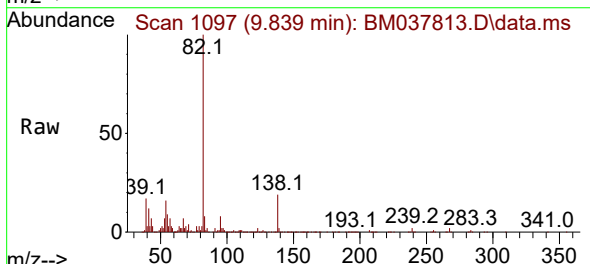




#25
2-Nitrophenol
Concen: 9.717 ng/ul
RT: 10.028 min Scan# 1129
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:139 Resp: 82359
Ion Ratio Lower Upper
139 100
65 43.5 36.6 54.8
109 25.9 21.2 31.8



#26
2,4-Dimethylphenol
Concen: 8.574 ng/ul
RT: 10.081 min Scan# 1138
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:107 Resp: 159588
Ion Ratio Lower Upper
107 100
121 53.7 41.8 62.8
122 93.5 73.1 109.7









#27
 Bis(2-Chloroethoxy)methane
 Concen: 8.708 ng/ul
 RT: 10.322 min Scan# 1179
 Delta R.T. -0.000 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01




Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048


Tgt Ion: 93 Resp: 208776
 Ion Ratio Lower Upper
 93 100
 95 35.8 27.9 41.9
 123 12.1 9.7 14.5

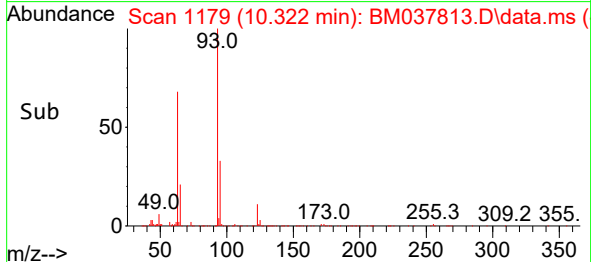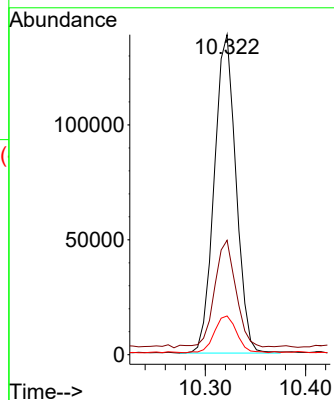

#29
 2,4-Dichlorophenol
 Concen: 10.387 ng/ul
 RT: 10.557 min Scan# 1219
 Delta R.T. -0.006 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01

Tgt Ion: 162 Resp: 145716
 Ion Ratio Lower Upper
 162 100
 164 62.3 50.7 76.1
 98 34.0 27.3 40.9



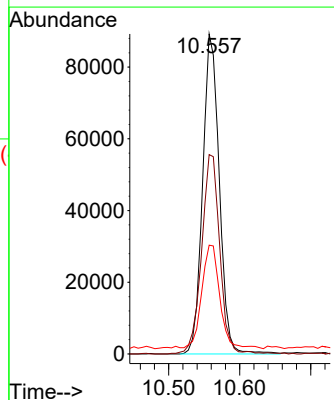





#30
Naphthalene
Concen: 9.898 ng/ul
RT: 10.969 min Scan# 1289
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:128 Resp: 525008
Ion Ratio Lower Upper
128 100
129 11.1 8.9 13.3
127 13.4 10.4 15.6

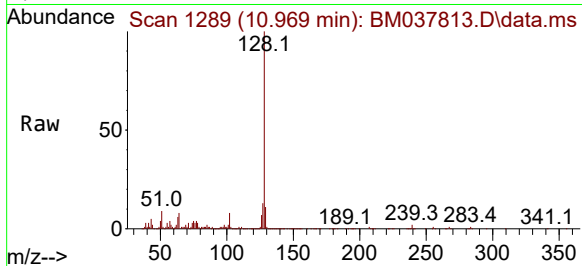

#32
4-Chloroaniline
Concen: 9.467 ng/ul
RT: 11.075 min Scan# 1307
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:127 Resp: 224507
Ion Ratio Lower Upper
127 100
129 32.4 26.9 40.3

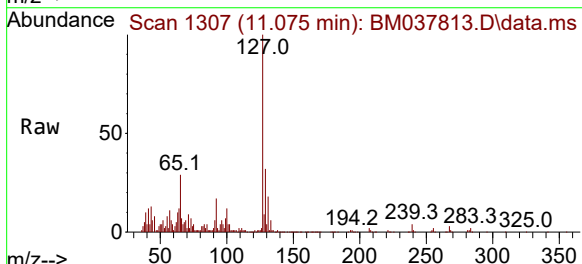



#33

Hexachlorobutadiene

Concen: 12.460 ng/ul

RT: 11.251 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion:225 Resp: 91761

Ion Ratio Lower Upper

225 100

223 61.2 49.3 73.9

227 65.0 49.4 74.0

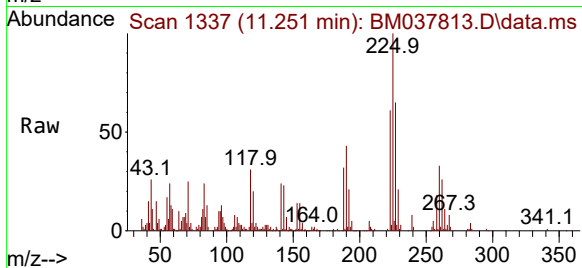

#34

Caprolactam

Concen: 8.356 ng/ul

RT: 11.845 min Scan# 1438

Delta R.T. -0.012 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01




Tgt Ion:113 Resp: 48825


Ion Ratio Lower Upper

113 100

55 241.8 186.2 279.2

56 142.3 119.8 179.8




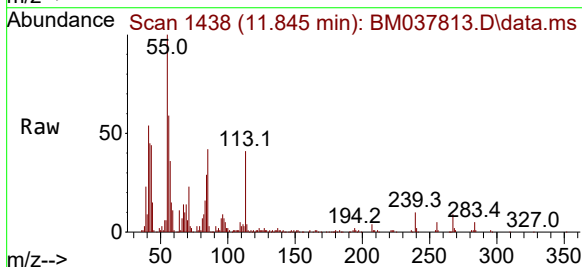




#35
 4-Chloro-3-methylphenol
 Concen: 8.424 ng/ul
 RT: 12.186 min Scan# 1496
 Delta R.T. -0.000 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01




Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048


Tgt Ion:107 Resp: 151068
 Ion Ratio Lower Upper
 107 100
 144 27.3 23.0 34.6
 142 86.9 69.1 103.7



#36
 2-Methylnaphthalene
 Concen: 9.813 ng/ul
 RT: 12.563 min Scan# 1560
 Delta R.T. -0.006 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01

Tgt Ion:142 Resp: 361574
 Ion Ratio Lower Upper
 142 100
 141 87.2 70.1 105.1





#37

1-Methylnaphthalene

Concen: 9.794 ng/ul

RT: 12.786 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion:142 Resp: 363040

Ion Ratio Lower Upper

142 100

141 89.7 73.4 110.2

116 3.1 2.6 4.0

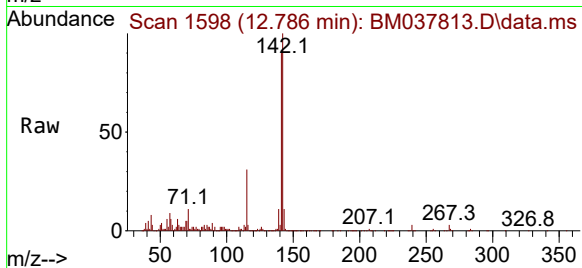

#39

1,2,4,5-Tetrachlorobenzene

Concen: 11.704 ng/ul

RT: 12.927 min Scan# 1622

Delta R.T. -0.000 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01

Tgt Ion:216 Resp: 183255




Ion Ratio Lower Upper


216 100

214 80.1 62.7 94.1

179 19.3 15.9 23.9

108 15.5 13.0 19.4




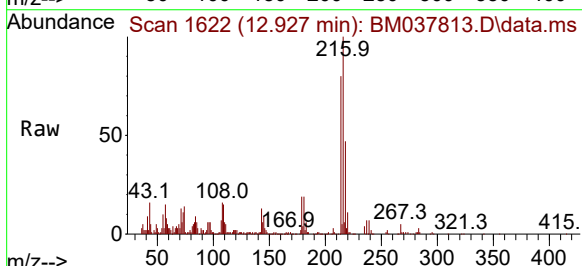




#40
Hexachlorocyclopentadiene
Concen: 9.624 ng/ul
RT: 12.910 min Scan# 1619
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:237 Resp: 93834
Ion Ratio Lower Upper
237 100
235 61.6 49.2 73.8
272 13.1 10.5 15.7

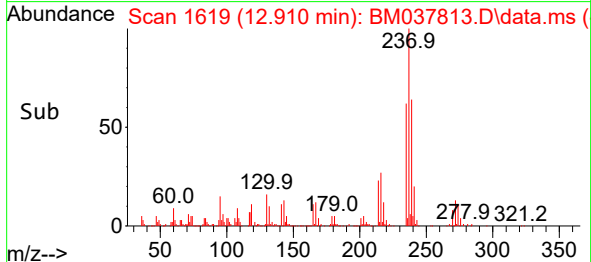

#41
2,4,6-Trichlorophenol
Concen: 10.277 ng/ul
RT: 13.163 min Scan# 1662
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:196 Resp: 115869
Ion Ratio Lower Upper
196 100
198 98.1 75.6 113.4
200 33.1 24.4 36.6




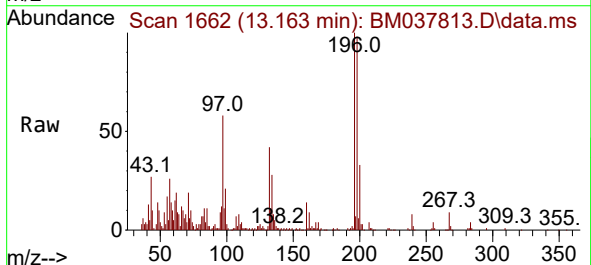




#42
2,4,5-Trichlorophenol
Concen: 10.118 ng/ul
RT: 13.233 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:196 Resp: 122055
Ion Ratio Lower Upper
196 100
198 99.4 76.1 114.1
200 31.7 24.8 37.2

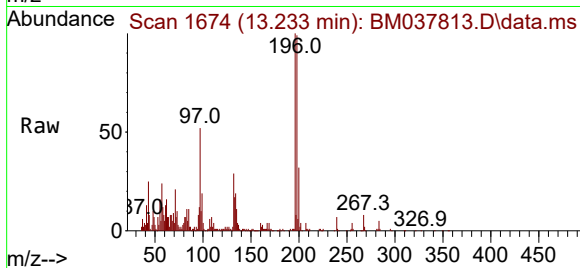

#43
1,1'-Biphenyl
Concen: 9.711 ng/ul
RT: 13.563 min Scan# 1730
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:154 Resp: 470237
Ion Ratio Lower Upper
154 100
153 40.5 31.4 47.0
76 12.9 10.2 15.2




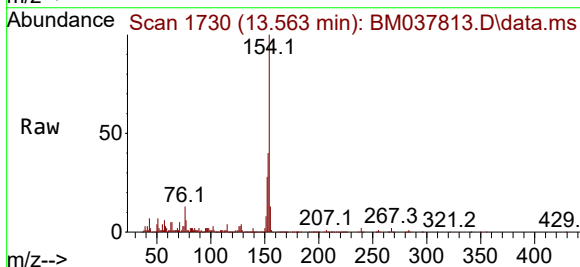




#44
2-Chloronaphthalene
Concen: 9.688 ng/ul
RT: 13.610 min Scan# 1738
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:162 Resp: 364622
Ion Ratio Lower Upper
162 100
164 32.9 26.5 39.7
127 37.2 30.5 45.7



#45
2-Nitroaniline
Concen: 7.051 ng/ul
RT: 13.810 min Scan# 1772
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion: 65 Resp: 100607
Ion Ratio Lower Upper
65 100
92 68.0 54.7 82.1
138 126.8 96.8 145.2









#47
Dimethylphthalate
Concen: 9.587 ng/ul
RT: 14.174 min Scan# 1834
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:163 Resp: 460262
Ion Ratio Lower Upper
163 100
194 4.1 3.6 5.4
164 10.4 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 9.787 ng/ul
RT: 14.298 min Scan# 1855
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:165 Resp: 90734
Ion Ratio Lower Upper
165 100
89 49.9 40.6 60.8
121 22.8 16.4 24.6









#50
Acenaphthylene
Concen: 9.923 ng/ul
RT: 14.451 min Scan# 1881
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:152 Resp: 597943
Ion Ratio Lower Upper
152 100
151 18.8 15.8 23.6
153 12.6 10.6 15.8

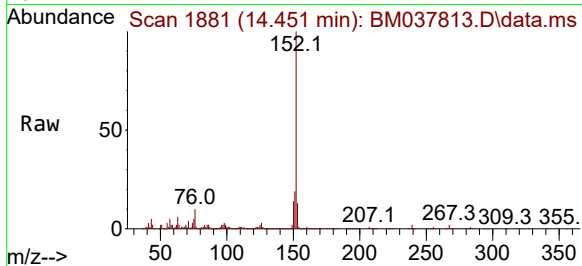

#51
3-Nitroaniline
Concen: 8.467 ng/ul
RT: 14.627 min Scan# 1911
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:138 Resp: 95250
Ion Ratio Lower Upper
138 100
108 10.1 7.8 11.8
92 103.2 83.8 125.6




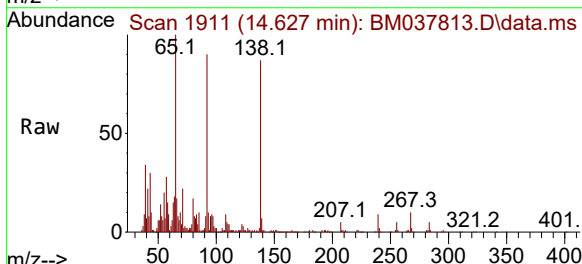




#52
Acenaphthene
Concen: 9.619 ng/ul
RT: 14.786 min Scan# 1938
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:153 Resp: 414559
Ion Ratio Lower Upper
153 100
152 47.2 37.0 55.4
154 85.9 69.8 104.6



#53
2,4-Dinitrophenol
Concen: 7.523 ng/ul
RT: 14.827 min Scan# 1945
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:184 Resp: 40917
Ion Ratio Lower Upper
184 100
63 60.4 43.4 65.0
154 47.5 39.7 59.5



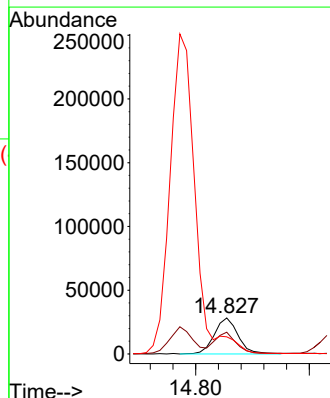





#55
4-Nitrophenol
Concen: 5.821 ng/ul
RT: 14.921 min Scan# 1961
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:109 Resp: 51897
Ion Ratio Lower Upper
109 100
139 169.7 131.6 197.4
65 139.1 109.4 164.0

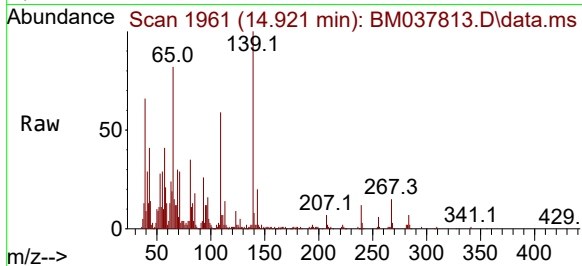

#56
Dibenzofuran
Concen: 9.957 ng/ul
RT: 15.121 min Scan# 1995
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:168 Resp: 560071
Ion Ratio Lower Upper
168 100
139 34.4 27.6 41.4

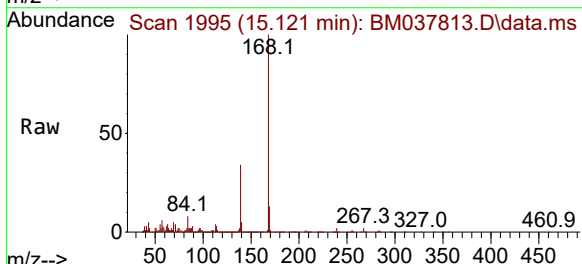



#57

2,4-Dinitrotoluene

Concen: 9.281 ng/ul

RT: 15.074 min Scan# 1988

Delta R.T. -0.006 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion:165 Resp: 126255

Ion Ratio Lower Upper

165 100

63 39.0 30.2 45.2

182 2.8 1.8 2.8

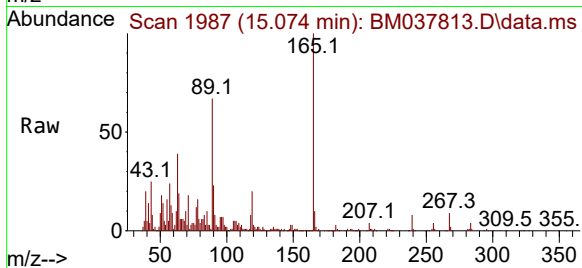

#58

2,3,4,6-Tetrachlorophenol

Concen: 11.116 ng/ul

RT: 15.339 min Scan# 2032

Delta R.T. -0.006 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01

Tgt Ion:232 Resp: 110023




Ion Ratio Lower Upper


232 100

131 42.7 32.7 49.1

130 2.4 1.8 2.6

166 30.5 22.2 33.4




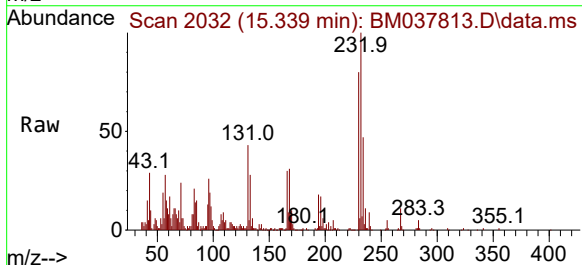




#59
Diethylphthalate
Concen: 9.043 ng/ul
RT: 15.527 min Scan# 2064
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:149 Resp: 468560
Ion Ratio Lower Upper
149 100
177 22.5 18.0 27.0
150 12.6 9.8 14.8

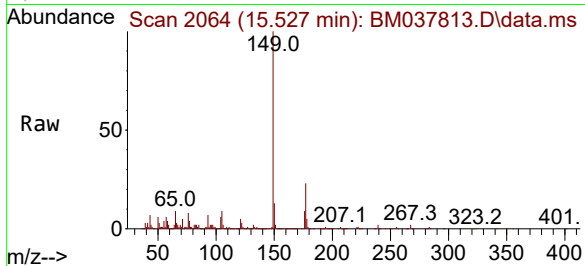

#61
Fluorene
Concen: 9.740 ng/ul
RT: 15.768 min Scan# 2105
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:166 Resp: 474584
Ion Ratio Lower Upper
166 100
165 92.7 77.0 115.6
167 12.9 10.5 15.7




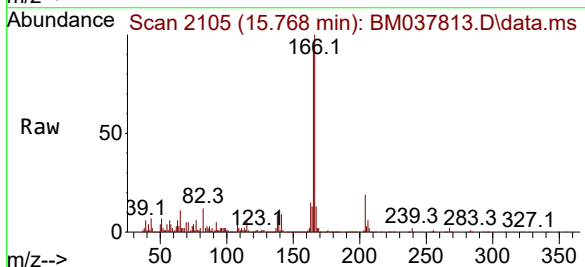




#62
4-Chlorophenyl-phenylether
Concen: 10.678 ng/ul
RT: 15.757 min Scan# 2103
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:204 Resp: 226971
Ion Ratio Lower Upper
204 100
206 32.3 26.2 39.4
141 53.1 44.7 67.1



#63
4-Nitroaniline
Concen: 9.464 ng/ul
RT: 15.780 min Scan# 2107
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:138 Resp: 101181
Ion Ratio Lower Upper
138 100
92 45.4 36.6 54.8
108 63.8 48.2 72.2



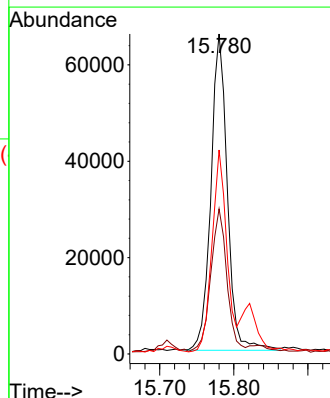





#66
 4,6-Dinitro-2-methylphenol
 Concen: 7.783 ng/ul
 RT: 15.839 min Scan# 2117
 Delta R.T. -0.000 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01




Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048


Tgt Ion:198 Resp: 61763
 Ion Ratio Lower Upper
 198 100
 182 4.7 2.9 4.3#
 77 20.4 17.5 26.3

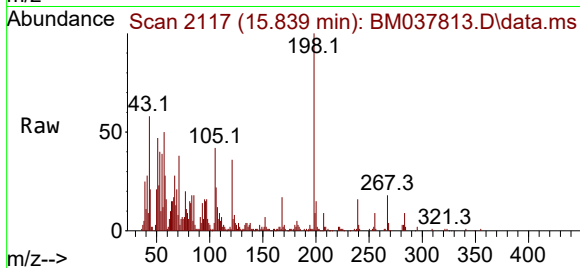

#67
 N-Nitrosodiphenylamine
 Concen: 9.209 ng/ul
 RT: 15.968 min Scan# 2139
 Delta R.T. -0.000 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01

Tgt Ion:169 Resp: 397750
 Ion Ratio Lower Upper
 169 100
 168 67.8 53.8 80.6
 167 36.1 29.5 44.3




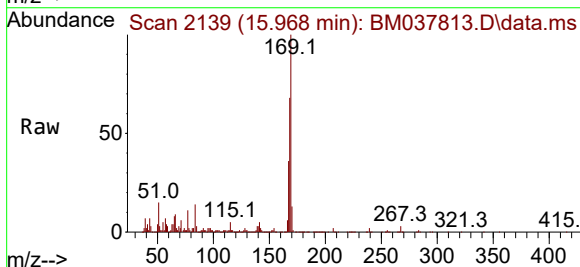




#68
4-Bromophenyl-phenylether
Concen: 12.796 ng/ul
RT: 16.651 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:248 Resp: 143062
Ion Ratio Lower Upper
248 100
250 101.2 78.1 117.1
141 60.3 51.6 77.4



#69
Hexachlorobenzene
Concen: 11.655 ng/ul
RT: 16.768 min Scan# 2275
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:284 Resp: 167356
Ion Ratio Lower Upper
284 100
142 29.1 24.5 36.7
249 28.9 22.9 34.3


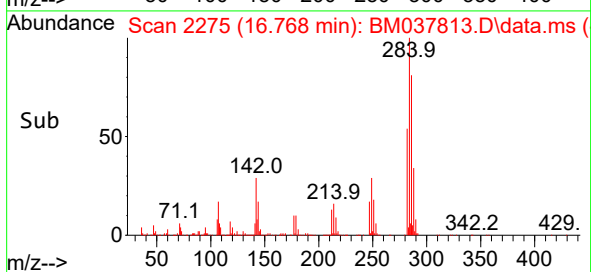






#70
Atrazine
Concen: 9.937 ng/ul
RT: 16.915 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:200 Resp: 145676
Ion Ratio Lower Upper
200 100
173 27.5 22.0 33.0
215 48.9 40.0 60.0

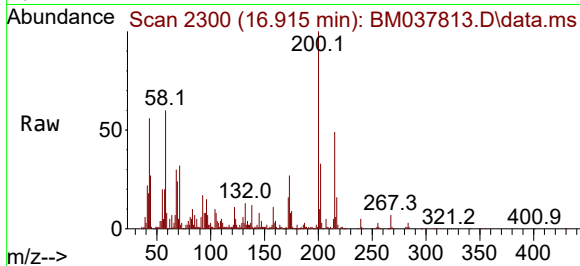

#71
Pentachlorophenol
Concen: 9.985 ng/ul
RT: 17.109 min Scan# 2333
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:266 Resp: 94932
Ion Ratio Lower Upper
266 100
264 63.0 50.3 75.5
268 61.3 52.2 78.2

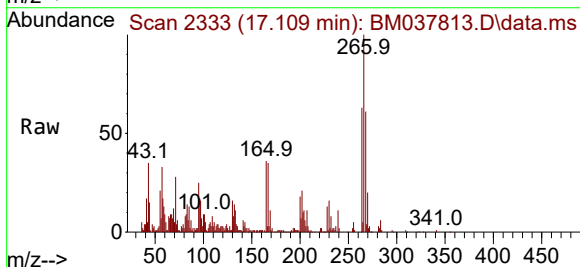



#72

Phenanthrene

Concen: 9.362 ng/ul

RT: 17.504 min Scan# 2400

Delta R.T. -0.000 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion:178 Resp: 762332

Ion Ratio Lower Upper

178 100

179 14.9 12.5 18.7

176 19.0 15.3 22.9

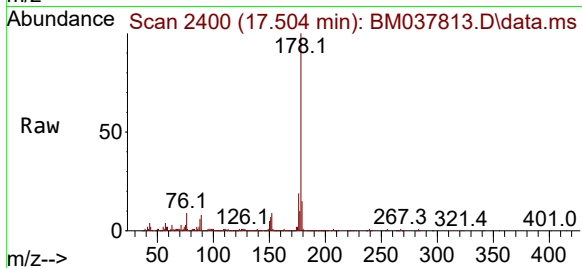

#74

Anthracene

Concen: 9.476 ng/ul

RT: 17.592 min Scan# 2415

Delta R.T. -0.006 min

Lab File: BM037813.D

Acq: 01 Dec 2022 17:01




Tgt Ion:178 Resp: 783365


Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.4

176 18.6 14.8 22.2




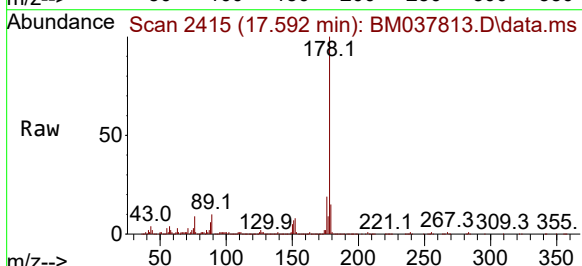




#75
1,2,3,4-Tetrachlorobenzene
Concen: 11.280 ng/uL
RT: 13.533 min Scan# 1725
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:216 Resp: 187577
Ion Ratio Lower Upper
216 100
214 76.6 63.0 94.6
218 46.9 40.0 60.0

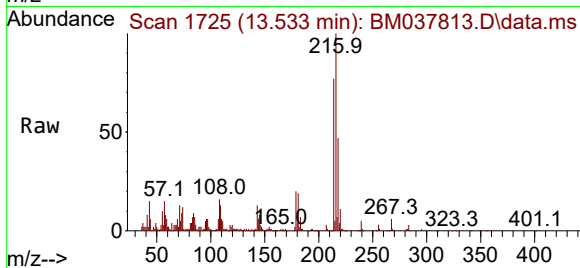

#76
Pentachlorobenzene
Concen: 11.490 ng/uL
RT: 15.039 min Scan# 1981
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:250 Resp: 203218
Ion Ratio Lower Upper
250 100
248 62.6 50.5 75.7
252 64.1 51.1 76.7




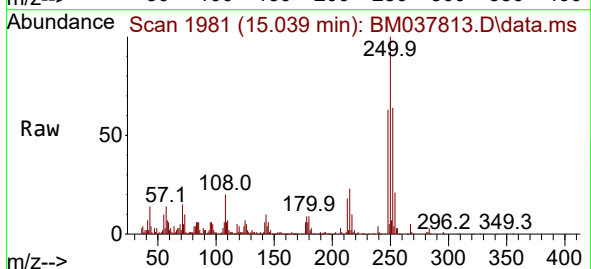




#77
 Carbazole
 Concen: 9.194 ng/ul
 RT: 17.862 min Scan# 2461
 Delta R.T. -0.000 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01




Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048


Tgt Ion:167 Resp: 722560
 Ion Ratio Lower Upper
 167 100
 166 21.4 17.2 25.8
 139 12.0 10.0 15.0

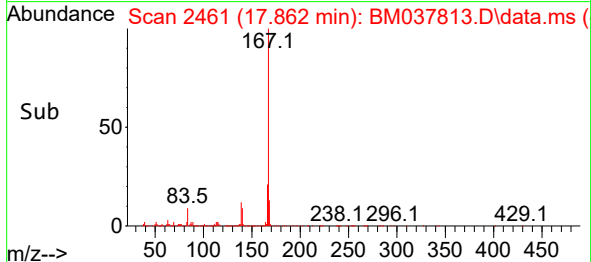

#78
 Di-n-butylphthalate
 Concen: 7.903 ng/ul
 RT: 18.415 min Scan# 2555
 Delta R.T. -0.000 min
 Lab File: BM037813.D
 Acq: 01 Dec 2022 17:01

Tgt Ion:149 Resp: 899113
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.2
 104 4.1 3.4 5.0









#80
Fluoranthene
Concen: 9.909 ng/ul
RT: 19.509 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:202 Resp: 906879
Ion Ratio Lower Upper
202 100
101 11.2 9.7 14.5
100 8.7 7.7 11.5

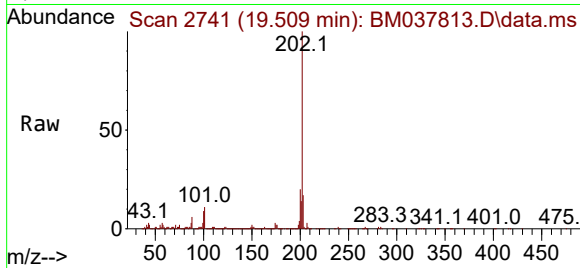

#82
Pyrene
Concen: 9.760 ng/ul
RT: 19.868 min Scan# 2802
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:202 Resp: 943447
Ion Ratio Lower Upper
202 100
101 14.4 11.0 16.4
100 12.2 9.0 13.6




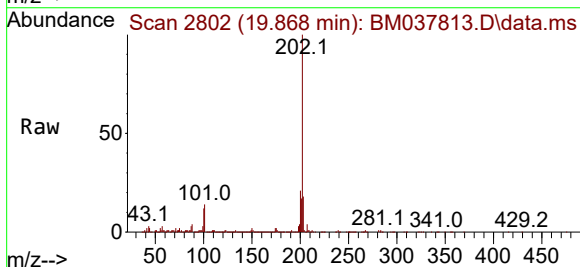




#83
Butylbenzylphthalate
Concen: 8.777 ng/ul
RT: 20.756 min Scan# 2953
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:149 Resp: 395247
Ion Ratio Lower Upper
149 100
91 62.5 51.7 77.5
206 22.3 17.1 25.7

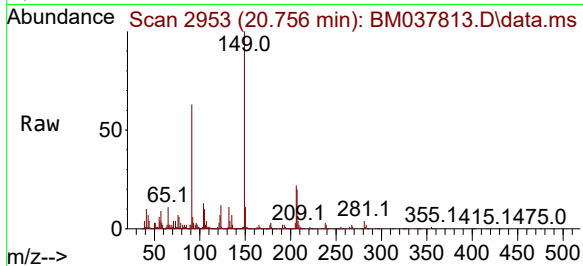

#84
3,3'-Dichlorobenzidine
Concen: 10.889 ng/ul
RT: 21.544 min Scan# 3087
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:252 Resp: 308312
Ion Ratio Lower Upper
252 100
254 65.3 52.2 78.4
126 10.1 8.8 13.2



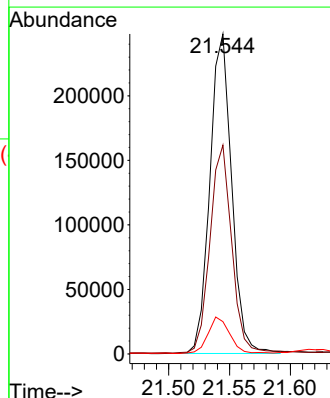
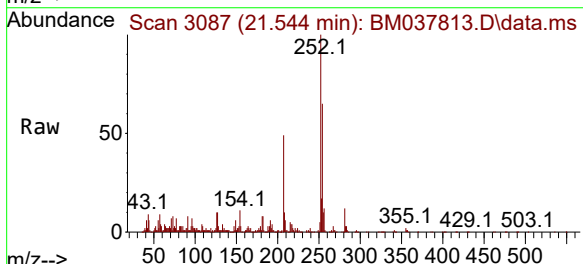




#85
Benzo(a)anthracene
Concen: 9.812 ng/ul
RT: 21.615 min Scan# 3099
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:228 Resp: 925398
Ion Ratio Lower Upper
228 100
229 19.5 16.2 24.2
226 27.2 22.3 33.5



#86
Bis(2-ethylhexyl)phthalate
Concen: 9.070 ng/ul
RT: 21.527 min Scan# 3084
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:149 Resp: 617104
Ion Ratio Lower Upper
149 100
167 29.0 23.3 34.9
279 4.2 3.6 5.4









#87
Chrysene
Concen: 9.680 ng/ul
RT: 21.668 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:228 Resp: 859124
Ion Ratio Lower Upper
228 100
226 29.9 24.2 36.2
229 19.1 15.8 23.6

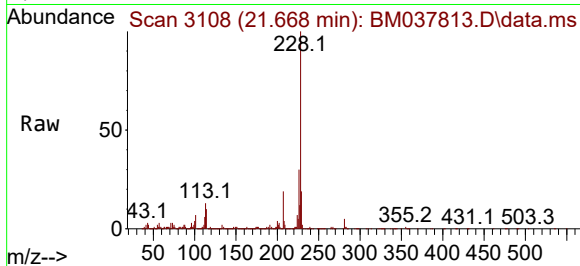

#89
Di-n-octyl phthalate
Concen: 8.700 ng/ul
RT: 22.474 min Scan# 3245
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:149 Resp: 1056748




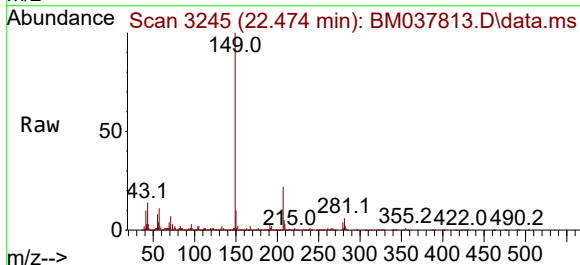




#90
Benzo(b)fluoranthene
Concen: 9.546 ng/ul
RT: 23.356 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:252 Resp: 922751
Ion Ratio Lower Upper
252 100
253 22.2 17.7 26.5
125 10.9 9.3 13.9



#91
Benzo(k)fluoranthene
Concen: 9.370 ng/ul
RT: 23.403 min Scan# 3403
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:252 Resp: 883278
Ion Ratio Lower Upper
252 100
253 21.9 17.8 26.8
125 11.5 9.3 13.9









#93
Benzo(a)pyrene
Concen: 9.496 ng/ul
RT: 24.003 min Scan# 3506
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:252 Resp: 797774
Ion Ratio Lower Upper
252 100
253 21.7 17.4 26.2
125 13.0 10.2 15.4



#94
Indeno(1,2,3-cd)pyrene
Concen: 9.287 ng/ul
RT: 26.715 min Scan# 3966
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:276 Resp: 895114
Ion Ratio Lower Upper
276 100
138 26.6 22.7 34.1
277 25.2 20.1 30.1









#95
Dibenzo(a,h)anthracene
Concen: 9.421 ng/ul
RT: 26.732 min Scan# 3970
Delta R.T. -0.006 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Instrument :
BNA_M
ClientSampleId :
SSTD010048

Tgt Ion:278 Resp: 815260
Ion Ratio Lower Upper
278 100
139 16.7 13.9 20.9
279 23.4 19.0 28.6



#96
Benzo(g,h,i)perylene
Concen: 9.189 ng/ul
RT: 27.515 min Scan# 4102
Delta R.T. -0.012 min
Lab File: BM037813.D
Acq: 01 Dec 2022 17:01

Tgt Ion:276 Resp: 771237
Ion Ratio Lower Upper
276 100
138 23.4 19.2 28.8
277 24.1 19.1 28.7

