




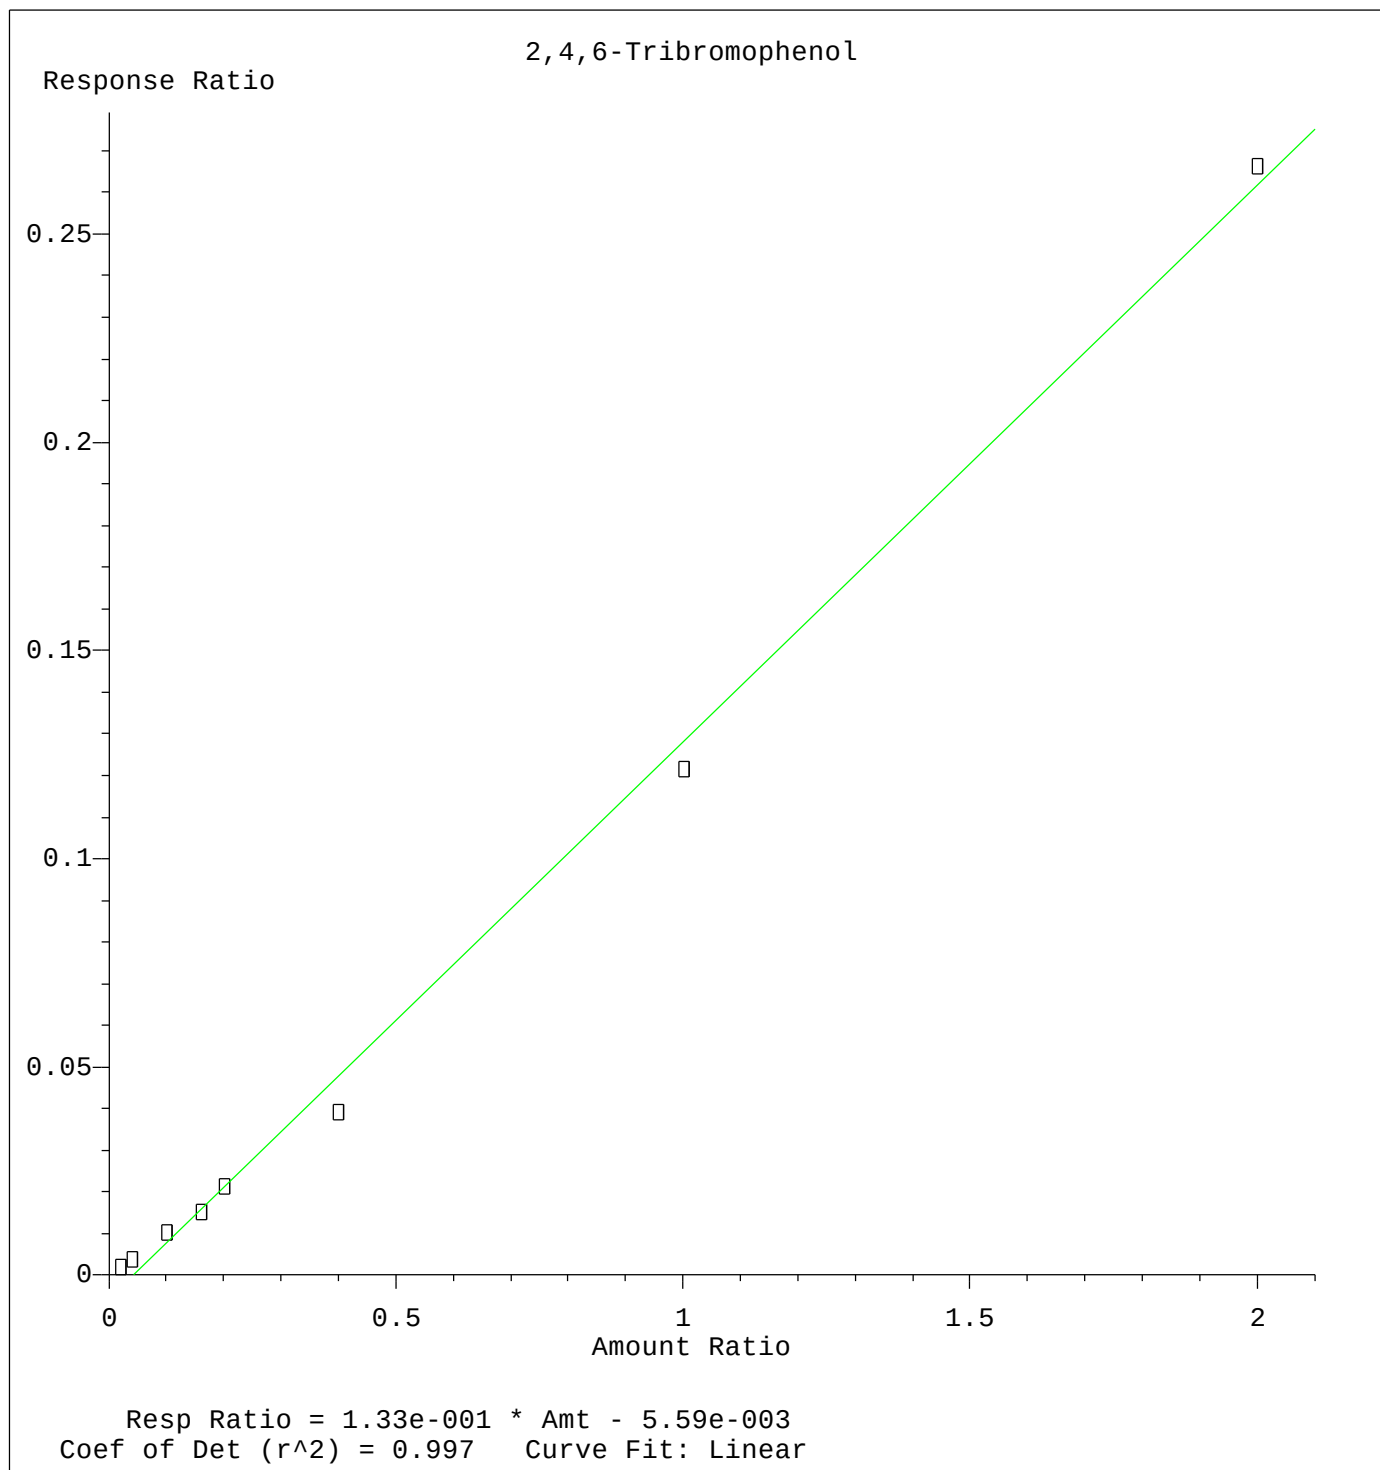


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
Calibration Table Last Updated: Wed Dec 02 16:19:00 2015

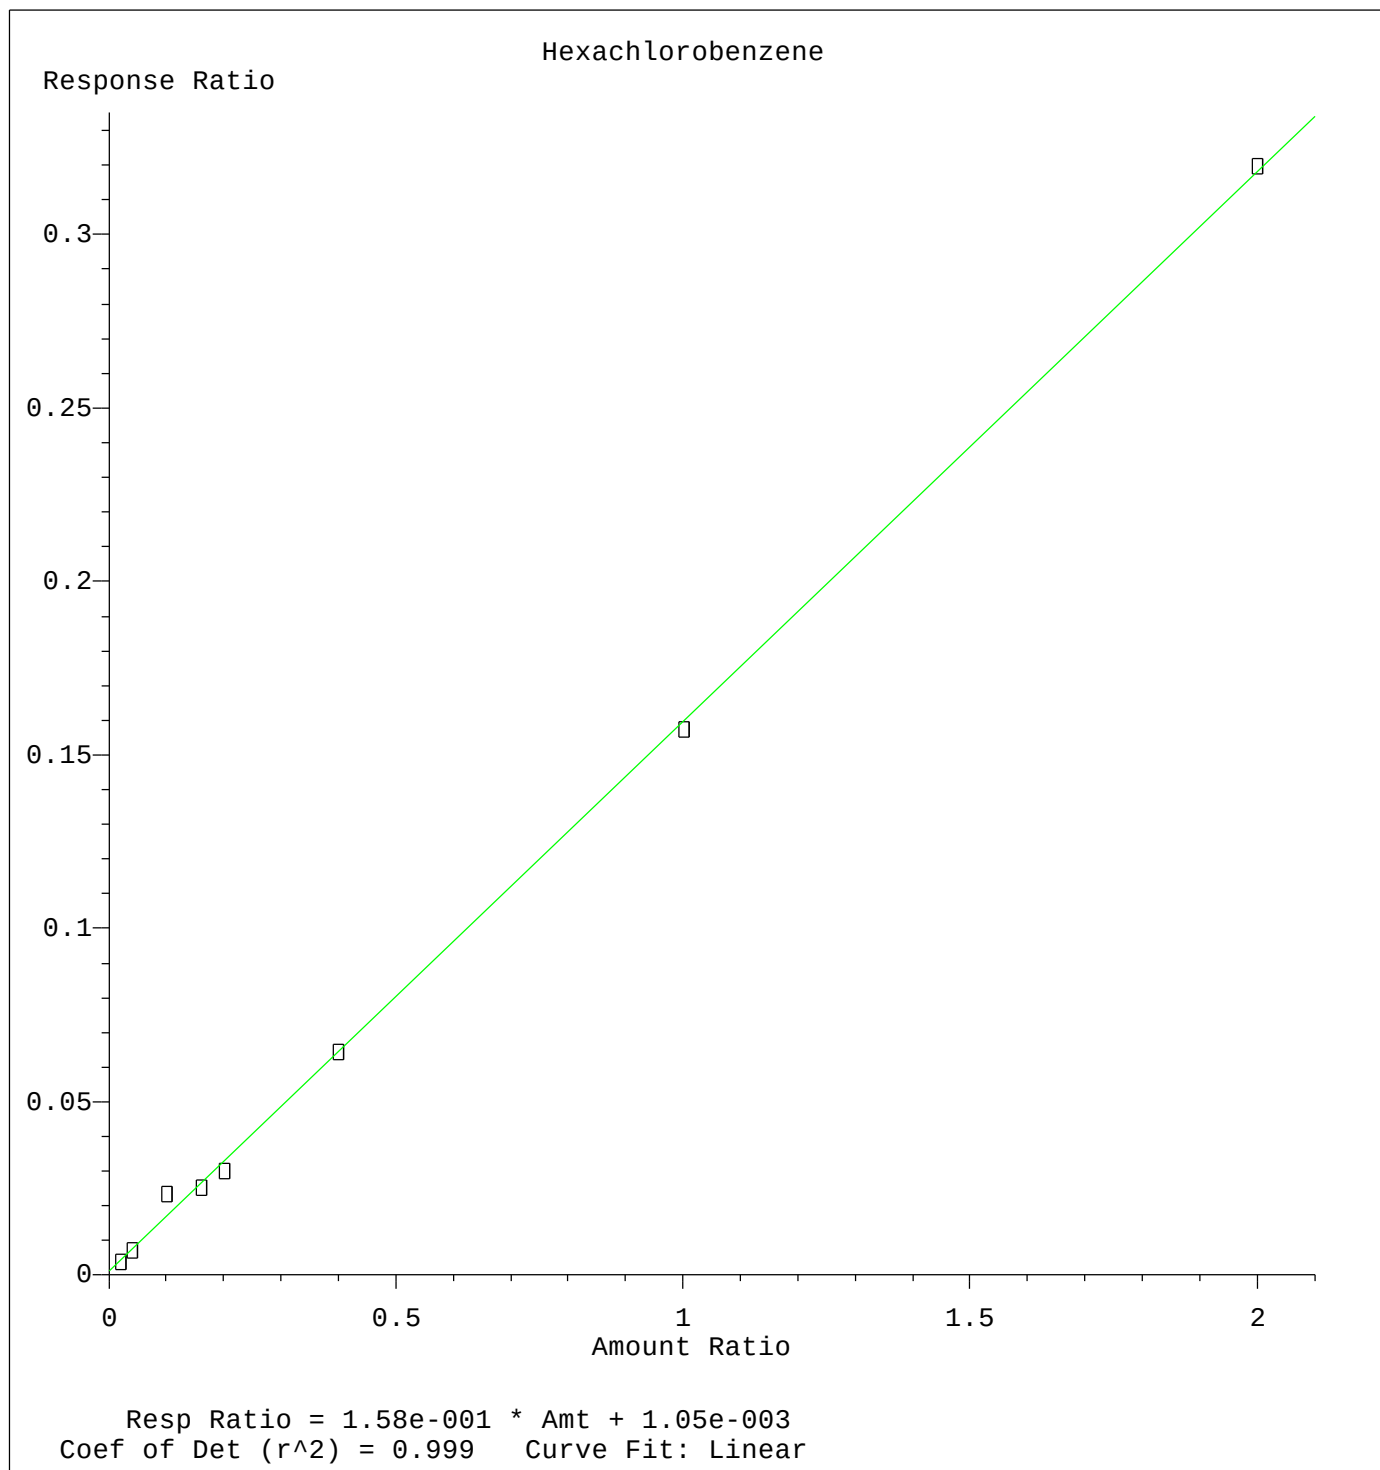

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
Calibration Table Last Updated: Wed Dec 02 16:19:00 2015

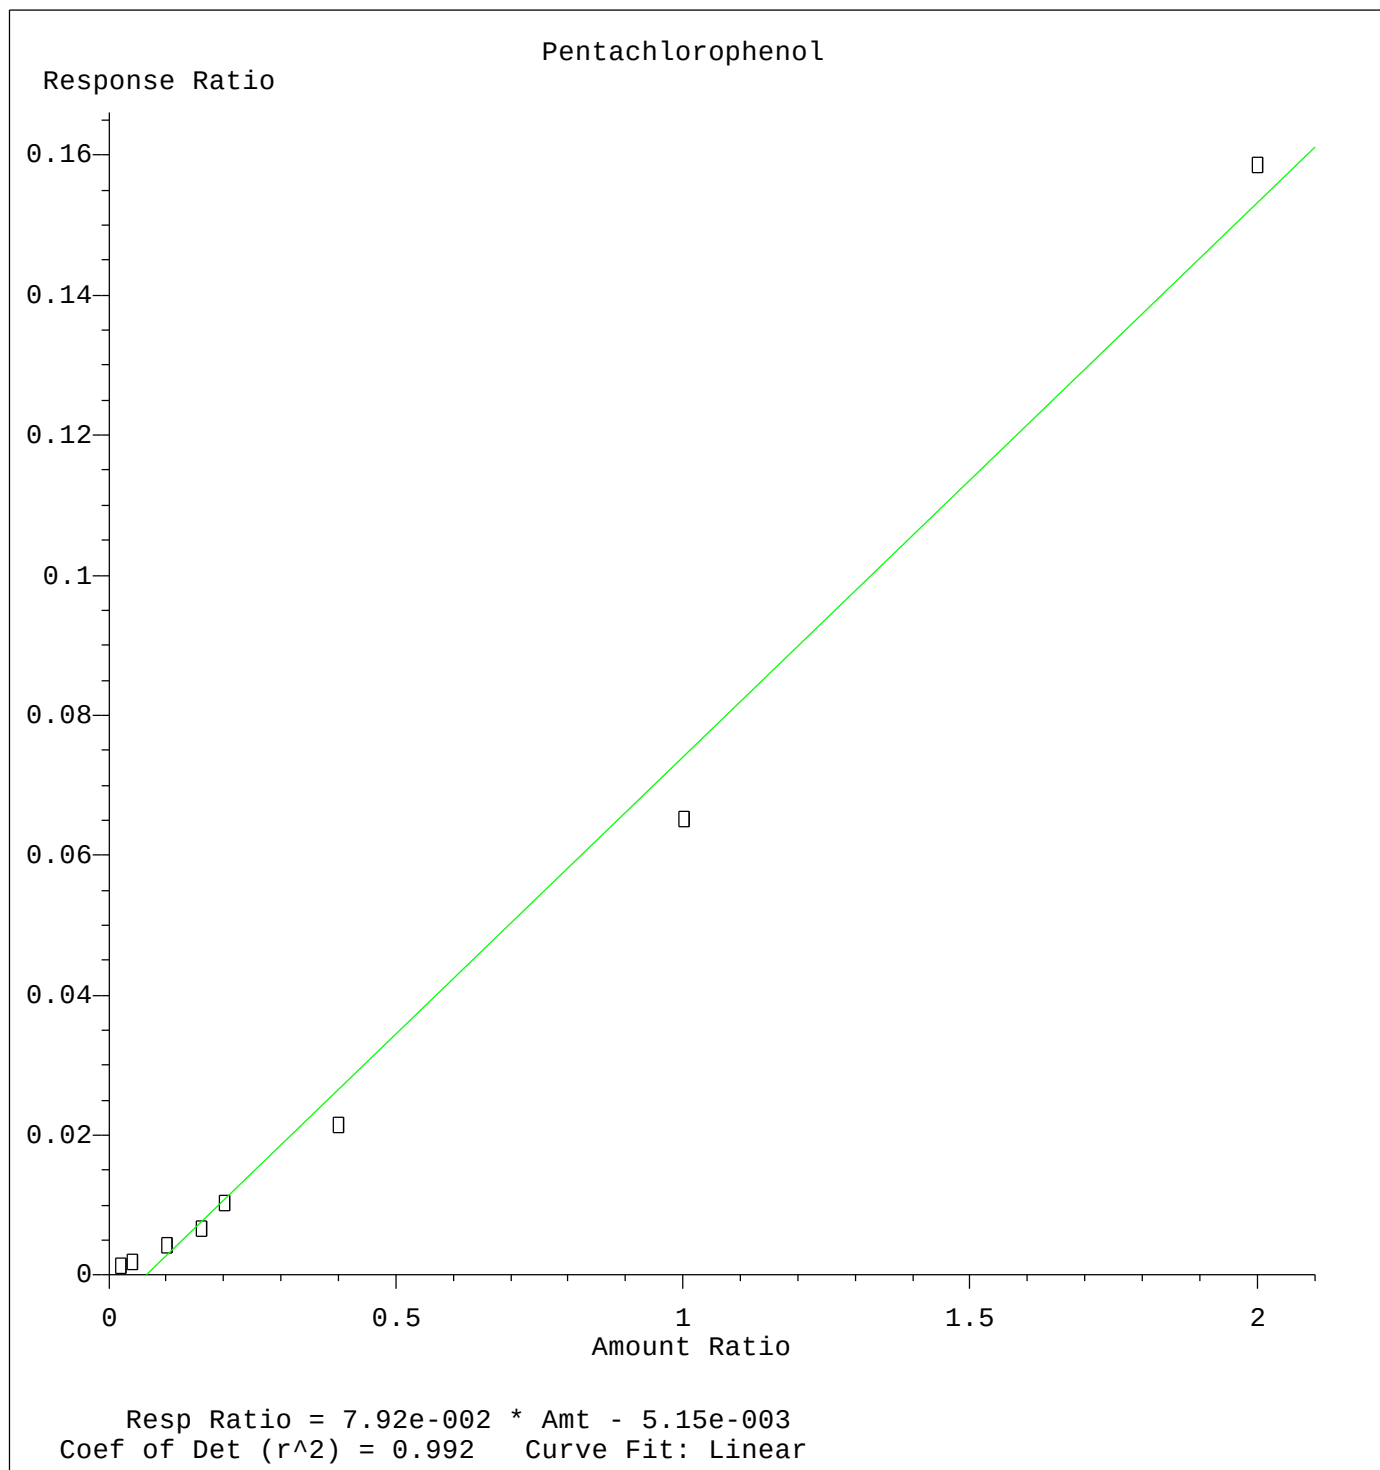


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
Calibration Table Last Updated: Wed Dec 02 16:19:00 2015

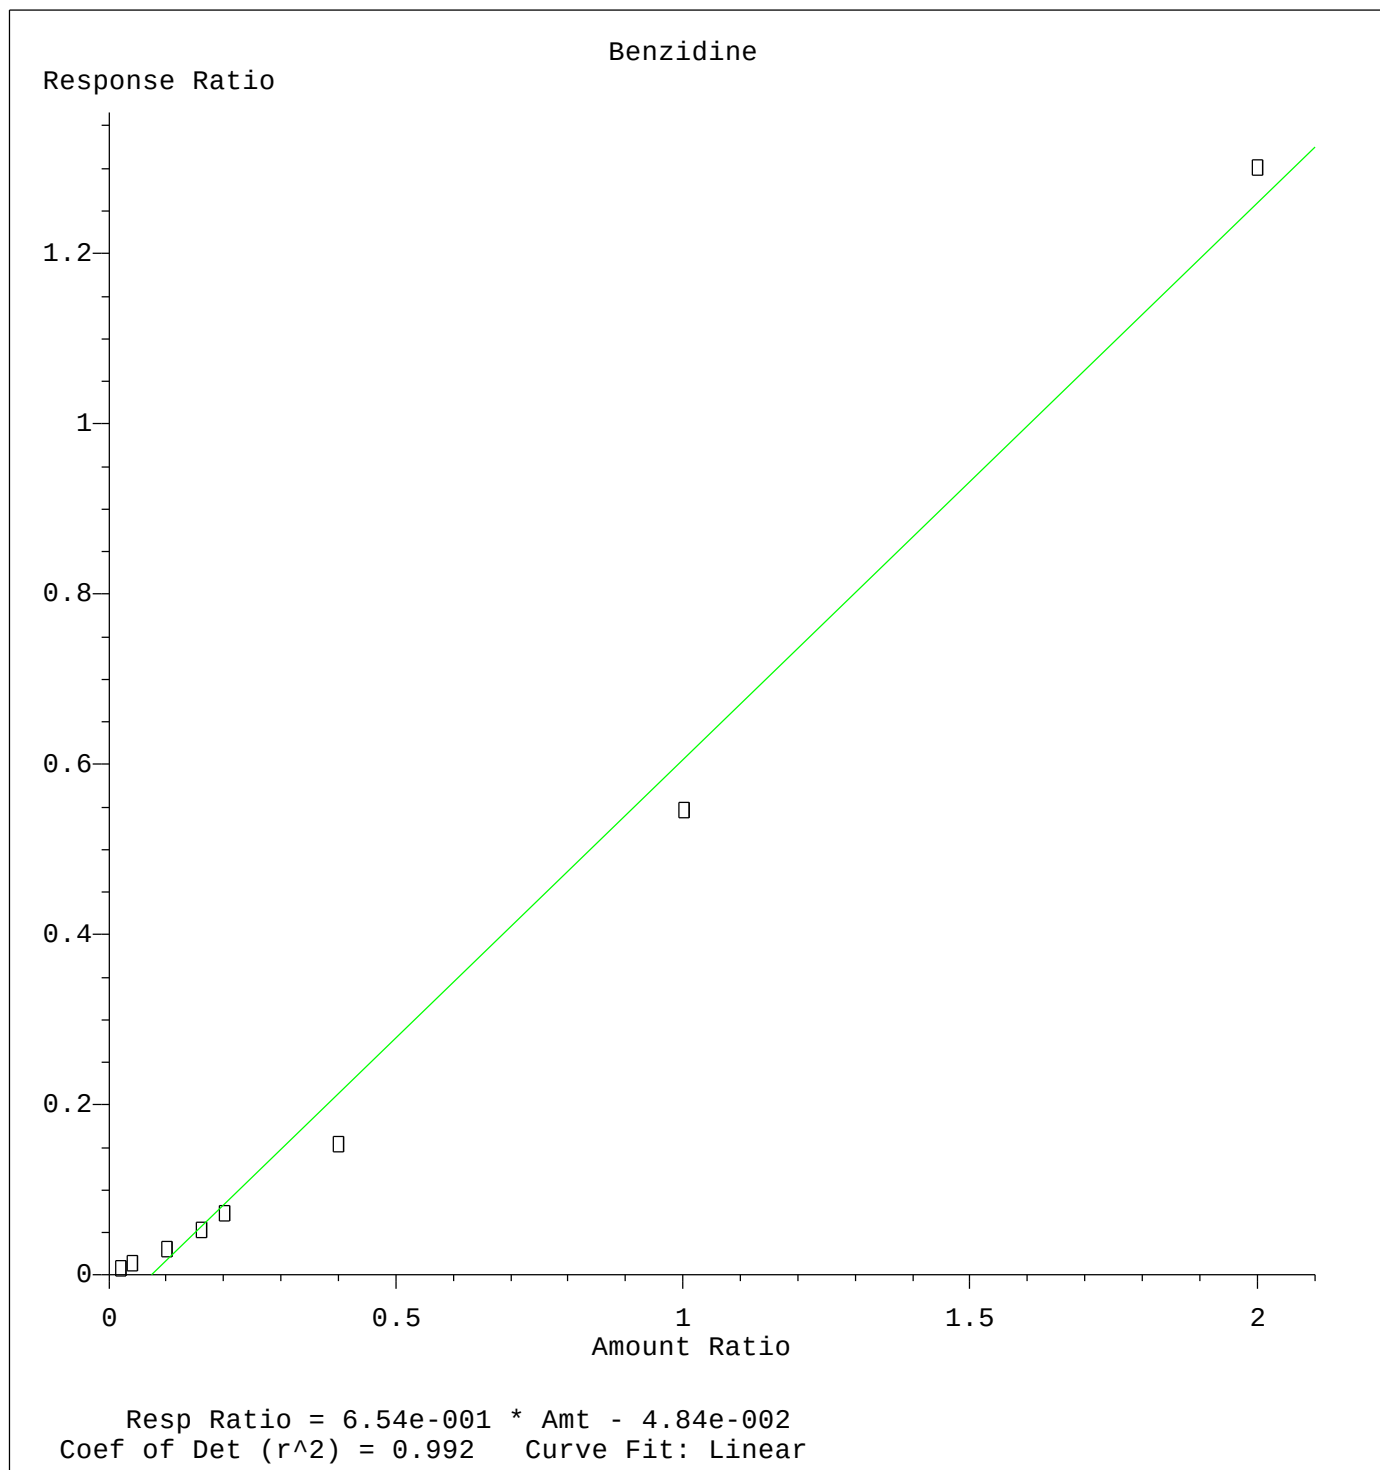

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
Calibration Table Last Updated: Wed Dec 02 16:19:00 2015

3,3'-Dichlorobenzidine

Response Ratio

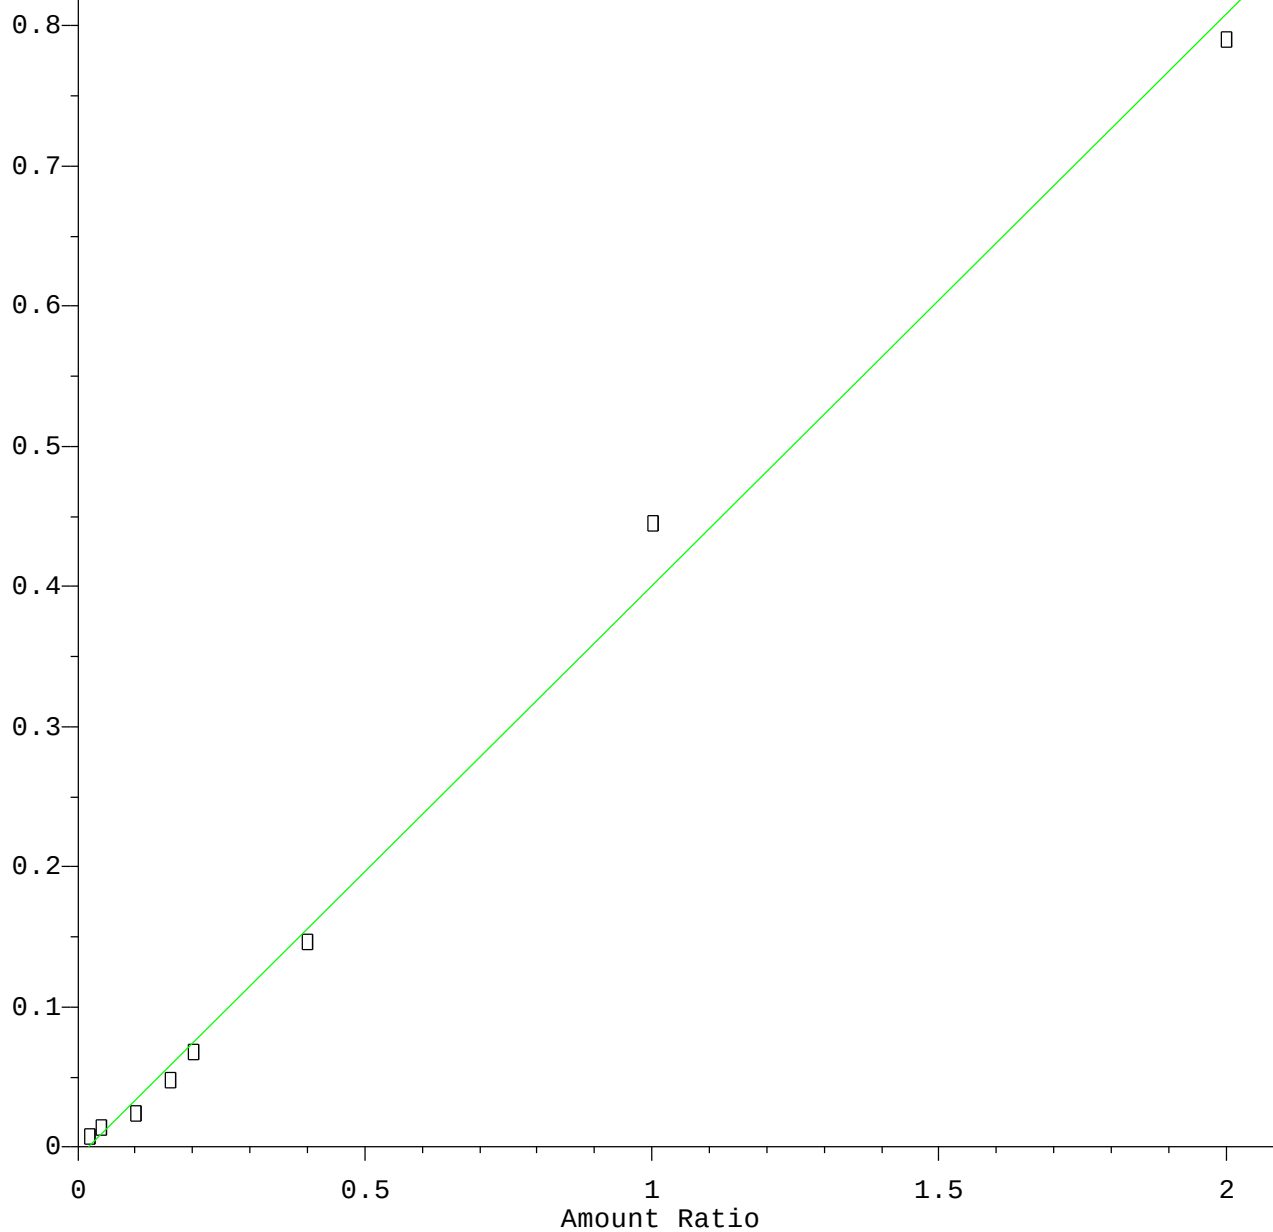


Resp Ratio = $4.08 \times 10^{-1} \times \text{Amt} - 7.19 \times 10^{-3}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
Calibration Table Last Updated: Wed Dec 02 16:19:00 2015

Bis(2-ethylhexyl)phthalate

Response Ratio

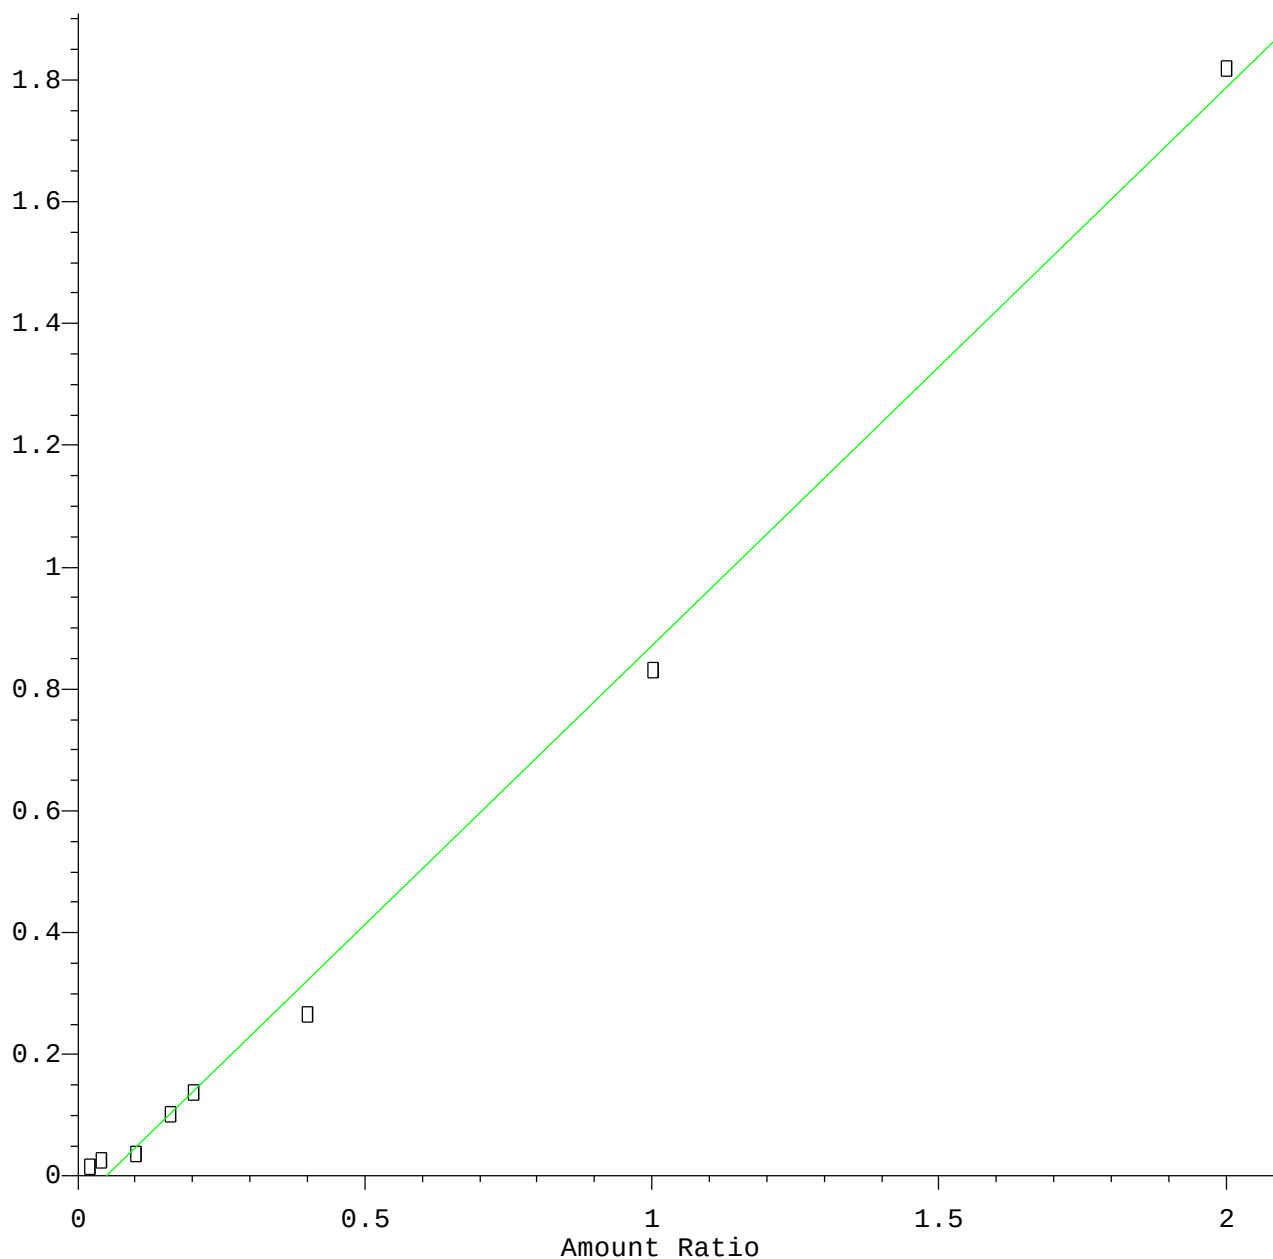

Resp Ratio = $9.16 \times 10^{-1} \times \text{Amt} - 4.56 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
Calibration Table Last Updated: Wed Dec 02 16:19:00 2015