


Data Path : Z:\HPCHEM1\BNA M\Data\BM120215\
 Data File : BM003350.D
 Acq On : 02 Dec 2015 10:03
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 16:19:00 2015

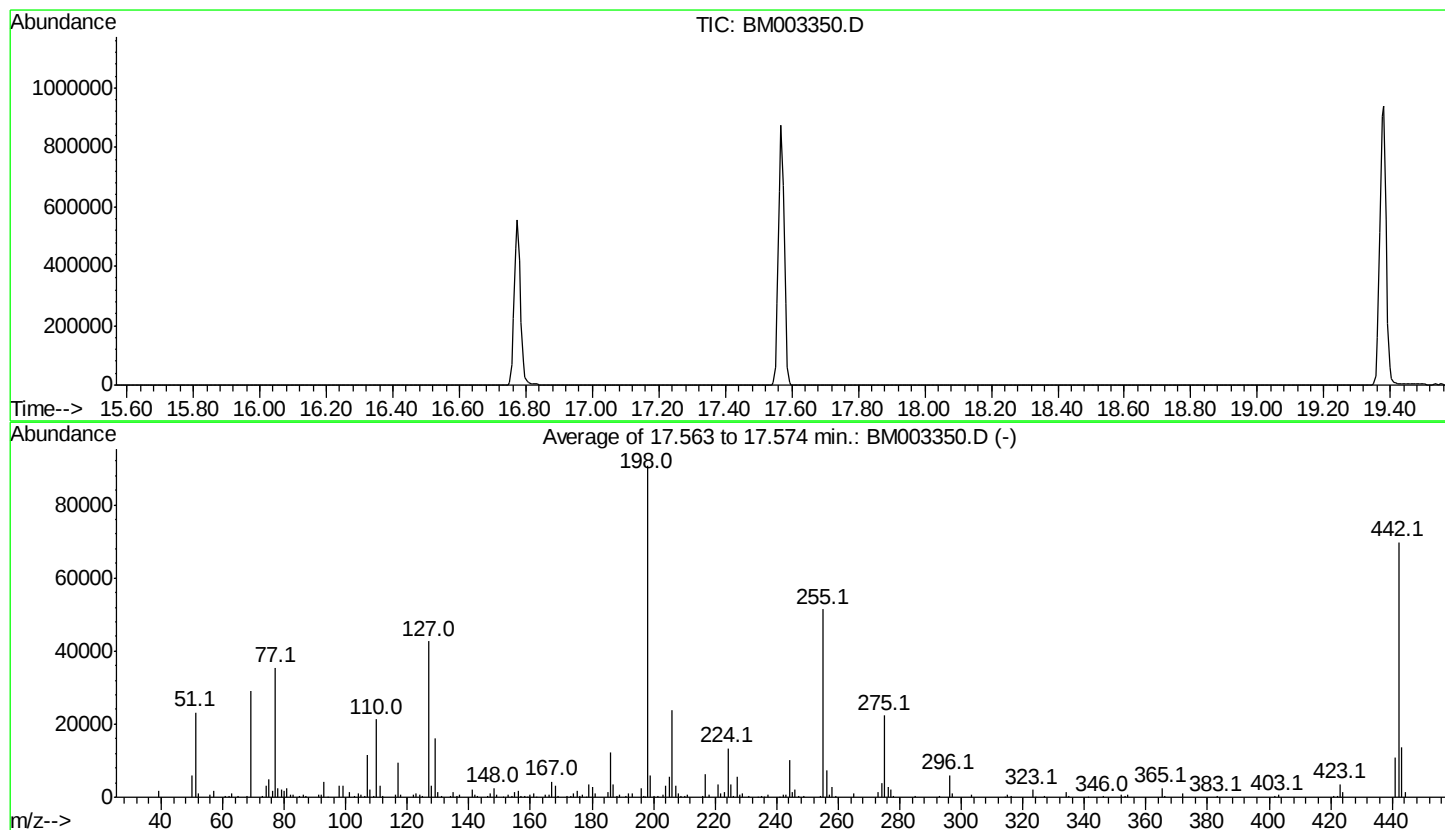

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	23253	PASS
68	69	0.00	2	1.8	520	PASS
69	198	0.00	100	32.0	29034	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	42685	PASS
197	198	0.00	2	0.4	324	PASS
198	198	100	100	100.0	90701	PASS
199	198	5	9	6.7	6120	PASS
275	198	10	60	24.6	22288	PASS
365	198	1	100	2.9	2599	PASS
441	442	0.01	24	15.4	10758	PASS
442	198	50	100	77.0	69845	PASS
443	442	15	24	19.3	13503	PASS