

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120216\
 Data File : BM008170.D
 Acq On : 02 Dec 2016 23:25
 Operator : UM/SJ
 Sample : H5733-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YA8Z4

Quant Time: Dec 03 00:58:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 03 00:55:35 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	546	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.48	136	1893	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.33	164	1084	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.18	188	145547	0.40	ng/ul	0.09
16) Chrysene-d12	21.29	240	1583	0.40	ng/ul	0.00
20) Perylene-d12	23.37	264	115254	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	840	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	1365	0.00	ng/ul	-0.02
Target Compounds						
9) Fluorene	15.32	166	318	0.07	ng/ul#	33
17) Pyrene	19.48	202	289	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120216\
Data File : BM008170.D
Acq On : 02 Dec 2016 23:25
Operator : UM/SJ
Sample : H5733-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YA8Z4

Quant Time: Dec 03 00:58:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 03 00:55:35 2016
Response via : Initial Calibration




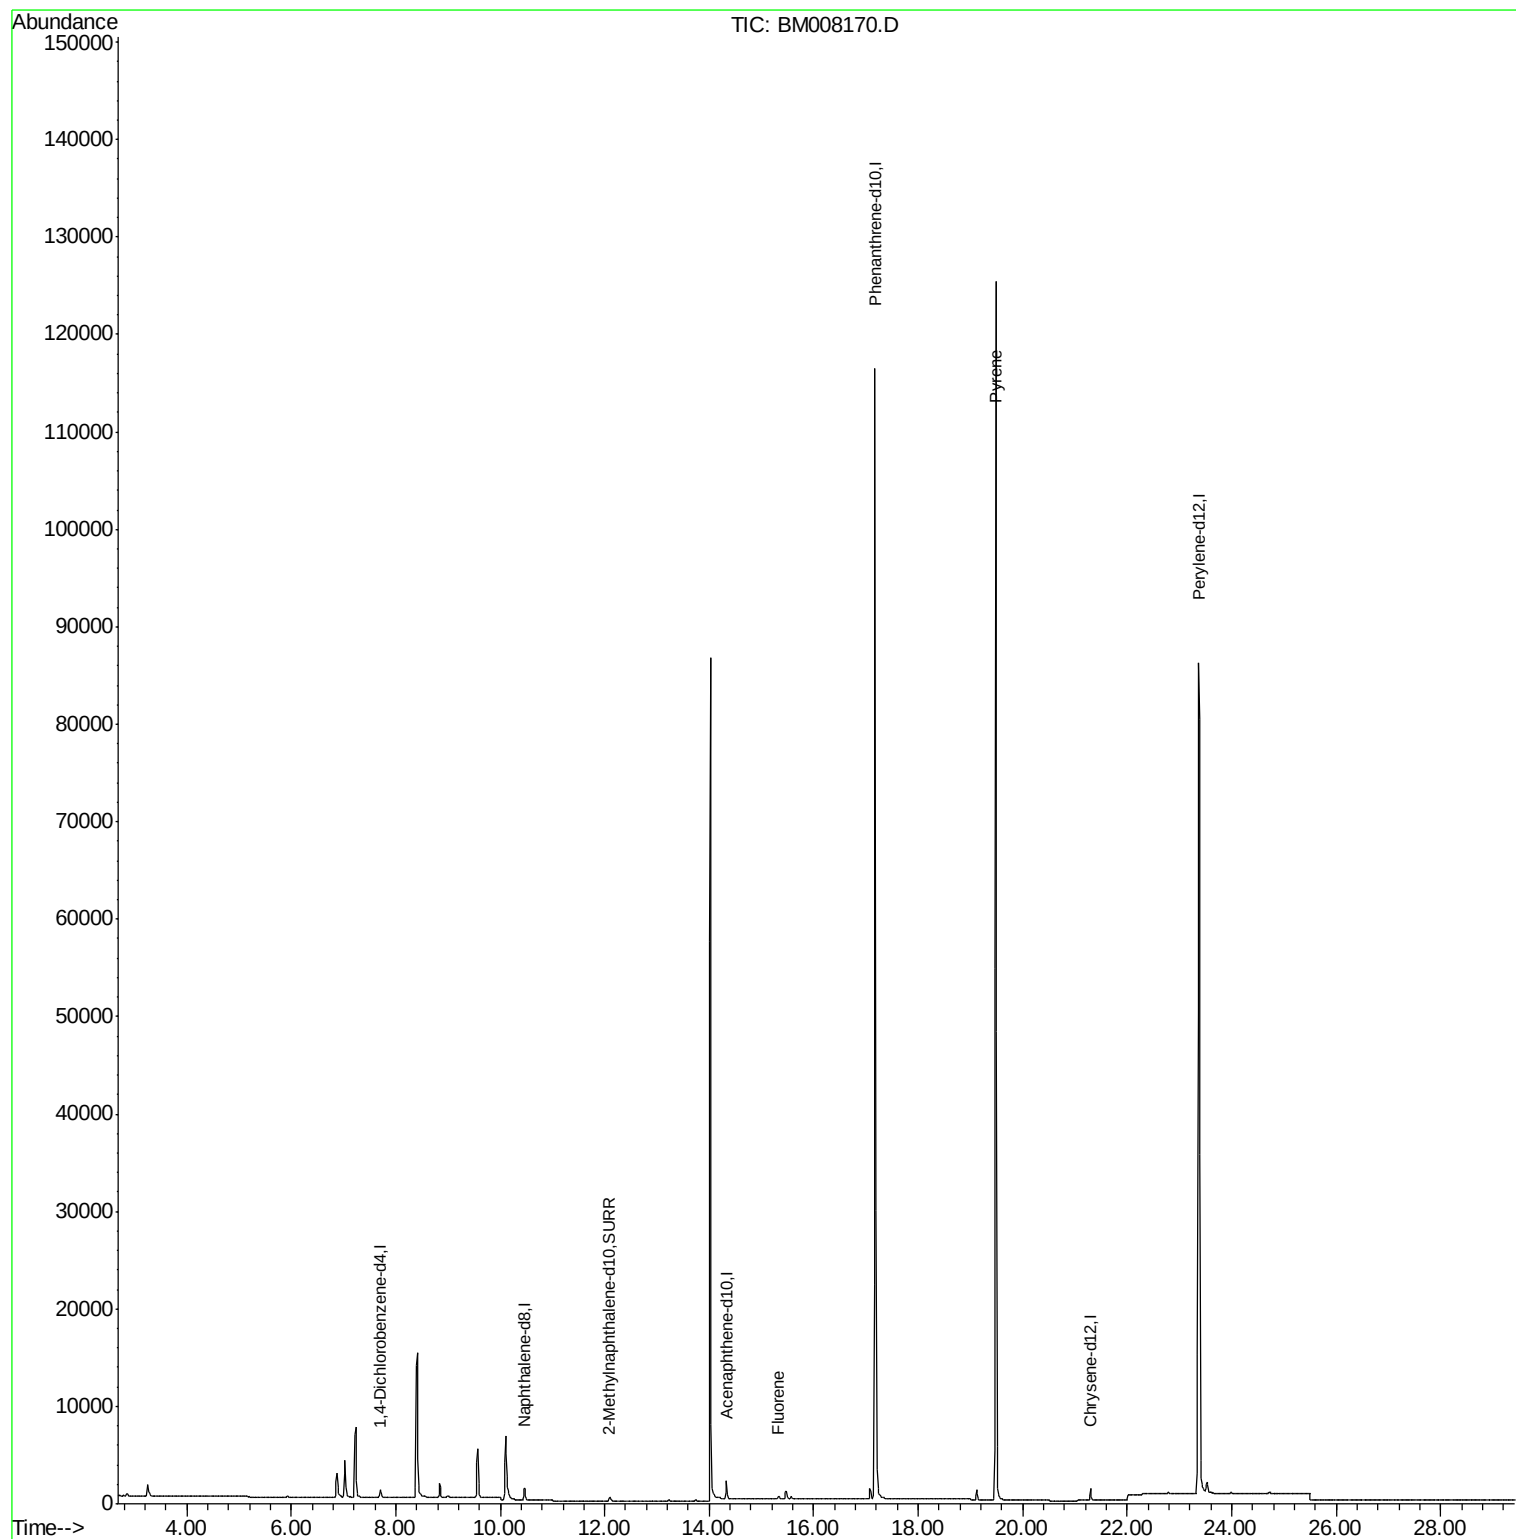


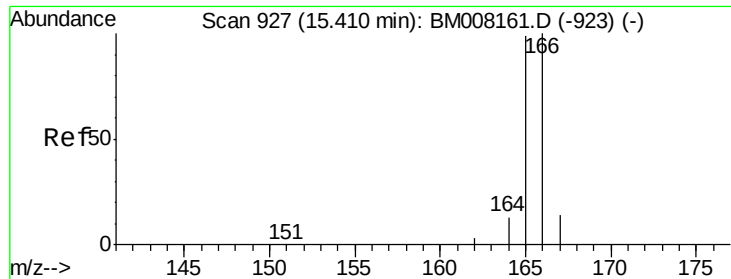

#9
Fluorene
 Concen: 0.07 ng/ul
 RT: 15.32 min Scan# 922
 Delta R.T. -0.09 min
 Lab File: BM008170.D
 Acq: 02 Dec 2016 23:25

Instrument :
 BNA_M
 ClientSampleId :
 YA8Z4

Tgt Ion:166 Resp: 318
 Ion Ratio Lower Upper
 166 100
 165 24.9 73.4 110.2#
 167 40.1 14.6 22.0#

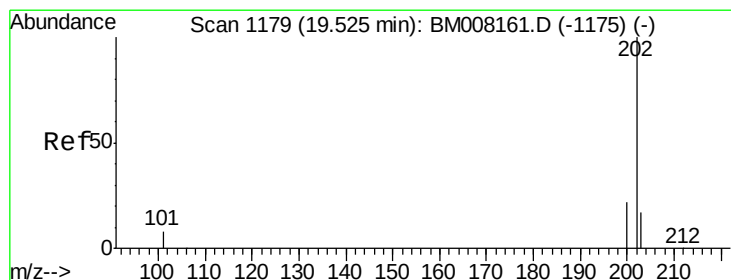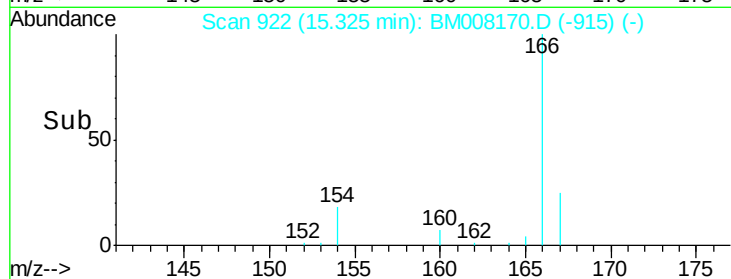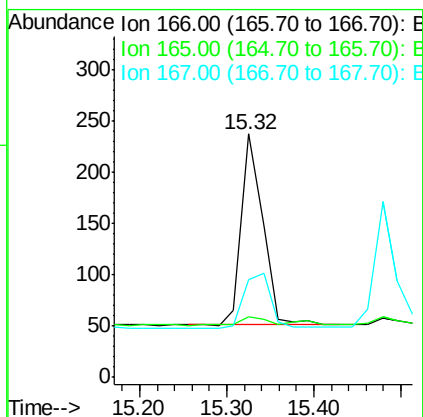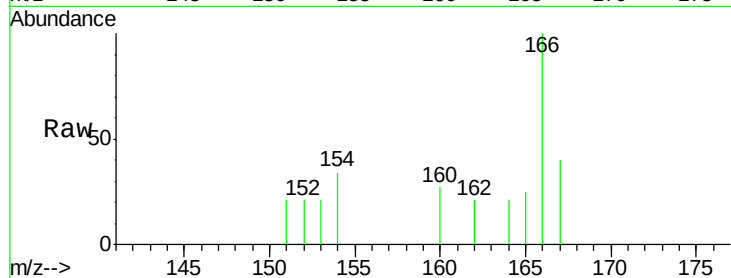

#17
Pyrene
 Concen: 0.05 ng/ul
 RT: 19.48 min Scan# 1176
 Delta R.T. -0.04 min
 Lab File: BM008170.D
 Acq: 02 Dec 2016 23:25

Tgt Ion:202 Resp: 289
 Ion Ratio Lower Upper
 202 100
 200 23.1 18.2 27.4
 203 172.9 15.6 23.4#

