

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120216\
 Data File : BM008173.D
 Acq On : 03 Dec 2016 01:12
 Operator : UM/SJ
 Sample : H5733-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YA8Y0

Quant Time: Dec 03 02:35:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 03 00:55:35 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	508	0.40	ng/ul	0.00
2) Naphthalene-d8	10.48	136	1664	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.33	164	977	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.18	188	161889	0.40	ng/ul	0.09
16) Chrysene-d12	21.30	240	1687	0.40	ng/ul	0.00
20) Perylene-d12	23.37	264	116691	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.10	152	896	0.38	ng/ul	0.01
14) Fluoranthene-d10	19.12	212	1597	0.00	ng/ul	-0.02
Target Compounds						
9) Fluorene	15.32	166	344	0.09	ng/ul#	32
17) Pyrene	19.48	202	316	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120216\
Data File : BM008173.D
Acq On : 03 Dec 2016 01:12
Operator : UM/SJ
Sample : H5733-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YA8Y0

Quant Time: Dec 03 02:35:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 03 00:55:35 2016
Response via : Initial Calibration

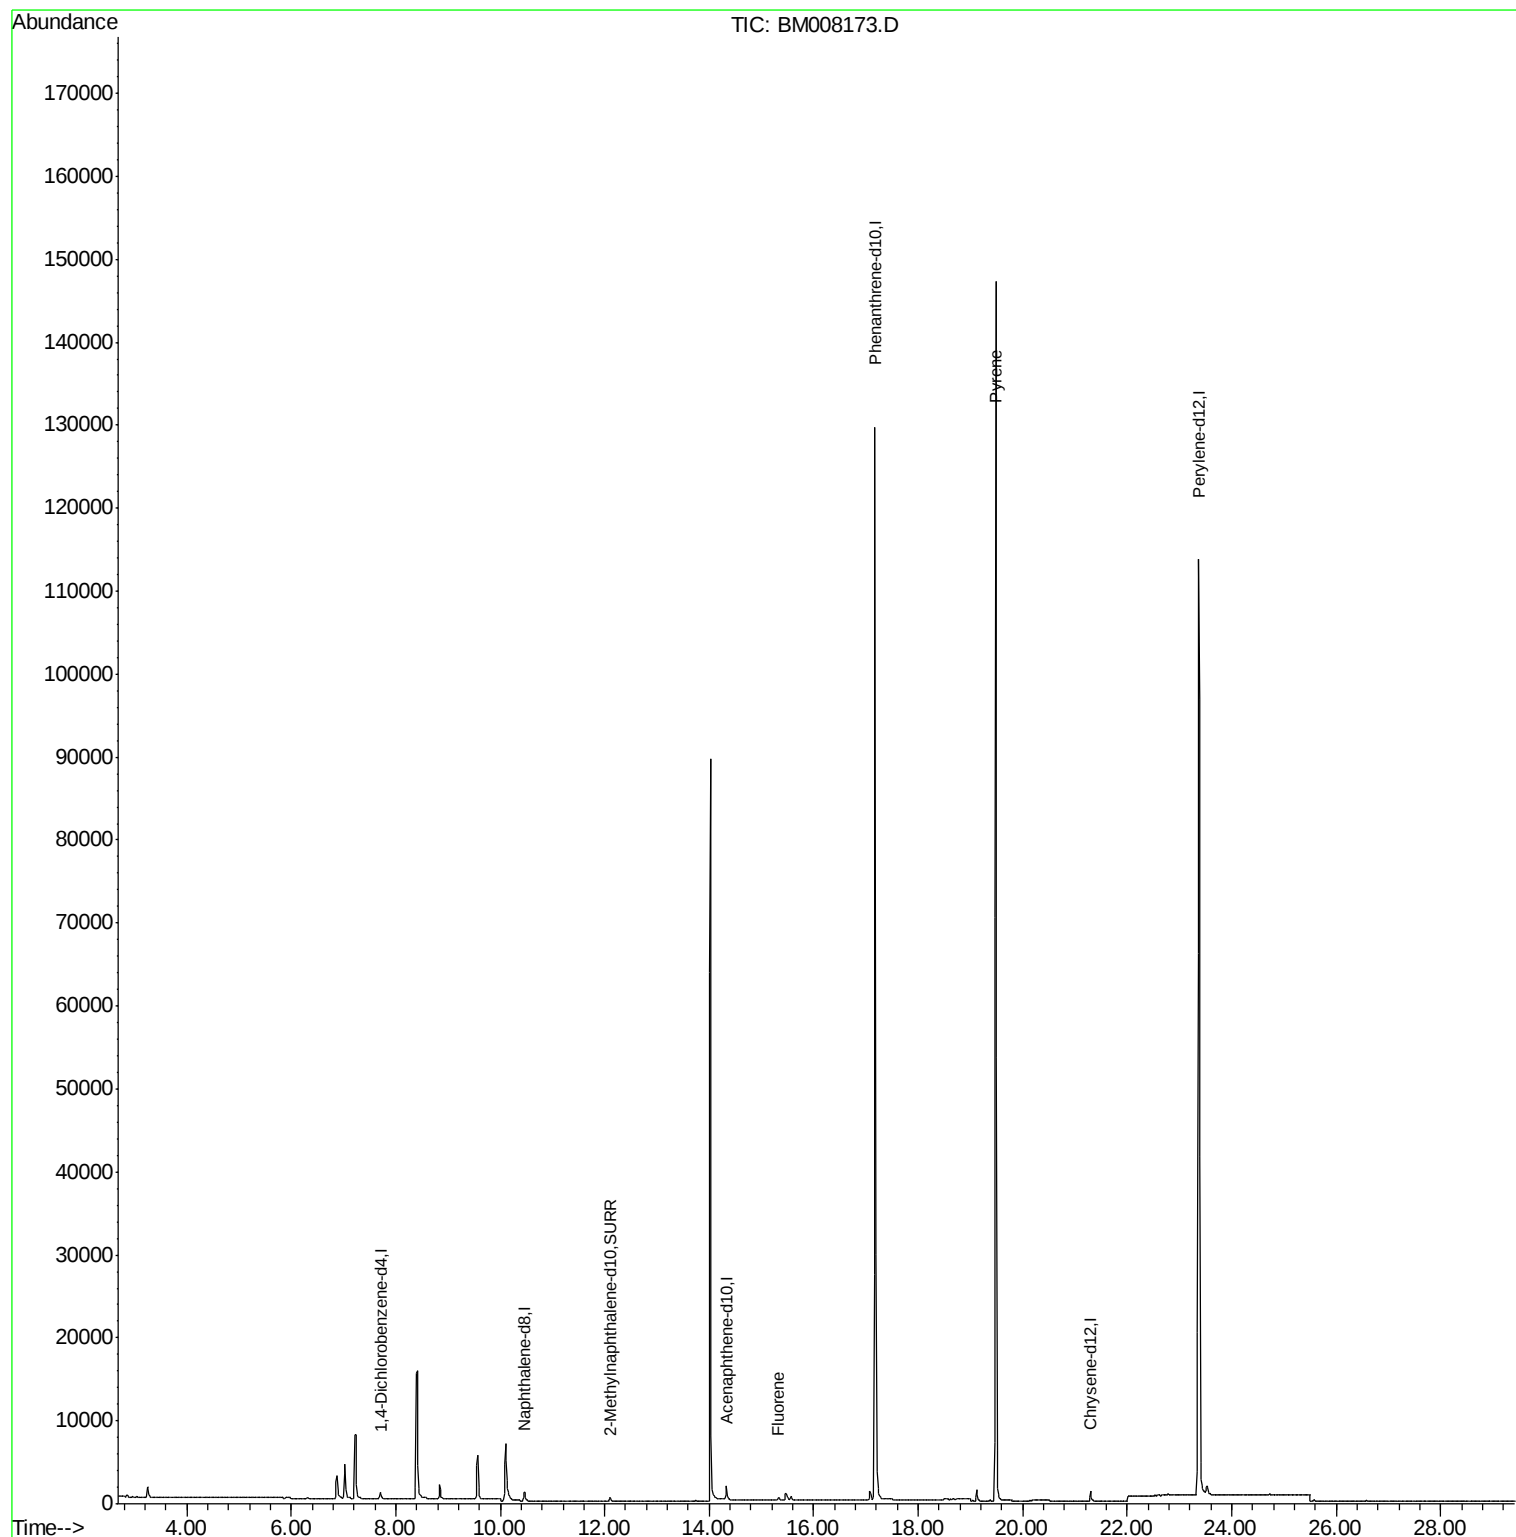

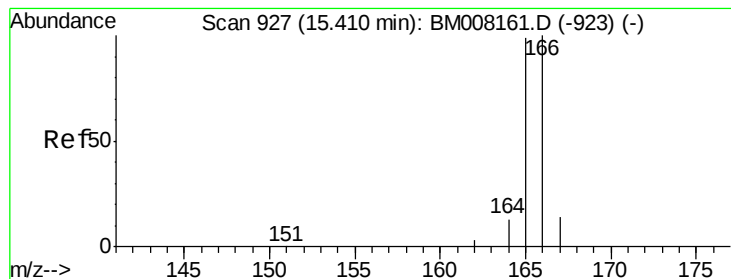

#9

Fluorene

Concen: 0.09 ng/ul

RT: 15.32 min Scan# 922

Delta R.T. -0.09 min

Lab File: BM008173.D

Acq: 03 Dec 2016 01:12

Instrument :

BNA_M

ClientSampleId :

YA8Y0





Tgt Ion:166 Resp: 344

Ion Ratio Lower Upper

166 100

165 22.9 73.4 110.2#

167 39.5 14.6 22.0#

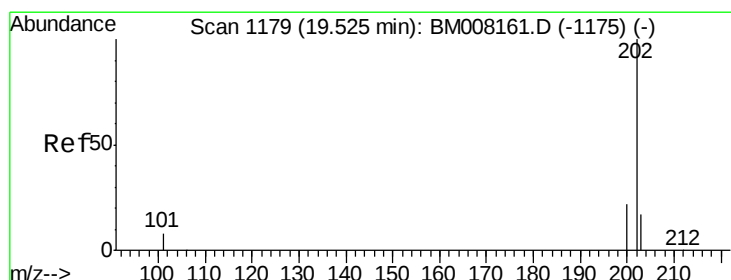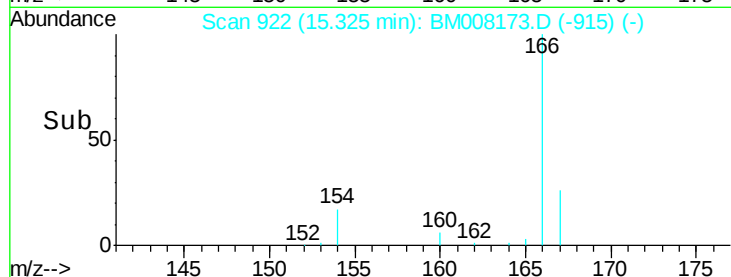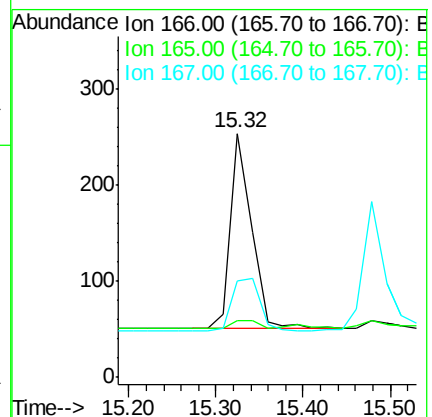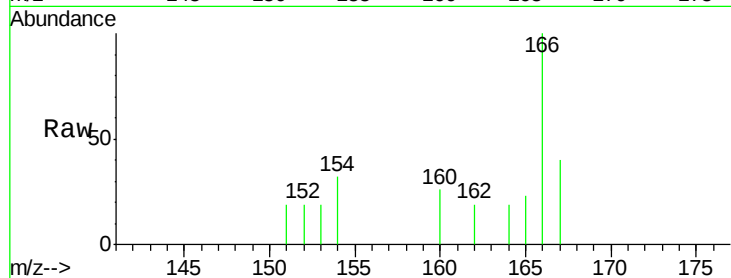

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.48 min Scan# 1176

Delta R.T. -0.04 min

Lab File: BM008173.D

Acq: 03 Dec 2016 01:12

Tgt Ion:202 Resp: 316

Ion Ratio Lower Upper

202 100

200 21.3 18.2 27.4

203 176.8 15.6 23.4#

