


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
Data File : BM008157.D
Acq On : 02 Dec 2016 15:39
Operator : UM/SJ
Sample : H5730-10MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 02 17:57:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 15:28:31 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4WH6MS

Manual Integrations
APPROVED

sohil
12/5/2016 11:17:33 AM

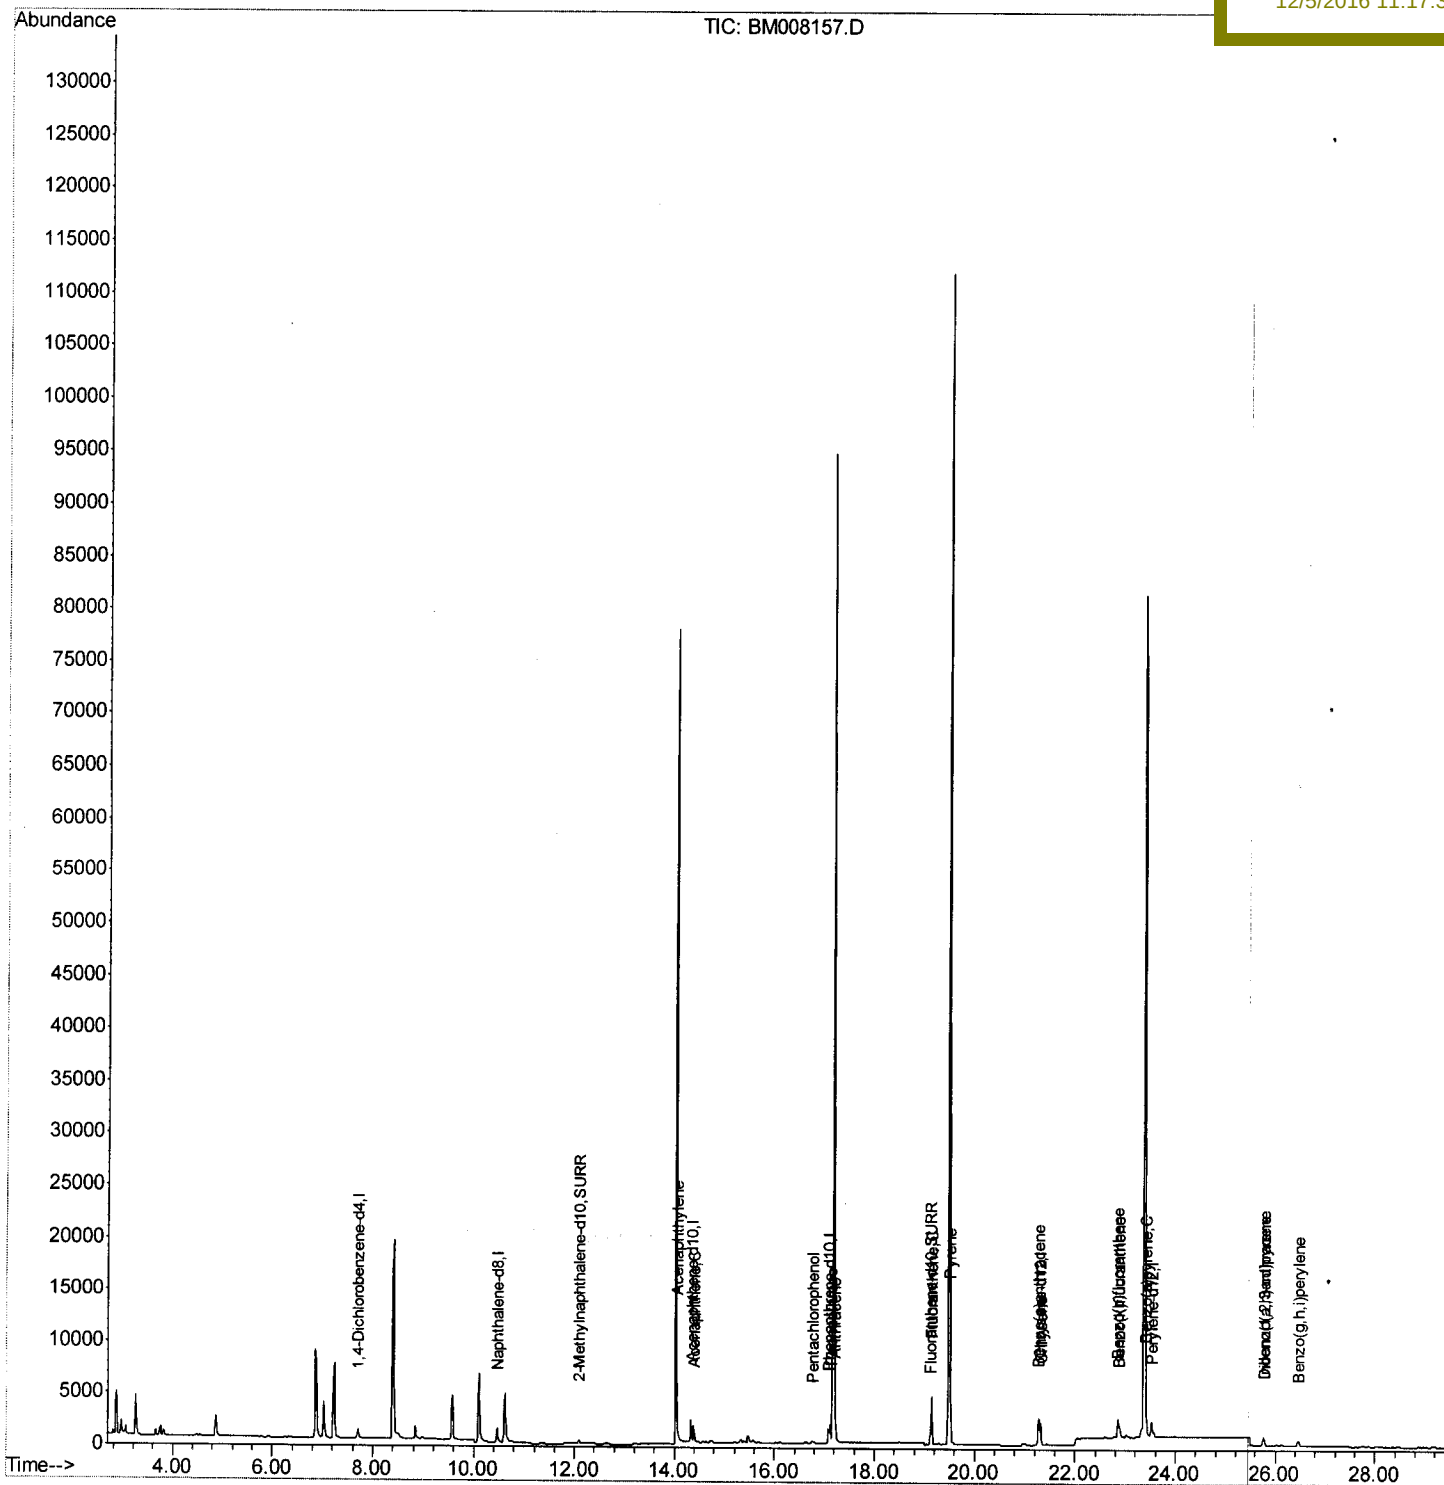

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

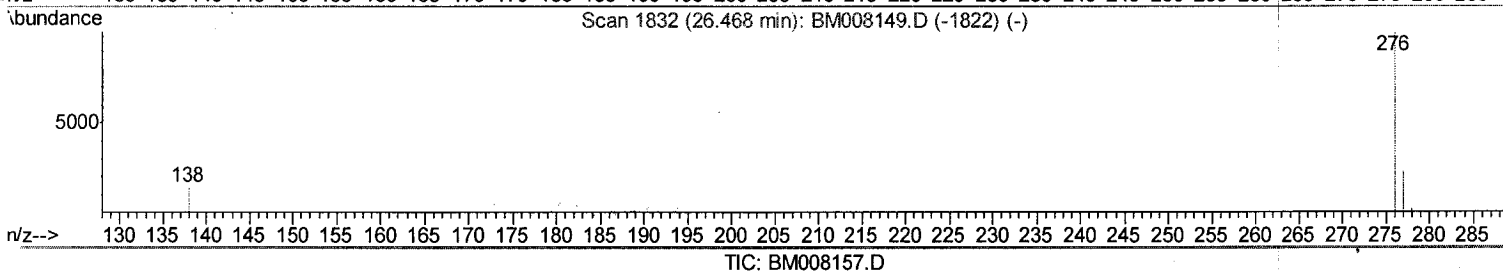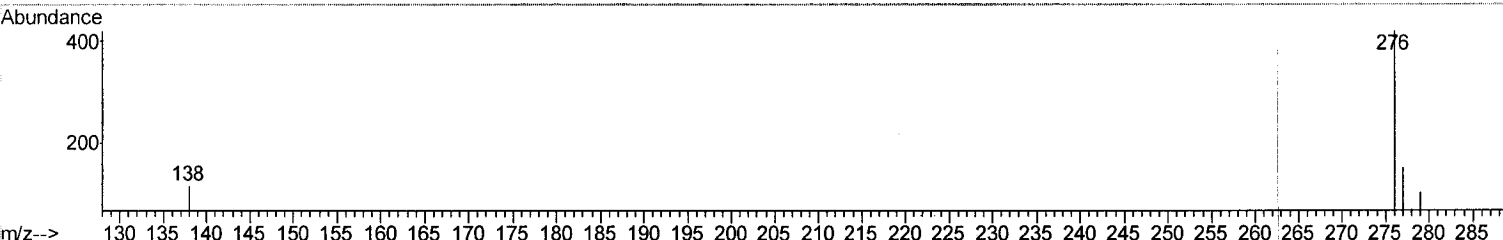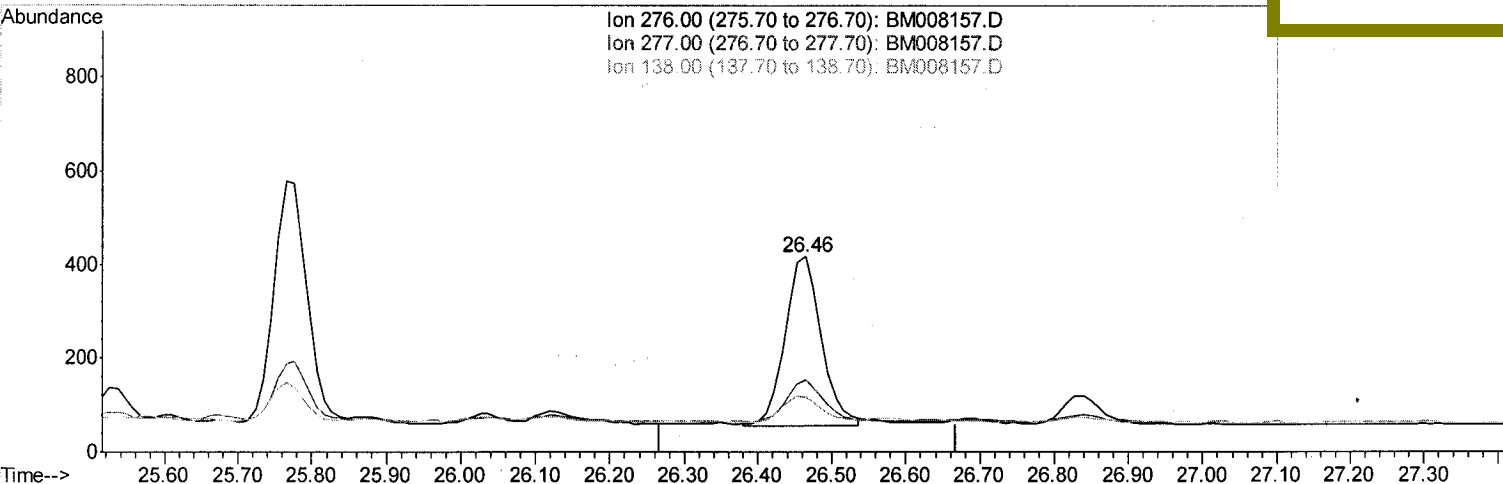

(26) Benzo(g,h,i)perylene

26.464min (-0.003) 0.17ng/ul m

response 1226

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	36.60#
138.00	25.60	27.99
0.00	0.00	0.00

9.9
 12/08/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

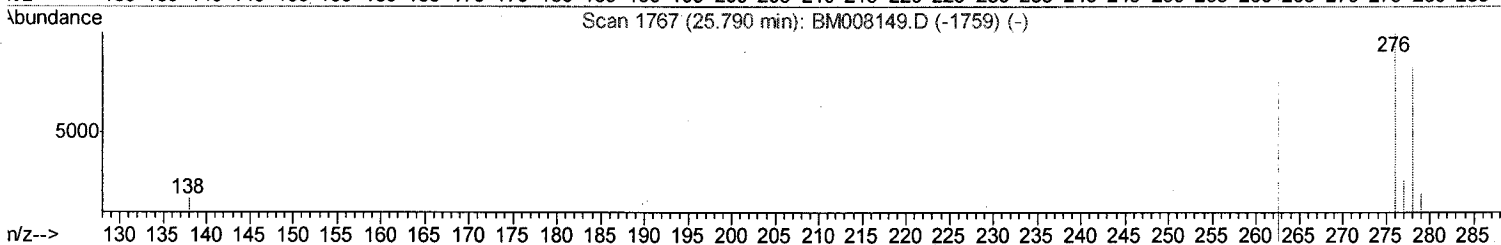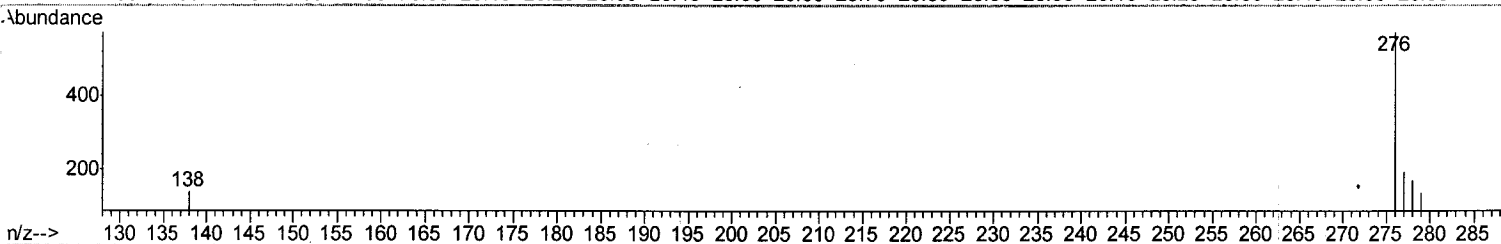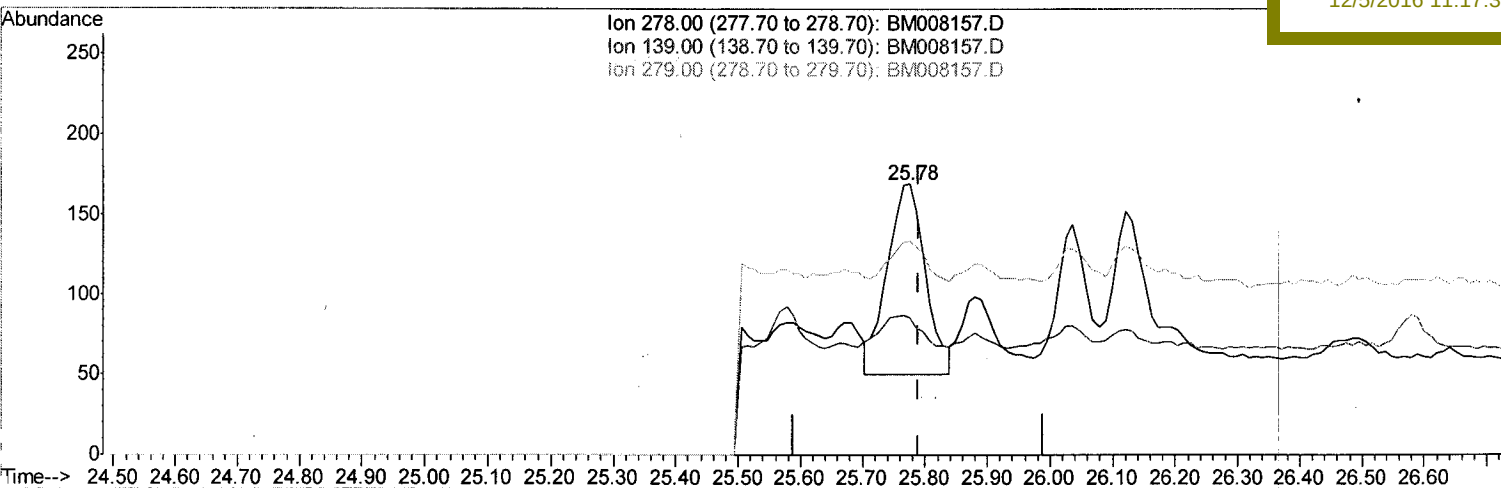

TIC: BM008157.D

(25) Dibenzo(a,h)anthracene

25.776min (-0.014) 0.08ng/ul m

response 508

Ion Exp% Act%

278.00 100 100

139.00 21.70 50.30#

279.00 32.40 79.29#

0.00 0.00 0.00

> 5.7
 12/06/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

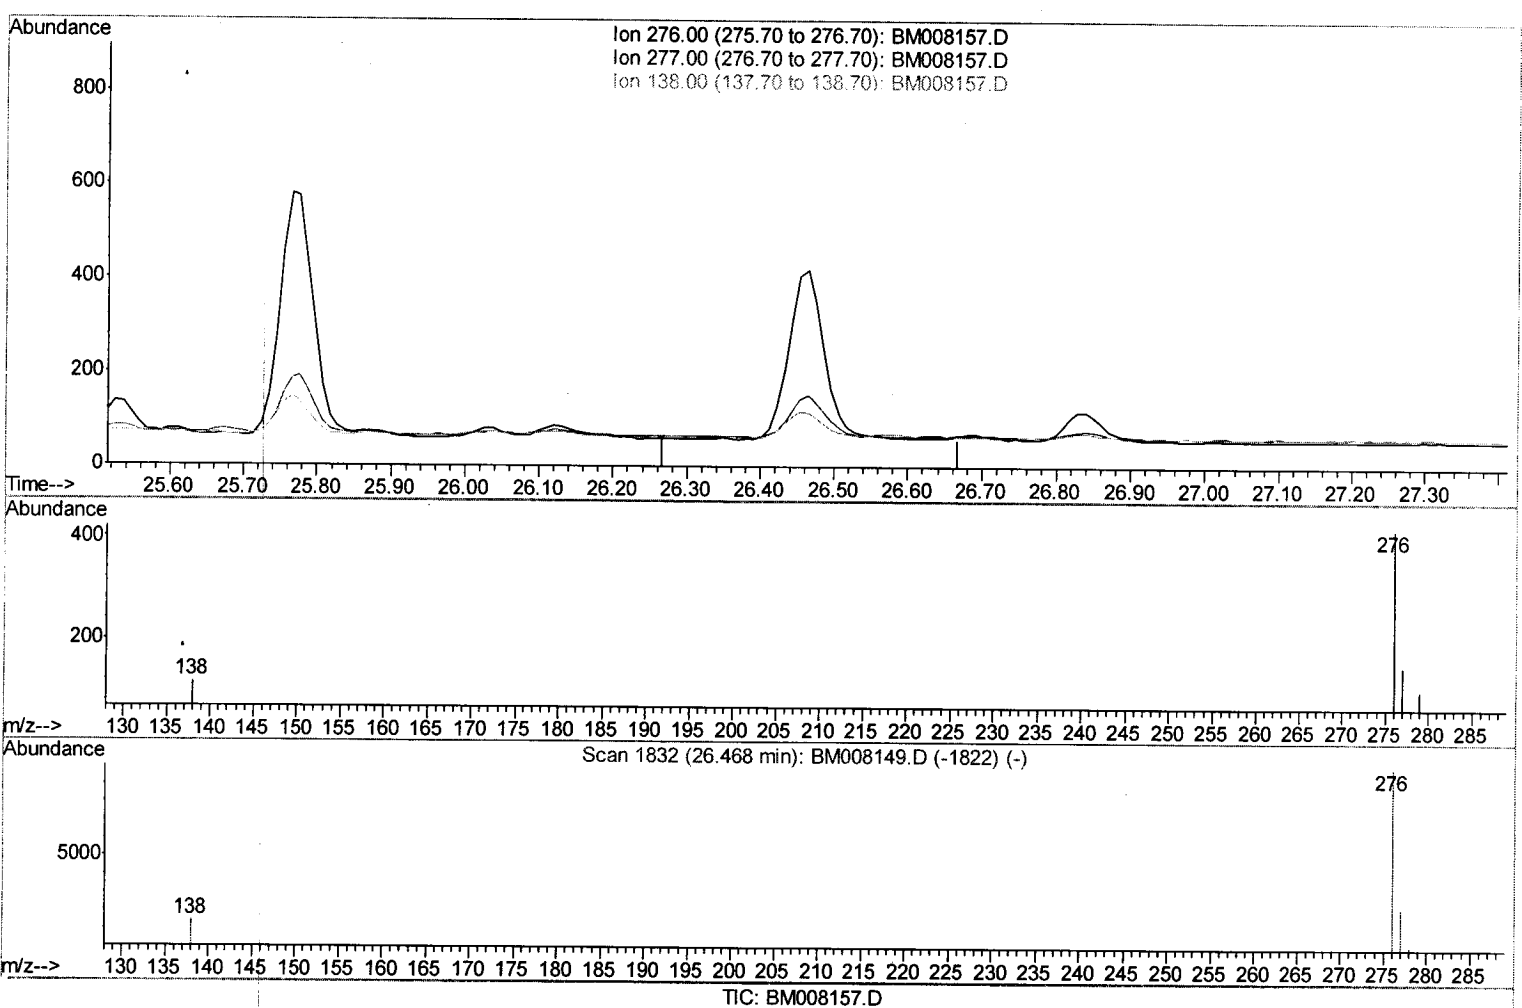

(26) Benzo(g,h,i)perylene

26.468min (-26.468) 0.00ng/ui

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

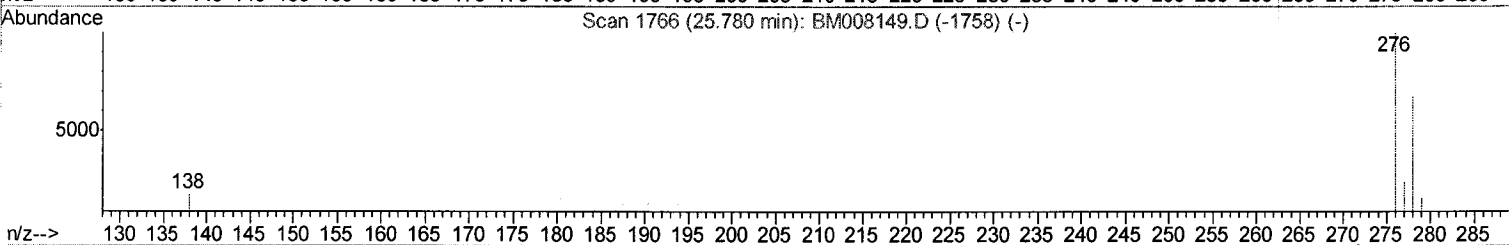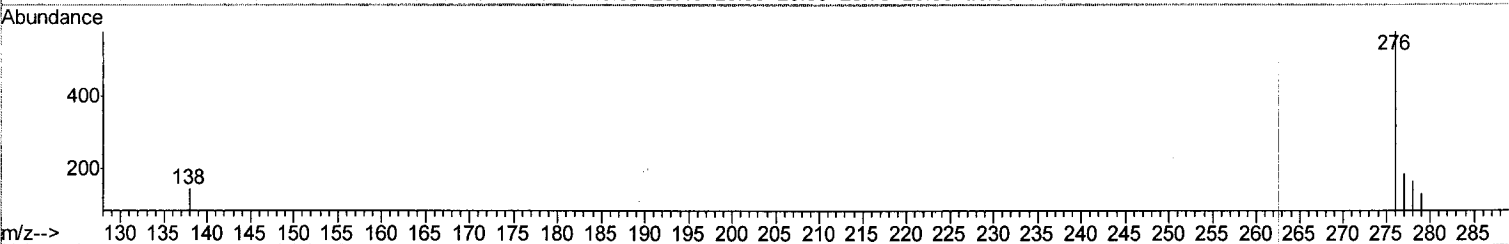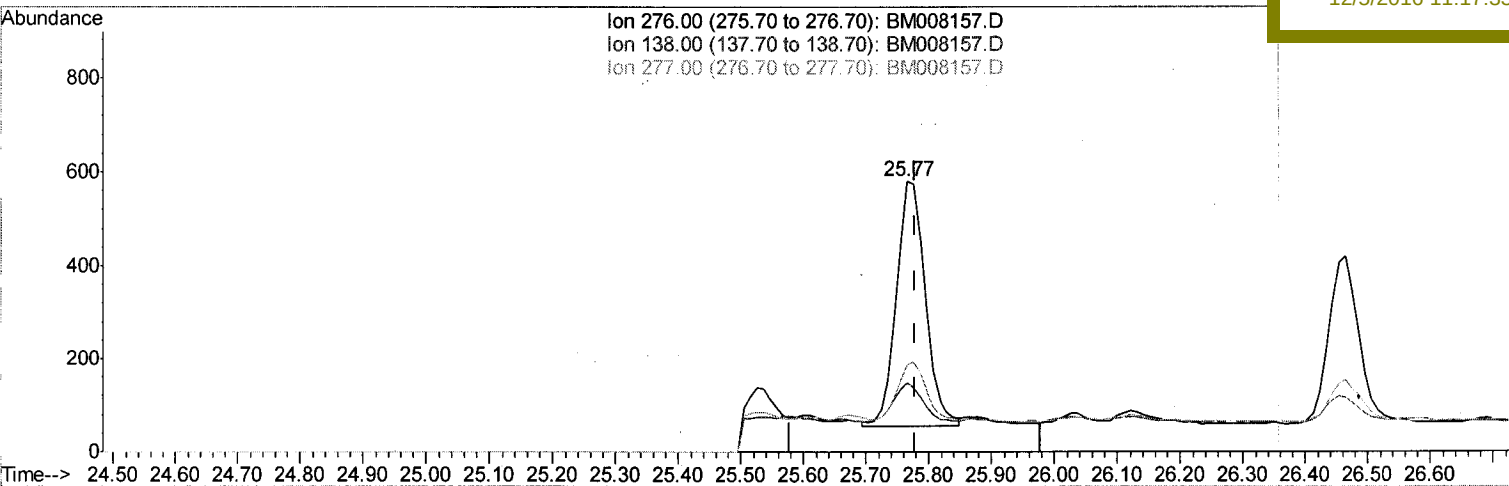

TIC: BM008157.D

(24) Indeno(1,2,3-cd)pyrene

25.766min (-0.014) 0.20ng/ul m

response 1669

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	59.08#
0.00	0.00	0.00

> 9.9
 12/02/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

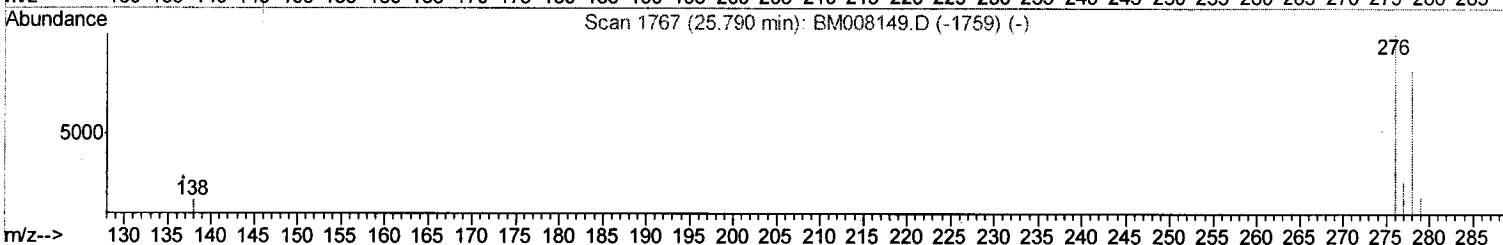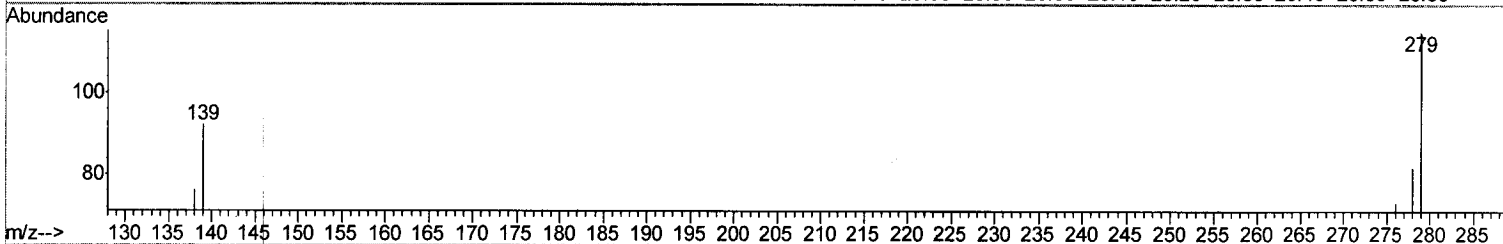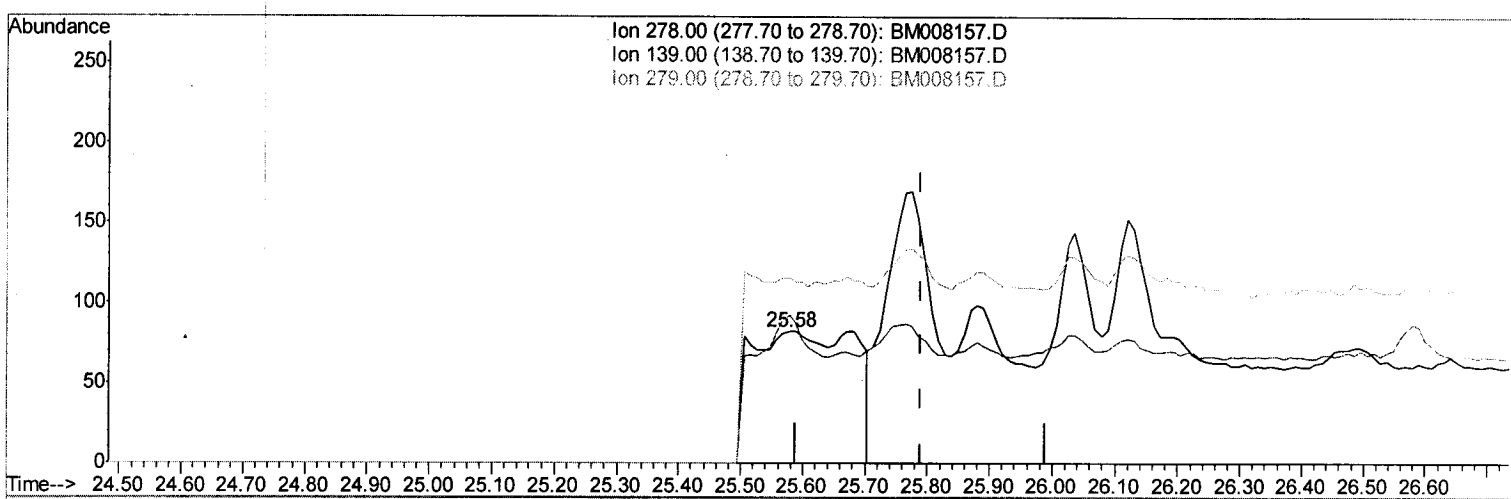

TIC: BM008157.D

(25) Dibenzo(a,h)anthracene

25.578min (-0.212) 0.14ng/ul

response 955

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	112.20#
279.00	32.40	140.24#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

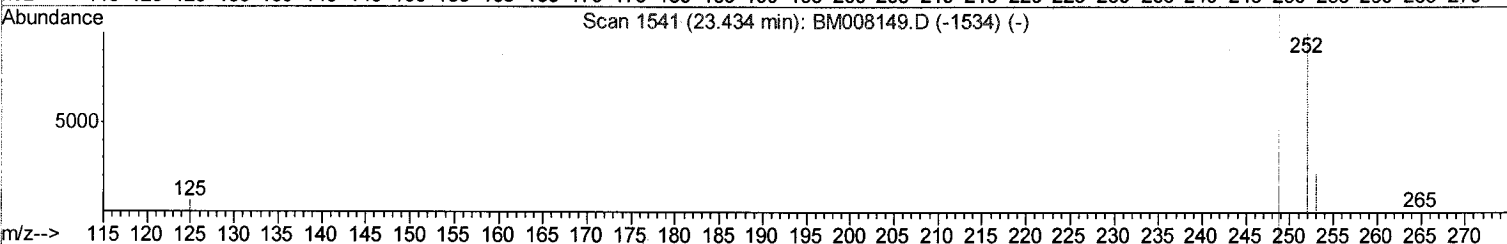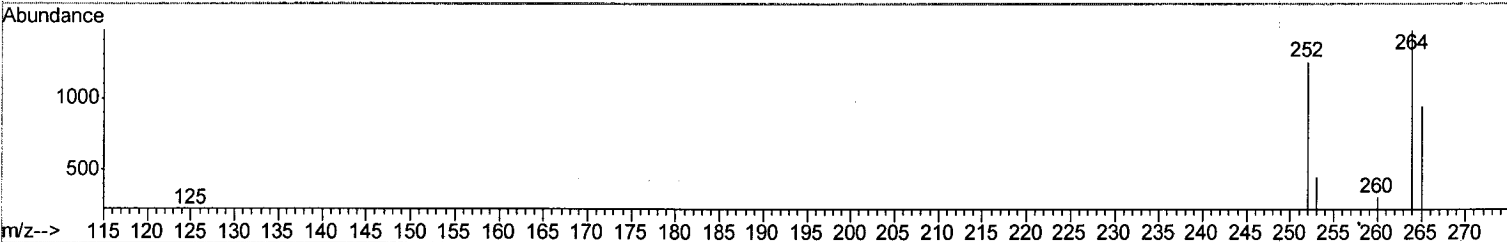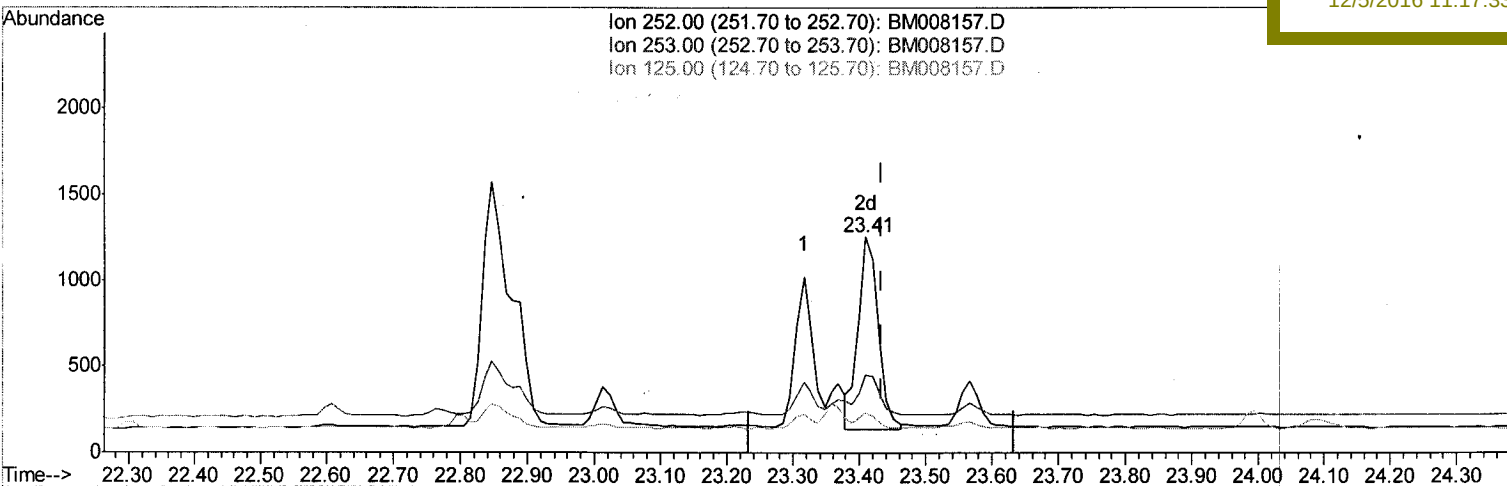

TIC: BM008157.D

(23) Benzo(a)pyrene (C)

23.410min (-0.024) 0.34ng/ul m

response 2318

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	35.73
125.00	22.60	18.34
0.00	0.00	0.00

> 5.9
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

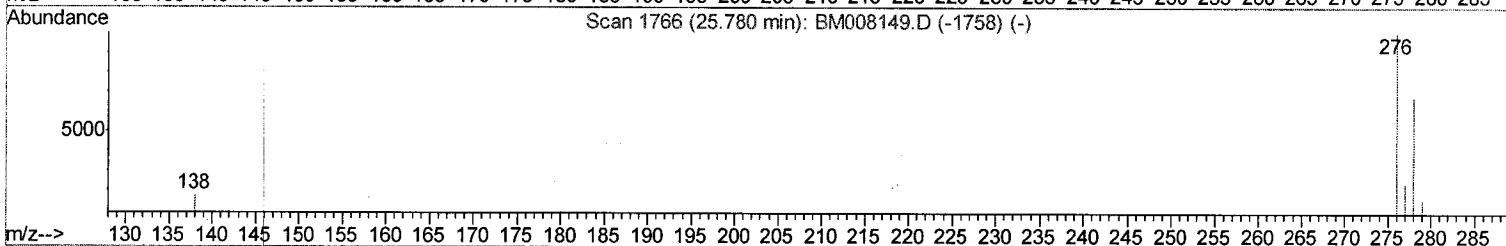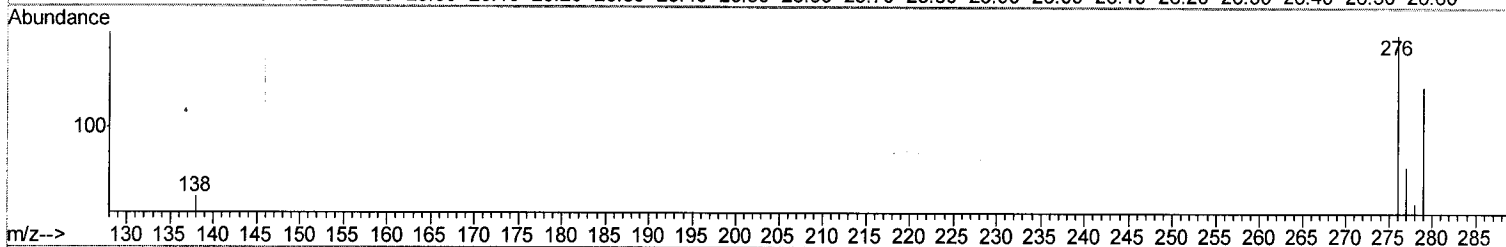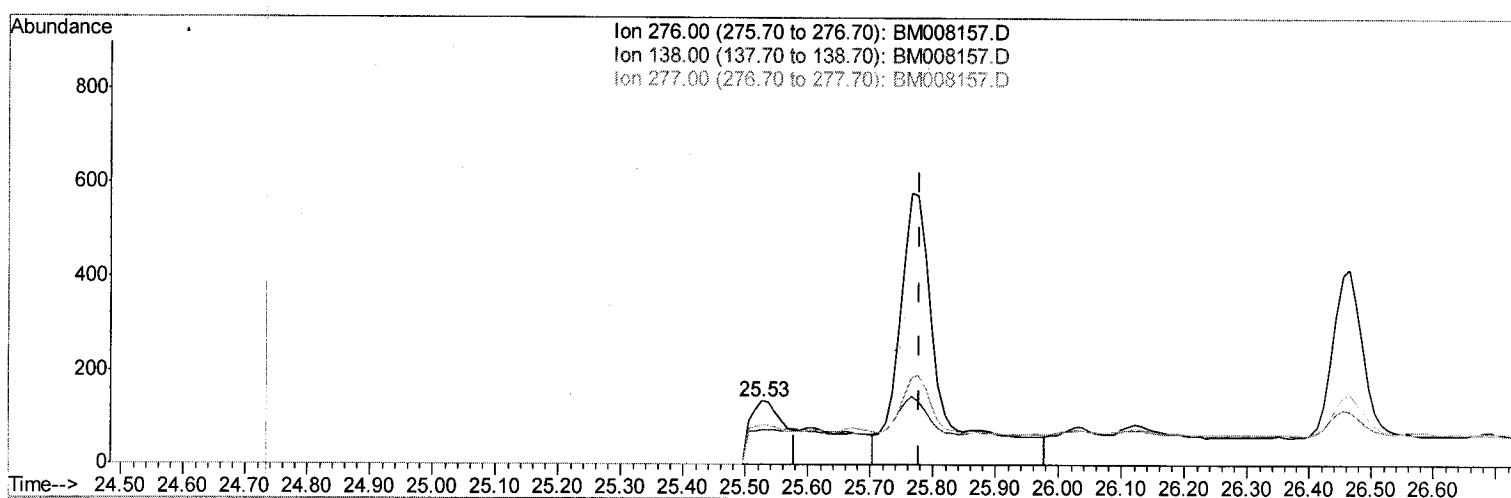

TIC: BM008157.D

(24) Indeno(1,2,3-cd)pyrene

25.526min (-0.254) 0.13ng/ul

response 1046

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	94.26#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

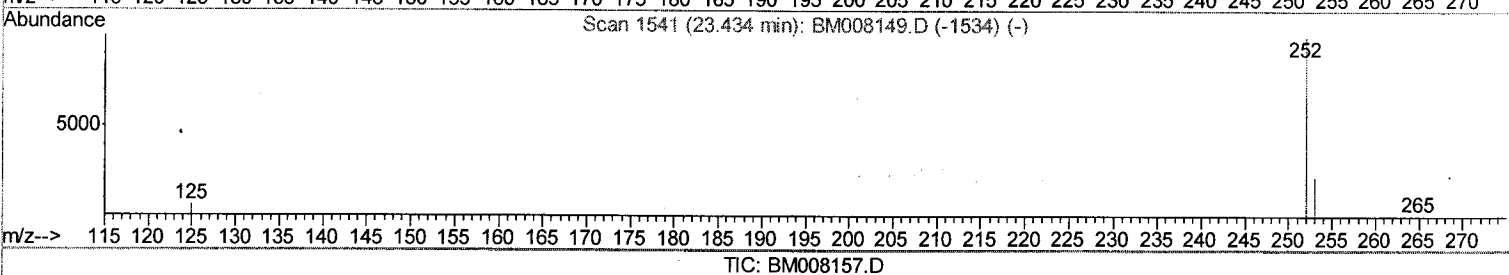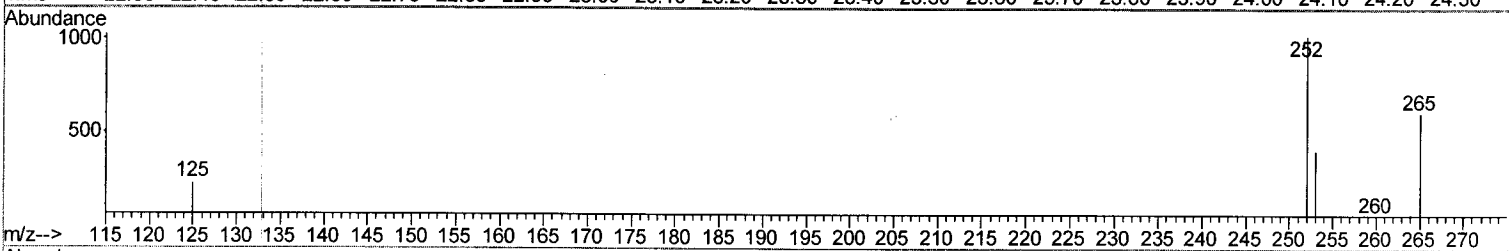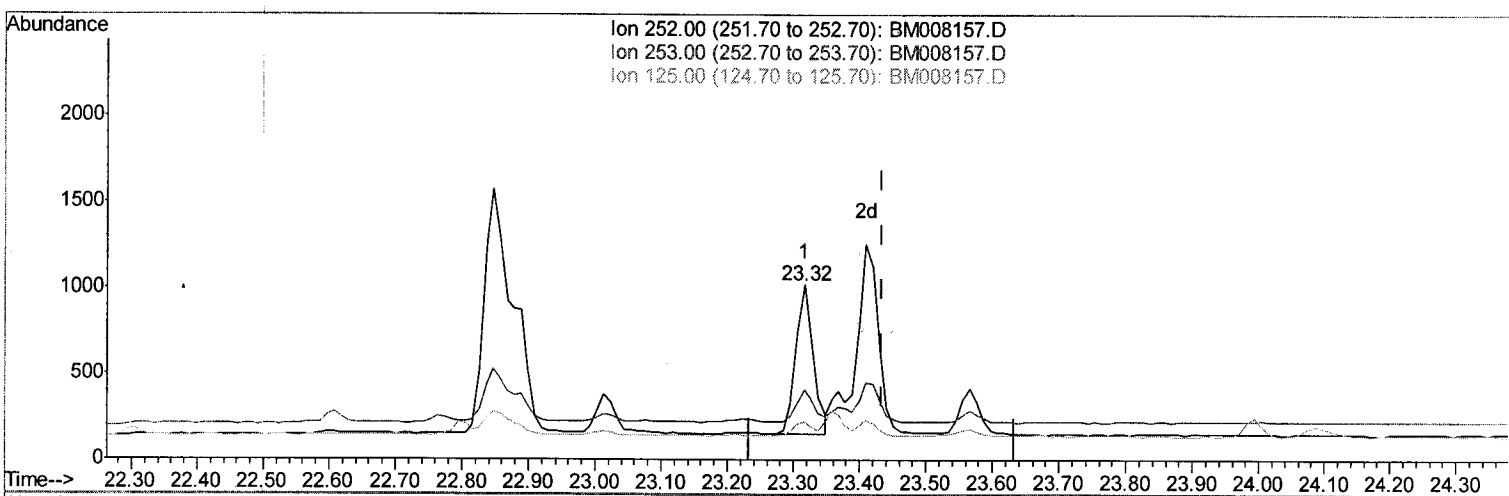

(23) Benzo(a)pyrene (C)

23.316min (-0.118) 0.24ng/ul

response 1601

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	39.65
125.00	22.60	21.98
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

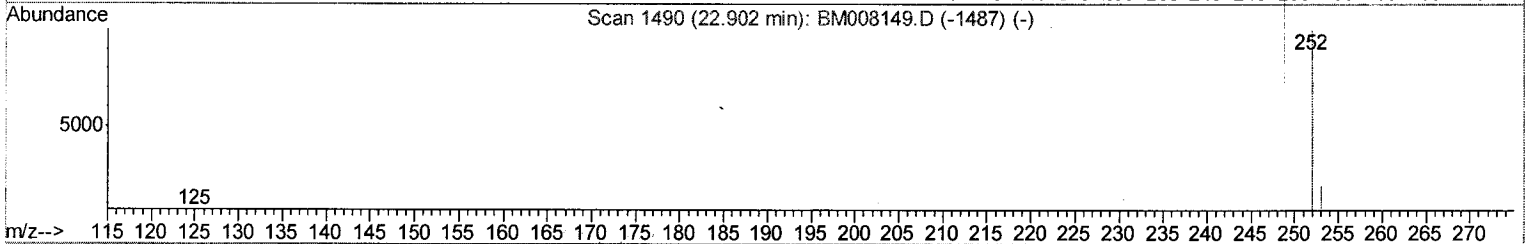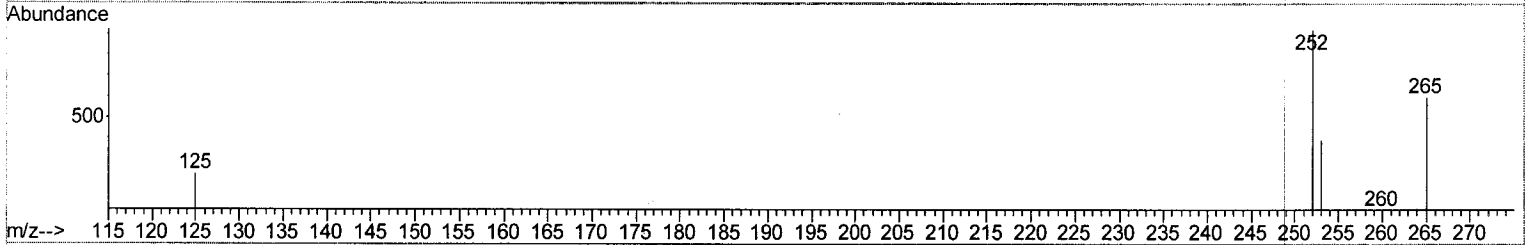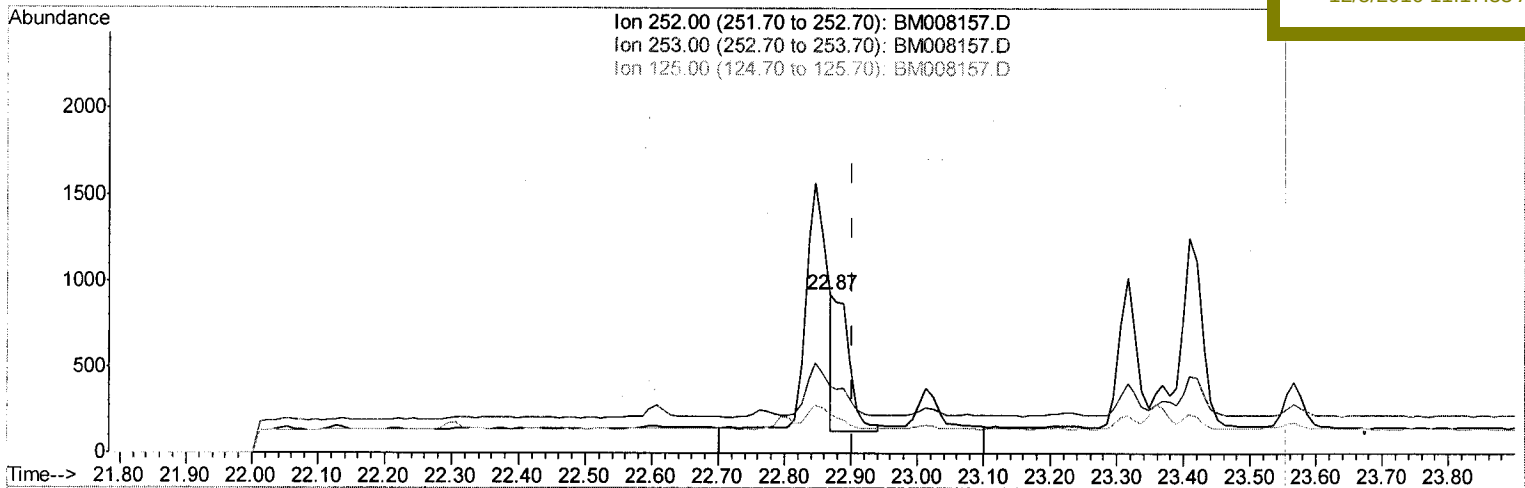

TIC: BM008157.D

(22) Benzo(k)fluoranthene

22.868min (-0.035) 0.18ng/ul m

response 1330

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	42.78#
125.00	17.10	24.54#
0.00	0.00	0.00

5.9
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

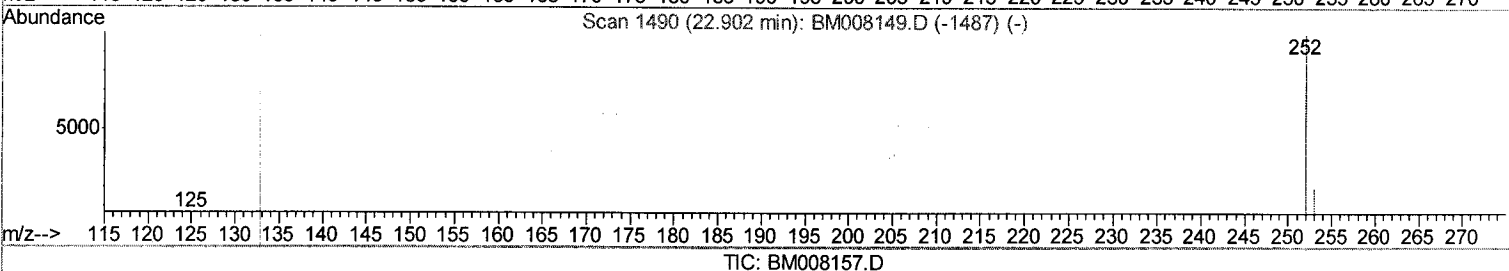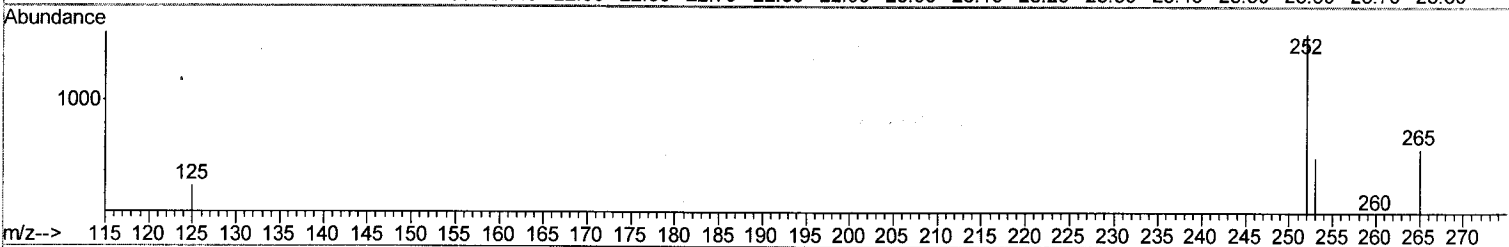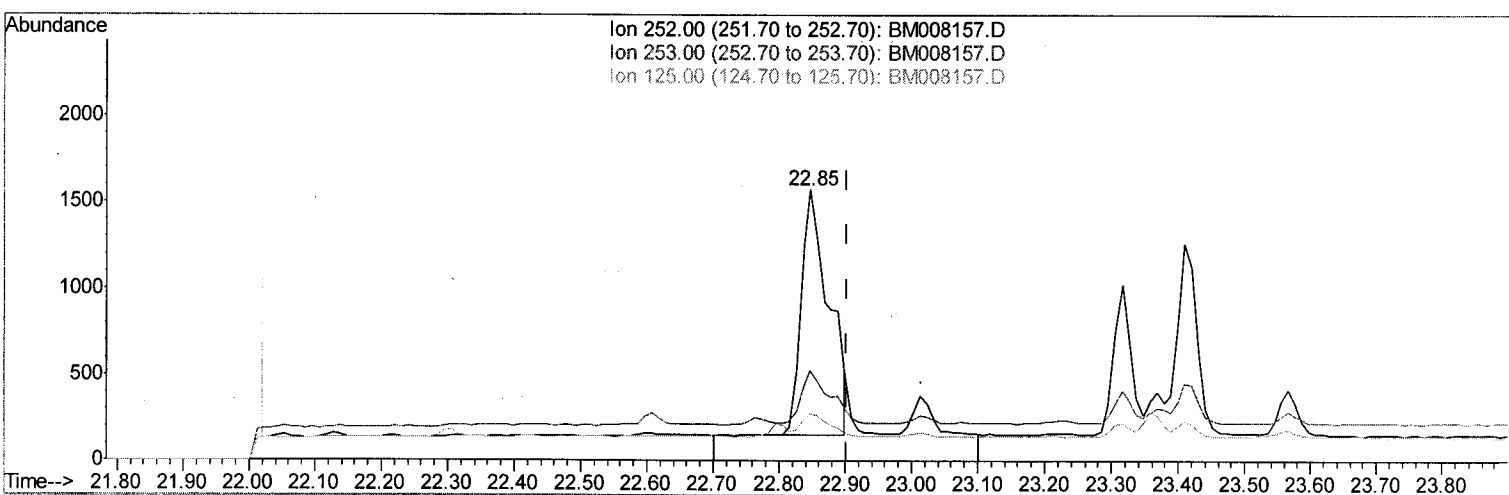

TIC: BM008157.D

(22) Benzo(k)fluoranthene

22.847min (-0.056) 0.56ng/ul

response 4170

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	33.50
125.00	17.10	17.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Quant Time: Dec 02 17:54:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

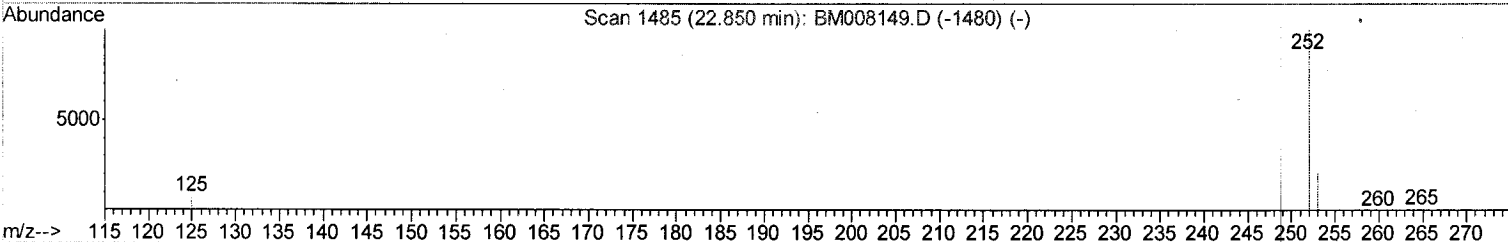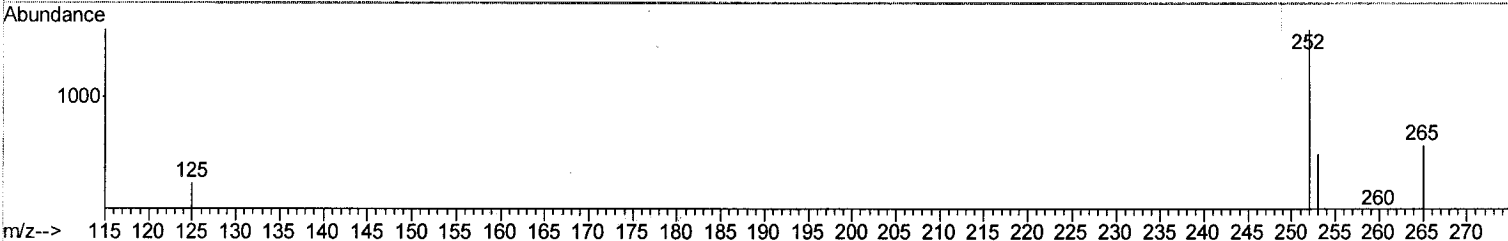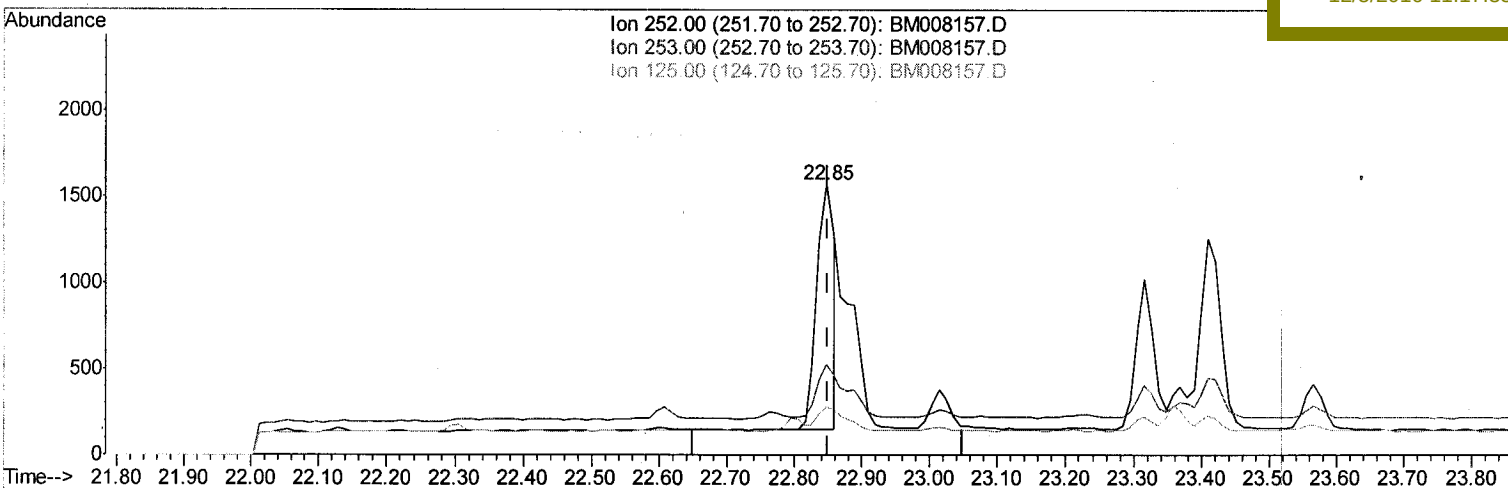

TIC: BM008157.D

(21) Benzo(b)fluoranthene

22.847min (-0.003) 0.35ng/ul

response 2542

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	33.50
125.00	17.50	17.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:53:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

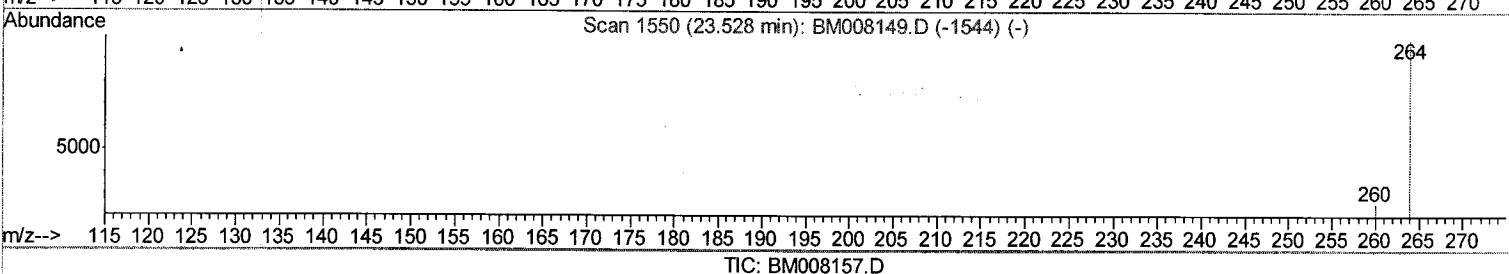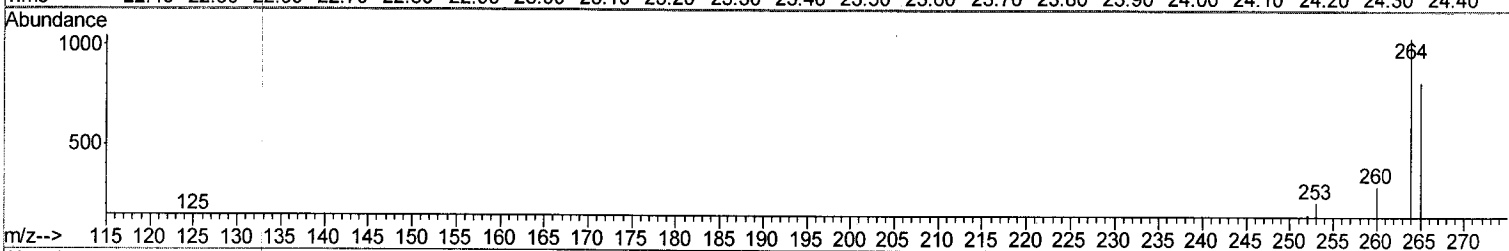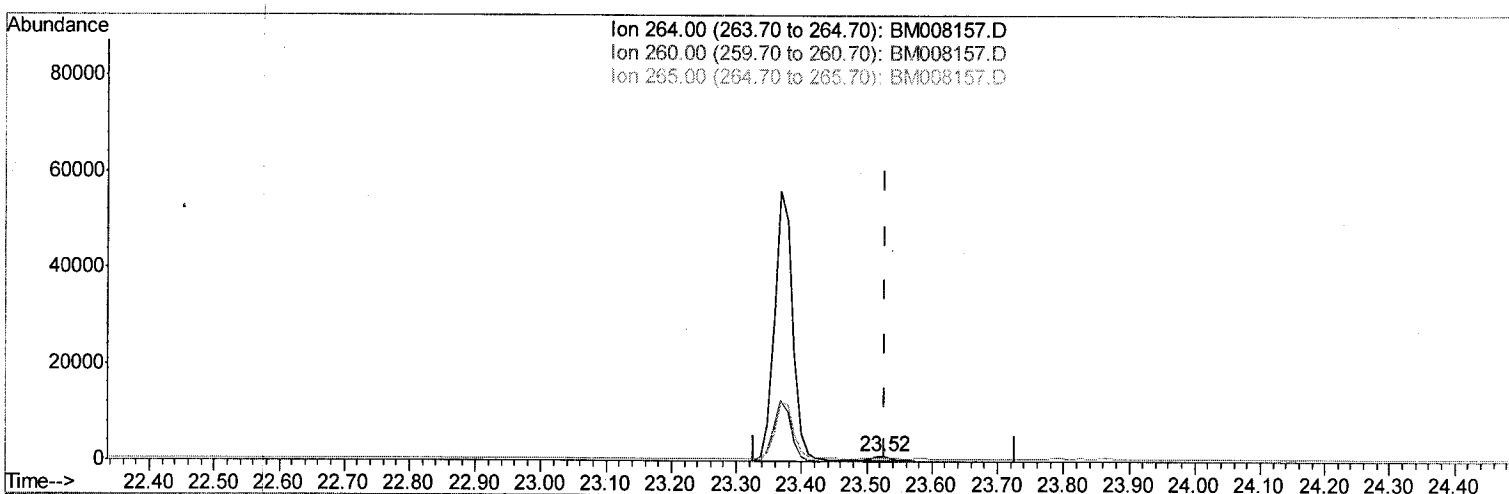

(20) Perylene-d12 (I)

23.524min (-0.003) 0.40ng/ul m

response 1806

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	28.80
265.00	103.50	79.04#
0.00	0.00	0.00

> 5.9
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Quant Time: Dec 02 17:53:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

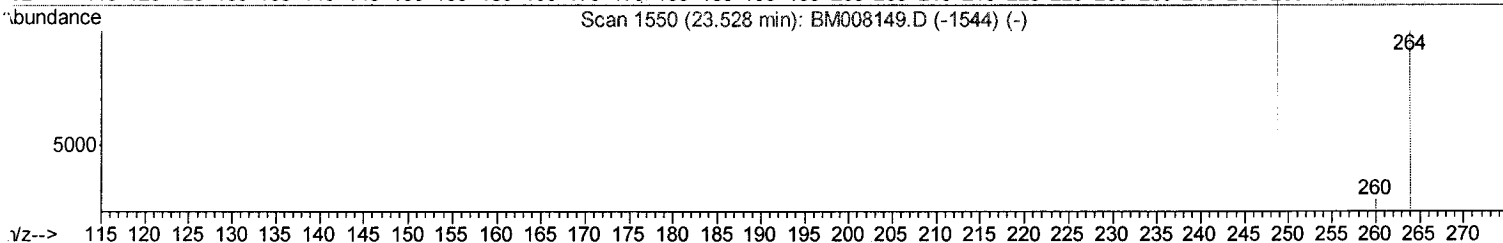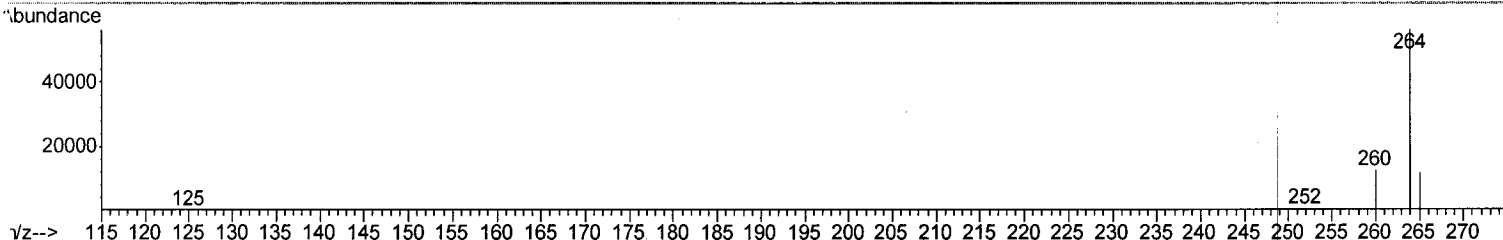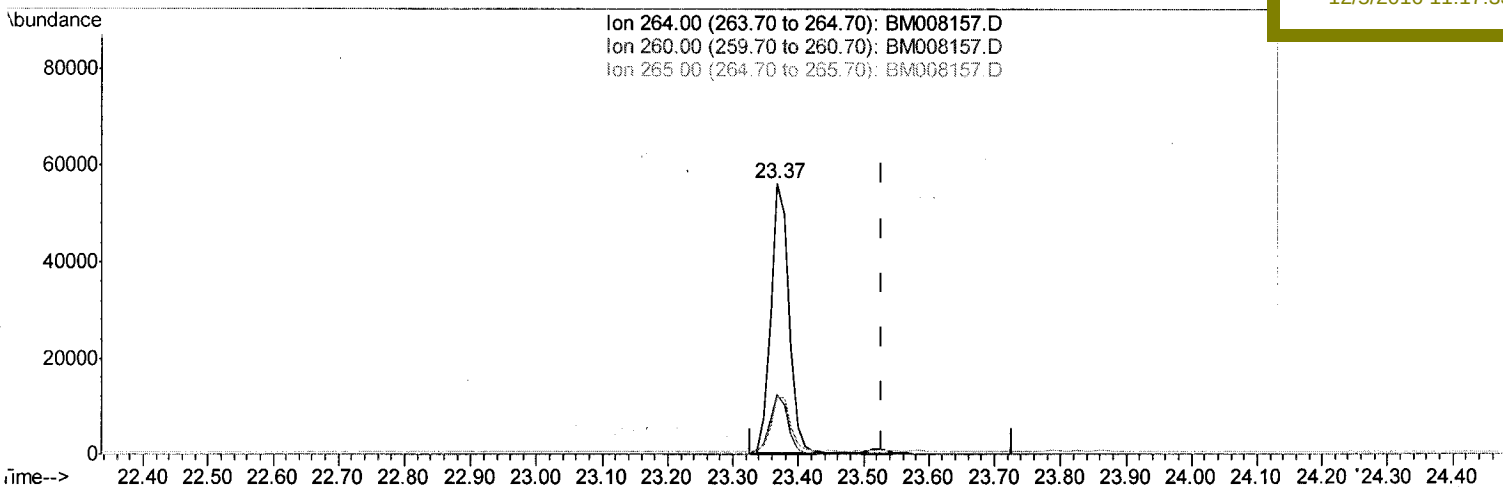

TIC: BM008157.D

(20) Perylene-d12 (I)

23.368min (-0.160) 0.40ng/ul

response 108093

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.27#
265.00	103.50	21.21#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:53:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

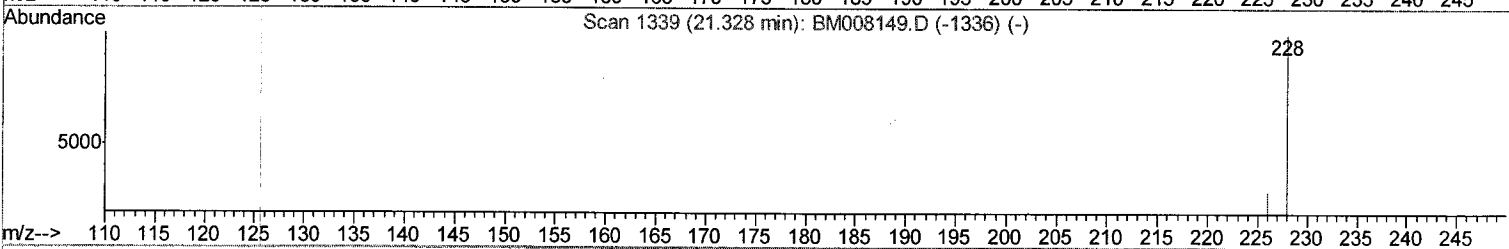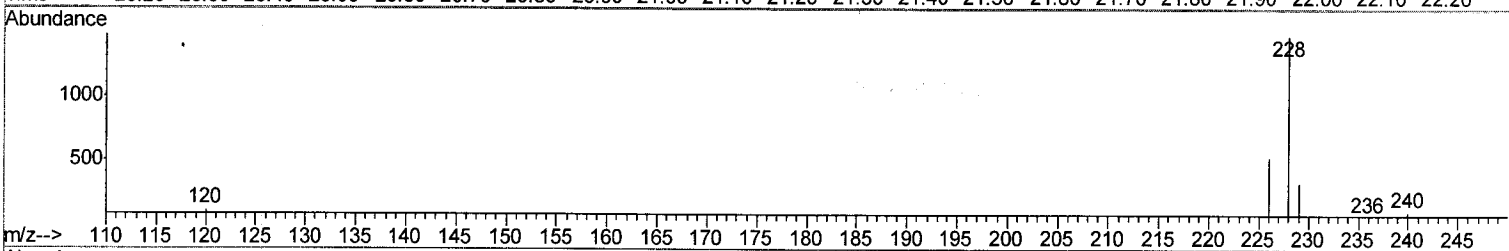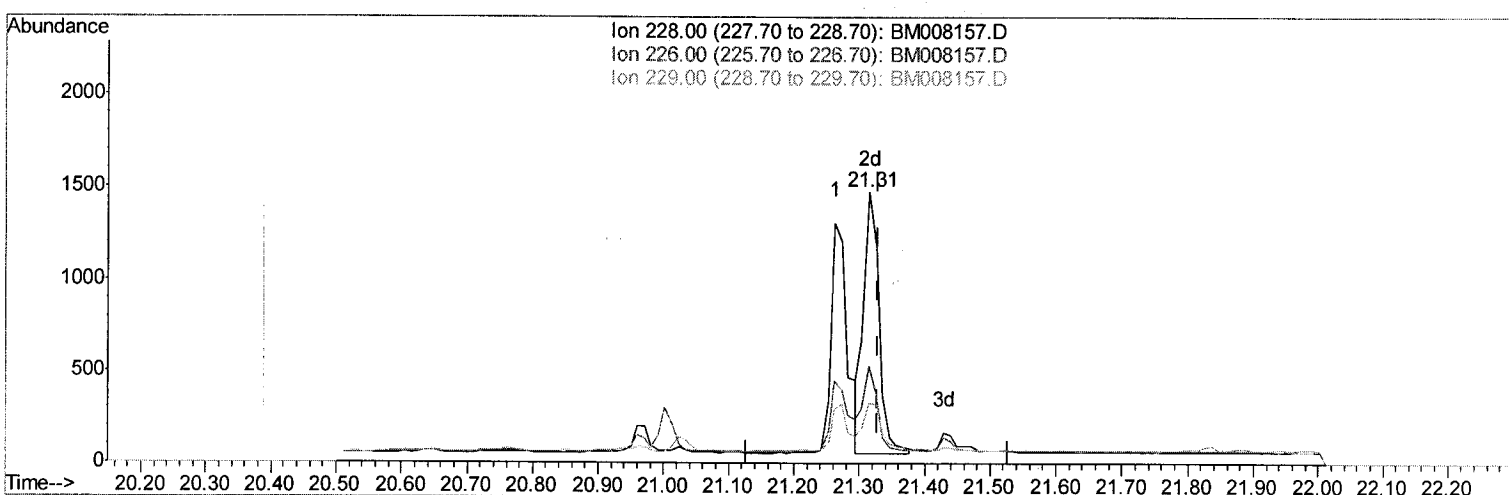

(19) Chrysene

21.315min (-0.014) 0.29ng/ul m

response 2294

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	35.78#
229.00	22.10	22.06
0.00	0.00	0.00

> 5.9
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Quant Time: Dec 02 17:53:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

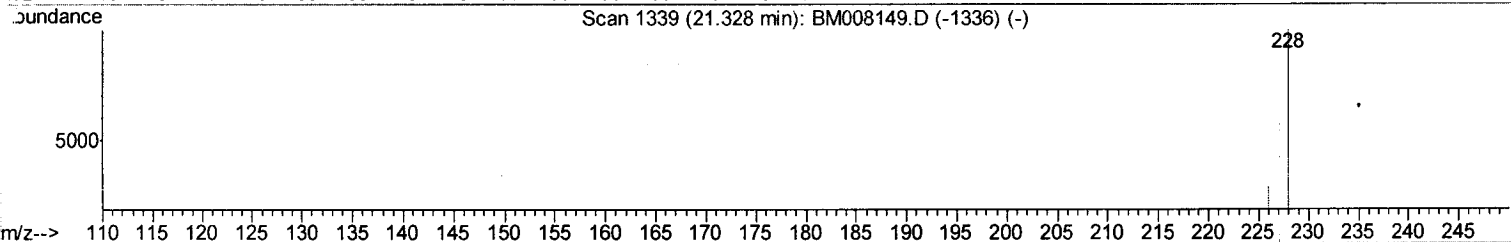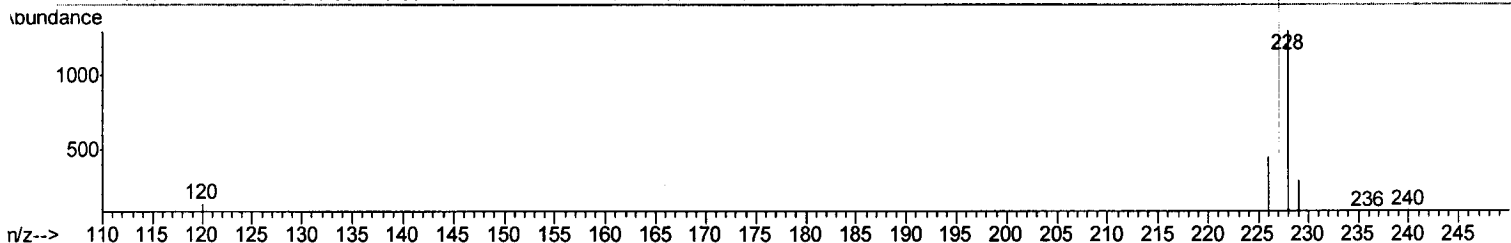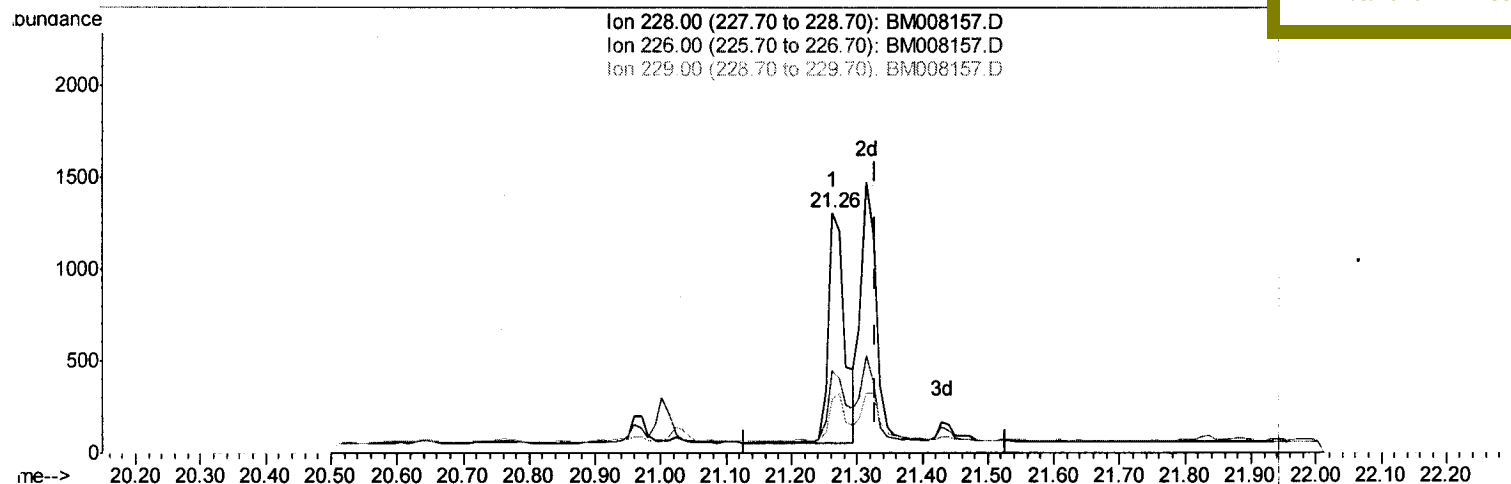

TIC: BM008157.D

(19) Chrysene

21.262min (-0.066) 0.29ng/ul

response 2217

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	34.15
229.00	22.10	22.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:50:29 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

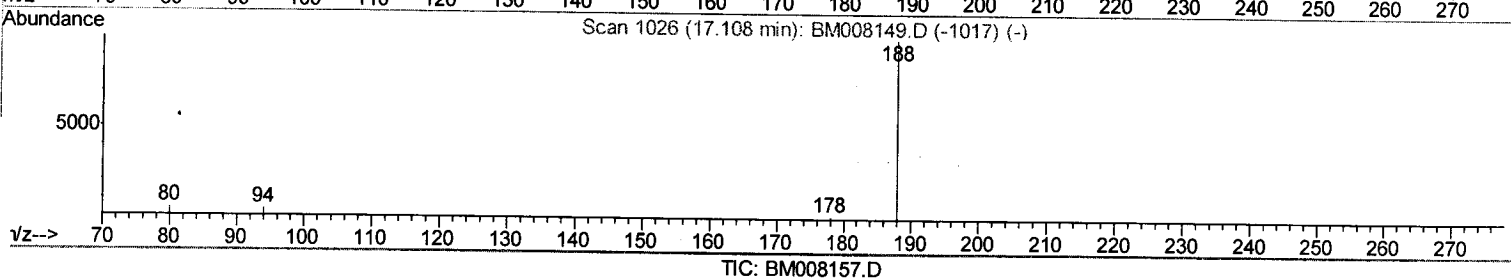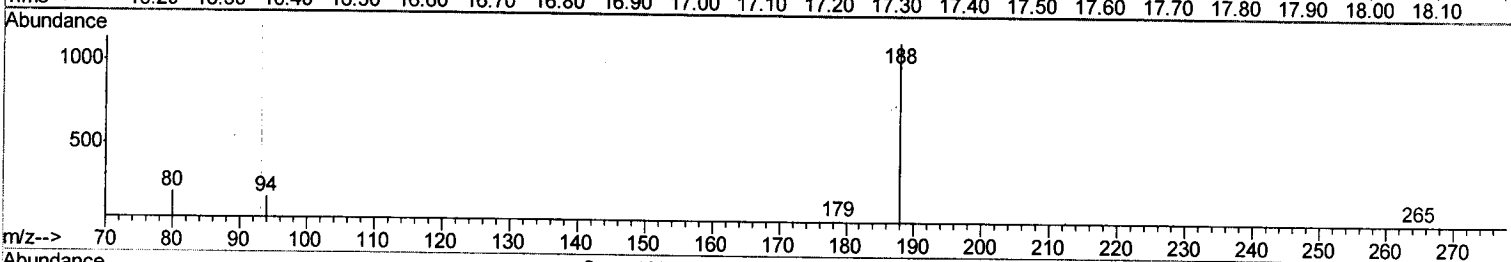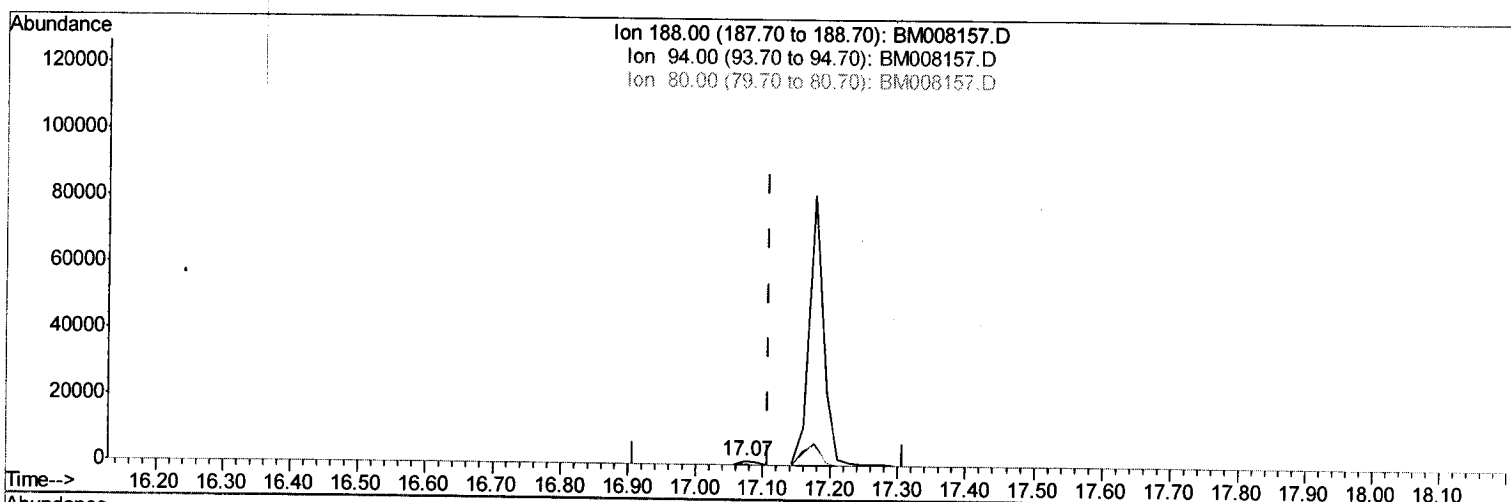

TIC: BM008157.D

(10) Phenanthrene-d10 (I)

17.073min (-0.034) 0.40ng/ul m

response 2266

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	15.28#
80.00	11.80	17.84#
0.00	0.00	0.00

5.7
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Quant Time: Dec 02 17:50:29 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

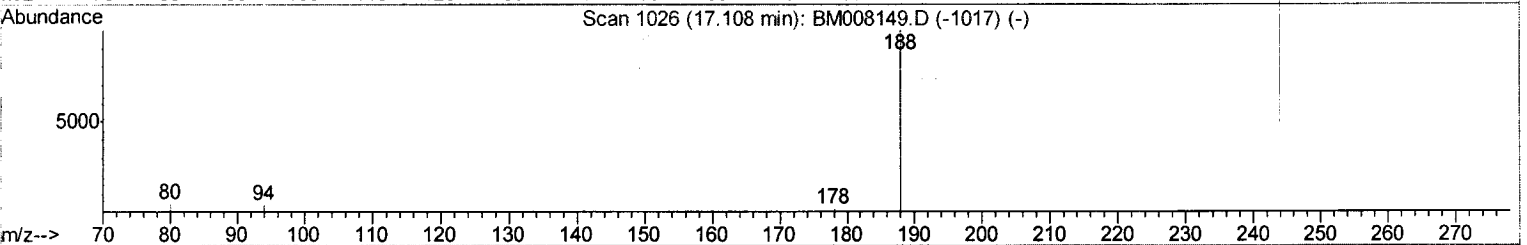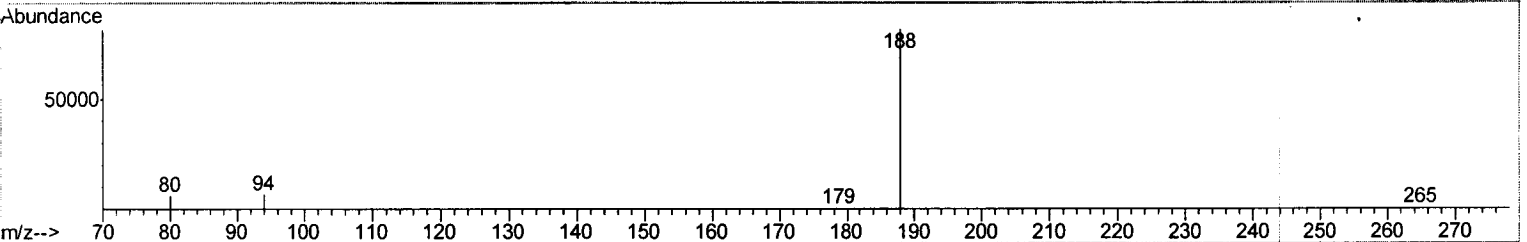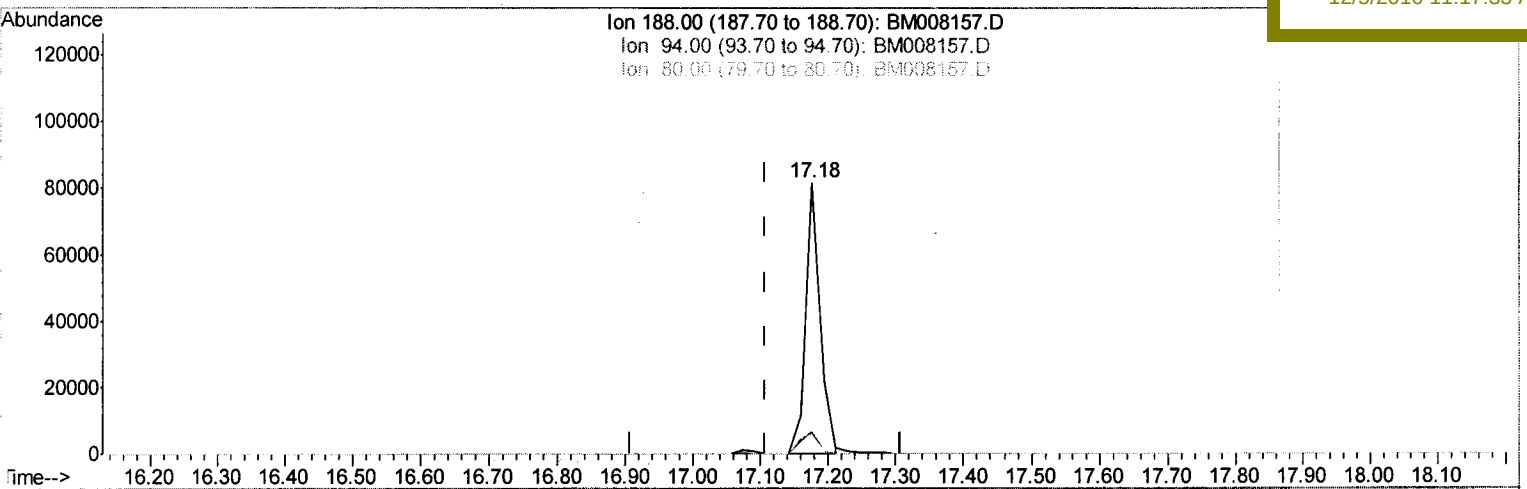

TIC: BM008157.D

(10) Phenanthrene-d10 (I)

17.176min (+0.069) 0.40ng/ul

response 120156

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.18#
80.00	11.80	7.54#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:57:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	632	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.48	136	2129	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.33	164	1258	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.07	188	2266m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.28	240	2037	0.40	ng/ul	-0.01
20) Perylene-d12	23.52	264	1806m	0.40	ng/ul	0.00

2 5.9
 12/06/16

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.09	152	784	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	1484	0.23	ng/ul	-0.02

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	14.04	152	430	0.08	ng/ul#	71
8) Acenaphthene	14.38	153	1096	0.25	ng/ul	92
11) Pentachlorophenol	16.76	266	166	0.21	ng/ul	97
12) Phenanthrene	17.12	178	2400	0.34	ng/ul	94
13) Anthracene	17.21	178	639	0.10	ng/ul#	80
15) Fluoranthene	19.14	202	4834	0.53	ng/ul	97
17) Pyrene	19.51	202	6809	0.96	ng/ul	99
18) Benzo(a)anthracene	21.26	228	2217	0.35	ng/ul	93
19) Chrysene	21.31	228	2294m	0.29	ng/ul	
21) Benzo(b)fluoranthene	22.85	252	3184m	0.44	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	1330m	0.18	ng/ul	
23) Benzo(a)pyrene	23.41	252	2318m	0.34	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.77	276	1669m	0.20	ng/ul	
25) Dibenzo(a,h)anthracene	25.78	278	508m	0.08	ng/ul	
26) Benzo(g,h,i)perylene	26.46	276	1226m	0.17	ng/ul	

2 5.9
 12/06/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008157.D
 Acq On : 02 Dec 2016 15:39
 Operator : UM/SJ
 Sample : H5730-10MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 A4WH6MS

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:33 AM

Quant Time: Dec 02 17:57:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

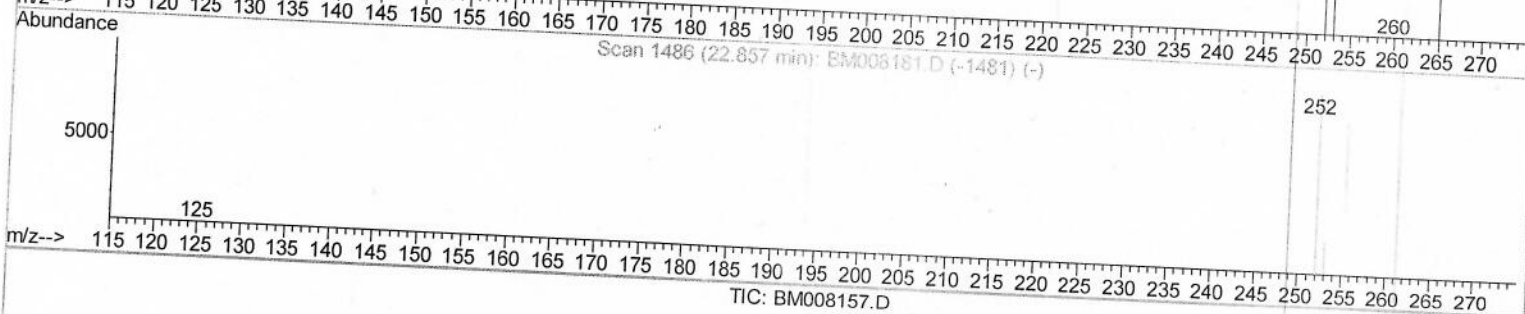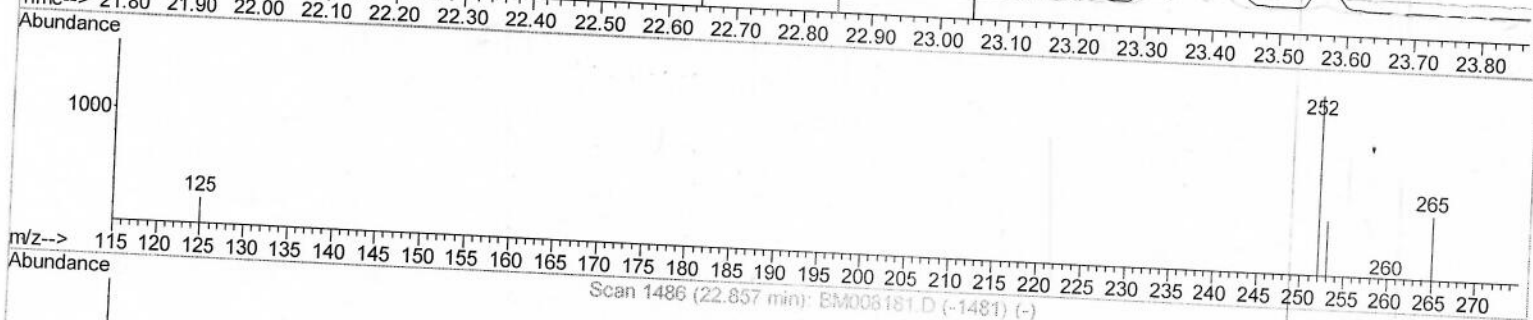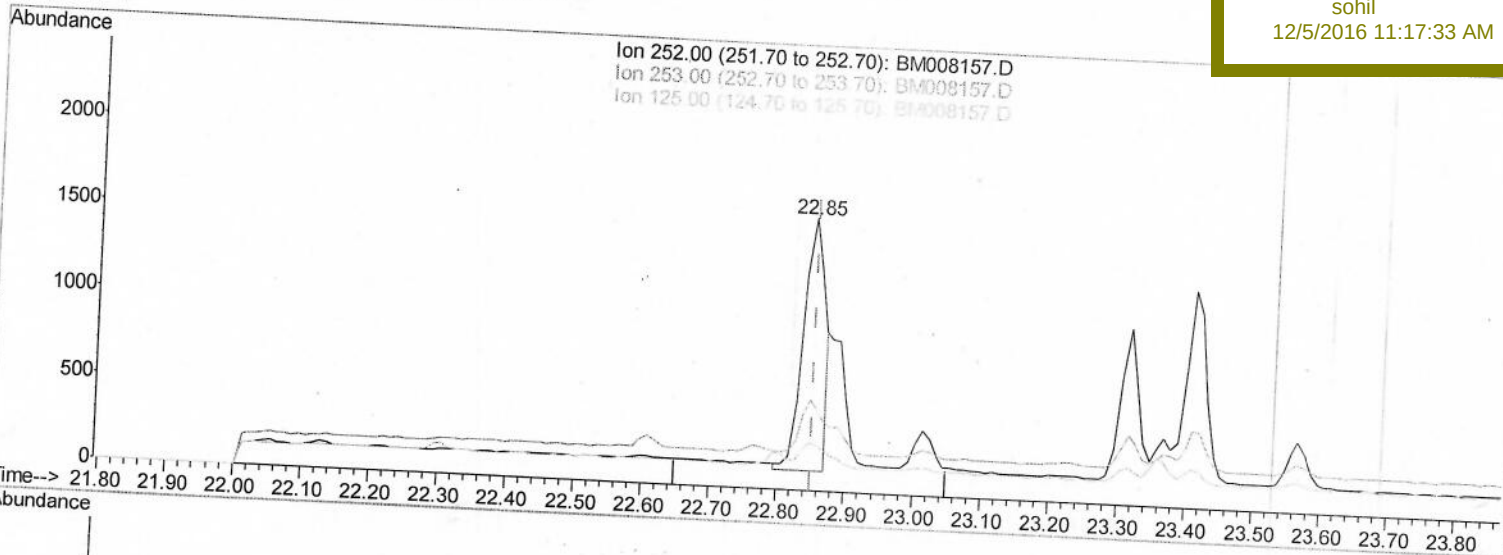

(21) Benzo(b)fluoranthene

22.847min (-0.003) 0.44ng/ul m

response 3184

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	33.50
125.00	17.50	17.58
0.00	0.00	0.00

> 5.7
 12/06/16