

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:02:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

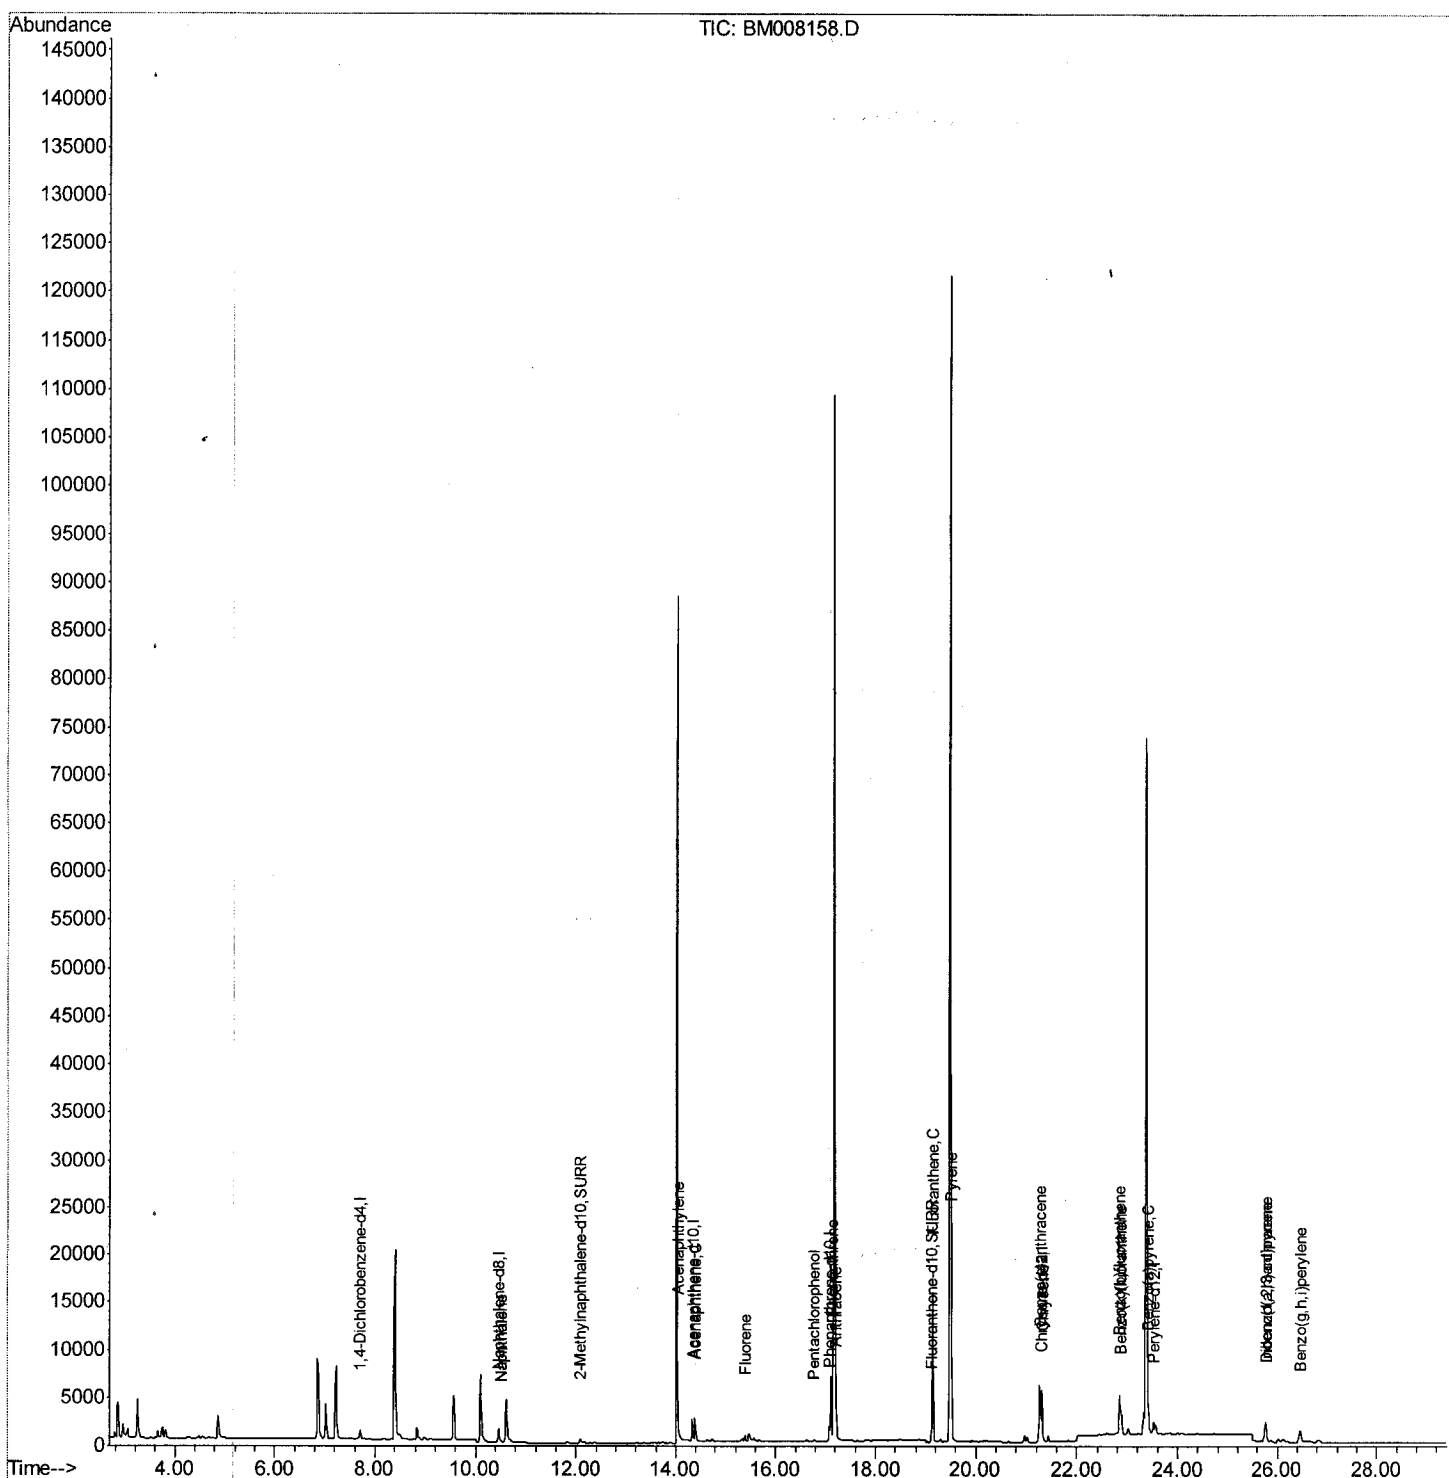

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
Data File : BM008158.D
Acq On : 02 Dec 2016 16:15
Operator : UM/SJ
Sample : H5730-11MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WH6MSD

Manual Integrations
APPROVED

sohil
12/5/2016 11:17:35 AM

Quant Time: Dec 02 17:58:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 15:28:31 2016
Response via : Initial Calibration

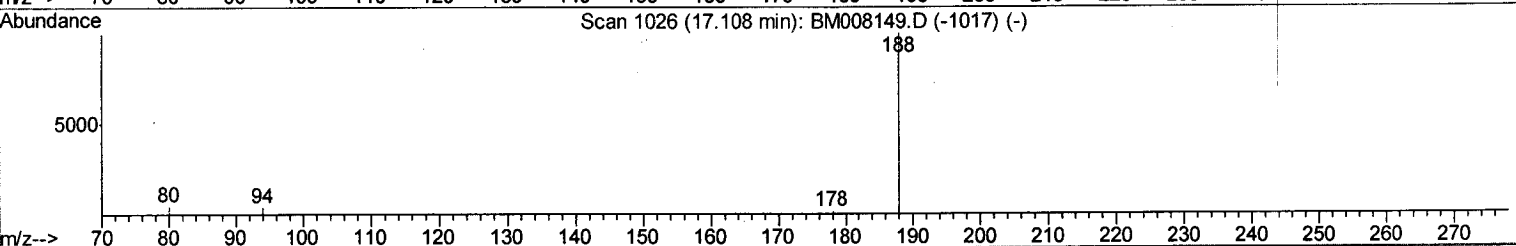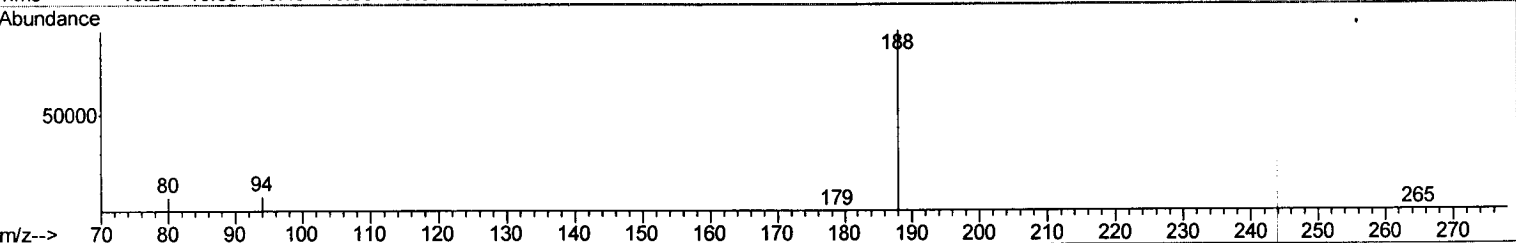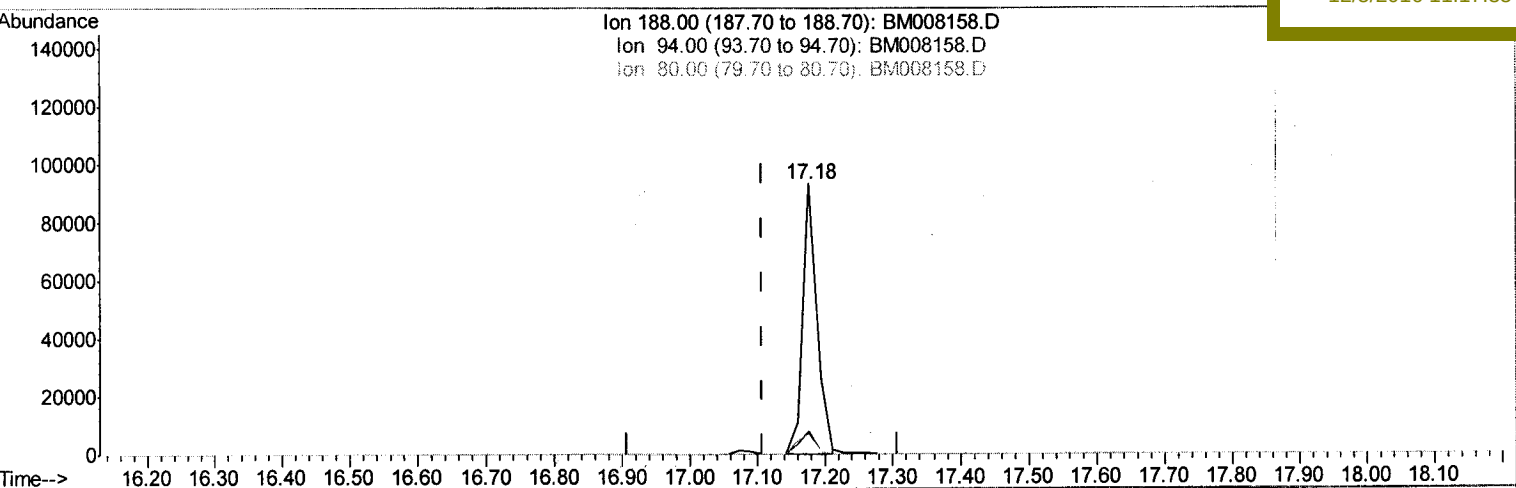

TIC: BM008158.D

(10) Phenanthrene-d10 (I)

17.176min (+0.068) 0.40ng/ui

response 136356

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.44#
80.00	11.80	7.78#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 17:58:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

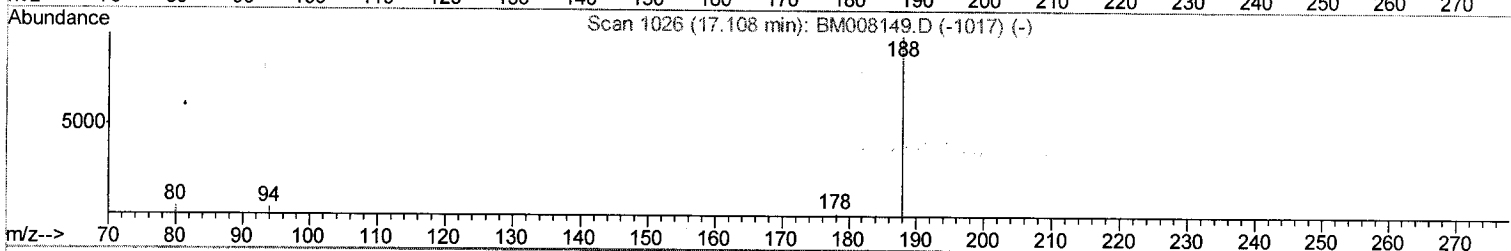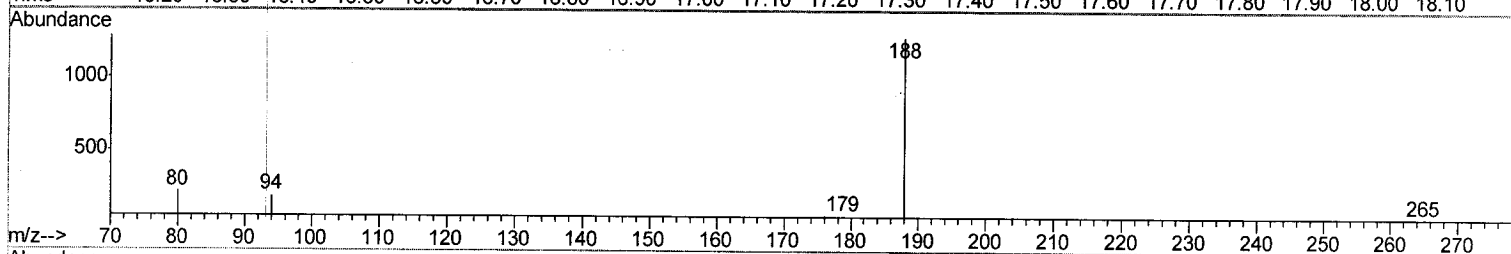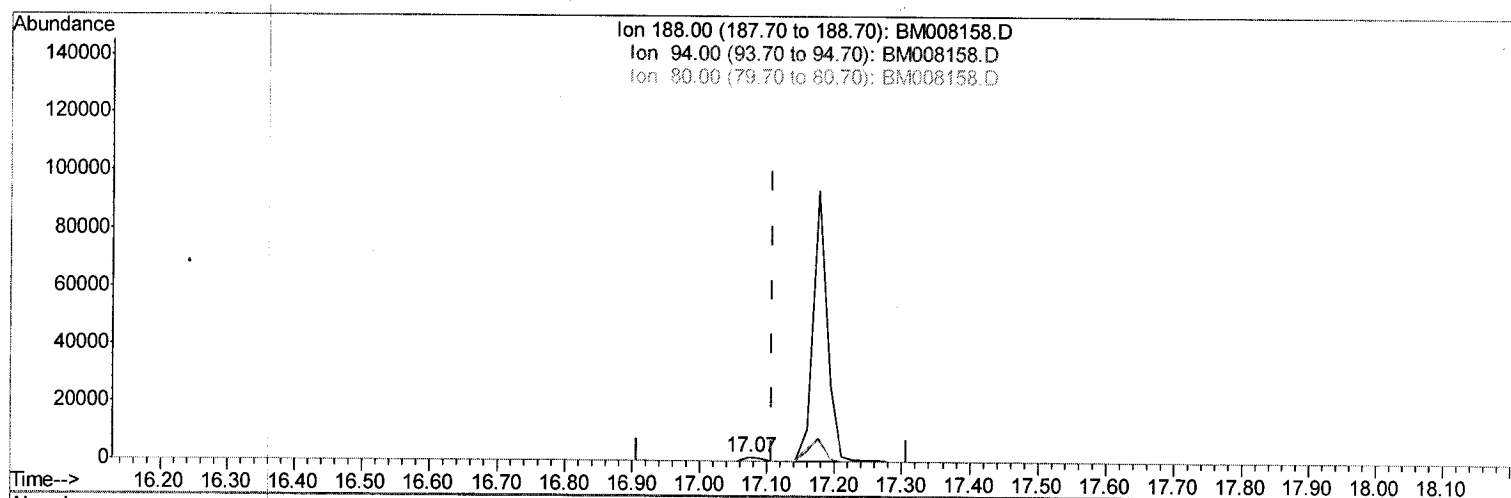

TIC: BM008158.D

(10) Phenanthrene-d10 (I)

17.073min (-0.035) 0.40ng/ul m

response 2474

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	14.52#
80.00	11.80	16.78#
0.00	0.00	0.00

75.3
 12106116




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
Data File : BM008158.D
Acq On : 02 Dec 2016 16:15
Operator : UM/SJ
Sample : H5730-11MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WH6MSD

Manual Integrations
APPROVED

sohil
12/5/2016 11:17:35 AM

Quant Time: Dec 02 17:59:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 15:28:31 2016
Response via : Initial Calibration

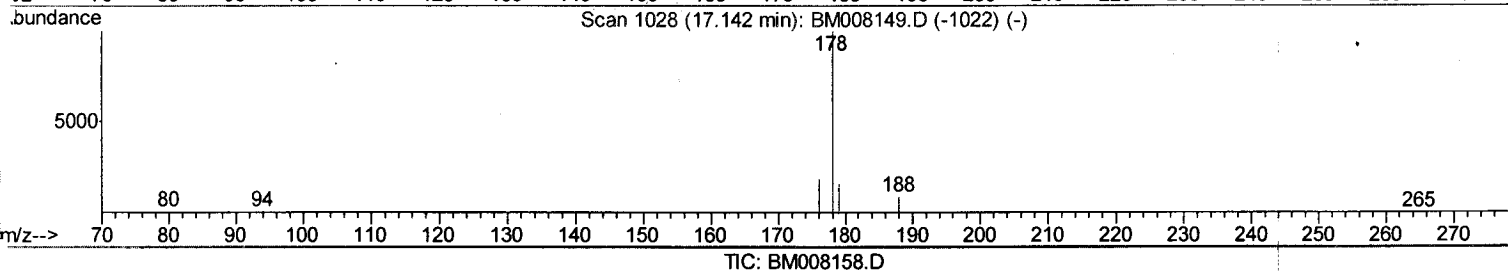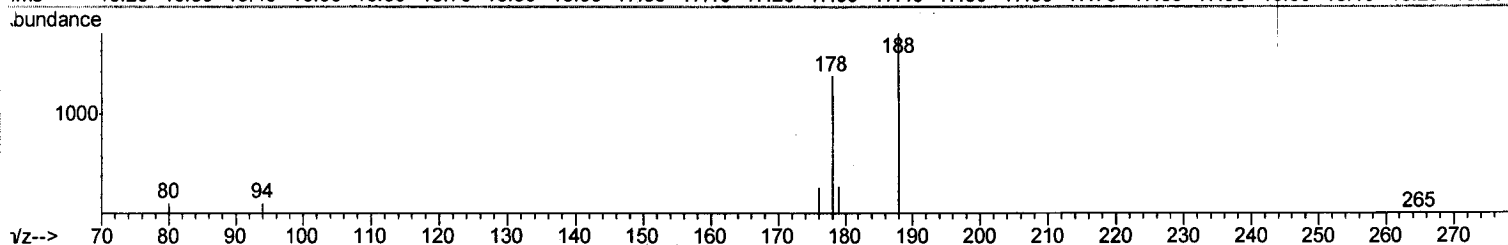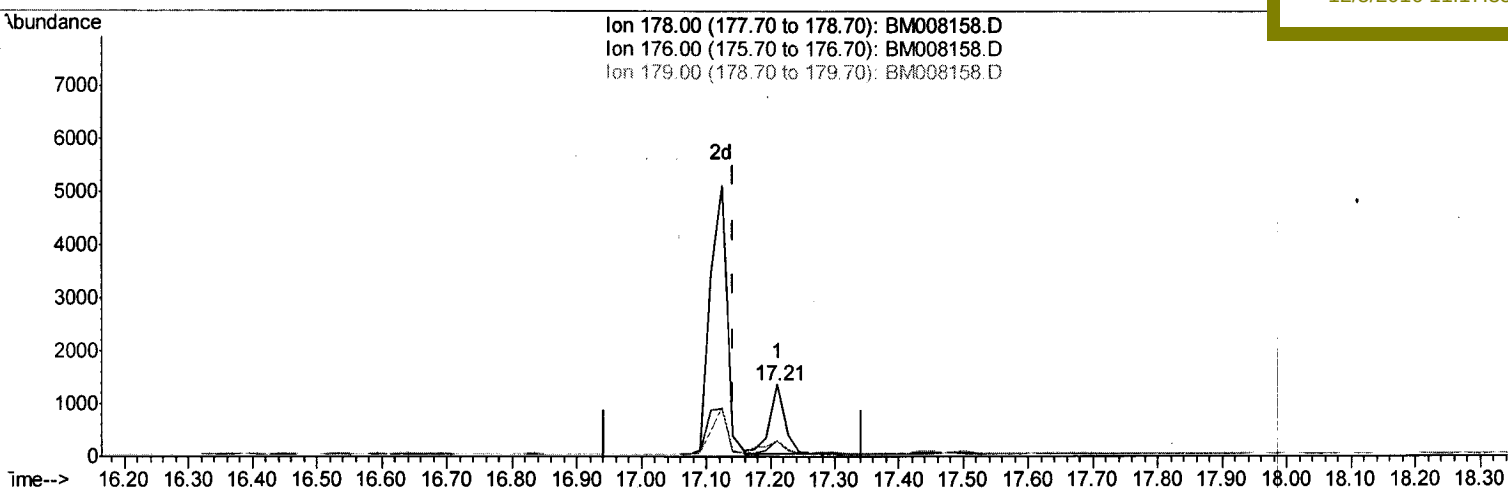

(12) Phenanthrene

17.210min (+0.068) 0.29ng/ul

response 2215

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	21.74
179.00	17.00	22.25#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 17:59:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

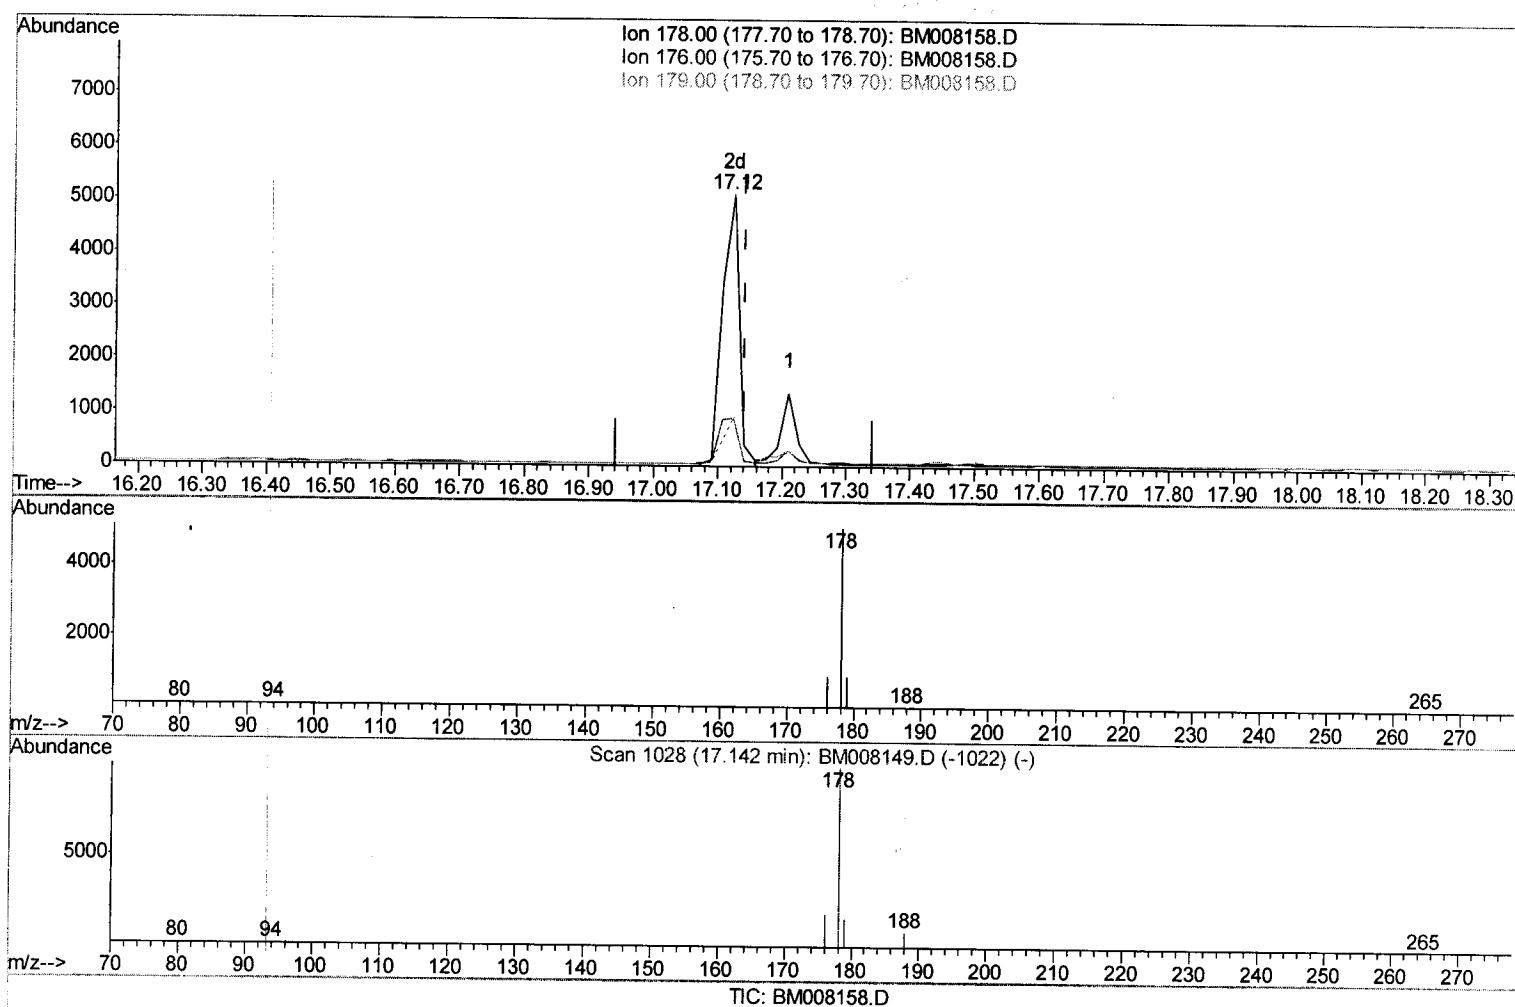

(12) Phenanthrene

17.125min (-0.017) 1.23ng/ul m

response 9465

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	17.84#
179.00	17.00	18.03
0.00	0.00	0.00

9.3
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Quant Time: Dec 02 17:59:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

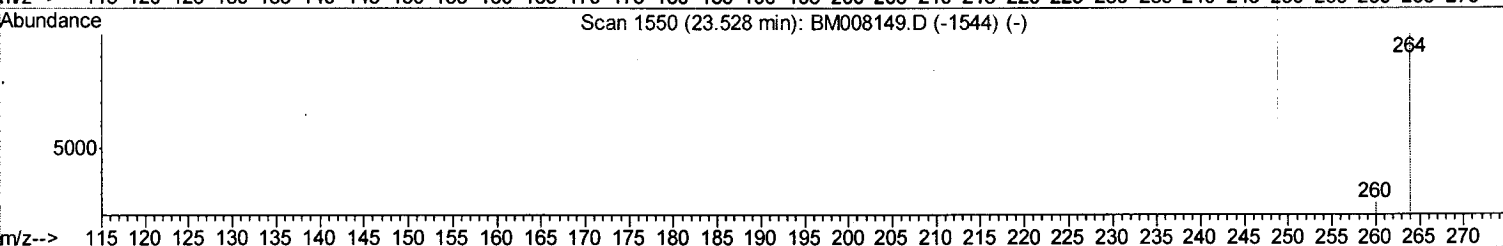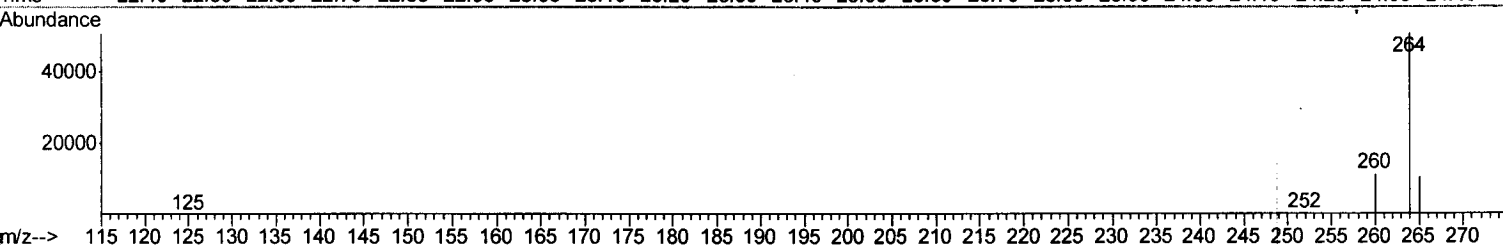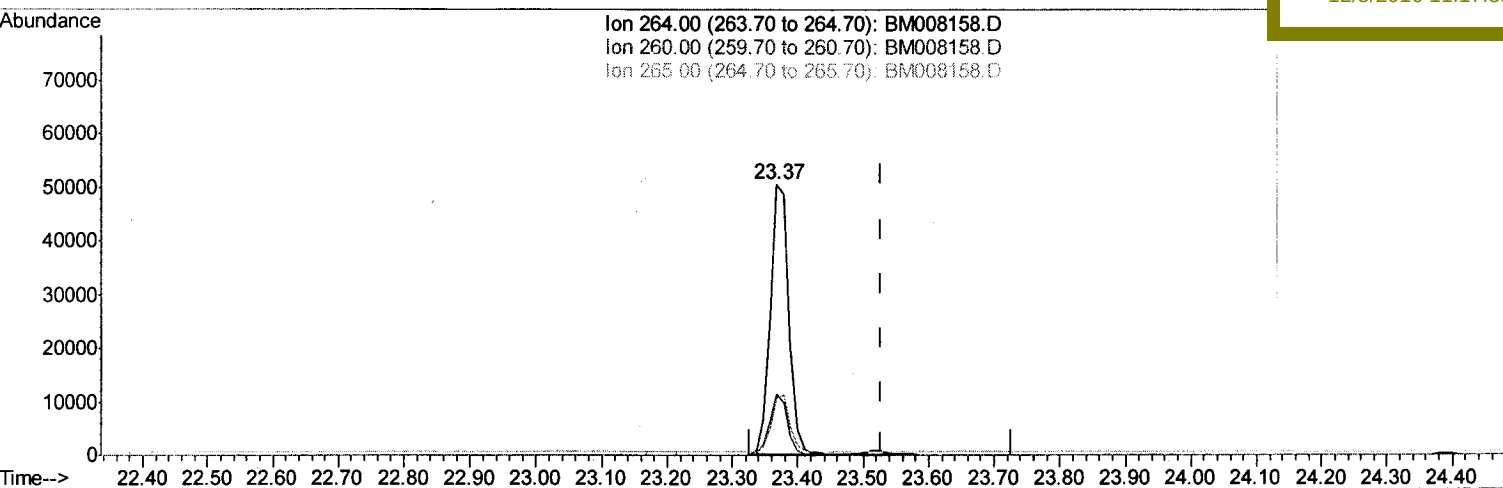

TIC: BM008158.D

(20) Perylene-d12 (I)

23.368min (-0.160) 0.40ng/ul

response 99117

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.63#
265.00	103.50	21.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 17:59:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

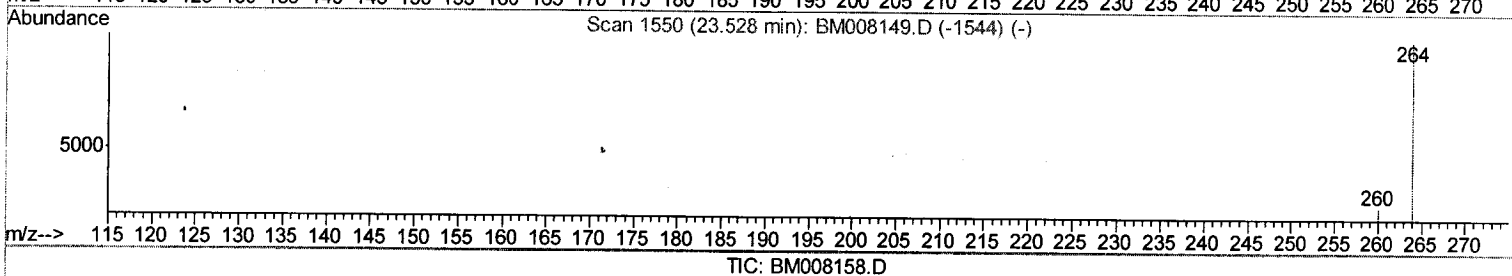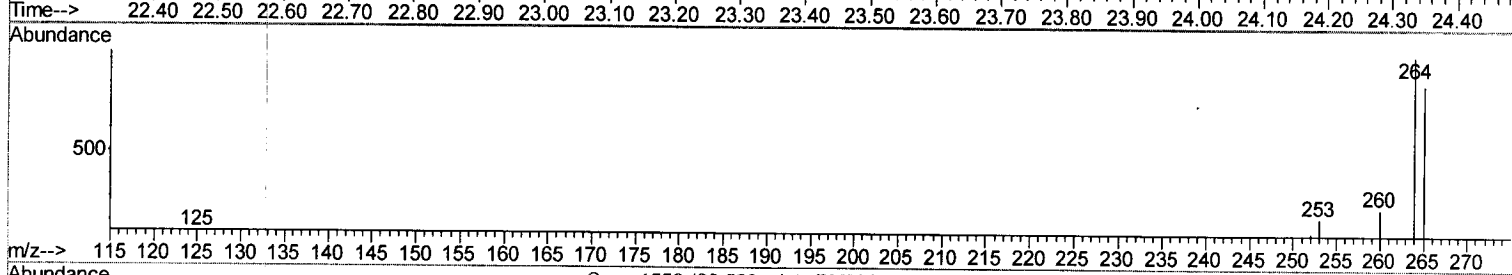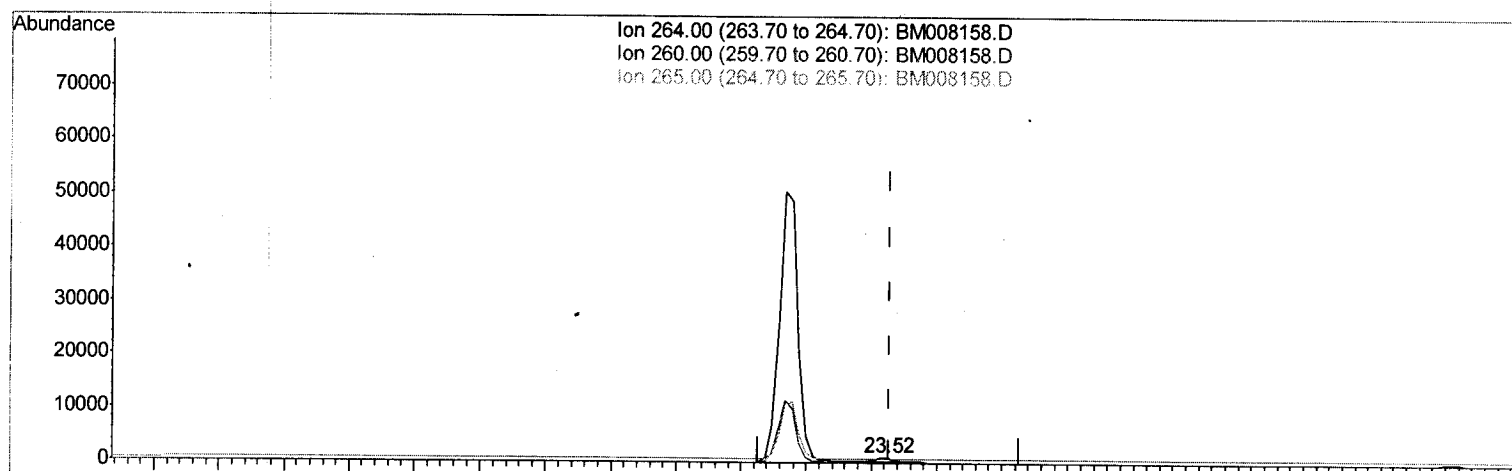

TIC: BM008158.D

(20) Perylene-d12 (I)

23.524min (-0.004) 0.40ng/ul m

response 1557

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	28.89
265.00	103.50	86.68
0.00	0.00	0.00

> S.J
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

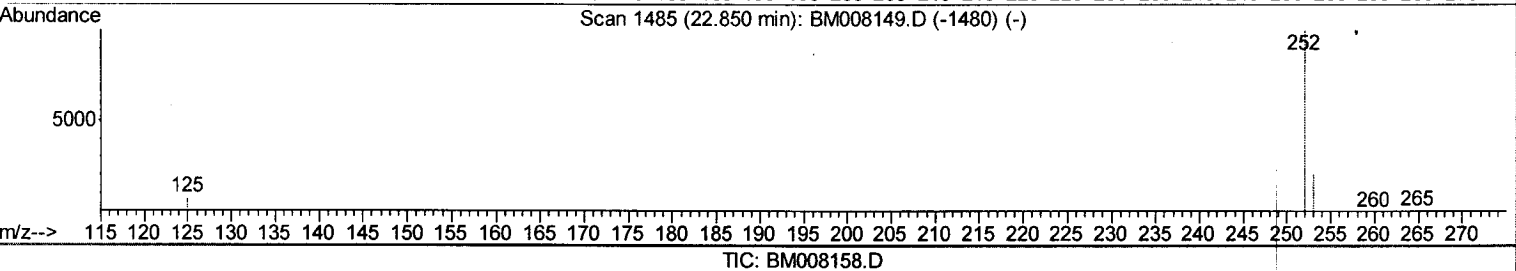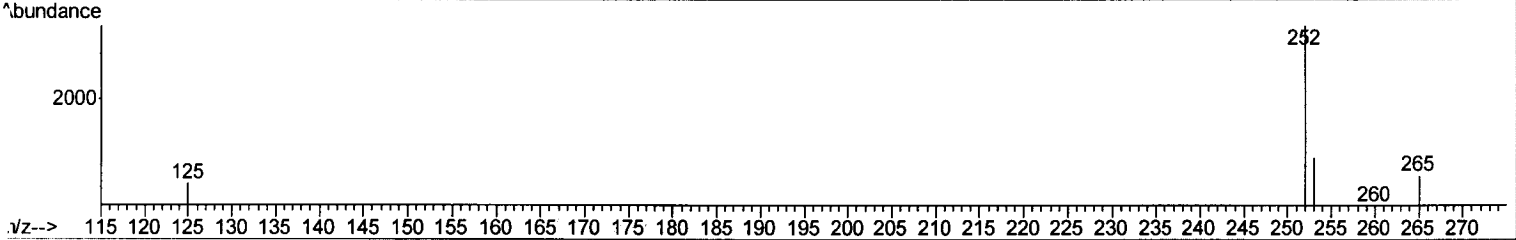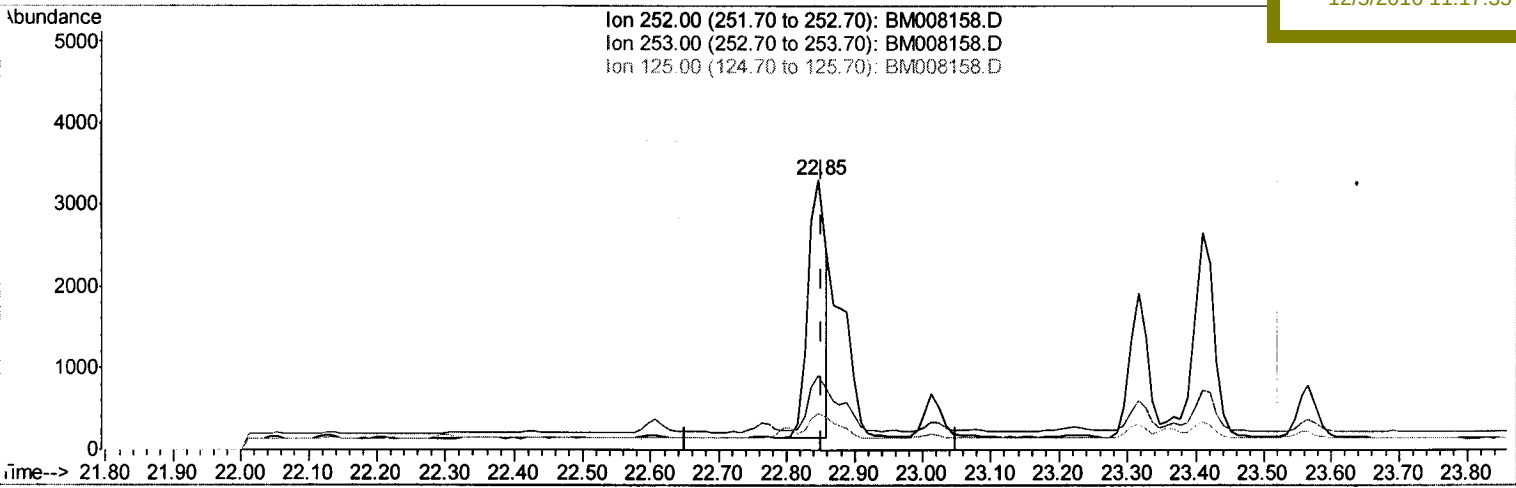

(21) Benzo(b)fluoranthene

22.847min (-0.004) 0.93ng/ul

response 5780

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.81
125.00	17.50	13.56
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

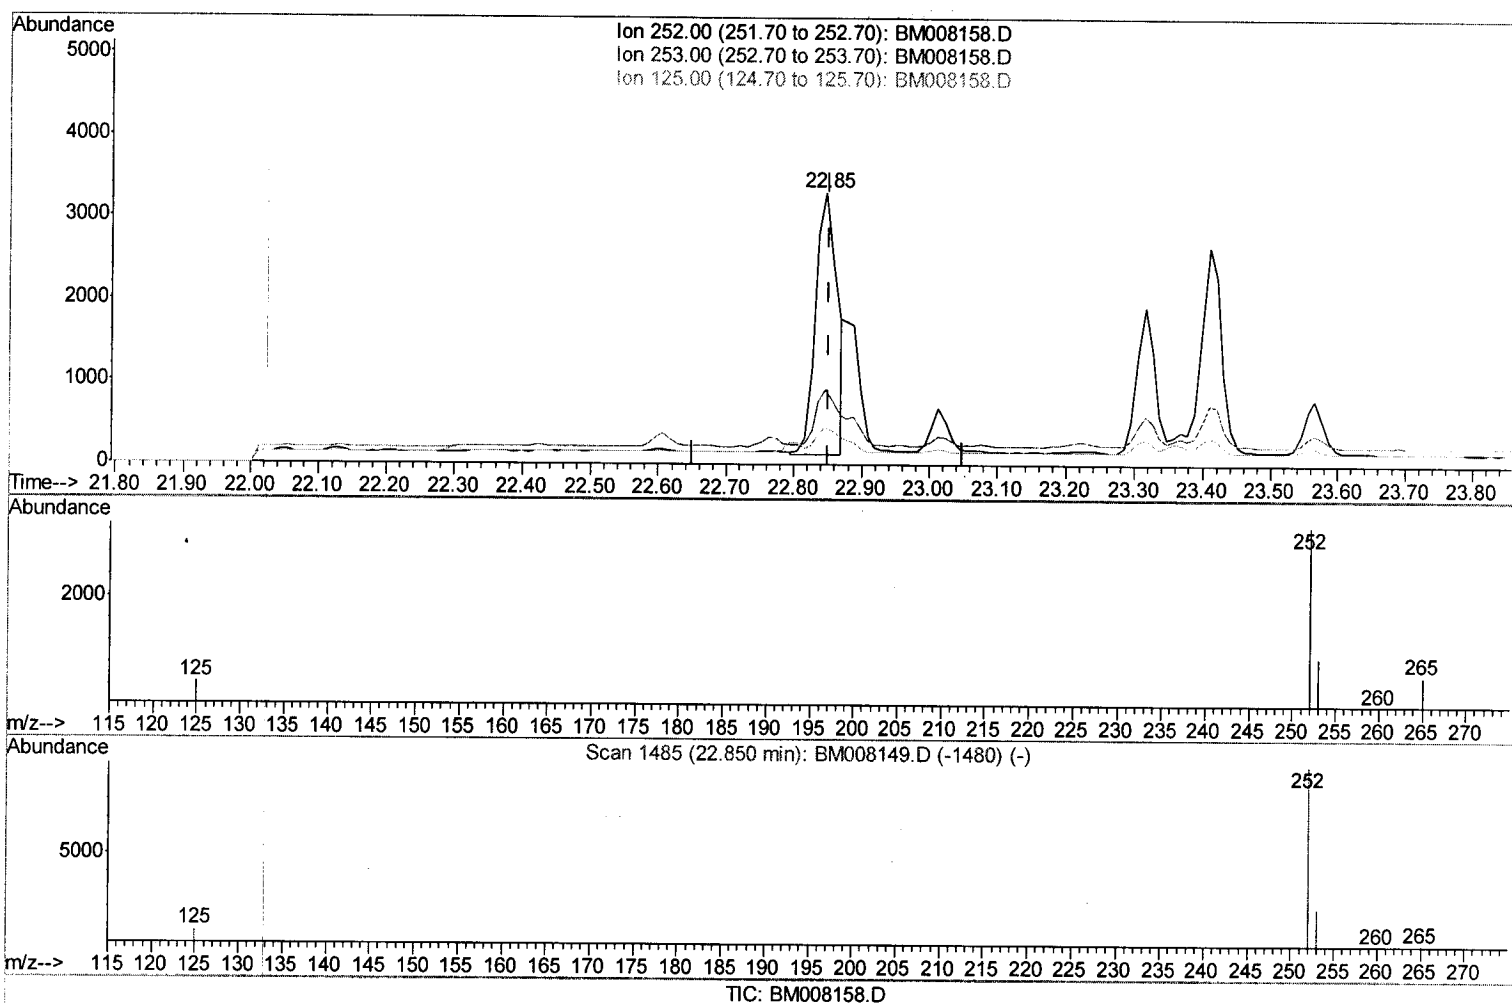

(21) Benzo(b)fluoranthene

22.847min (-0.004) 1.12ng/ul m

response 6952

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.81
125.00	17.50	13.56
0.00	0.00	0.00

5.5
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
Data File : BM008158.D
Acq On : 02 Dec 2016 16:15
Operator : UM/SJ
Sample : H5730-11MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WH6MSD

Manual Integrations
APPROVED

sohil
12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 15:28:31 2016
Response via : Initial Calibration

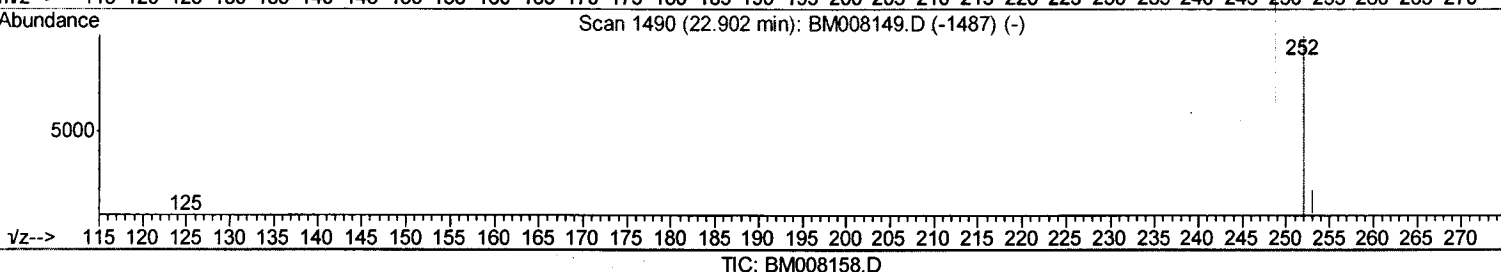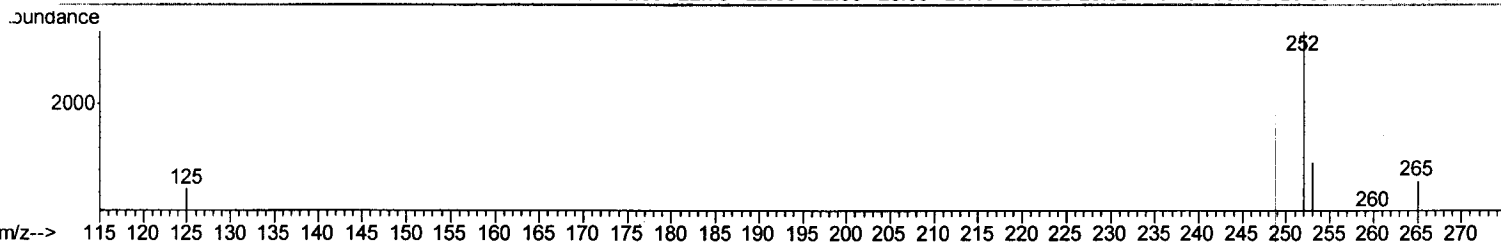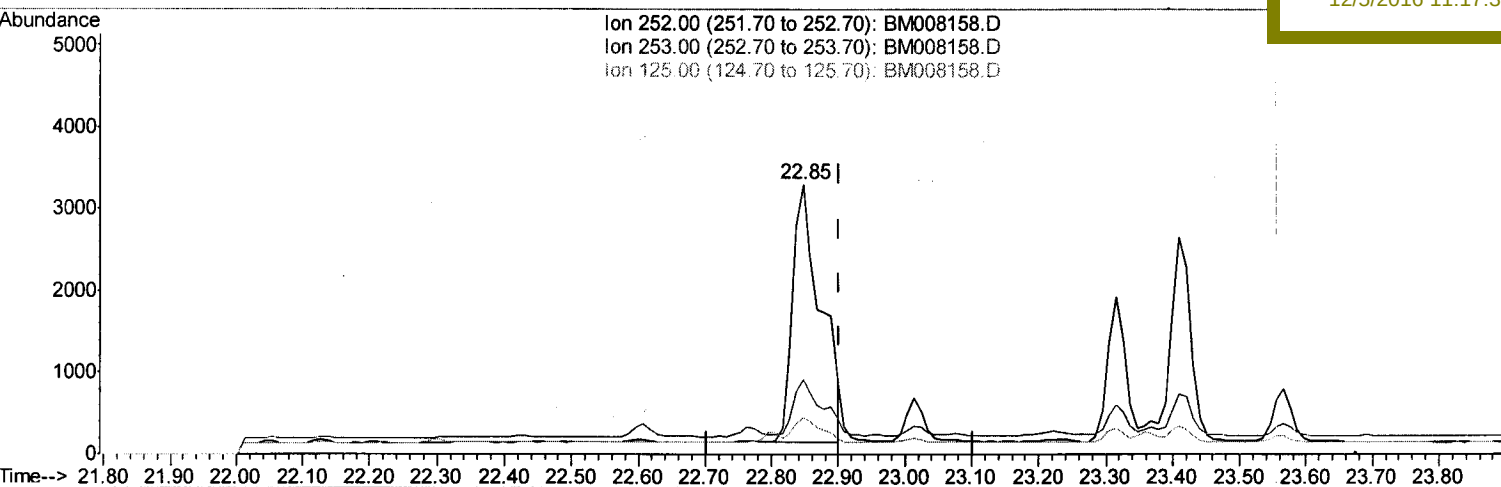

(22) Benzo(k)fluoranthene

22.847min (-0.056) 1.44ng/ul

response 9210

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	27.81
125.00	17.10	13.56#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

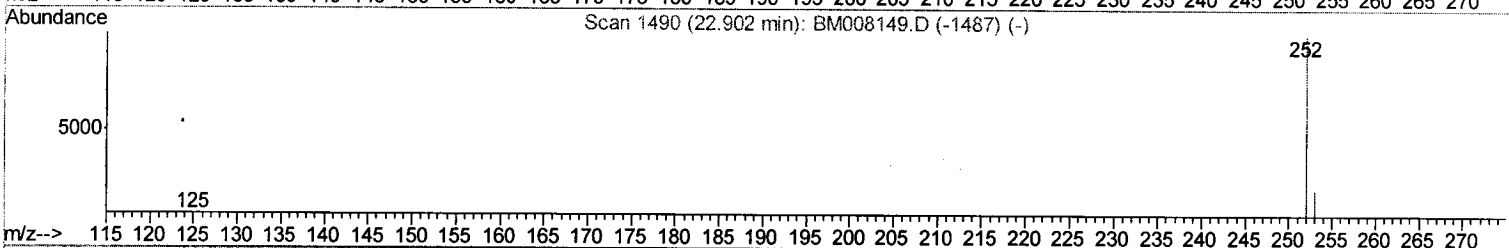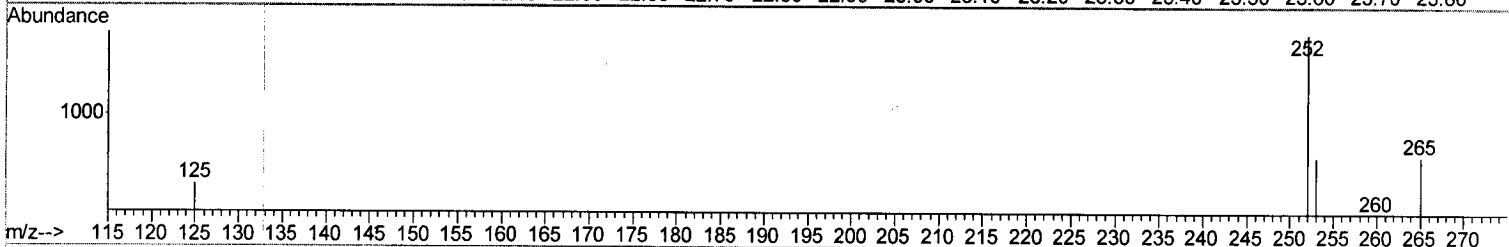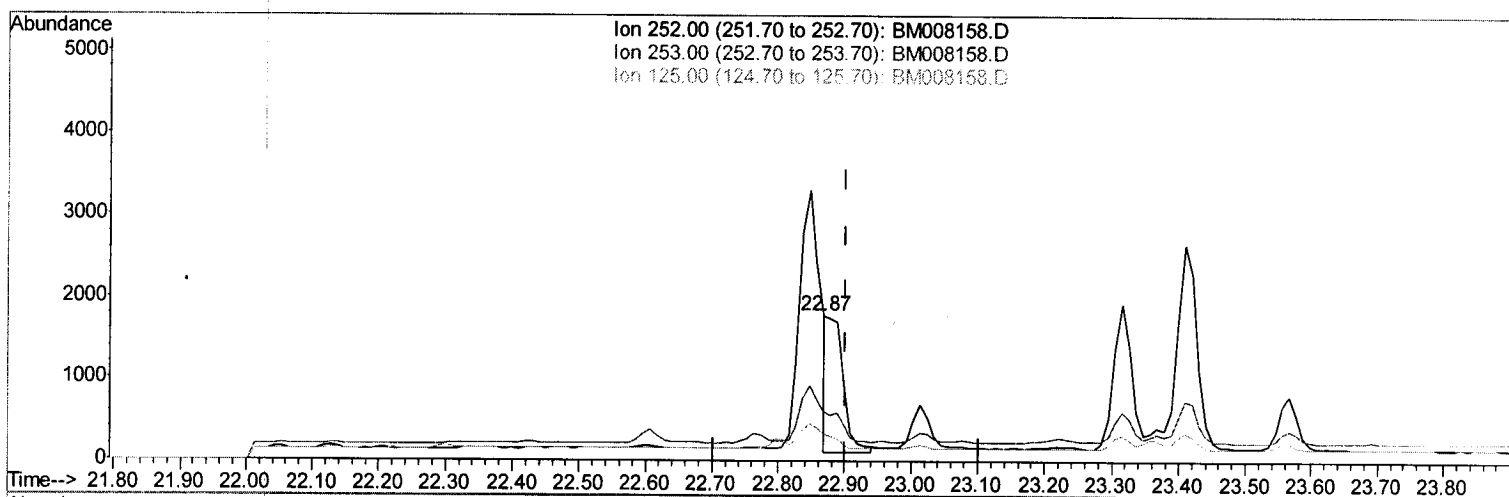

TIC: BM008158.D

(22) Benzo(k)fluoranthene

22.868min (-0.035) 0.44ng/ul m

response 2811

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	33.76
125.00	17.10	18.31
0.00	0.00	0.00

> 9.7
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
Data File : BM008158.D
Acq On : 02 Dec 2016 16:15
Operator : UM/SJ
Sample : H5730-11MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 02 18:00:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 15:28:31 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4WH6MSD

Manual Integrations
APPROVED

sohil
12/5/2016 11:17:35 AM

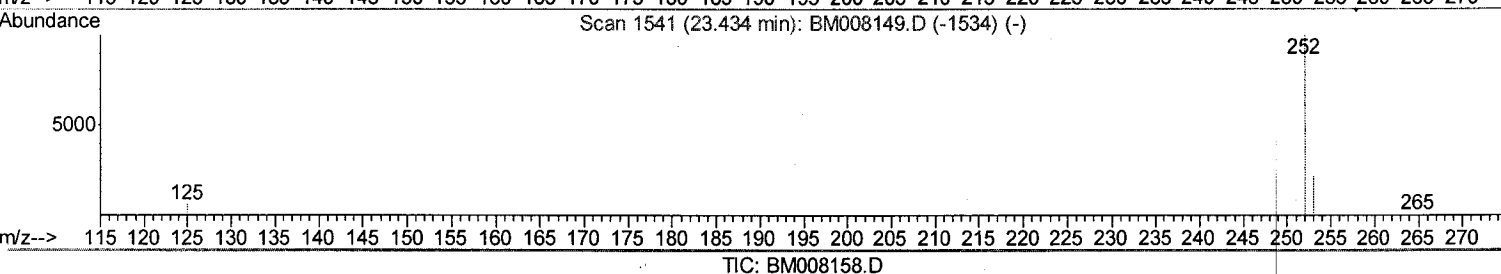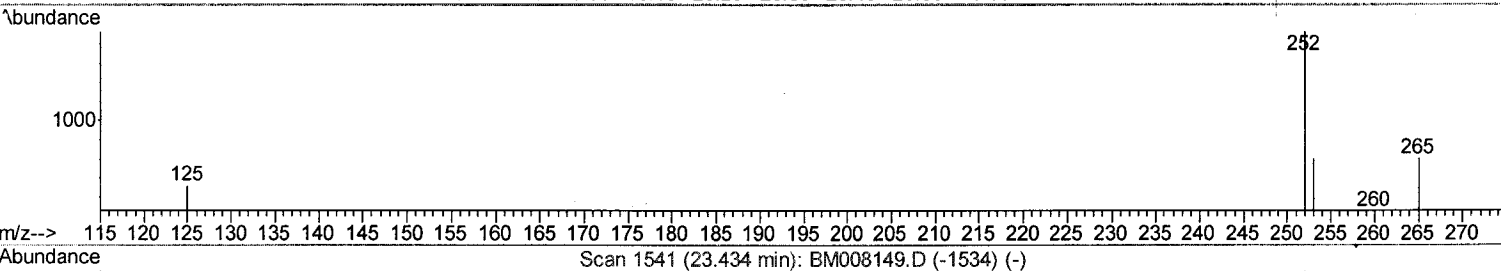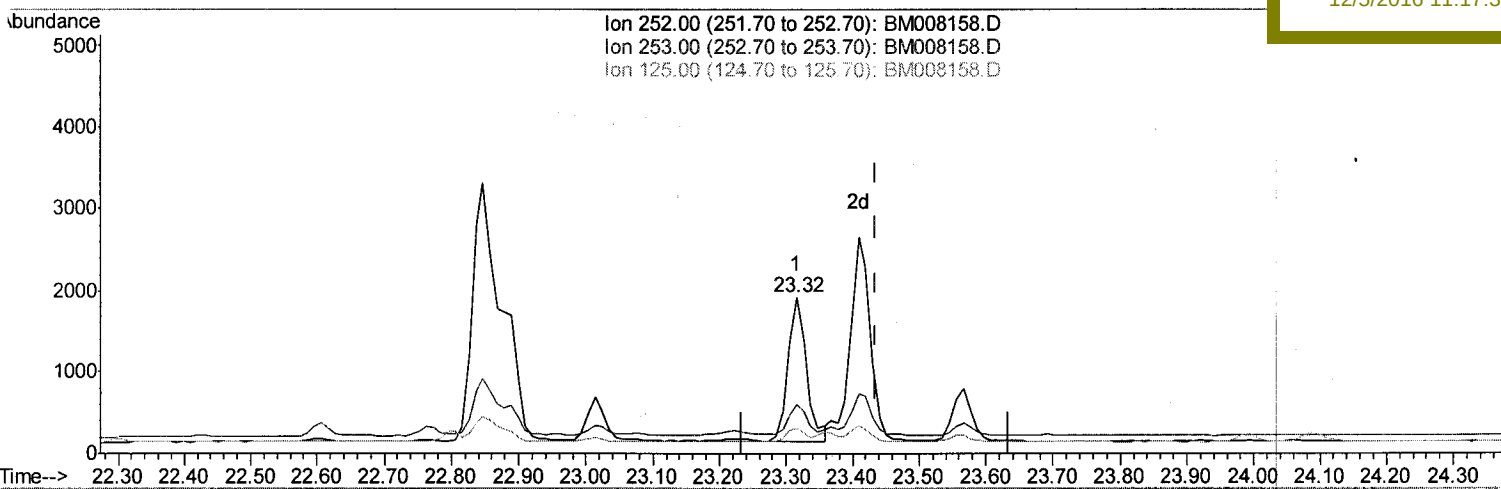

(23) Benzo(a)pyrene (C)

23.316min (-0.118) 0.58ng/ul

response 3363

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	31.45
125.00	22.60	16.40#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

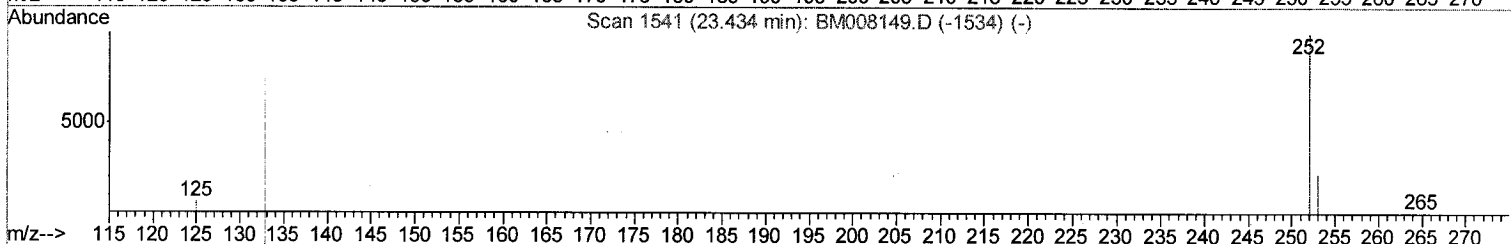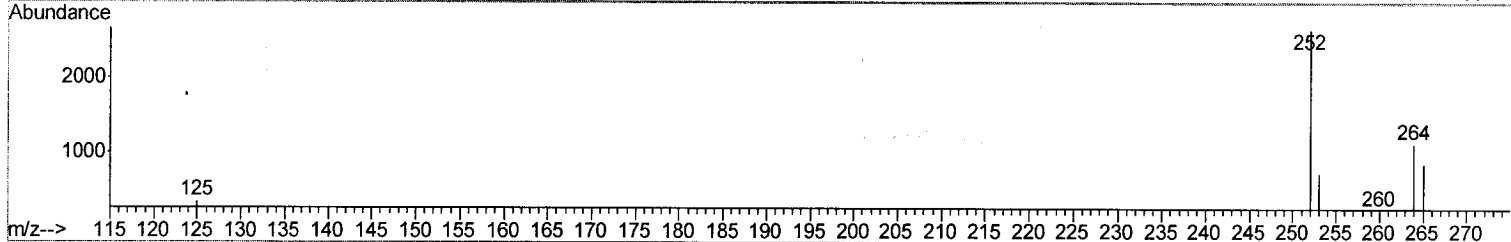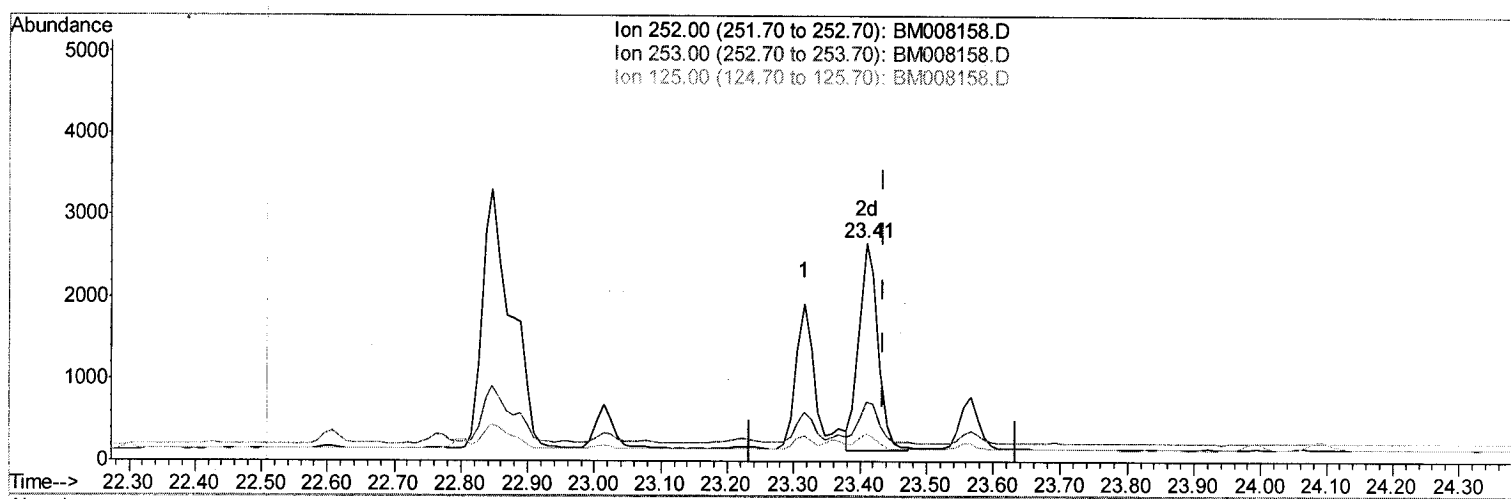

(23) Benzo(a)pyrene (C)

23.410min (-0.024) 0.87ng/ul m

response 5074

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	27.88#
125.00	22.60	12.83#
0.00	0.00	0.00

> 5.9
 12/06/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 A4WH6MSD

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
 12/5/2016 11:17:35 AM

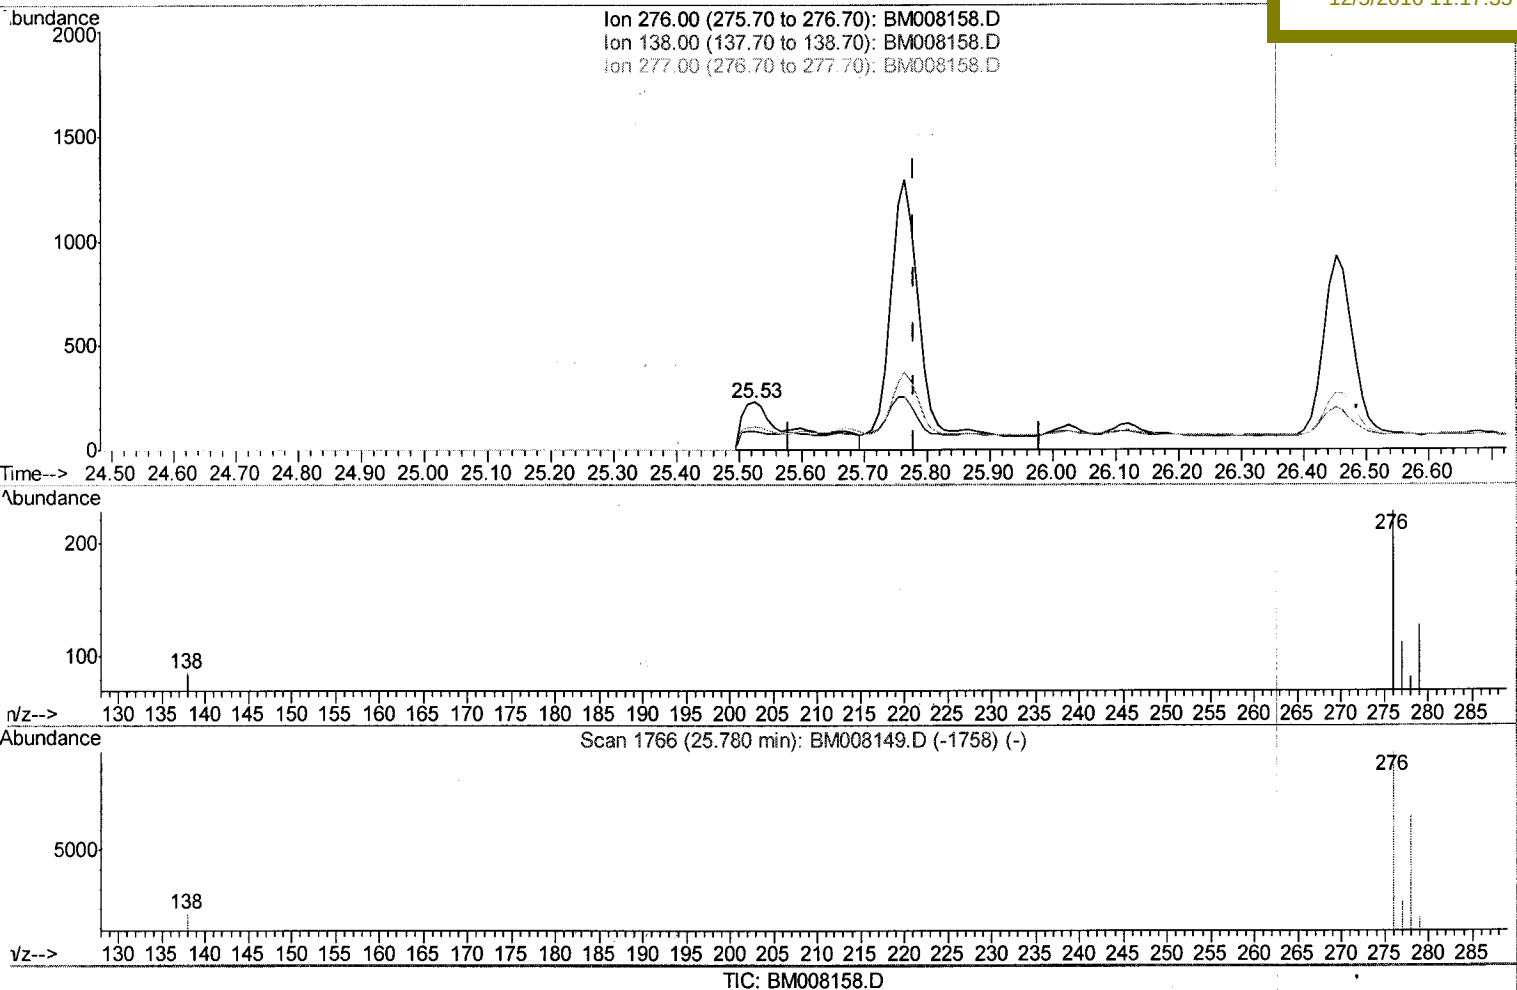

(24) Indeno(1,2,3-cd)pyrene

25.526min (-0.254) 0.19ng/ul

response 1374

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	71.03#
277.00	24.50	56.62#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

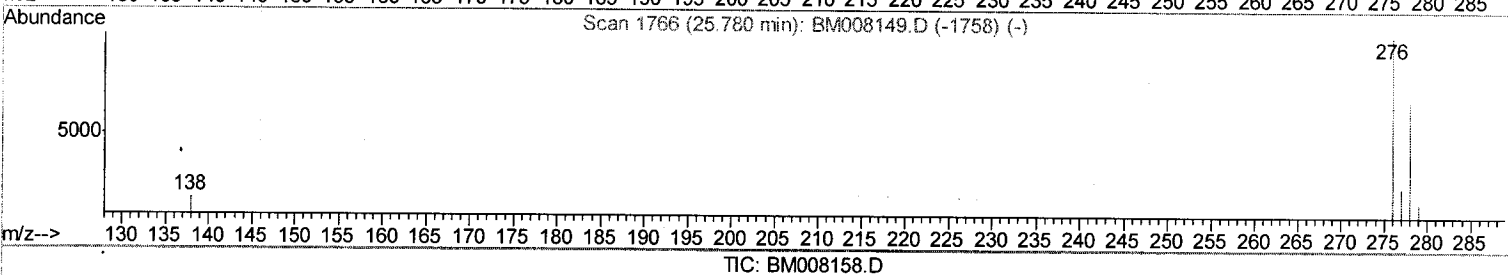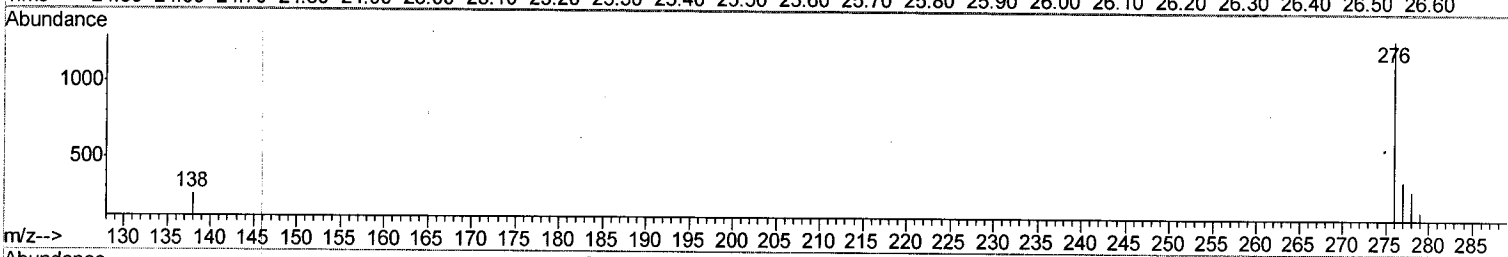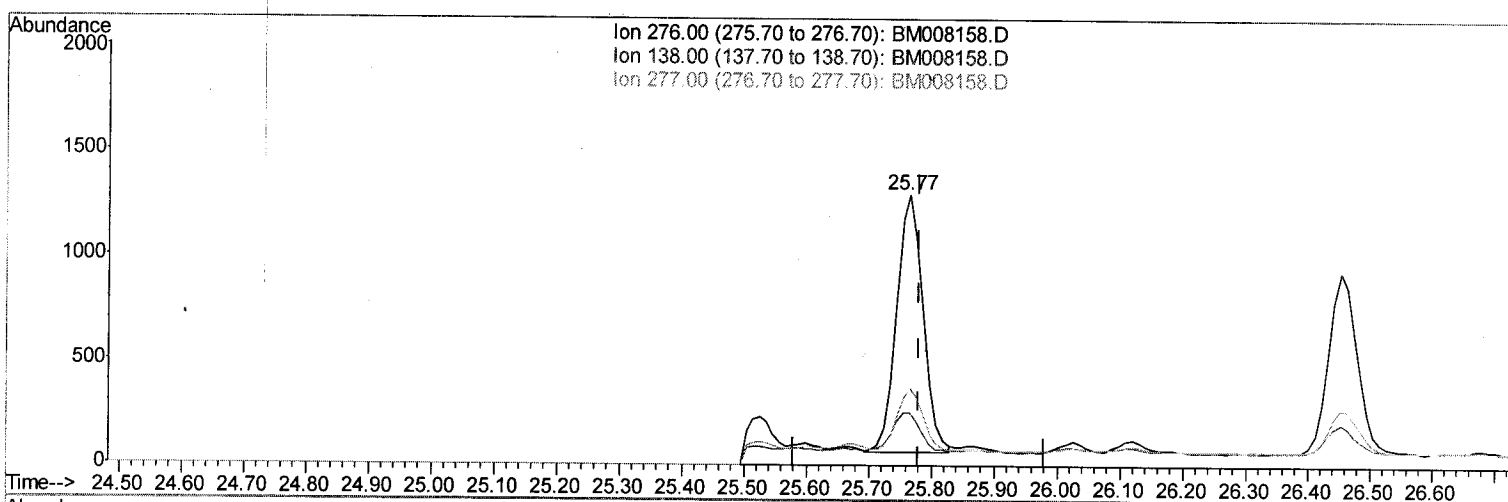

(24) Indeno(1,2,3-cd)pyrene

25.766min (-0.014) 0.49ng/ul m

response 3546

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	27.52
277.00	24.50	21.94
0.00	0.00	0.00

25.7
 12/06/16




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
Data File : BM008158.D
Acq On : 02 Dec 2016 16:15
Operator : UM/SJ
Sample : H5730-11MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WH6MSD

Quant Time: Dec 02 18:00:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 15:28:31 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
12/5/2016 11:17:35 AM

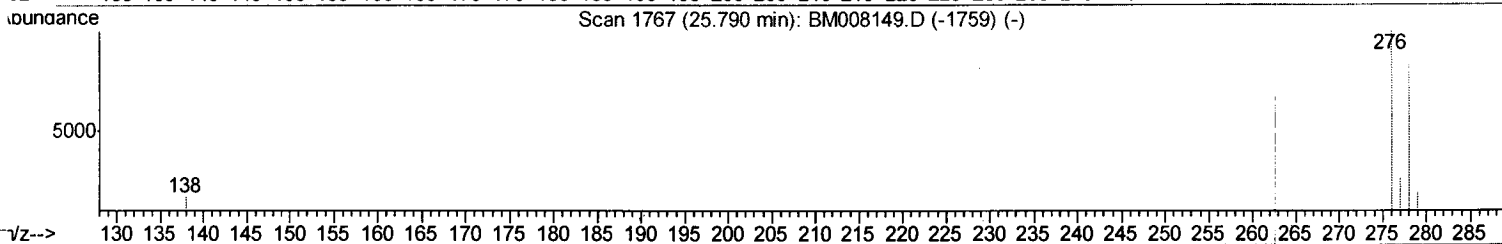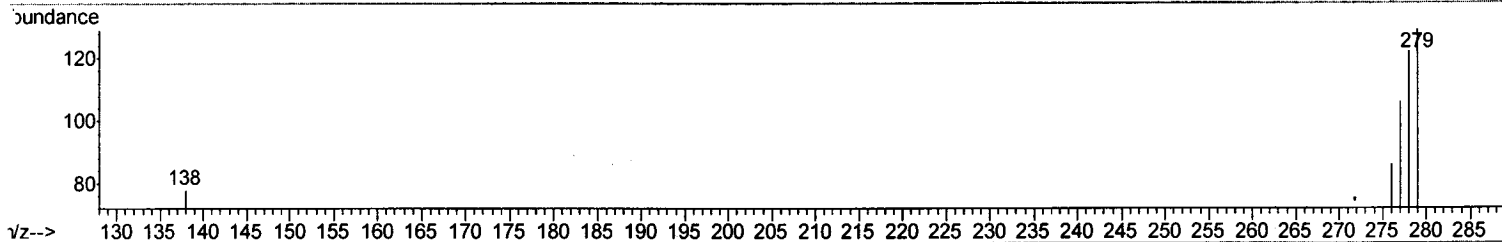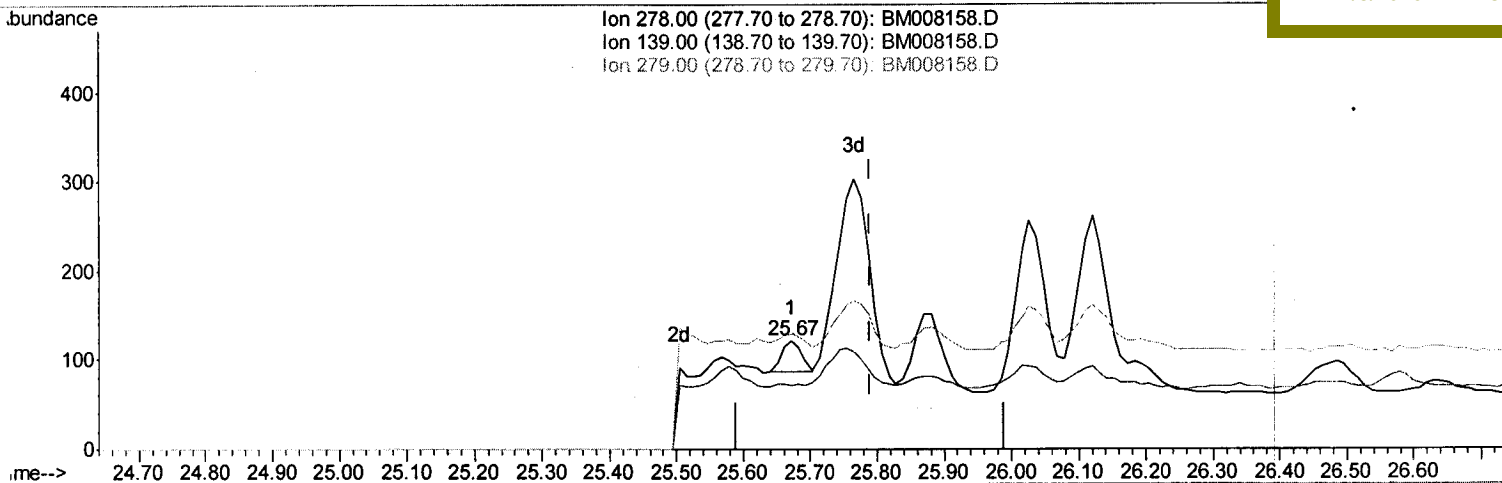

TIC: BM008158.D

(25) Dibenzo(a,h)anthracene

25.672min (-0.118) 0.01ng/ul

response 69

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	59.02#
279.00	32.40	105.74#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

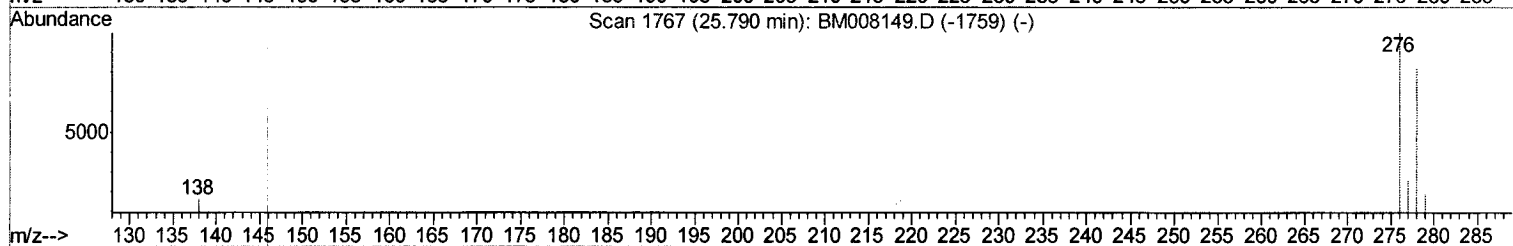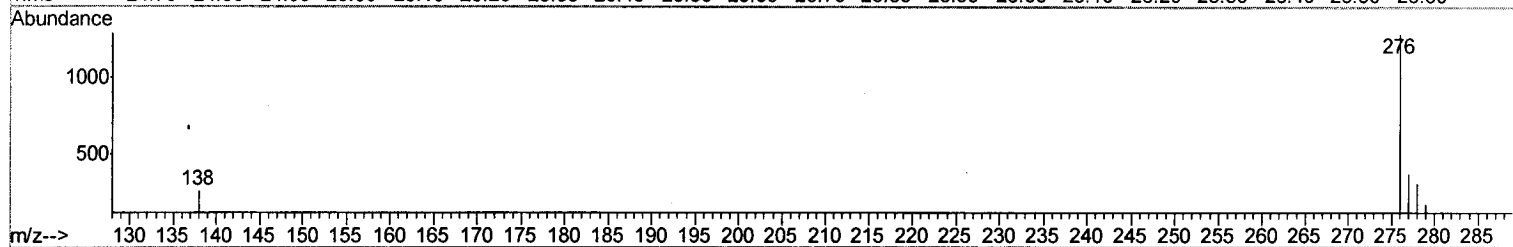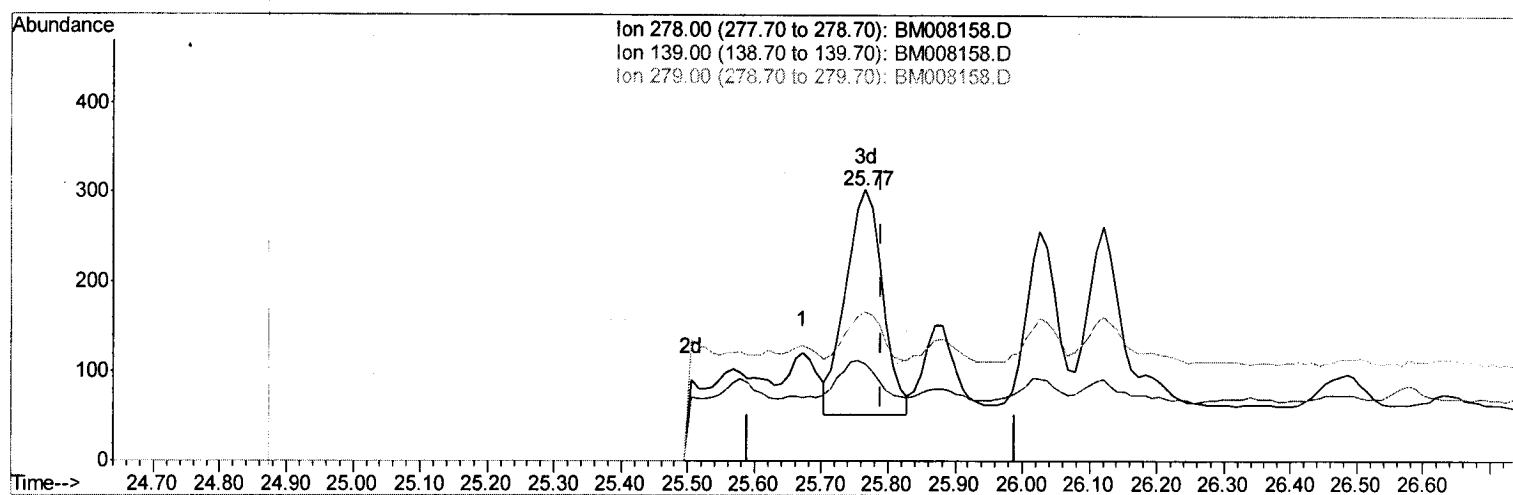

TIC: BM008158.D

(25) Dibenzo(a,h)anthracene

25.766min (-0.024) 0.17ng/ul m

response 953

Ion Exp% Act%

278.00 100 100

139.00 21.70 35.97#

279.00 32.40 55.12#

0.00 0.00 0.00

75.9
 12/06/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

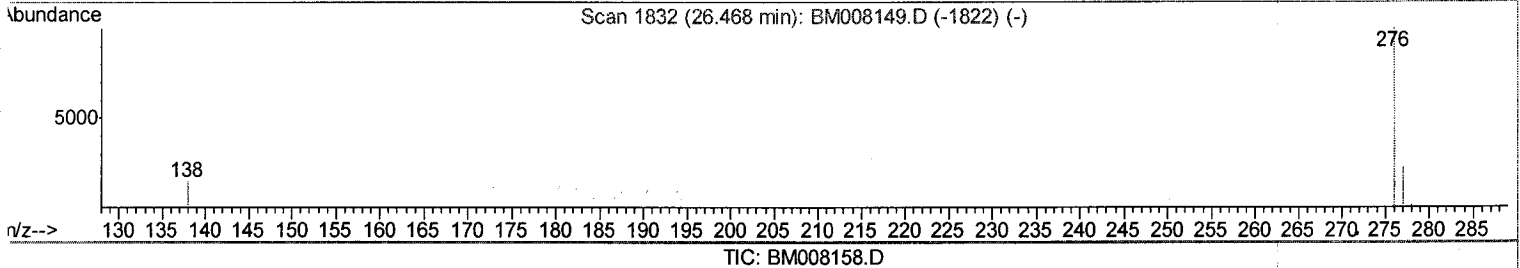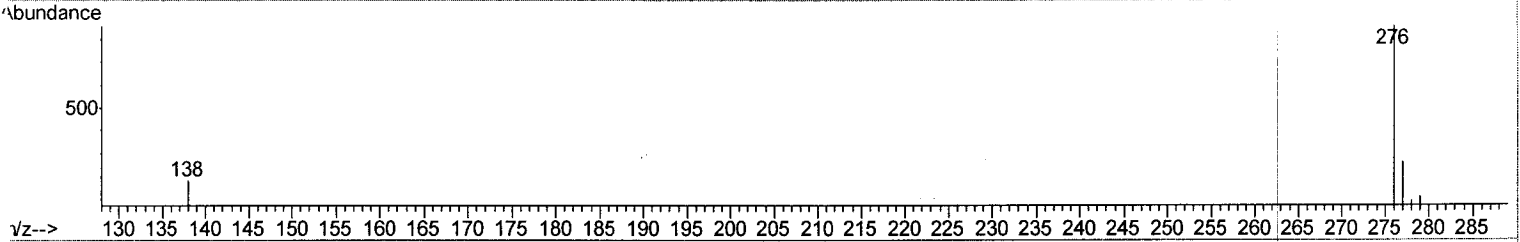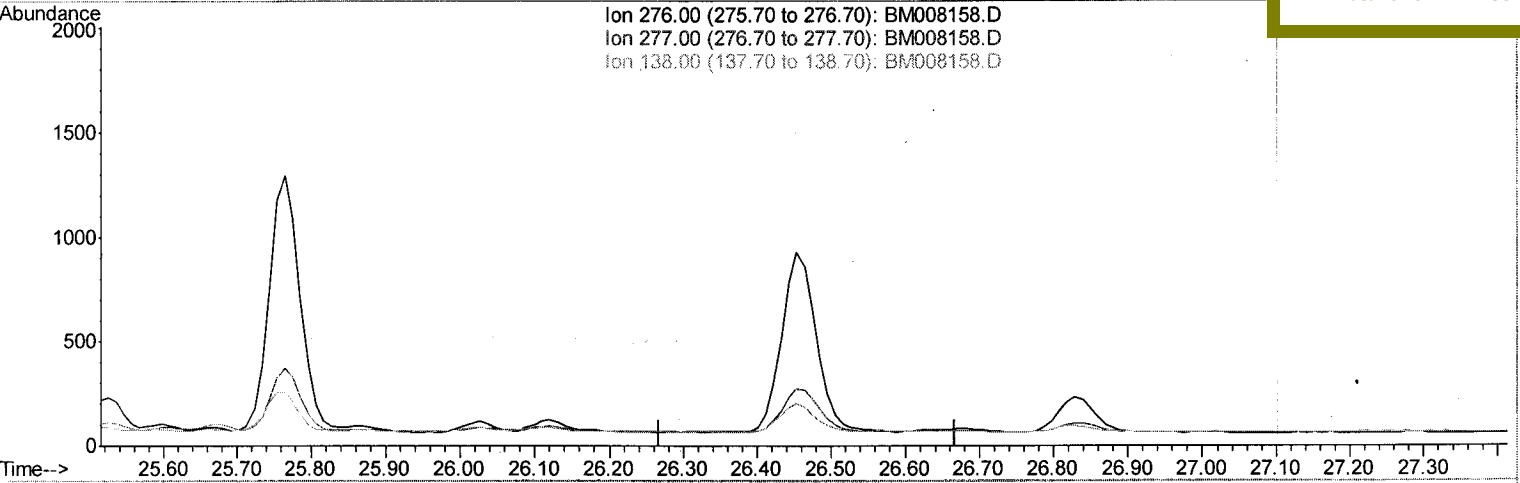

(26) Benzo(g,h,i)perylene

26.468min (-26.468) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:00:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

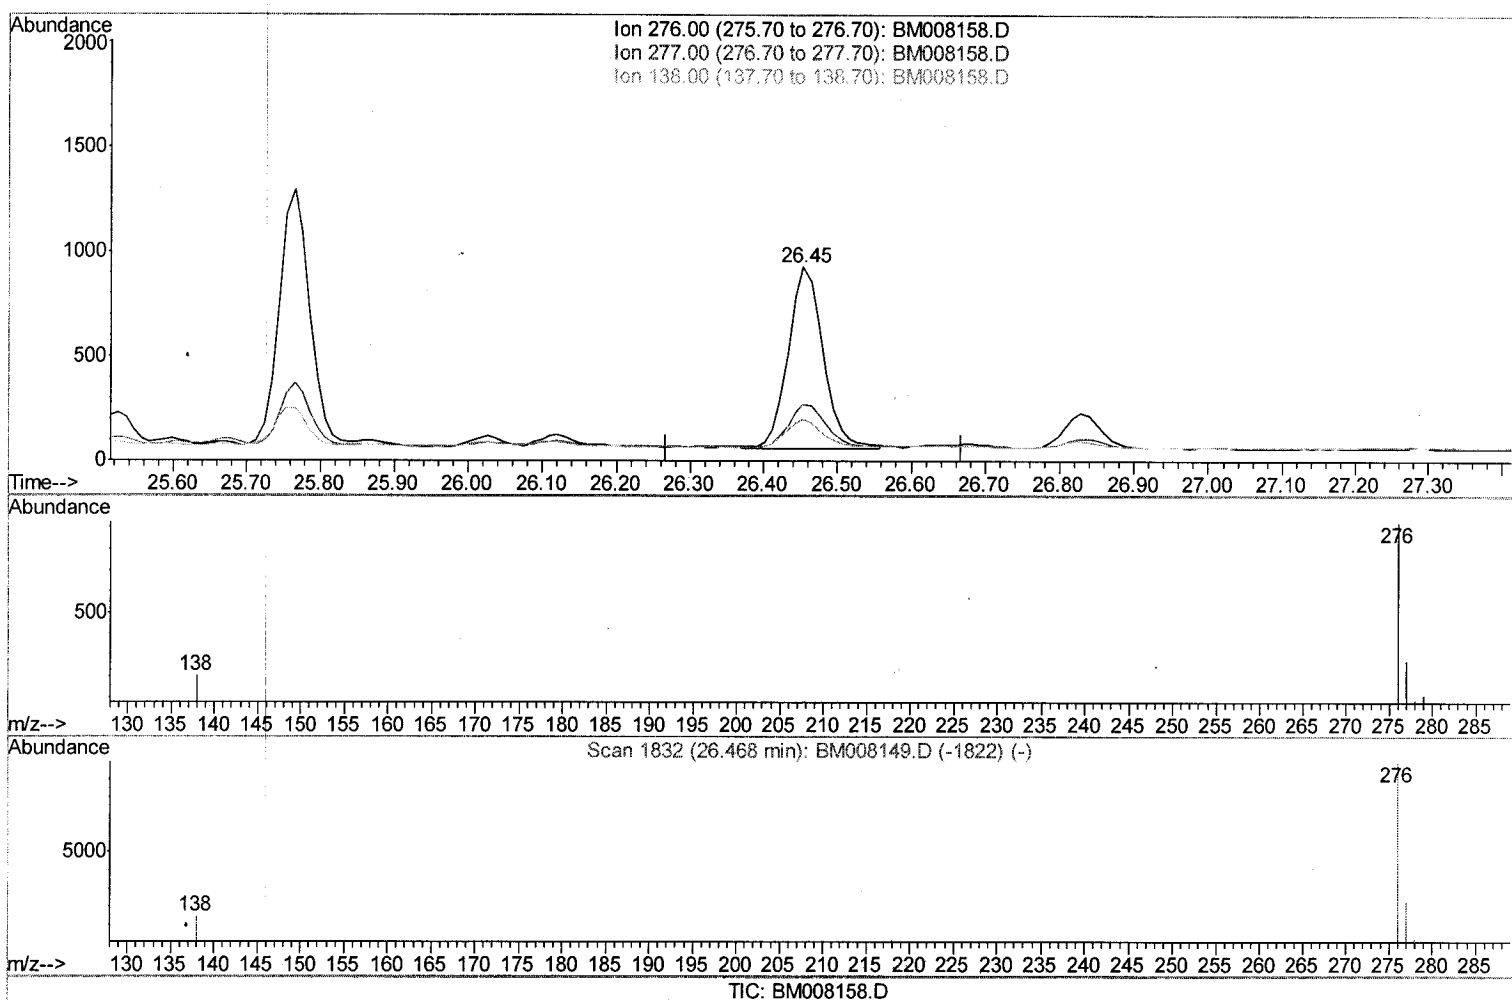

(26) Benzo(g,h,i)perylene

26.454min (-0.014) 0.45ng/ul m

response 2861

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	29.27
138.00	25.60	21.81
0.00	0.00	0.00

75.5
 12/06/16

Data Path : Z:\HPCHEM1\BNA_M\Data\BM120216\
 Data File : BM008158.D
 Acq On : 02 Dec 2016 16:15
 Operator : UM/SJ
 Sample : H5730-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH6MSD

Manual Integrations
 APPROVED

sohil
 12/5/2016 11:17:35 AM

Quant Time: Dec 02 18:02:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 15:28:31 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	598	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.48	136	2109	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.33	164	1314	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.07	188	2474m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.28	240	1955	0.40	ng/ul	-0.01
20) Perylene-d12	23.52	264	1557m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.08	152	831	0.28	ng/ul	-0.01
14) Fluoranthene-d10	19.12	212	1647	0.24	ng/ul	-0.02

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.52	128	208	0.04	ng/ul#	43
7) Acenaphthylene	14.04	152	627	0.11	ng/ul#	81
8) Acenaphthene	14.38	153	1602	0.35	ng/ul	91
9) Fluorene	15.39	166	522	0.10	ng/ul#	96
11) Pentachlorophenol	16.76	266	198	0.23	ng/ul	96
12) Phenanthrene	17.12	178	9465m	1.23	ng/ul	
13) Anthracene	17.21	178	2170	0.30	ng/ul#	95
15) Fluoranthene	19.14	202	15506	1.56	ng/ul	94
17) Pyrene	19.51	202	15904	2.34	ng/ul	98
18) Benzo(a)anthracene	21.26	228	5386	0.90	ng/ul	98
19) Chrysene	21.31	228	5487	0.74	ng/ul	96
21) Benzo(b)fluoranthene	22.85	252	6952m	1.12	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	2811m	0.44	ng/ul	
23) Benzo(a)pyrene	23.41	252	5074m	0.87	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.77	276	3546m	0.49	ng/ul	
25) Dibenzo(a,h)anthracene	25.77	278	953m	0.17	ng/ul	
26) Benzo(g,h,i)perylene	26.45	276	2861m	0.45	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed