

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120222\
 Data File : BM037829.D
 Acq On : 02 Dec 2022 15:10
 Operator : CG/JU
 Sample : N5738-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBNH4

Quant Time: Dec 02 21:48:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 02 01:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	190817	20.000	ng/u1	0.00
20) Naphthalene-d8	10.922	136	920633	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.728	164	611424	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1323910	20.000	ng/u1	0.00
79) Chrysene-d12	21.633	240	1054545	20.000	ng/u1	0.00
88) Perylene-d12	24.121	264	860762	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	15566	3.827	ng/uL	0.00
4) Pyridine-d5	3.875	84	110623	8.410	ng/u1	0.00
7) Phenol-d5	7.252	99	376143	21.880	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	231836	23.115	ng/u1	0.00
11) 2-Chlorophenol-d4	7.628	132	313894	24.149	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	254596	18.622	ng/u1	0.00
21) Nitrobenzene-d5	9.269	128	167137	22.854	ng/u1	0.00
24) 2-Nitrophenol-d4	9.999	143	179870	23.769	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	316357	22.542	ng/u1	0.00
31) 4-Chloroaniline-d4	11.057	131	226528	10.523	ng/u1	0.00
46) Dimethylphthalate-d6	14.134	166	976487	23.258	ng/u1	0.00
49) Acenaphthylene-d8	14.422	160	1180137	23.112	ng/u1	0.00
54) 4-Nitrophenol-d4	14.916	143	170455	19.560	ng/u1	0.00
60) Fluorene-d10	15.716	176	910844	23.913	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.828	200	120669	17.303	ng/u1	0.00
73) Anthracene-d10	17.563	188	1339106	21.994	ng/u1	0.00
81) Pyrene-d10	19.845	212	1575906	28.850	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.956	264	978461	22.691	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.928	105	60180	2.791	ng/u1	96
71) Pentachlorophenol	17.116	266	291790	29.904	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120222\
Data File : BM037829.D
Acq On : 02 Dec 2022 15:10
Operator : CG/JU
Sample : N5738-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNH4

Quant Time: Dec 02 21:48:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 02 01:14:59 2022
Response via : Initial Calibration




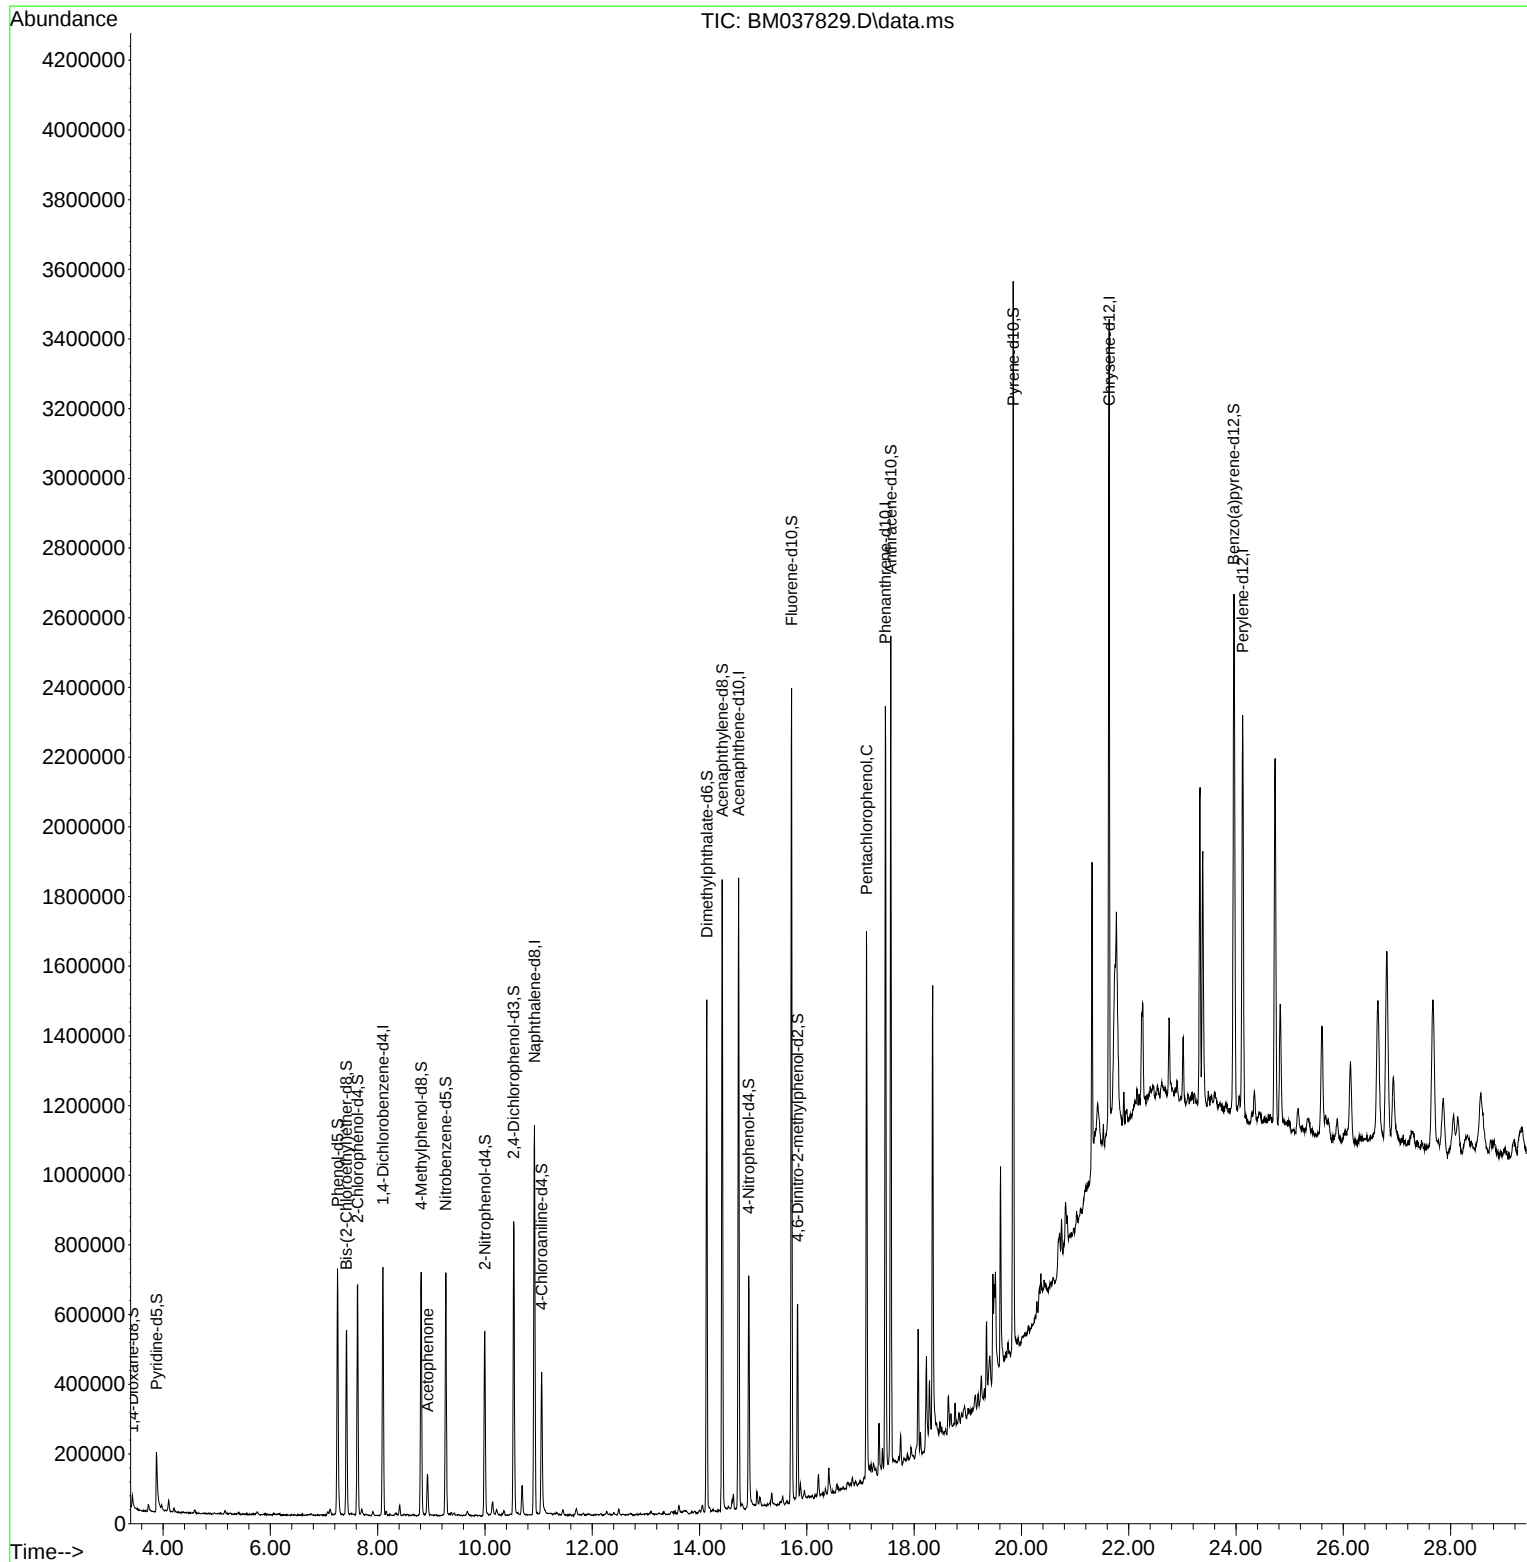


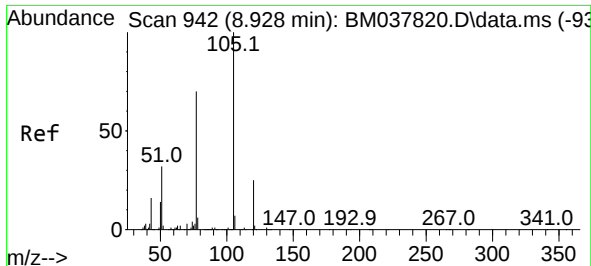

#16
Acetophenone
Concen: 2.791 ng/ul
RT: 8.928 min Scan# 942
Delta R.T. -0.000 min
Lab File: BM037829.D
Acq: 02 Dec 2022 15:10

Instrument :
BNA_M
ClientSampleId :
GBNH4

Tgt Ion:105 Resp: 60180
Ion Ratio Lower Upper
105 100
77 76.8 59.0 88.4
51 33.7 24.4 36.6

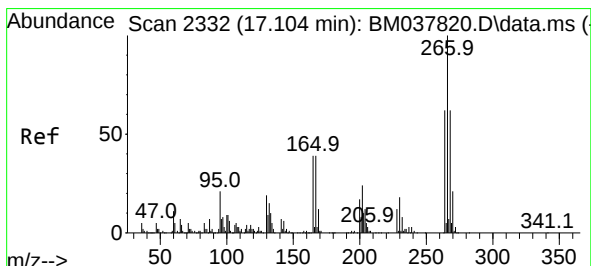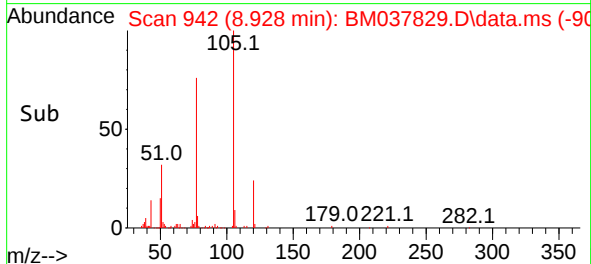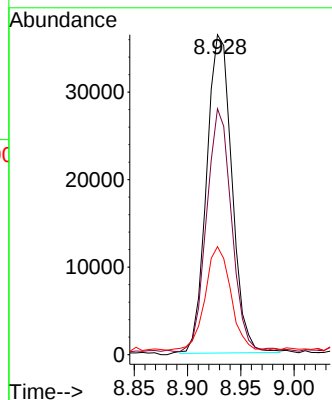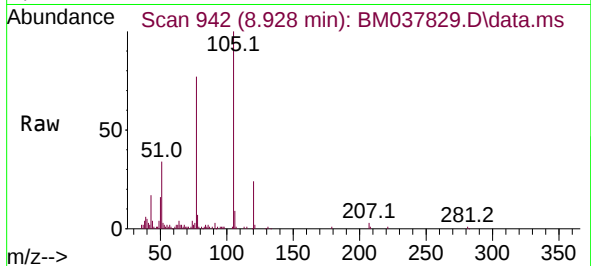

#71
Pentachlorophenol
Concen: 29.904 ng/ul
RT: 17.116 min Scan# 2334
Delta R.T. 0.006 min
Lab File: BM037829.D
Acq: 02 Dec 2022 15:10

Tgt Ion:266 Resp: 291790
Ion Ratio Lower Upper
266 100
264 62.5 50.3 75.5
268 63.3 52.2 78.2

