

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120222\
 Data File : BM037821.D
 Acq On : 02 Dec 2022 10:17
 Operator : CG/JU
 Sample : PB149301BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK301

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	3	7	16	rVB	33162	59014	1.29%	0.139%
2	3.593	33	35	39	rBV5	4147	5127	0.11%	0.012%
3	3.864	78	81	103	rBV	347163	711831	15.58%	1.678%
4	4.199	135	138	145	rVB4	11240	21422	0.47%	0.051%
5	5.581	369	373	376	rBV6	4255	7282	0.16%	0.017%
6	6.357	501	505	509	rVB7	2666	4786	0.10%	0.011%
7	6.405	509	513	515	rBV5	3038	4718	0.10%	0.011%
8	6.887	593	595	598	rBV4	4150	4652	0.10%	0.011%
9	7.246	649	656	663	rBV	577015	906137	19.84%	2.136%
10	7.416	678	685	693	rBV	498570	756862	16.57%	1.784%
11	7.622	713	720	726	rBV	562245	887526	19.43%	2.092%
12	7.834	753	756	760	rBV6	3142	4934	0.11%	0.012%
13	8.093	793	800	809	rBV	571629	927187	20.30%	2.186%
14	8.798	913	920	934	rBV	710536	1126300	24.66%	2.655%
15	8.957	944	947	953	rVV7	2814	4859	0.11%	0.011%
16	9.034	957	960	966	rVB8	3282	5569	0.12%	0.013%
17	9.263	991	999	1010	rBV	571798	940242	20.58%	2.217%
18	9.992	1114	1123	1131	rBV	416175	686167	15.02%	1.618%
19	10.528	1206	1214	1223	rBV	663645	1103893	24.17%	2.603%
20	10.916	1272	1280	1288	rBV	907420	1479623	32.39%	3.488%
21	11.051	1295	1303	1321	rBV	737094	1257782	27.53%	2.965%
22	12.486	1543	1547	1552	rBV2	14181	20577	0.45%	0.049%
23	13.604	1734	1737	1742	rBV6	4684	7285	0.16%	0.017%
24	14.128	1819	1826	1833	rBV	1325263	1744812	38.20%	4.114%
25	14.416	1869	1875	1887	rBV2	1507532	2212637	48.44%	5.217%
26	14.722	1919	1927	1936	rBV	1483623	2098720	45.94%	4.948%
27	14.904	1950	1958	1967	rBV	535487	851291	18.64%	2.007%
28	15.133	1992	1997	1999	rBV6	3037	5558	0.12%	0.013%
29	15.710	2088	2095	2103	rBV	2010699	2809020	61.49%	6.623%
30	15.816	2107	2113	2124	rBV	487201	689826	15.10%	1.626%
31	15.945	2130	2135	2139	rVB6	9355	15992	0.35%	0.038%
32	16.251	2186	2187	2192	rBV5	4572	6169	0.14%	0.015%
33	16.639	2250	2253	2256	rBV5	2809	4820	0.11%	0.011%
34	17.139	2335	2338	2341	rBV4	5662	8202	0.18%	0.019%
35	17.251	2351	2357	2359	rBV7	5347	10289	0.23%	0.024%
36	17.457	2386	2392	2400	rBV	1886087	2603301	56.99%	6.138%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120222\
 Data File : BM037821.D
 Acq On : 02 Dec 2022 10:17
 Operator : CG/JU
 Sample : PB149301BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK301

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Title : SVOA CALIBRATION

37	17.557	2402	2409	2419	rVV2	2364281	3297407	72.18%	7.774%
38	17.833	2453	2456	2460	rBV6	3717	5711	0.13%	0.013%
39	18.415	2553	2555	2559	rBV5	5941	5887	0.13%	0.014%
40	19.404	2720	2723	2728	rVB4	30324	37886	0.83%	0.089%
41	19.474	2731	2735	2738	rBV	32117	42752	0.94%	0.101%
42	19.745	2779	2781	2785	rVB4	19901	19907	0.44%	0.047%
43	19.839	2791	2797	2807	rBV	3167935	4017550	87.95%	9.472%
44	21.627	3096	3101	3110	rVB	2511374	3234872	70.81%	7.627%
45	23.950	3489	3496	3508	rVB2	2156118	4568091	100.00%	10.770%
46	24.109	3516	3523	3531	rVB	1582879	3190256	69.84%	7.522%




Sum of corrected areas: 42414731

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120222\
Data File : BM037821.D
Acq On : 02 Dec 2022 10:17
Operator : CG/JU
Sample : PB149301BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK301

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

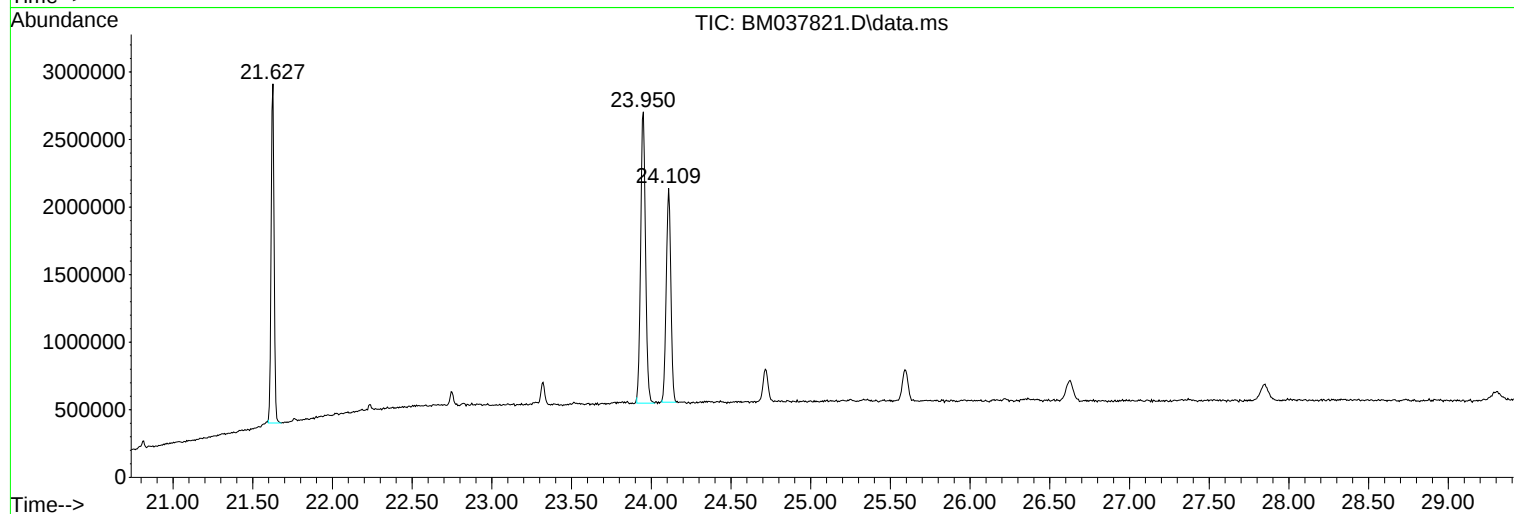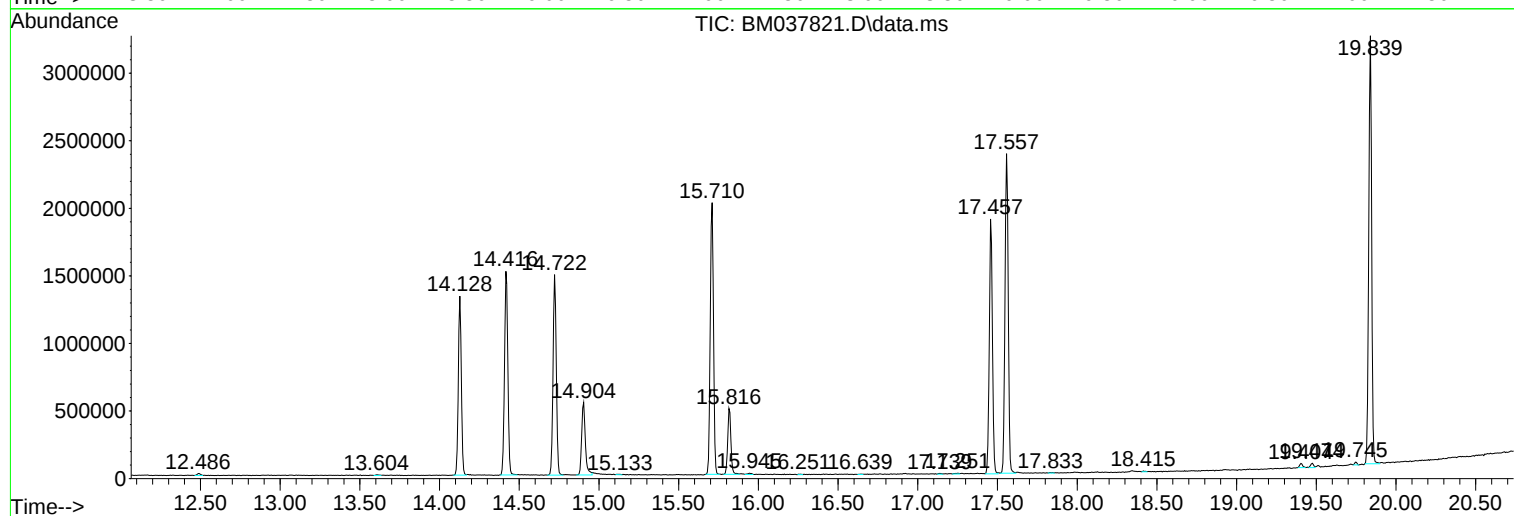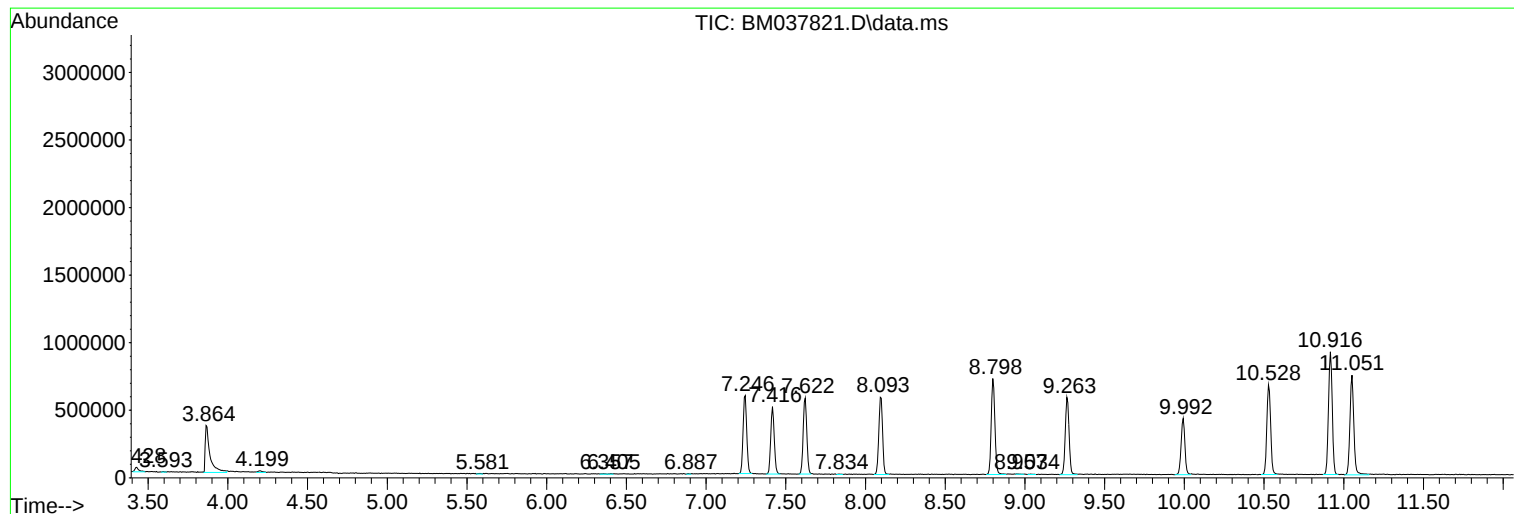

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120222\
Data File : BM037821.D
Acq On : 02 Dec 2022 10:17
Operator : CG/JU
Sample : PB149301BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK301

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120222\
Data File : BM037821.D
Acq On : 02 Dec 2022 10:17
Operator : CG/JU
Sample : PB149301BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK301

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc