


Data Path : Z:\HPCHEM1\BNA M\Data\BM120315\
 Data File : BM003367.D
 Acq On : 03 Dec 2015 09:27
 Operator : UM/IZ
 Sample : DFTPP53
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP53

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION
 Last Update : Fri Dec 04 00:04:27 2015

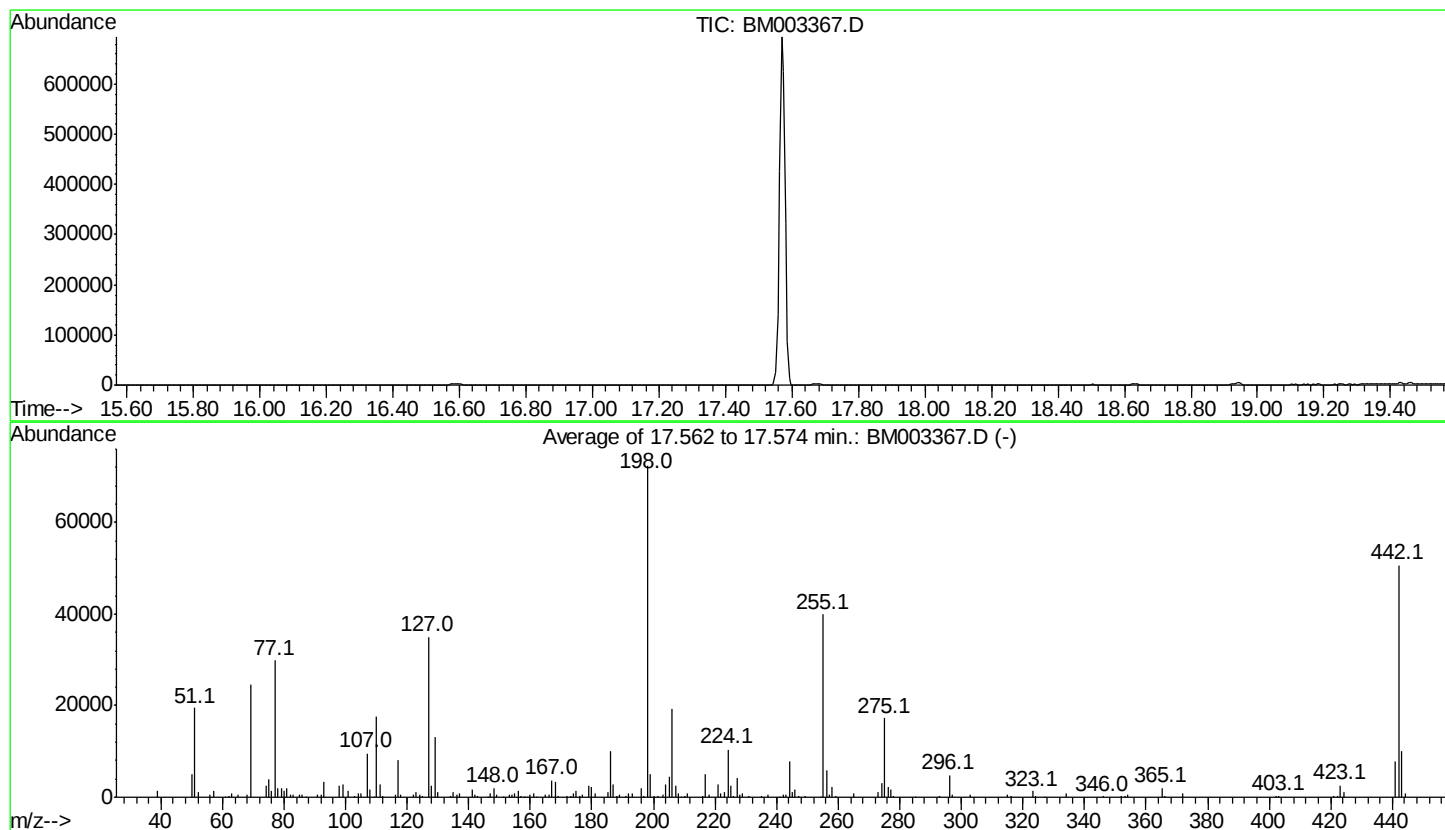

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	19512	PASS
68	69	0.00	2	1.8	434	PASS
69	198	0.00	100	33.9	24546	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	35018	PASS
197	198	0.00	2	0.6	406	PASS
198	198	100	100	100.0	72408	PASS
199	198	5	9	6.9	4967	PASS
275	198	10	60	23.8	17266	PASS
365	198	1	100	2.7	1962	PASS
441	443	0.01	100	77.7	7826	PASS
442	198	50	100	69.9	50640	PASS
443	442	15	24	19.9	10077	PASS

Scan 2456 (17.533 min): BM003367.D
DFTPP53

m/z	Abundance
73.00	332.0
207.00	476.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

m/z	Abundance
39.00	1310.0
50.10	4544.0
51.10	17408.0
52.00	943.0
56.00	528.0
57.00	1282.0
62.00	303.0
63.00	748.0
65.00	426.0
68.00	425.0
69.00	20816.0
74.00	2194.0
75.00	3463.0
76.10	1166.0
77.10	24992.0
78.00	1812.0
79.00	1688.0
80.00	1371.0
81.00	1653.0
82.00	494.0
83.00	449.0
84.90	410.0
86.00	555.0
91.00	377.0
92.00	443.0
93.00	3039.0
98.00	2272.0
99.00	2540.0
101.00	1074.0
103.00	314.0
104.00	596.0
105.00	638.0
107.00	7805.0
108.00	1387.0
110.00	13802.0
111.00	2381.0
112.00	327.0
116.10	452.0
117.00	6382.0
117.90	616.0
121.90	464.0
123.00	853.0
123.90	362.0
124.90	385.0
127.00	27880.0
128.00	2349.0
129.00	10582.0
130.00	1000.0
135.00	887.0
136.10	334.0
137.00	764.0
141.00	1451.0
142.00	492.0
142.90	308.0
147.00	731.0
148.00	1719.0
148.90	442.0
153.00	509.0
154.00	384.0
155.00	644.0
156.00	1192.0
157.00	302.0
160.00	468.0
161.00	689.0
165.00	488.0
166.10	407.0
167.00	2927.0
168.00	3112.0
169.00	375.0
173.00	315.0
174.00	581.0
175.00	1051.0
176.90	466.0
179.00	1944.0
180.00	1845.0
181.00	830.0
185.00	945.0
186.10	7436.0
187.00	2271.0
188.00	318.0
188.90	511.0
192.00	541.0
193.00	684.0
196.00	1563.0
196.80	307.0
198.00	53624.0
199.00	3699.0
200.00	350.0
203.00	431.0
204.00	1923.0
205.10	3236.0
206.10	14238.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

207.10	2450.0
208.00	577.0
211.10	528.0
217.00	3386.0
218.00	473.0
221.00	2226.0
221.80	496.0
223.00	736.0
224.10	7277.0
225.10	1936.0
226.10	306.0
227.10	2984.0
227.90	444.0
229.00	658.0
237.00	570.0
242.10	416.0
243.10	439.0
244.10	5405.0
245.10	863.0
246.00	1071.0
255.10	27024.0
256.10	4346.0
257.00	494.0
258.00	1563.0
265.00	626.0
273.00	934.0
274.00	2002.0
275.10	11270.0
276.10	1712.0
277.10	1004.0
296.00	3089.0
297.00	558.0
303.00	386.0
315.00	375.0
323.10	914.0
334.00	570.0
354.10	331.0
365.10	1115.0
372.00	374.0
423.10	1378.0
424.10	648.0
441.10	4283.0
442.10	27344.0
443.10	5574.0
444.00	526.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

m/z	Abundance
39.10	1740.0
50.10	6045.0
51.10	23088.0
52.00	1230.0
56.00	659.0
57.00	1699.0
60.90	342.0
62.10	321.0
63.00	1005.0
65.00	625.0
68.00	502.0
69.00	29480.0
73.00	407.0
74.00	3158.0
75.00	4921.0
76.10	1706.0
77.10	36008.0
78.10	2470.0
79.00	2106.0
80.00	1765.0
81.00	2457.0
82.00	648.0
83.00	568.0
85.00	565.0
86.00	677.0
91.00	531.0
92.00	779.0
93.00	4038.0
98.00	3094.0
99.00	3206.0
101.00	1564.0
103.00	450.0
104.00	903.0
105.00	840.0
107.00	11499.0
108.00	1859.0
109.00	390.0
110.00	21296.0
111.00	3374.0
111.90	388.0
116.00	646.0
117.00	9754.0
118.00	886.0
122.00	848.0
123.00	1182.0
124.00	599.0
125.00	471.0
127.00	42320.0
128.00	3163.0
129.00	15997.0
130.00	1423.0
134.00	441.0
135.00	1323.0
136.00	550.0
137.00	940.0
141.00	2006.0
142.00	742.0
143.00	529.0
146.00	384.0
147.00	1061.0
148.00	2572.0
149.00	641.0
150.90	338.0
153.00	544.0
154.00	529.0
155.00	1182.0
156.00	1822.0
157.00	388.0
157.80	400.0
158.90	334.0
160.00	610.0
161.00	1141.0
162.00	316.0
165.00	724.0
166.00	557.0
167.00	4394.0
168.00	3733.0
169.00	504.0
171.90	444.0
173.00	472.0
174.00	836.0
175.00	1823.0
176.10	446.0
177.00	788.0
179.00	3075.0
180.00	2918.0
181.00	1120.0
185.00	1396.0
186.10	11930.0
187.10	3398.0
188.00	443.0
189.00	787.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

191.00	357.0
192.00	1136.0
193.00	1198.0
196.00	2488.0
196.80	482.0
198.00	86472.0
199.00	5899.0
200.00	457.0
201.50	372.0
203.00	535.0
204.00	3245.0
205.10	5207.0
206.10	22992.0
207.10	3473.0
208.10	739.0
208.90	380.0
210.10	368.0
211.00	941.0
216.00	451.0
217.00	6085.0
218.00	792.0
221.10	3502.0
221.80	886.0
223.00	1320.0
224.10	12236.0
225.10	2909.0
226.00	473.0
227.00	4948.0
228.00	779.0
229.00	1094.0
231.00	429.0
235.00	312.0
237.00	794.0
242.00	671.0
243.10	646.0
244.10	9191.0
245.10	1211.0
246.00	1814.0
247.00	335.0
249.10	302.0
255.10	47144.0
256.10	6761.0
257.00	755.0
258.00	2840.0
259.00	413.0
265.10	1033.0
273.00	1430.0
274.00	3545.0
275.10	20448.0
276.10	2671.0
277.00	1921.0
278.00	400.0
293.00	388.0
296.10	5765.0
297.00	730.0
303.00	625.0
315.00	598.0
316.10	389.0
323.10	1540.0
324.10	343.0
334.10	1008.0
346.00	370.0
352.00	484.0
353.10	340.0
354.10	547.0
365.10	2234.0
366.00	319.0
372.10	820.0
402.10	430.0
403.10	501.0
421.00	335.0
422.00	434.0
423.10	2817.0
424.10	1285.0
441.10	8991.0
442.10	58504.0
443.10	11696.0
444.10	1098.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

m/z	Abundance
39.00	1255.0
50.10	4450.0
51.10	18040.0
52.00	912.0
56.00	537.0
57.00	1284.0
62.00	312.0
63.10	853.0
65.00	441.0
68.00	377.0
69.00	23344.0
74.00	2399.0
75.00	3642.0
76.00	1209.0
77.10	28728.0
78.00	2016.0
79.00	1865.0
80.00	1437.0
81.00	2016.0
82.00	564.0
83.00	454.0
85.00	505.0
86.00	601.0
87.00	315.0
91.00	446.0
92.00	572.0
93.00	3409.0
98.00	2497.0
99.00	2447.0
101.00	1295.0
102.90	392.0
104.00	700.0
105.00	662.0
107.00	9380.0
108.00	1475.0
110.00	17360.0
111.00	2674.0
111.90	395.0
116.00	517.0
117.00	8313.0
118.00	555.0
122.00	704.0
123.00	1013.0
123.90	433.0
124.90	418.0
127.00	34856.0
128.00	2380.0
129.00	12793.0
130.00	1197.0
134.00	363.0
135.00	1184.0
136.00	526.0
137.00	748.0
141.00	1736.0
141.90	583.0
143.00	415.0
147.00	856.0
148.00	1990.0
149.00	553.0
153.00	602.0
153.90	441.0
155.10	944.0
156.00	1599.0
157.00	368.0
158.00	324.0
160.00	591.0
161.10	997.0
165.00	674.0
166.00	501.0
167.00	4001.0
168.00	2875.0
169.00	342.0
172.00	301.0
173.00	401.0
174.00	734.0
175.00	1668.0
176.10	396.0
177.00	639.0
179.00	2690.0
180.00	2306.0
181.00	897.0
185.00	1359.0
186.10	10496.0
187.00	2932.0
188.00	337.0
189.00	722.0
191.10	328.0
192.00	807.0
193.00	1037.0
196.00	2179.0
196.80	430.0
198.00	77128.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

199.00	5303.0
200.00	328.0
201.40	385.0
203.00	489.0
204.00	2864.0
205.10	4875.0
206.10	20680.0
207.10	3015.0
208.00	822.0
210.00	417.0
210.90	807.0
216.00	378.0
217.00	5545.0
218.00	603.0
221.10	2846.0
221.80	762.0
223.00	1190.0
224.10	11540.0
225.10	2921.0
226.10	419.0
227.00	4939.0
228.00	598.0
229.00	1002.0
231.10	387.0
235.00	412.0
237.00	626.0
241.10	303.0
242.00	512.0
243.10	685.0
244.10	9032.0
245.00	1109.0
246.00	1824.0
247.00	398.0
249.00	368.0
254.10	352.0
255.10	45448.0
256.10	6483.0
257.00	551.0
258.10	2701.0
259.00	452.0
265.00	1077.0
273.00	1280.0
274.10	3430.0
275.10	20080.0
276.10	2577.0
277.00	1845.0
278.00	354.0
285.10	354.0
293.10	339.0
296.00	5485.0
297.10	785.0
303.10	580.0
315.00	643.0
316.10	327.0
323.10	1733.0
324.00	324.0
327.00	395.0
334.10	1333.0
346.00	351.0
352.00	536.0
353.00	462.0
354.10	627.0
365.10	2539.0
366.10	330.0
372.10	961.0
402.10	374.0
403.10	582.0
421.10	462.0
422.10	482.0
423.10	3353.0
424.10	1319.0
441.10	10205.0
442.10	66072.0
443.10	12961.0
444.10	1239.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53