

Data File : BM017877.D

Acq On : 03 Dec 2018 11:24

Operator : JU/SJ

Sample : SSTDCCC020

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Dec 04 00:12:16 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Dec 03 00:28:52 2018

Response via : Initial Calibration

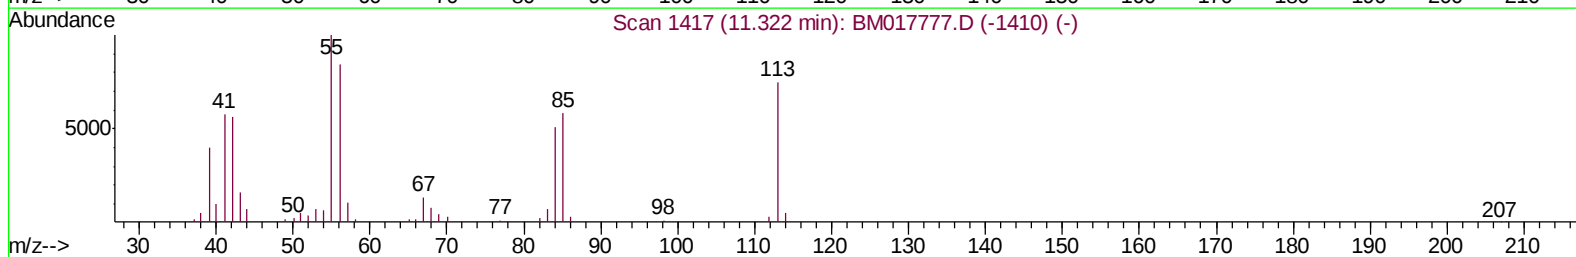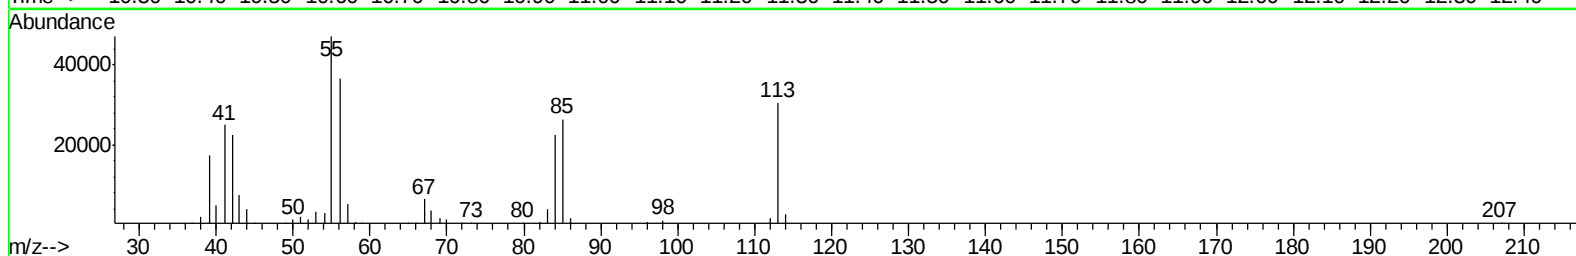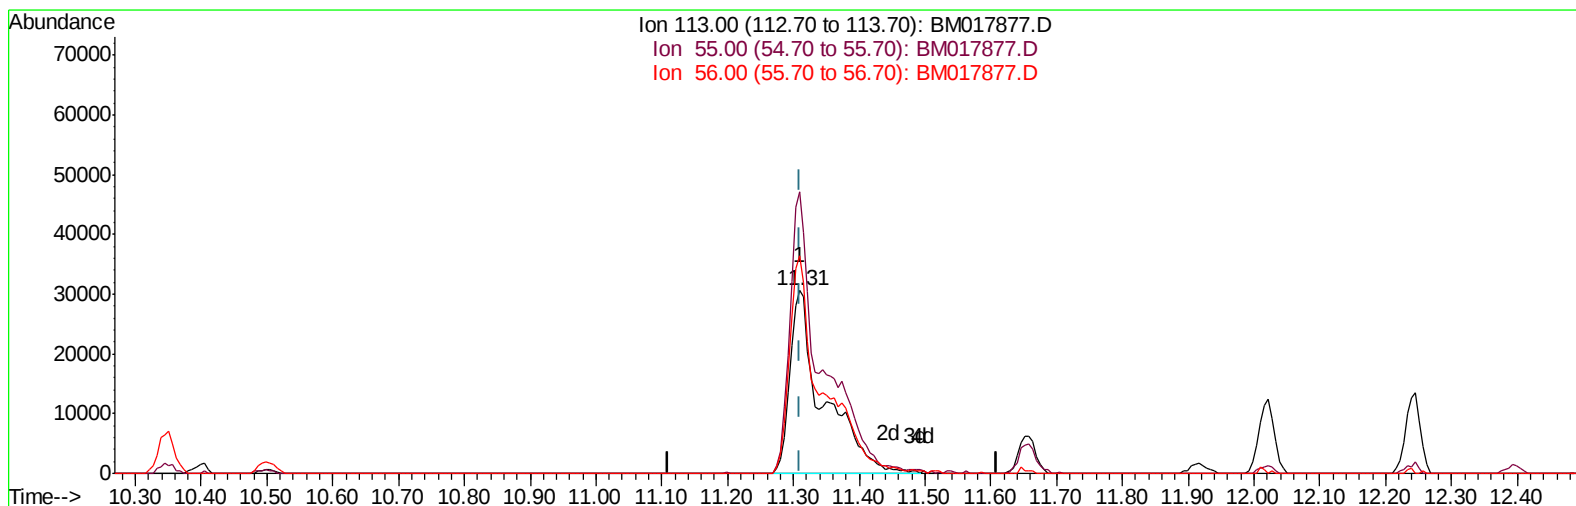

TIC: BM017877.D

(32) Caprolactam

11.310min (-0.000) 19.07ng/ul m

response 107780

Ion	Exp%	Act%
113.00	100	100
55.00	138.30	154.34
56.00	110.30	119.28
0.00	0.00	0.00