
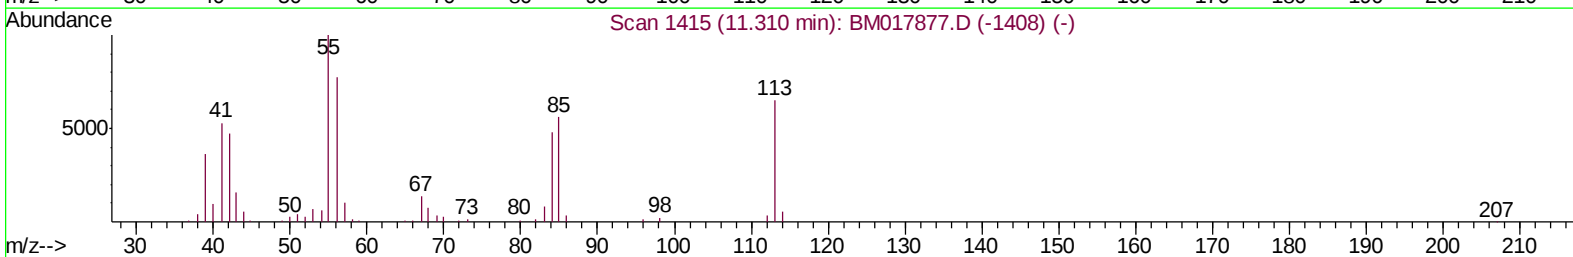
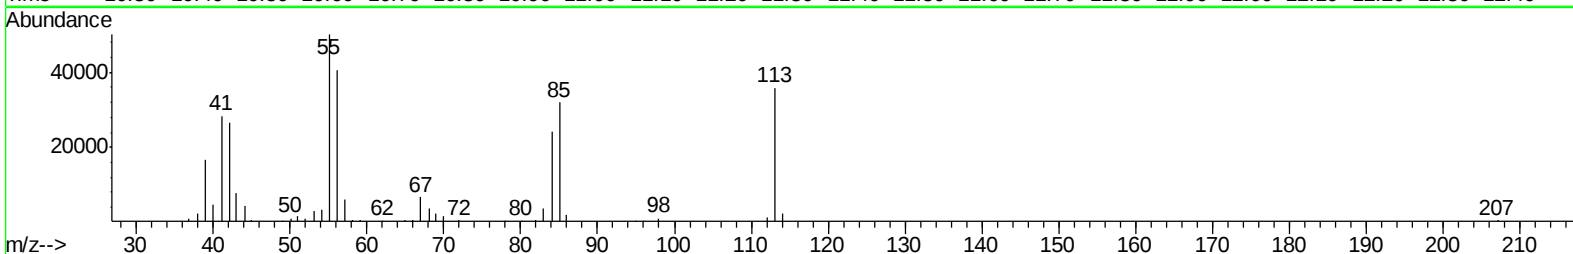


Data File : BM017879.D
Acq On : 03 Dec 2018 16:25
Operator : JU/SJ
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 04 00:22:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 04 00:18:53 2018
Response via : Initial Calibration

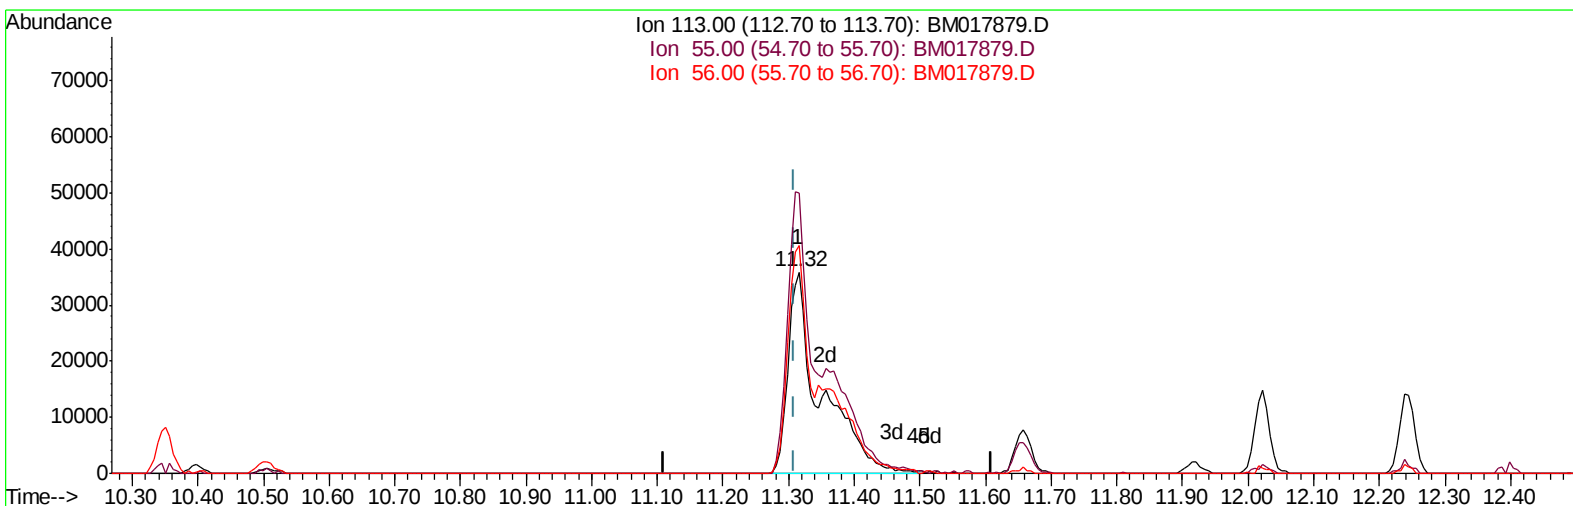

TIC: BM017879.D

(32) Caprolactam

11.316min (+0.006) 19.07ng/ul m

response 124640

Ion	Exp%	Act%
113.00	100	100
55.00	138.30	139.67
56.00	110.30	113.13
0.00	0.00	0.00