




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM120324\  
Data File : BM048811.D  
Acq On : 02 Dec 2024 18:43  
Operator : RC/JU  
Sample : SST0.420  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SSTD0.4001

Manual IntegrationsAPPROVED

Quant Time: Dec 03 00:12:40 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM120324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 03 00:10:10 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2024  
Supervised By :mohammad ahmed 12/05/2024

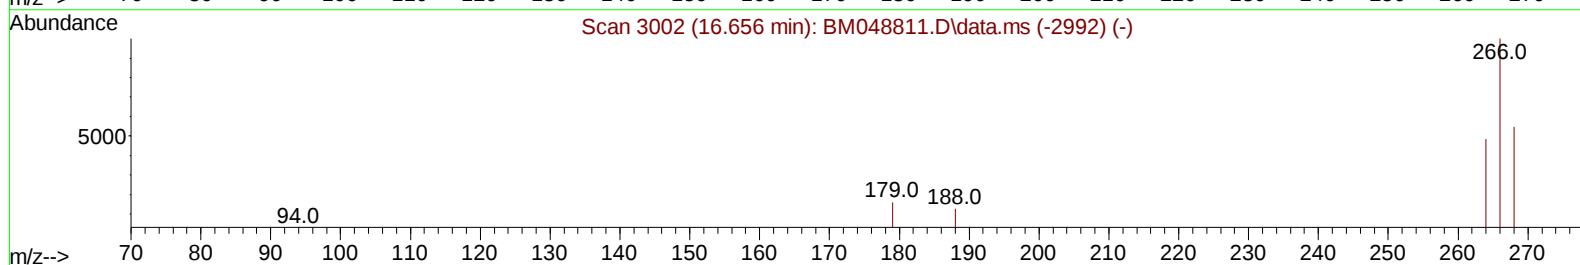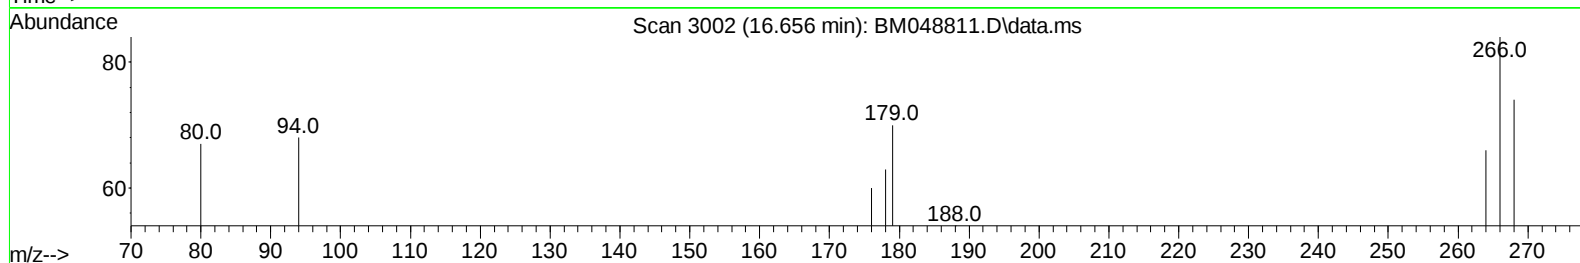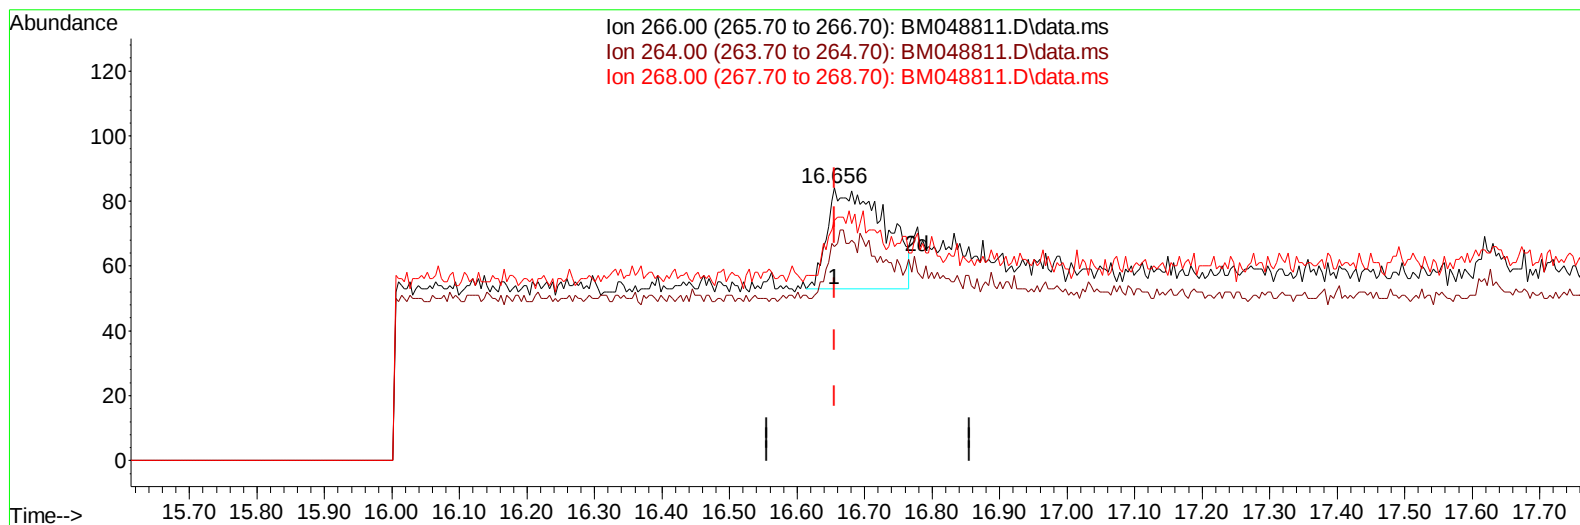

TIC: BM048811.D\data.ms

(14) Pentachloropheno1

16.656min ( 0.000) 0.07 ng/u1

response 182

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 266.00 | 100.00 | 100.00 |
| 264.00 | 19.10  | 29.12# |
| 268.00 | 0.00   | 0.00   |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM120324\  
Data File : BM048811.D  
Acq On : 02 Dec 2024 18:43  
Operator : RC/JU  
Sample : SST0.420  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SSTD0.4001

Manual IntegrationsAPPROVED

Quant Time: Dec 03 00:12:40 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM120324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 03 00:10:10 2024  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2024  
Supervised By :mohammad ahmed 12/05/2024

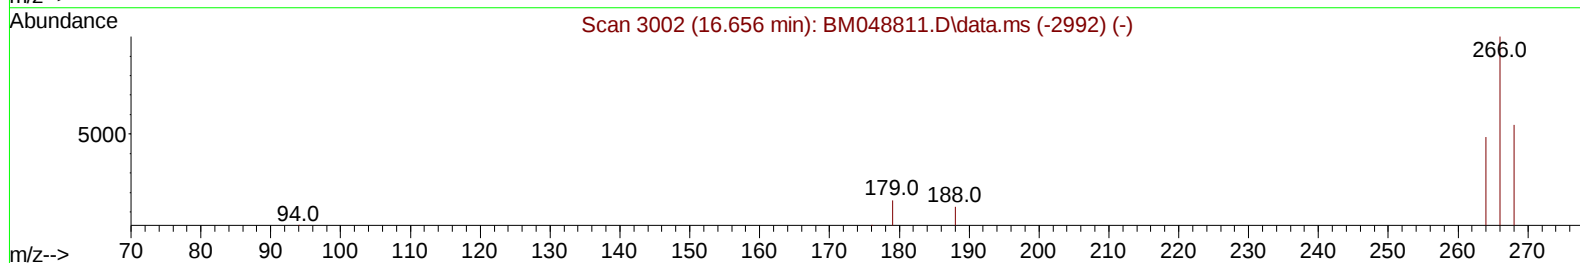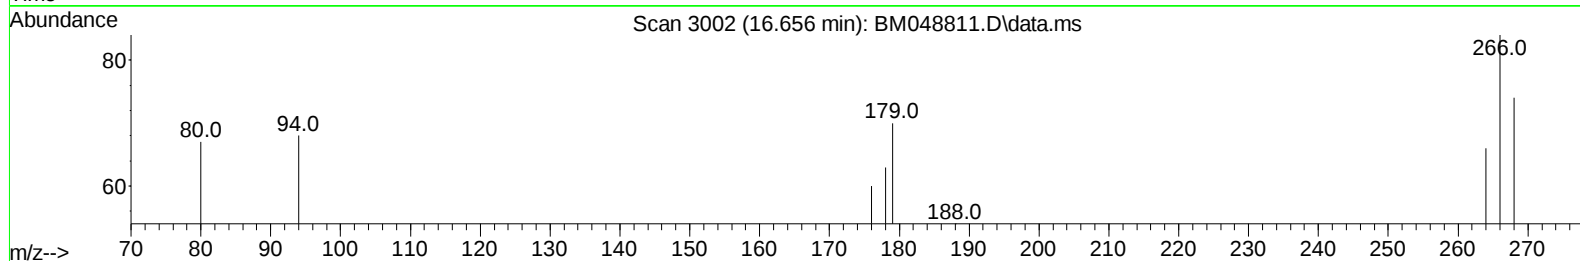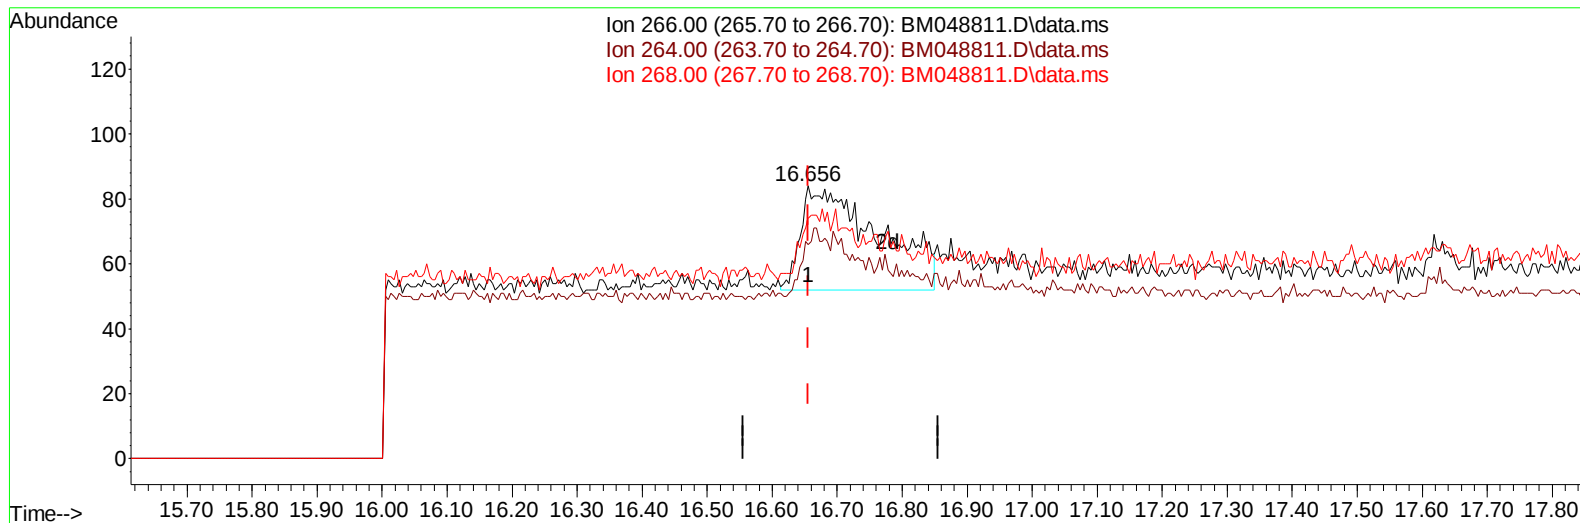

TIC: BM048811.D\data.ms

(14) Pentachloropheno1

16.656min ( 0.000) 0.11 ng/u1 m

response 263

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 266.00 | 100.00 | 100.00 |
| 264.00 | 19.10  | 20.15  |
| 268.00 | 0.00   | 0.00   |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM120324\  
 Data File : BM048811.D  
 Acq On : 02 Dec 2024 18:43  
 Operator : RC/JU  
 Sample : SSTD0.420  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SSTD0.4001

Manual IntegrationsAPPROVED

Quant Time: Dec 03 00:12:40 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM120324.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Dec 03 00:10:10 2024  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2024  
 Supervised By :mohammad ahmed 12/05/2024

| Compound                    | R.T.   | Q   | Ion | Response | Conc  | Units | Dev(Min) |
|-----------------------------|--------|-----|-----|----------|-------|-------|----------|
| -----                       |        |     |     |          |       |       |          |
| Internal Standards          |        |     |     |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.611  | 152 |     | 3158     | 0.400 | ng/ul | 0.00     |
| 4) Naphthalene-d8           | 10.375 | 136 |     | 8838     | 0.400 | ng/ul | 0.00     |
| 9) Acenaphthene-d10         | 14.243 | 164 |     | 4778     | 0.400 | ng/ul | 0.00     |
| 13) Phenanthrene-d10        | 16.989 | 188 |     | 8953     | 0.400 | ng/ul | 0.00     |
| 17) Chrysene-d12            | 21.186 | 240 |     | 5613     | 0.400 | ng/ul | 0.00     |
| 23) Perylene-d12            | 23.370 | 264 |     | 6682     | 0.400 | ng/ul | 0.00     |
| System Monitoring Compounds |        |     |     |          |       |       |          |
| 3) 1,4-Dioxane-d8           | 3.176  | 96  |     | 1680     | 0.440 | ng/ul | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 11.976 | 152 |     | 4327     | 0.374 | ng/ul | 0.00     |
| 18) Fluoranthene-d10        | 19.021 | 212 |     | 7255     | 0.388 | ng/ul | 0.00     |
| Target Compounds            |        |     |     |          |       |       |          |
|                             |        |     |     |          |       |       | Qvalue   |
| 2) 1,4-Dioxane              | 3.206  | 88  |     | 2029     | 0.476 | ng/ul | 100      |
| 5) Naphthalene              | 10.425 | 128 |     | 9049     | 0.400 | ng/ul | 100      |
| 7) 2-Methylnaphthalene      | 12.053 | 142 |     | 5181     | 0.349 | ng/ul | 99       |
| 8) 1-Methylnaphthalene      | 12.267 | 142 |     | 5523     | 0.368 | ng/ul | 99       |
| 10) Acenaphthylene          | 13.961 | 152 |     | 8491     | 0.375 | ng/ul | 100      |
| 11) Acenaphthene            | 14.303 | 153 |     | 6129     | 0.398 | ng/ul | 100      |
| 12) Fluorene                | 15.298 | 166 |     | 6378     | 0.372 | ng/ul | 100      |
| 14) Pentachlorophenol       | 16.656 | 266 |     | 263m     | 0.105 | ng/ul |          |
| 15) Phenanthrene            | 17.031 | 178 |     | 8876     | 0.347 | ng/ul | 100      |
| 16) Anthracene              | 17.124 | 178 |     | 8015     | 0.314 | ng/ul | 100      |
| 19) Fluoranthene            | 19.053 | 202 |     | 10395    | 0.364 | ng/ul | 100      |
| 20) Pyrene                  | 19.416 | 202 |     | 10881    | 0.357 | ng/ul | 100      |
| 21) Benzo(a)anthracene      | 21.172 | 228 |     | 6127     | 0.230 | ng/ul | 100      |
| 22) Chrysene                | 21.222 | 228 |     | 10143    | 0.400 | ng/ul | 100      |
| 24) Benzo(b)fluoranthene    | 22.721 | 252 |     | 7122     | 0.255 | ng/ul | 100      |
| 25) Benzo(k)fluoranthene    | 22.764 | 252 |     | 10529    | 0.378 | ng/ul | 100      |
| 26) Benzo(a)pyrene          | 23.273 | 252 |     | 7616     | 0.295 | ng/ul | 100      |
| 27) Indeno(1,2,3-cd)pyrene  | 25.547 | 276 |     | 9949     | 0.291 | ng/ul | 100      |
| 28) Dibenzo(a,h)anthracene  | 25.564 | 278 |     | 7588     | 0.298 | ng/ul | 100      |
| 29) Benzo(g,h,i)perylene    | 26.195 | 276 |     | 8703     | 0.321 | ng/ul | 100      |
| -----                       |        |     |     |          |       |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

