


Data Path : Z:\HPCHEM1\BNA M\DATA\BM120415\
 Data File : BM003372.D
 Acq On : 03 Dec 2015 13:40
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 16:19:00 2015

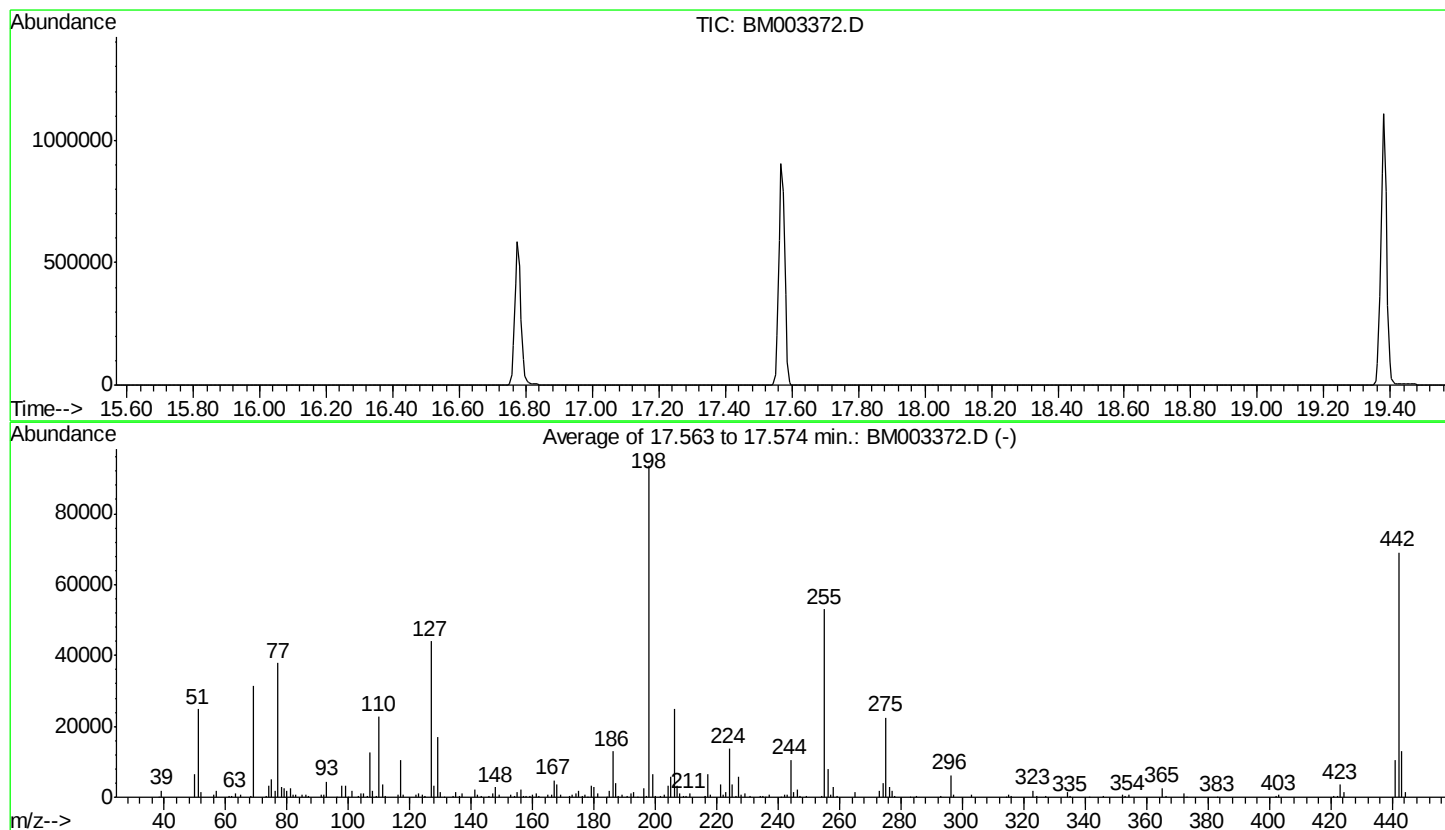

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	24805	PASS
68	69	0.00	2	1.6	507	PASS
69	198	0.00	100	33.5	31320	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	43973	PASS
197	198	0.00	2	0.3	302	PASS
198	198	100	100	100.0	93554	PASS
199	198	5	9	6.8	6350	PASS
275	198	10	60	24.1	22559	PASS
365	198	1	100	2.8	2594	PASS
441	442	0.01	24	15.3	10541	PASS
442	198	50	100	73.8	69000	PASS
443	442	15	24	19.1	13195	PASS