

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM120417\
 Data File : BM013165.D
 Acq On : 04 Dec 2017 14:15
 Operator : SJ/JU
 Sample : I6646-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0245

Quant Time: Dec 05 04:21:28 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 05 04:17:47 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	190234	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	779188	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	484842	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	1180068	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1347127	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	1245013	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.24	96	7330	1.91	ng/uL	0.00
5) Phenol-d5	6.88	99	168437	10.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	108829	11.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	140714	10.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	145155	10.32	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	76325	12.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	74826	11.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	143151	10.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	159899	12.77	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	517402	11.99	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	634253	11.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	66180	8.83	ng/ul	0.00
57) Fluorene-d10	15.34	176	461584	12.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	60359	8.13	ng/ul	0.00
70) Anthracene-d10	17.19	188	729745	12.35	ng/ul	0.00
76) Pyrene-d10	19.48	212	843240	12.56	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	774601	12.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.80	163	115939	2.810	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM120417\
Data File : BM013165.D
Acq On : 04 Dec 2017 14:15
Operator : SJ/JU
Sample : I6646-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0245

Quant Time: Dec 05 04:21:28 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 05 04:17:47 2017
Response via : Initial Calibration

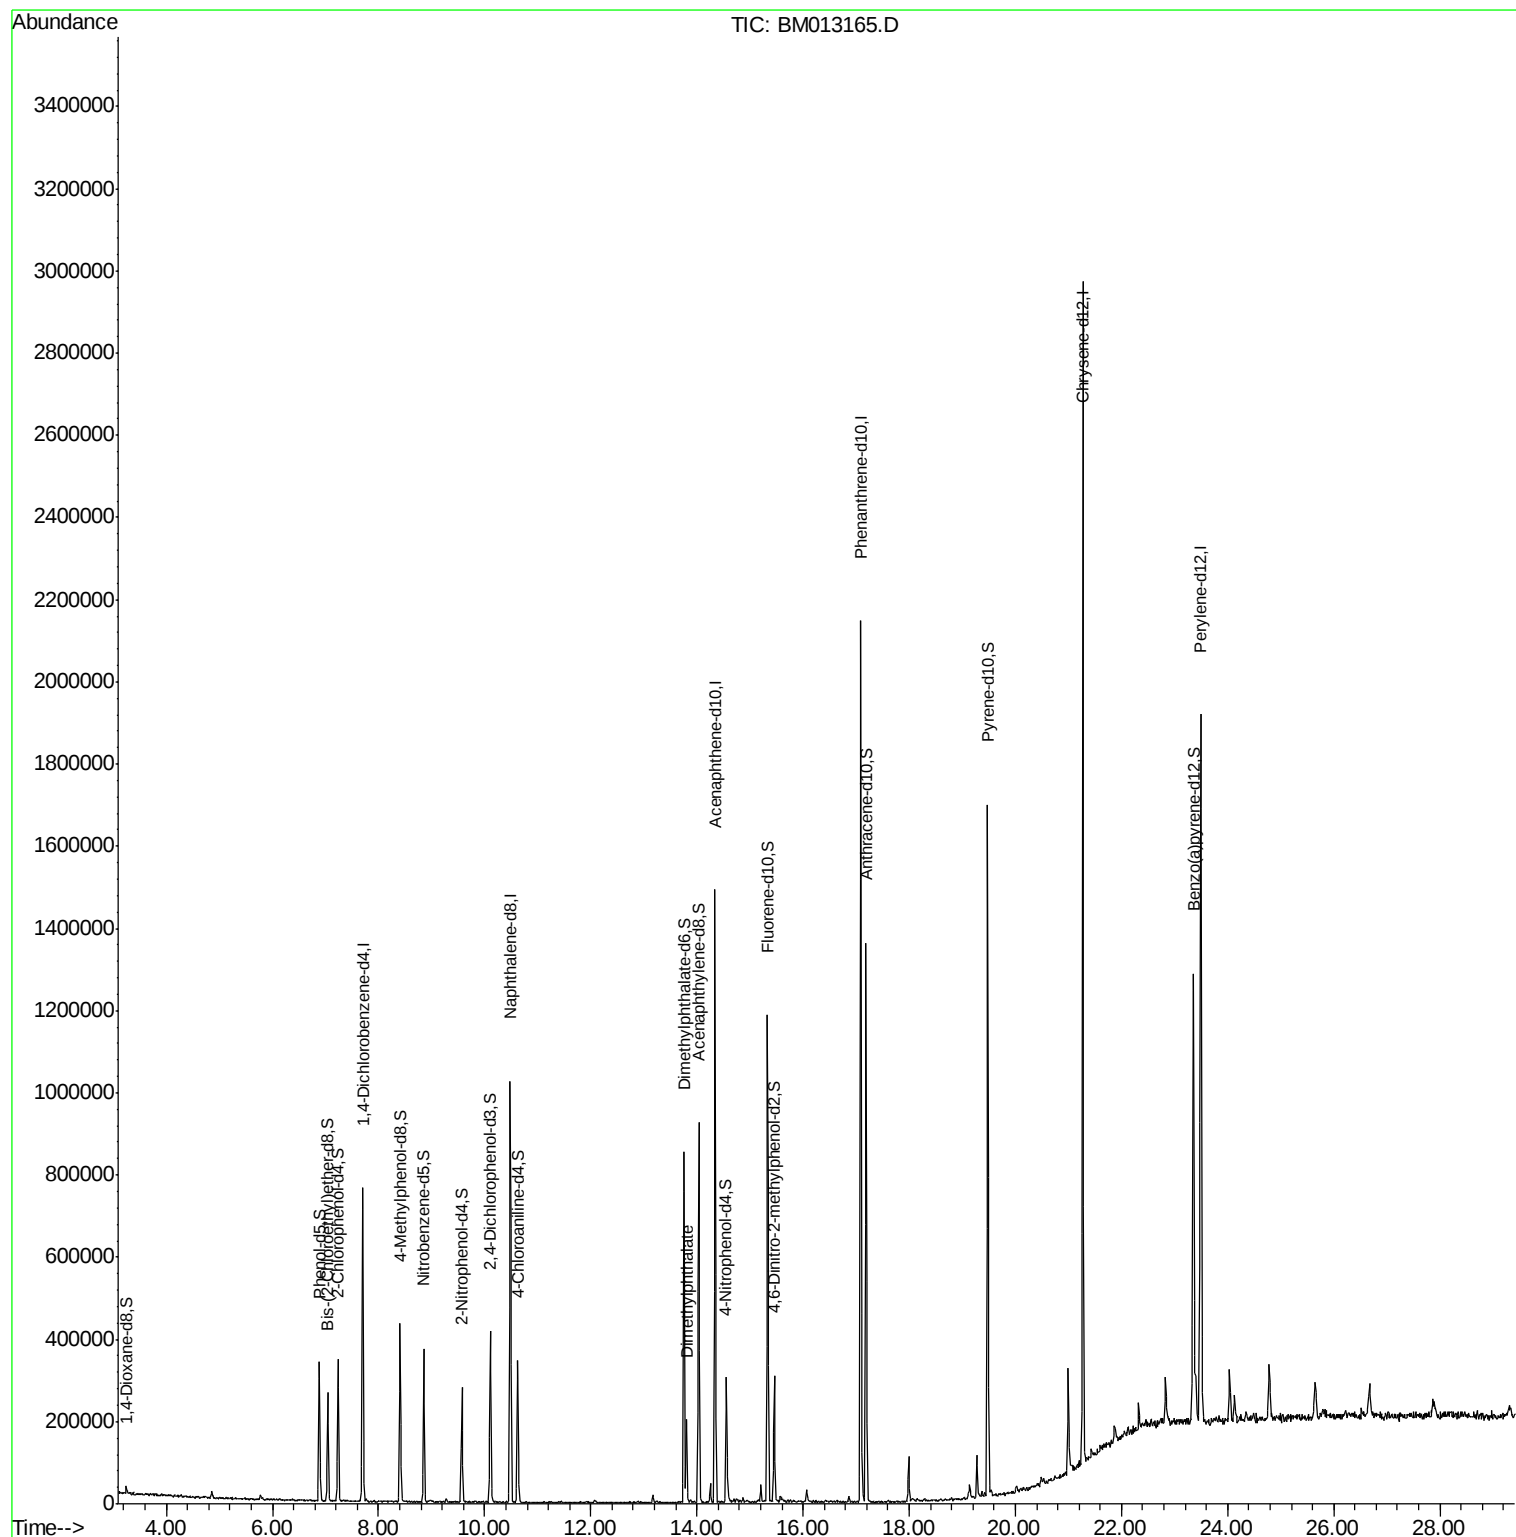

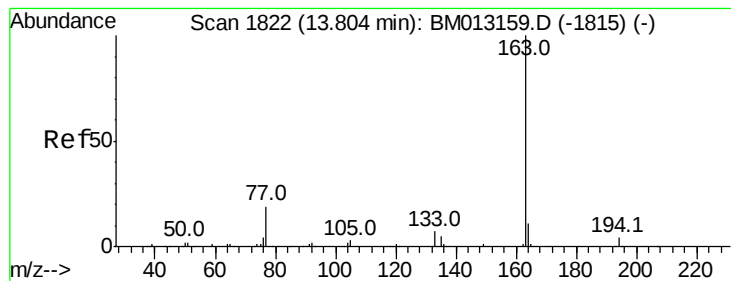

#44

Dimethylphthalate

Concen: 2.810 ng/ul

RT: 13.80 min Scan# 1822

Delta R.T. 0.00 min

Lab File: BM013165.D

Acq: 04 Dec 2017 14:15

Instrument :

BNA_M

ClientSampleId :

C0245



Tot Ion:163 Resp: 115939

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.7 8.2 12.4

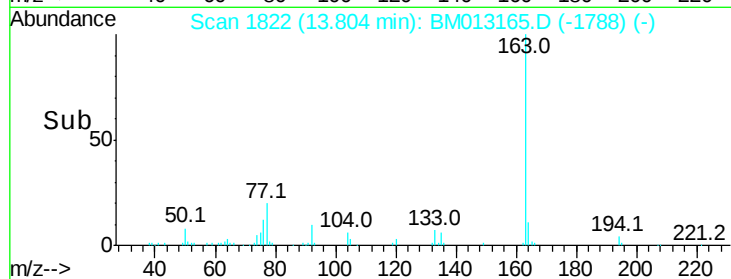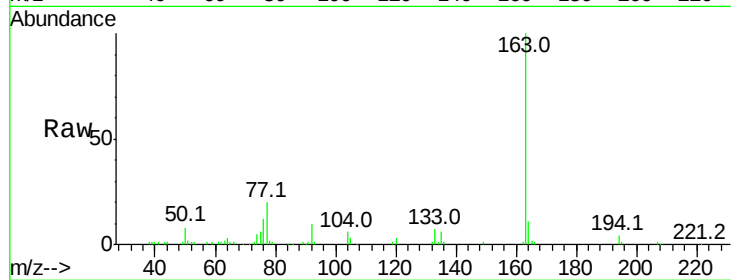

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

