

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM120417\
 Data File : BM013171.D
 Acq On : 04 Dec 2017 17:48
 Operator : SJ/JU
 Sample : I6646-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0261

Quant Time: Dec 05 05:08:14 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 05 04:53:13 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	302423	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	1313451	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	787836	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	1835335	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1862911	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	1512333	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	11295	1.85	ng/uL	0.00
5) Phenol-d5	6.88	99	293638	11.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	185870	12.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	242372	11.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	234353	10.48	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	131926	12.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	130010	11.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	251177	10.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	178146	8.44	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	818605	11.68	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1053622	12.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	108660	8.92	ng/ul	0.00
57) Fluorene-d10	15.34	176	739070	12.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	94965	8.23	ng/ul	0.00
70) Anthracene-d10	17.19	188	1126122	12.25	ng/ul	0.00
76) Pyrene-d10	19.48	212	1249925	13.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	928937	12.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.80	163	154414	2.303	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM120417\
Data File : BM013171.D
Acq On : 04 Dec 2017 17:48
Operator : SJ/JU
Sample : I6646-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0261

Quant Time: Dec 05 05:08:14 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 05 04:53:13 2017
Response via : Initial Calibration

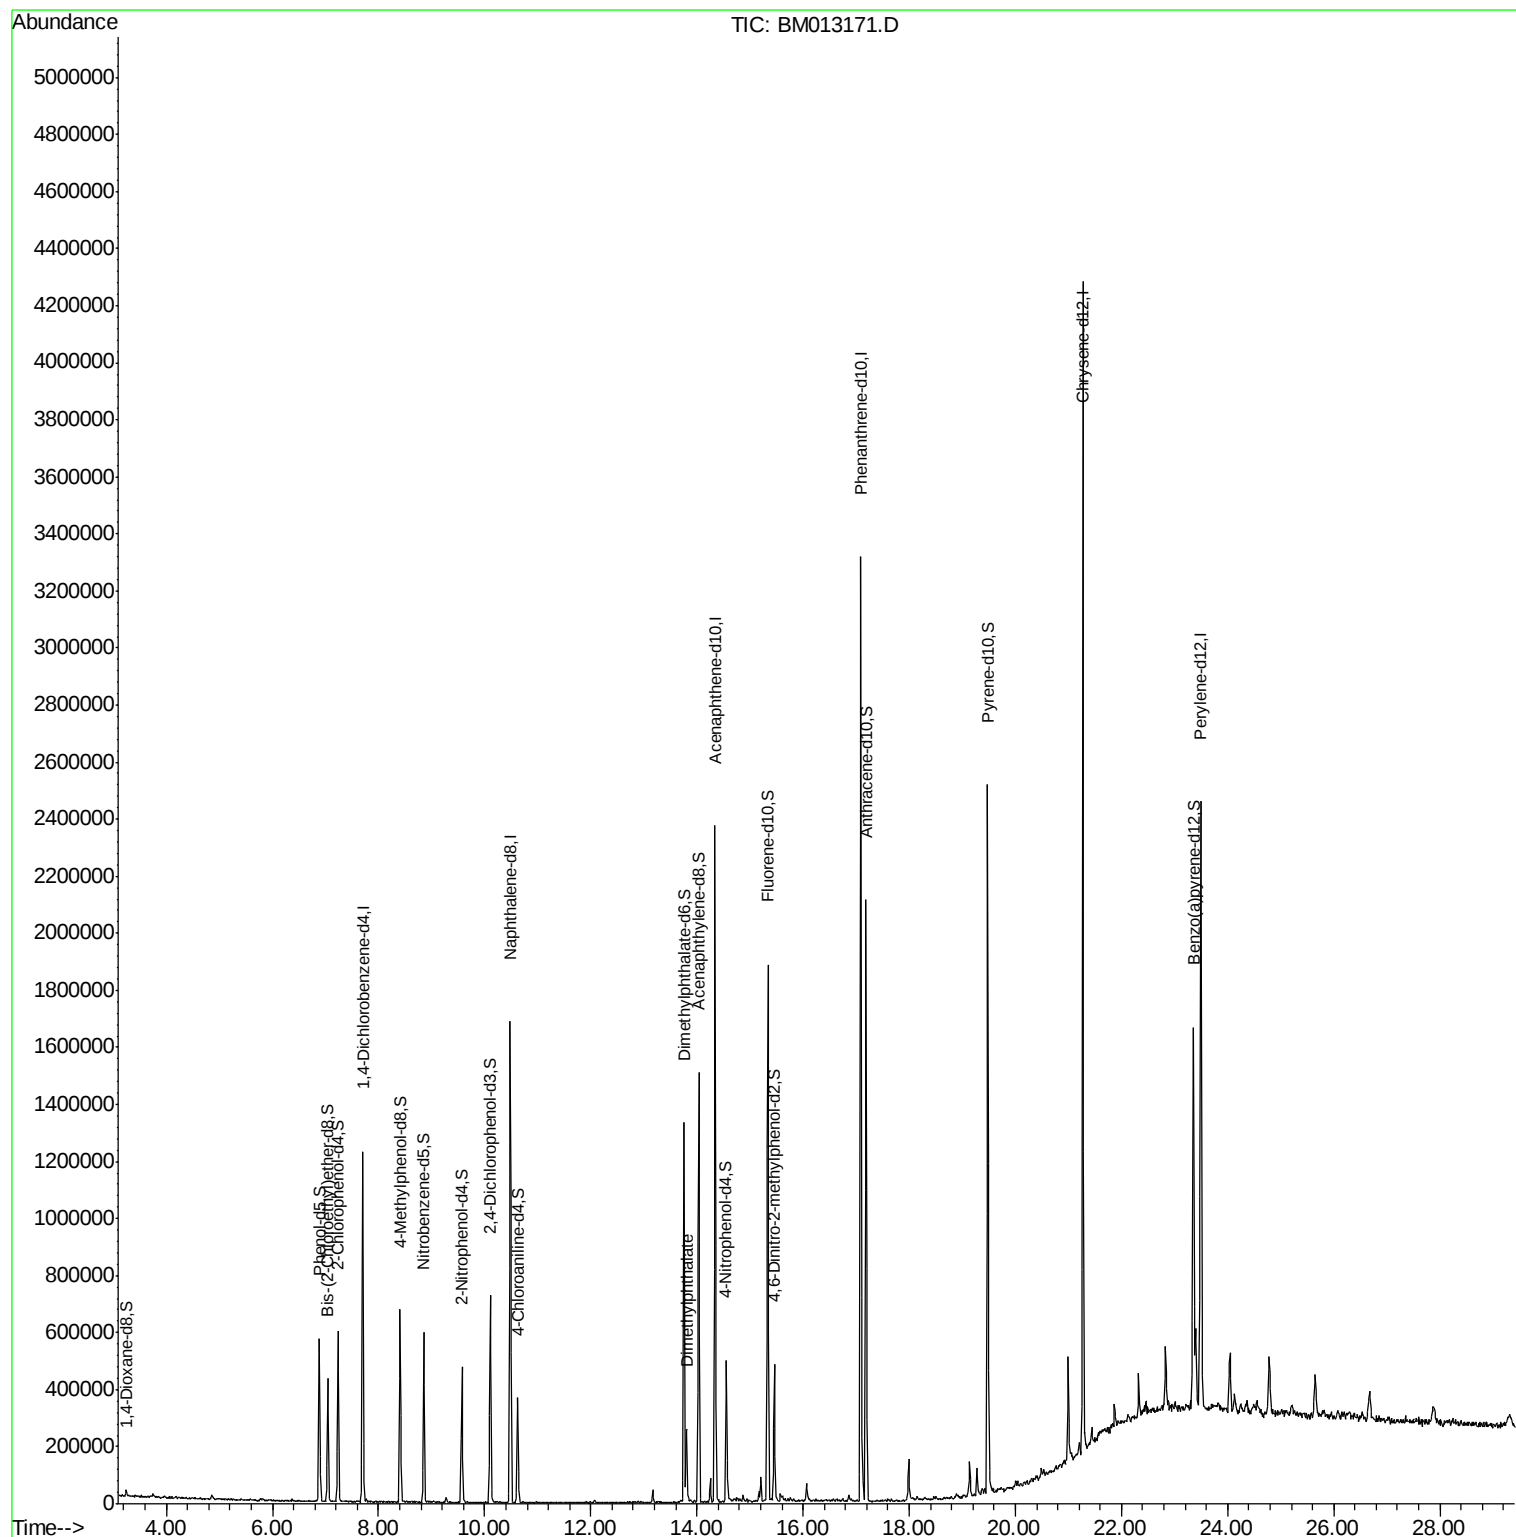

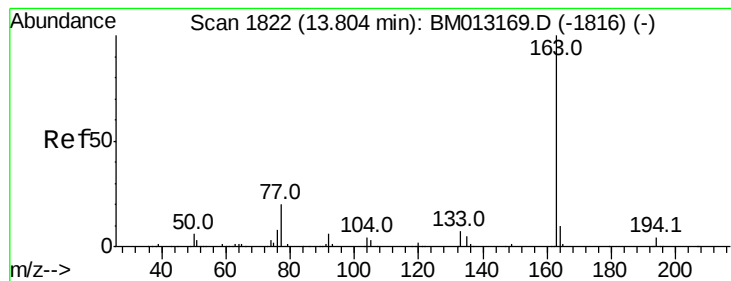

#44
 Dimethylphthalate
 Concen: 2.303 ng/ul
 RT: 13.80 min Scan# 1822
 Delta R.T. 0.00 min
 Lab File: BM013171.D
 Acq: 04 Dec 2017 17:48

Instrument :
 BNA_M
 ClientSampleId :
 C0261

Tot Ion:163 Resp: 154414
 Ion Ratio Lower Upper
 163 100
 194 3.8 3.5 5.3
 164 9.5 8.2 12.4

