
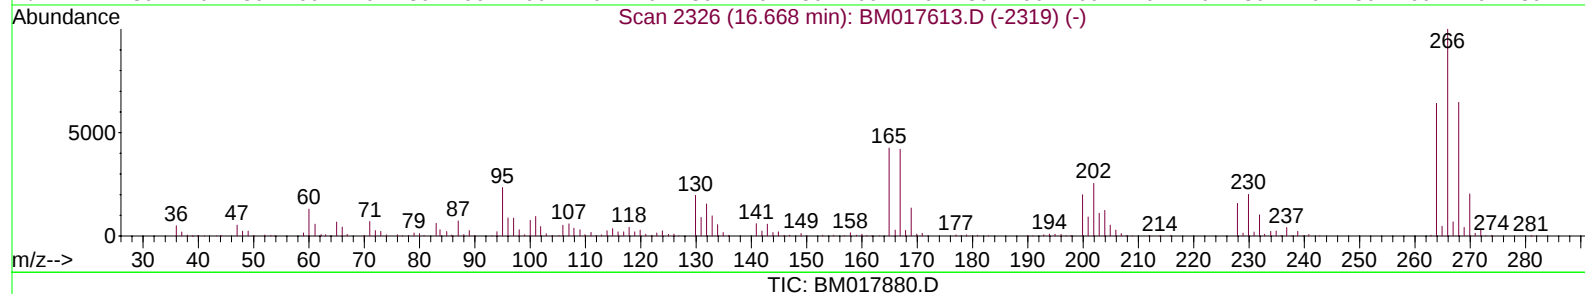
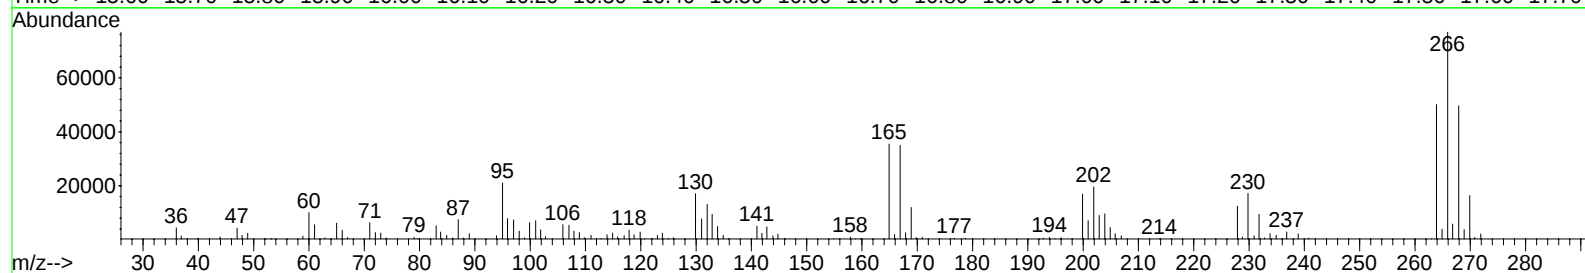


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM120418\
Data File : BM017880.D
Acq On : 03 Dec 2018 18:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 09:58:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

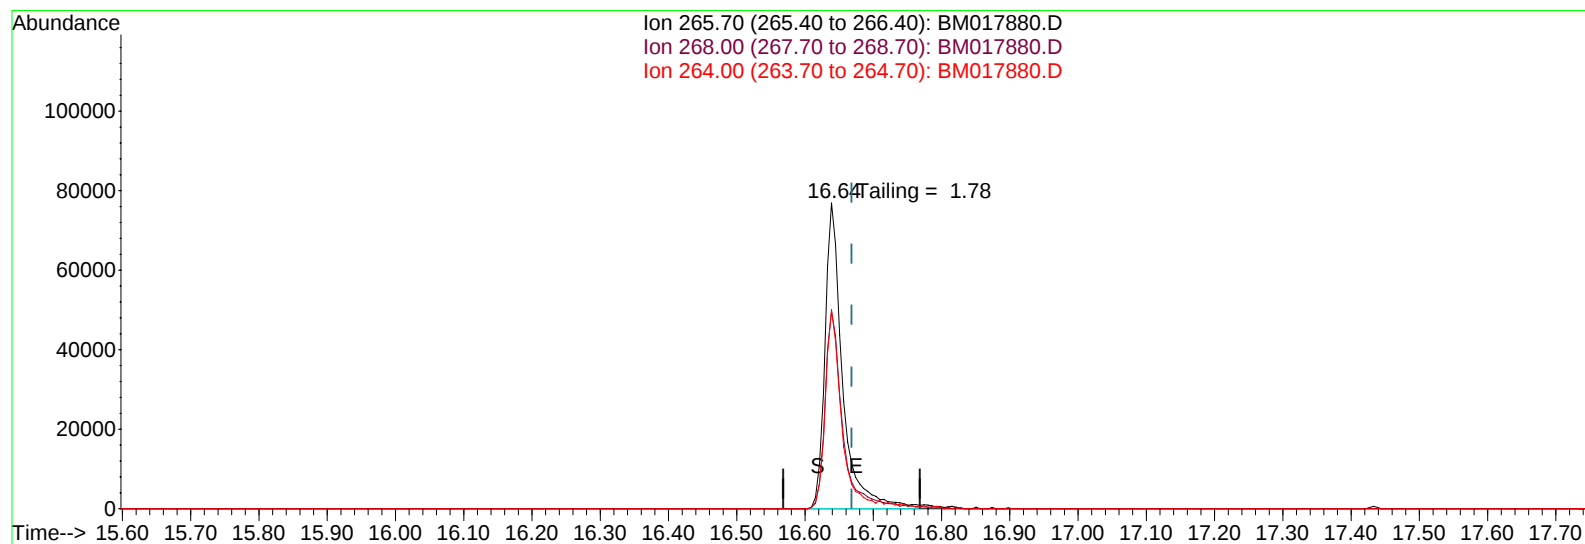

(70) Pentachlorophenol (C)




16.639min (-0.029) 0.00ng

response 137470

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	64.52
264.00	64.10	65.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM120418\
Data File : BM017880.D
Acq On : 03 Dec 2018 18:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 09:58:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

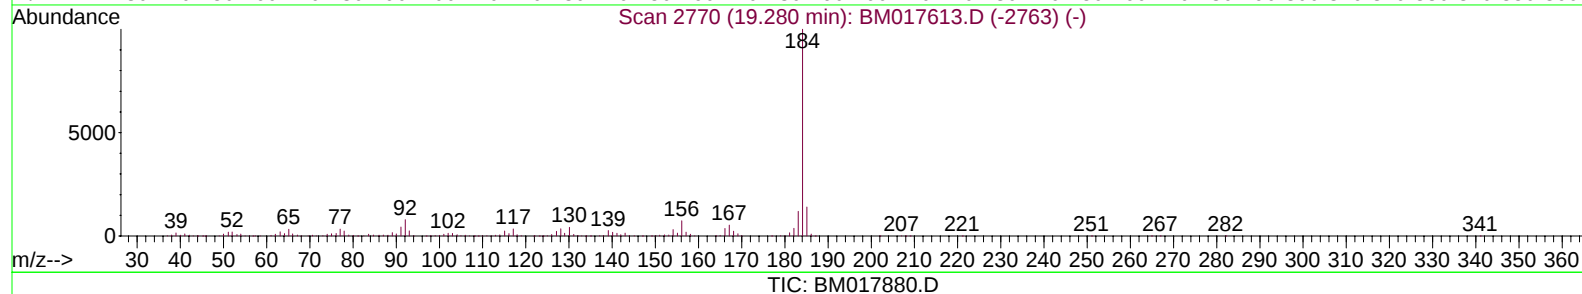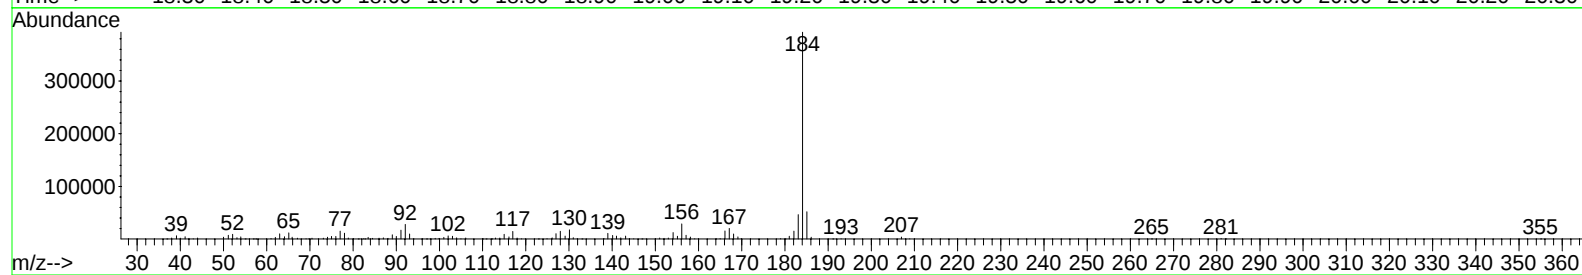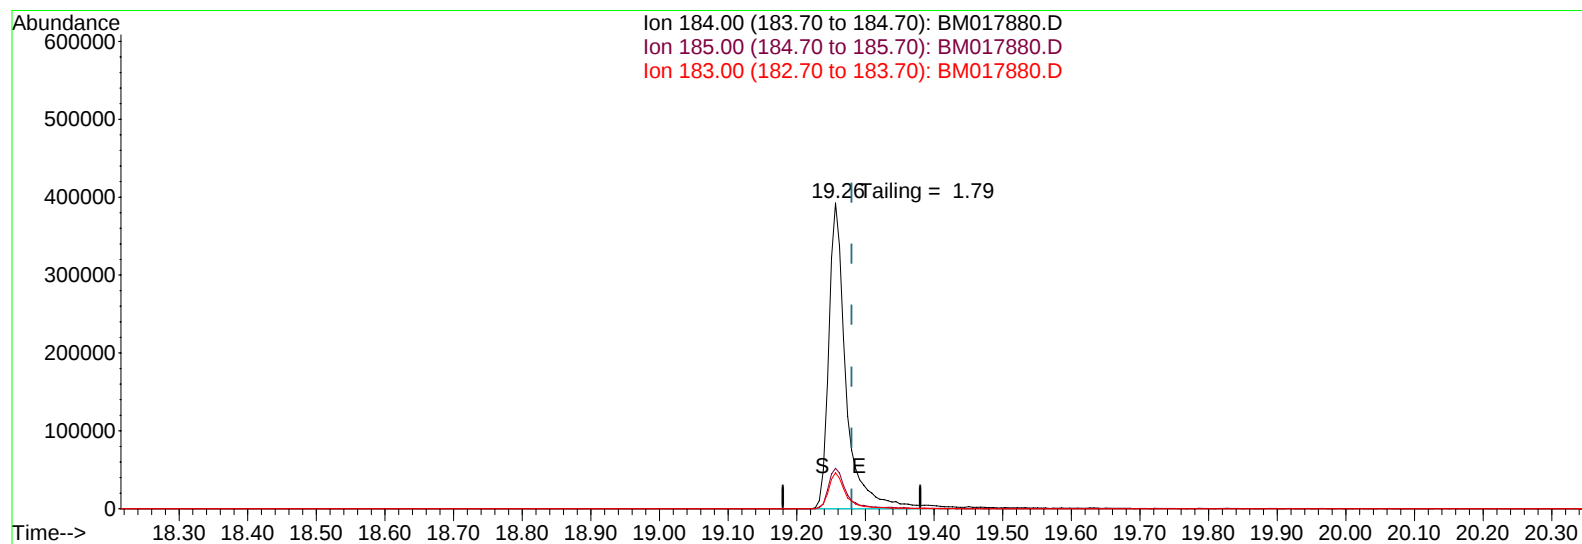

(77) Benzidine

19.256min (-0.024) 0.00ng

response 678582

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.25
183.00	11.90	11.80
0.00	0.00	0.00