

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120418\
 Data File : BM017900.D
 Acq On : 04 Dec 2018 11:38
 Operator : JU/SJ
 Sample : J6042-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB4Y7

Quant Time: Dec 04 12:18:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 04 00:18:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	222425	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	973642	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	530712	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	1128287	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	998783	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	947398	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	0.00	176	0d	0.00	ng/ul	
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
78) Pyrene-d10	0.00	212	0d	0.00	ng/ul	
89) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
69) Phenanthrene	17.02	178	83062	1.287	ng/ul	97
76) Fluoranthene	19.05	202	132200	1.742	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120418\
Data File : BM017900.D
Acq On : 04 Dec 2018 11:38
Operator : JU/SJ
Sample : J6042-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB4Y7

Quant Time: Dec 04 12:18:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 04 00:18:53 2018
Response via : Initial Calibration

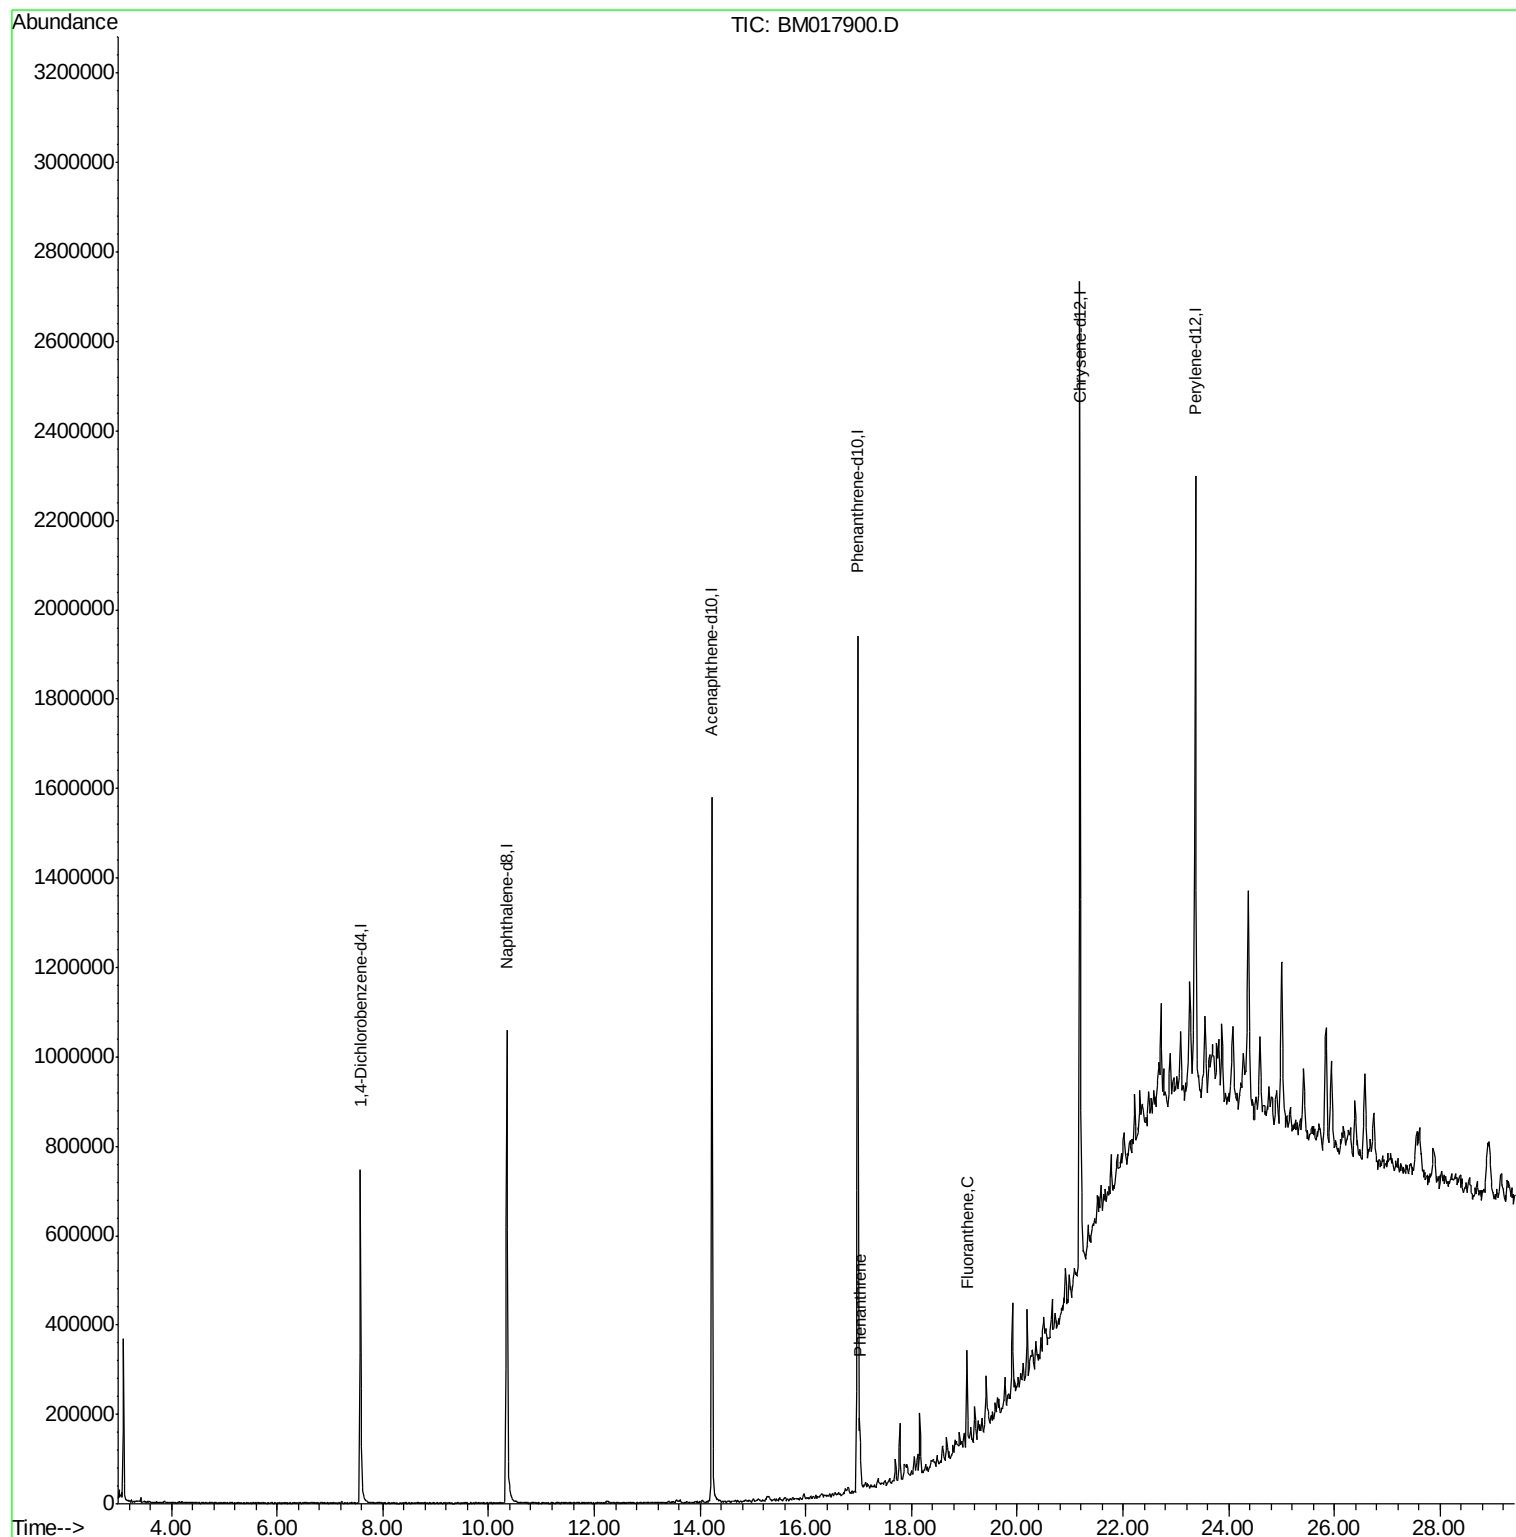

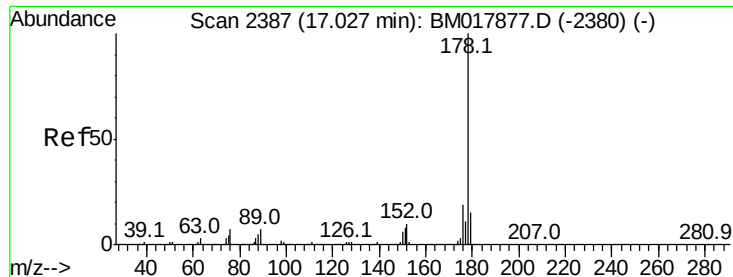

#69

Phenanthrene

Concen: 1.287 ng/ul

RT: 17.02 min Scan# 2386

Delta R.T. -0.01 min

Lab File: BM017900.D

Acq: 04 Dec 2018 11:38

Instrument :


BNA_M

ClientSampleId :

CB4Y7

Tot Ion:178 Resp: 83062

Ion	Ratio	Lower	Upper
178	100		
179	15.6	11.8	17.8
176	20.4	15.0	22.6



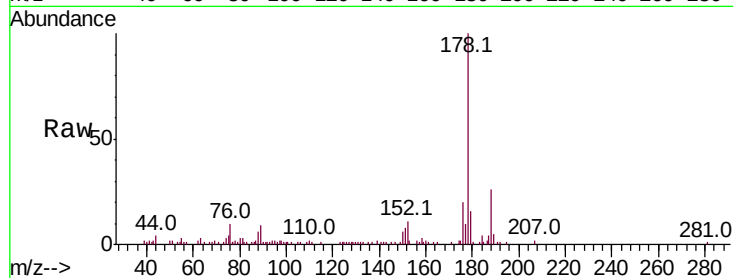


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

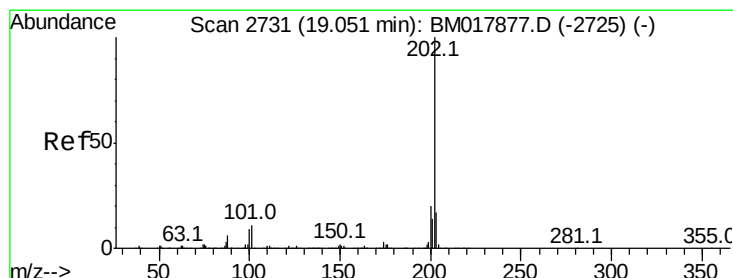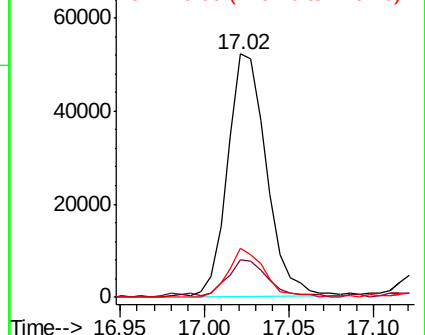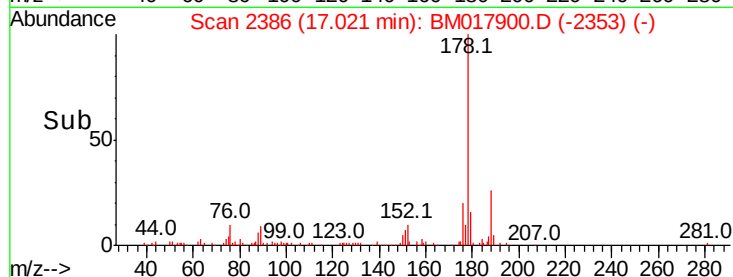

#76

Fluoranthene

Concen: 1.742 ng/ul

RT: 19.05 min Scan# 2731


Delta R.T. -0.00 min

Lab File: BM017900.D

Acq: 04 Dec 2018 11:38

Tgt Ion:202 Resp: 132200

Ion	Ratio	Lower	Upper
202	100		
101	9.5	8.4	12.6
100	8.2	6.6	9.8

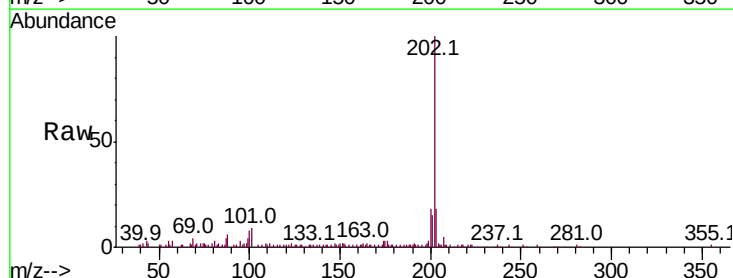

Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

