


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM120418\
 Data File : BM017880.D
 Acq On : 03 Dec 2018 18:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

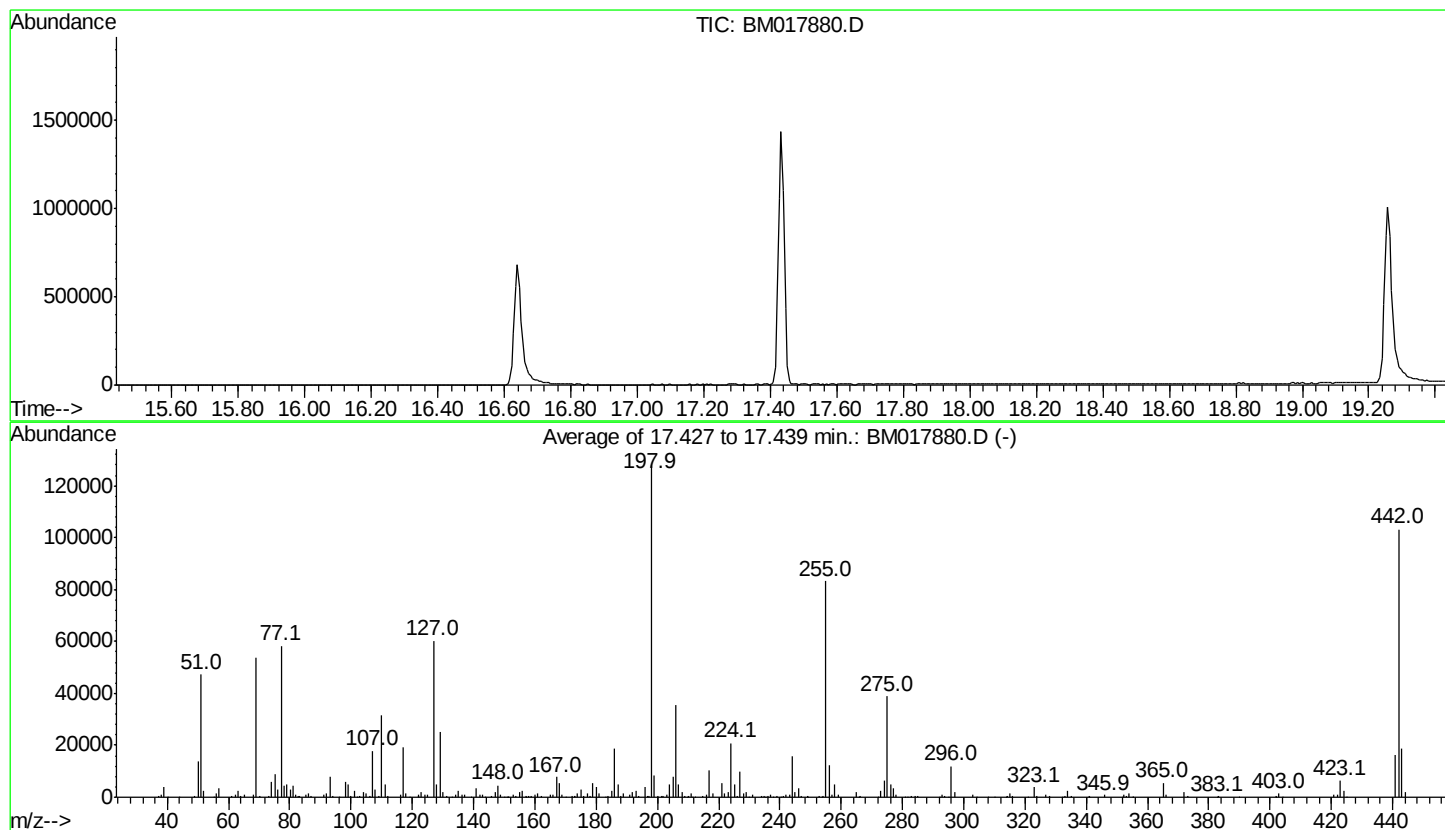

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	47274	PASS
68	69	0.00	2	1.7	931	PASS
69	198	0.00	100	42.0	53661	PASS
70	69	0.00	2	0.6	310	PASS
127	198	10	80	47.2	60280	PASS
197	198	0.00	2	0.5	682	PASS
198	198	100	100	100.0	127730	PASS
199	198	5	9	6.5	8315	PASS
275	198	10	60	30.4	38810	PASS
365	198	1	100	4.4	5615	PASS
441	198	0.01	100	12.7	16203	PASS
442	198	50	100	80.7	103090	PASS
443	442	15	24	18.3	18890	PASS