

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120420\
 Data File : BM028030.D
 Acq On : 04 Dec 2020 14:52
 Operator : JU/CG
 Sample : PB133233BL
 Misc : MDL-WATER-BL-02
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	44	48	62	rVB	72083	101086	2.54%	0.208%
2	3.934	123	127	144	rBV	903742	1399794	35.24%	2.886%
3	4.293	184	188	194	rBV	13497	20795	0.52%	0.043%
4	4.540	225	230	234	rBV6	2608	4217	0.11%	0.009%
5	5.381	369	373	380	rVB4	3049	5551	0.14%	0.011%
6	7.422	712	720	732	rBV	1023392	1595038	40.16%	3.289%
7	7.598	741	750	762	rBV	781111	1228679	30.93%	2.534%
8	7.810	778	786	796	rBV	1045736	1661291	41.83%	3.426%
9	8.292	860	868	876	rBV	785591	1267332	31.91%	2.613%
10	8.992	978	987	998	rBV	1182837	1864544	46.94%	3.845%
11	9.469	1059	1068	1082	rBV	894999	1489906	37.51%	3.072%
12	10.192	1183	1191	1199	rBV	696991	1160673	29.22%	2.393%
13	10.733	1275	1283	1295	rBV	1129066	1862303	46.89%	3.840%
14	11.128	1342	1350	1357	rVB	973376	1701980	42.85%	3.510%
15	11.251	1363	1371	1382	rBV	1094301	1889102	47.56%	3.895%
16	12.692	1611	1616	1621	rVB	17726	28267	0.71%	0.058%
17	14.304	1884	1890	1896	rBV	1810256	2404501	60.54%	4.958%
18	14.363	1896	1900	1904	rVB2	3942	6561	0.17%	0.014%
19	14.610	1935	1942	1950	rBV	2110968	2994091	75.38%	6.174%
20	14.910	1986	1993	2000	rBV	1395545	2052796	51.68%	4.233%
21	15.074	2014	2021	2039	rBV	805142	1199270	30.19%	2.473%
22	15.304	2056	2060	2063	rVB4	6324	7147	0.18%	0.015%
23	15.892	2153	2160	2167	rBV	2531145	3562979	89.70%	7.347%
24	15.992	2171	2177	2192	rBV	746450	987901	24.87%	2.037%
25	16.127	2196	2200	2204	rVB2	29335	38889	0.98%	0.080%
26	16.621	2278	2284	2287	rBV5	2727	5235	0.13%	0.011%
27	16.662	2287	2291	2296	rVB4	10895	13212	0.33%	0.027%
28	17.415	2413	2419	2424	rBV2	4661	7831	0.20%	0.016%
29	17.627	2449	2455	2462	rBV	1518116	2161331	54.41%	4.457%
30	17.727	2465	2472	2489	rVB	2586190	3637324	91.58%	7.500%
31	19.615	2790	2793	2797	rBV	26566	33530	0.84%	0.069%
32	19.868	2832	2836	2841	rBV	28746	42852	1.08%	0.088%
33	19.980	2849	2855	2861	rBV	3004460	3971946	100.00%	8.190%
34	21.733	3148	3153	3161	rBV	1727692	2161705	54.42%	4.458%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120420\
Data File : BM028030.D
Acq On : 04 Dec 2020 14:52
Operator : JU/CG
Sample : PB133233BL
Misc : MDL-WATER-BL-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
Title : SVOA CALIBRATION

35	23.986	3529	3536	3546	rVB	1930176	3863451	97.27%	7.967%
36	24.138	3556	3562	3569	rVB	1054667	2062577	51.93%	4.253%


Sum of corrected areas: 48495687

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120420\
Data File : BM028030.D
Acq On : 04 Dec 2020 14:52
Operator : JU/CG
Sample : PB133233BL
Misc : MDL-WATER-BL-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK233

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

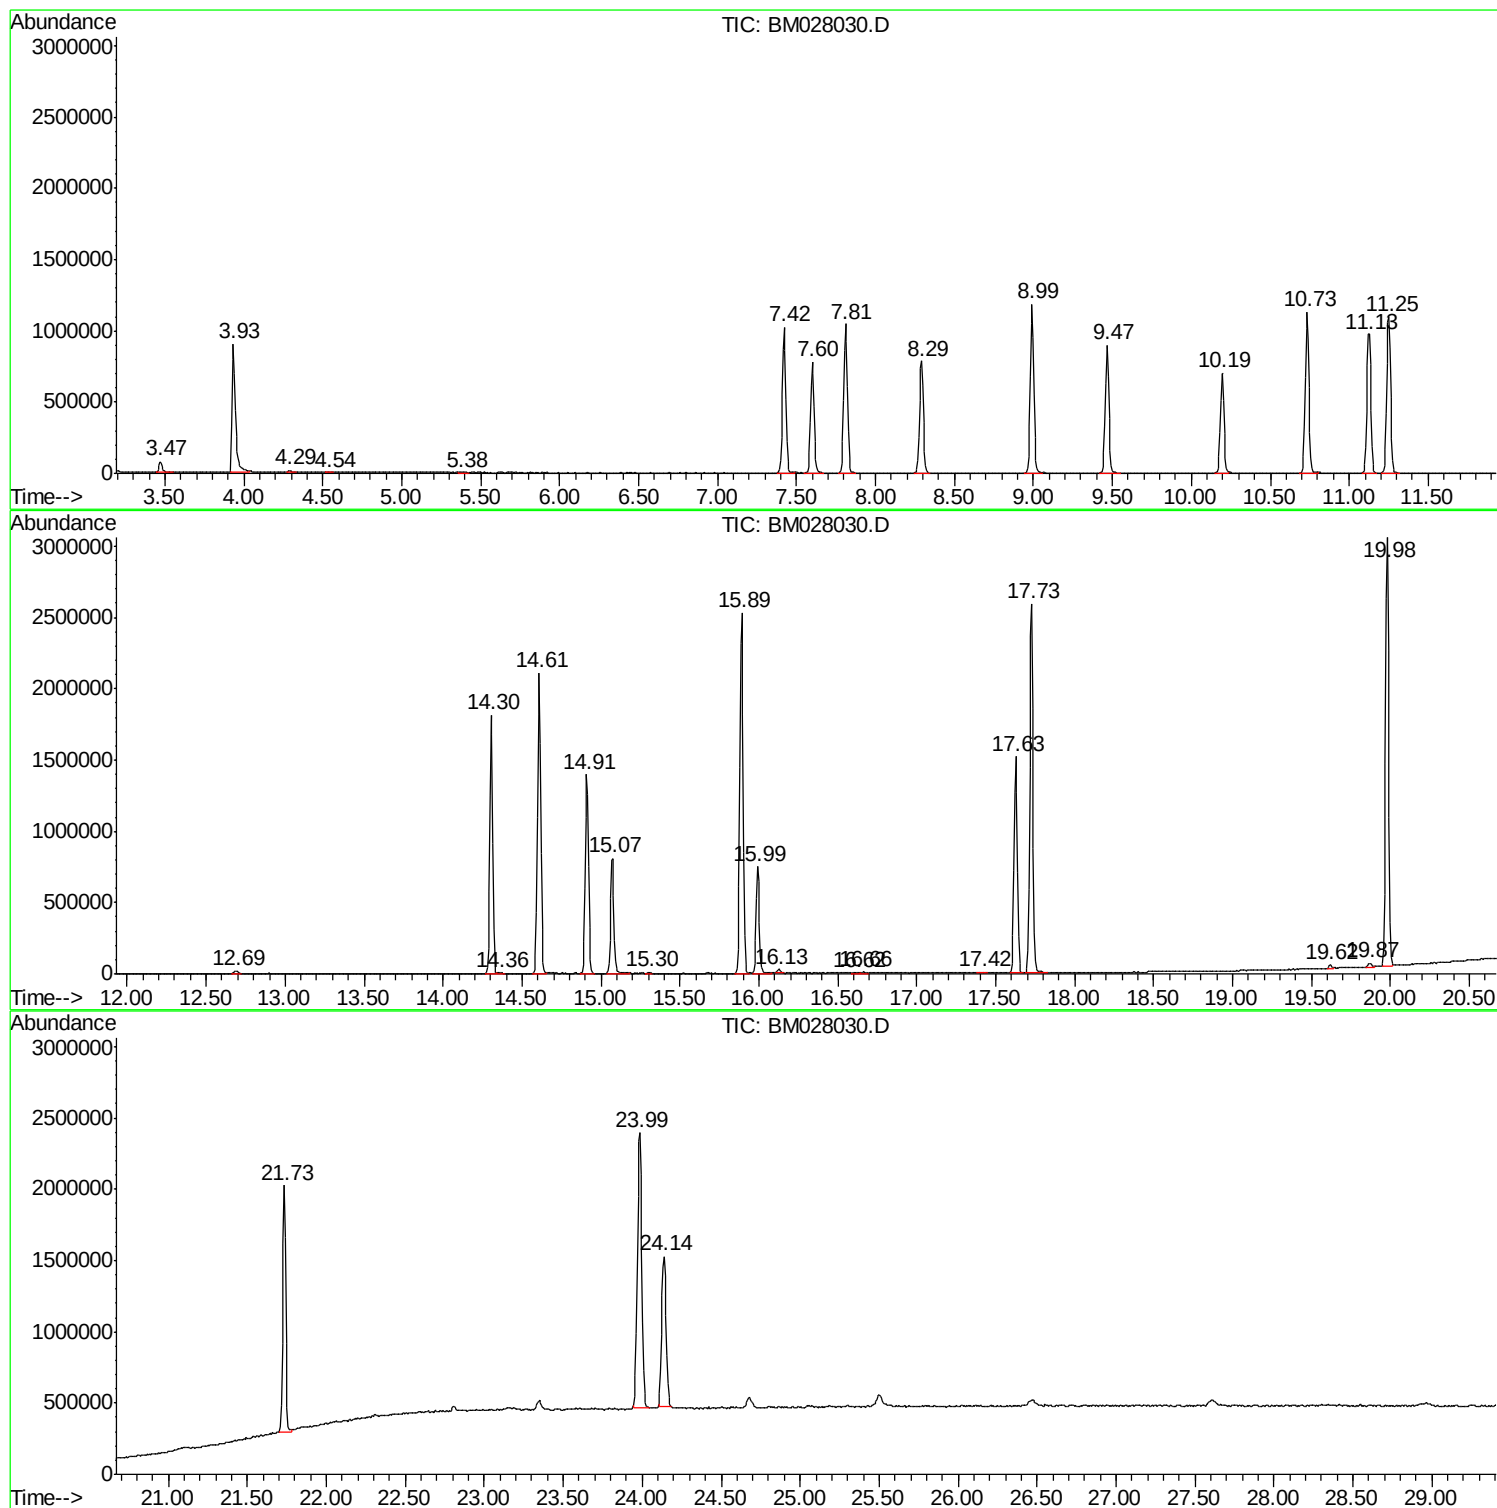

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120420\
Data_File : BM028030.D
Acq_On : 04 Dec 2020 14:522
Operator : JU/CGG
Sample : PB133233BLL
Misc : MDL-WATER-BL-022
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
SBLK233

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SEAM-EPA-BM120320.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
