
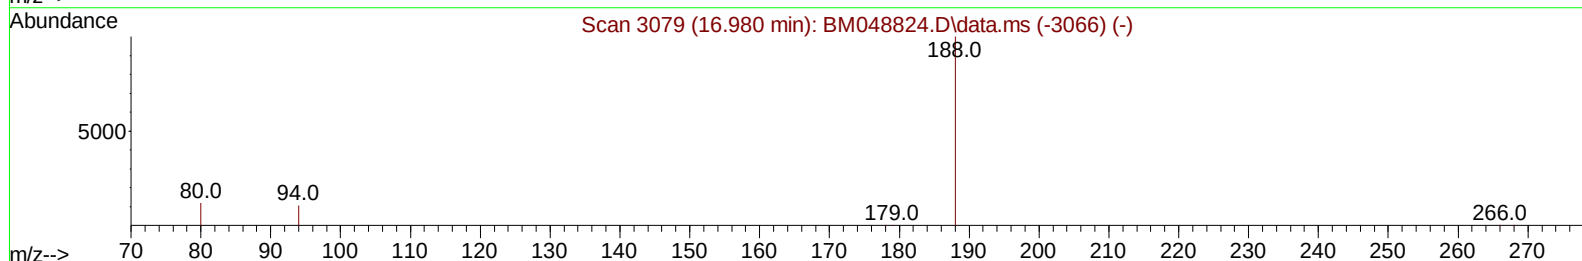
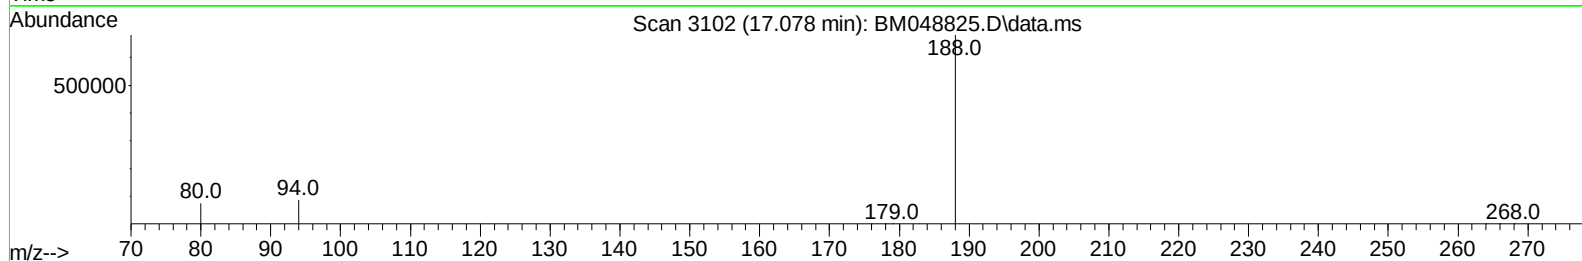


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120424\
Data File : BM048825.D
Acq On : 04 Dec 2024 09:40
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 14:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

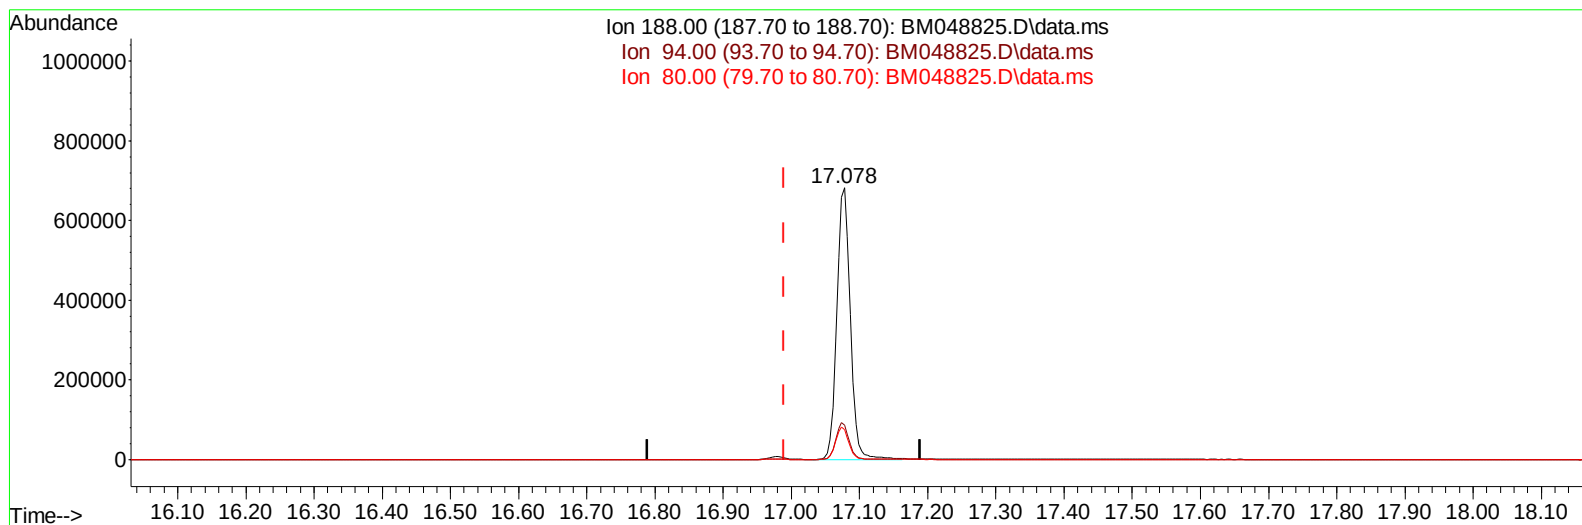

TIC: BM048825.D\data.ms

(13) Phenanthrene-d10 (I)




17.078min (+ 0.089) 0.40 ng/u1

response 932421

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.56
80.00	12.50	10.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120424\
Data File : BM048825.D
Acq On : 04 Dec 2024 09:40
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 14:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

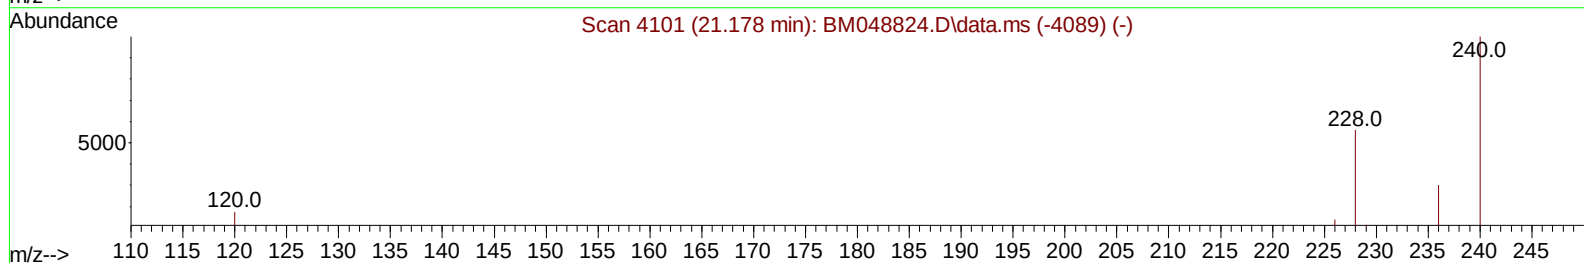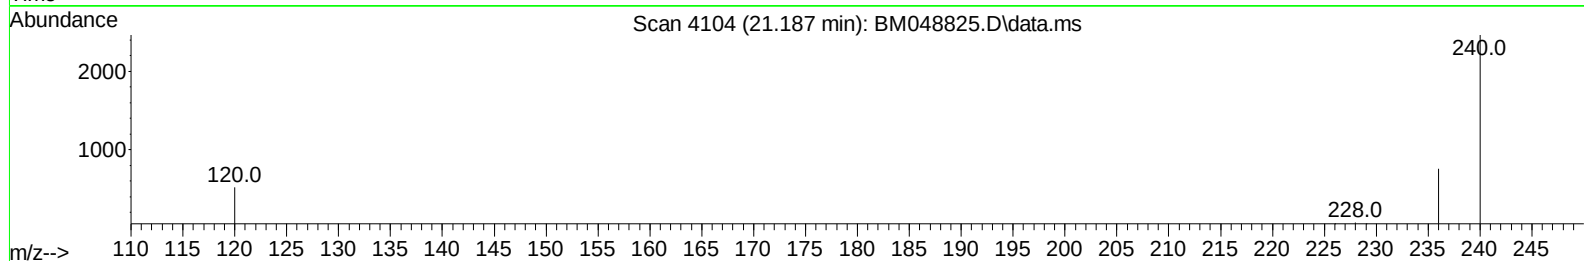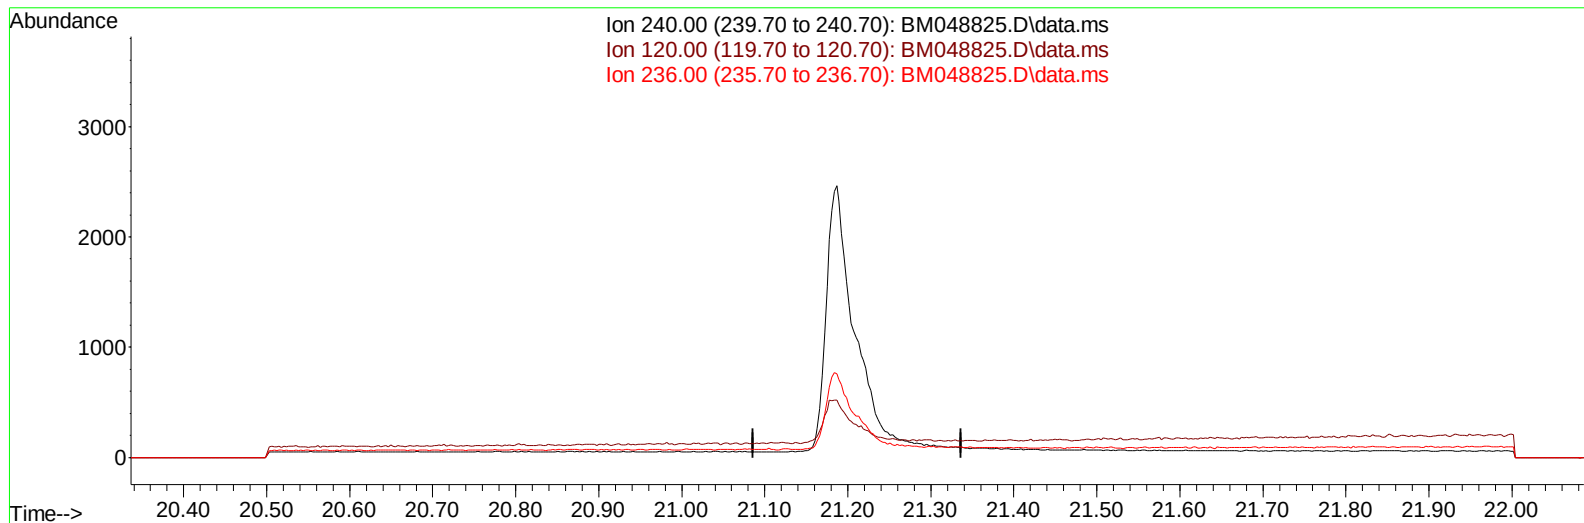

TIC: BM048825.D\data.ms

(17) Chrysene-d12




21.186min (-21.186) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120424\
Data File : BM048825.D
Acq On : 04 Dec 2024 09:40
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 14:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

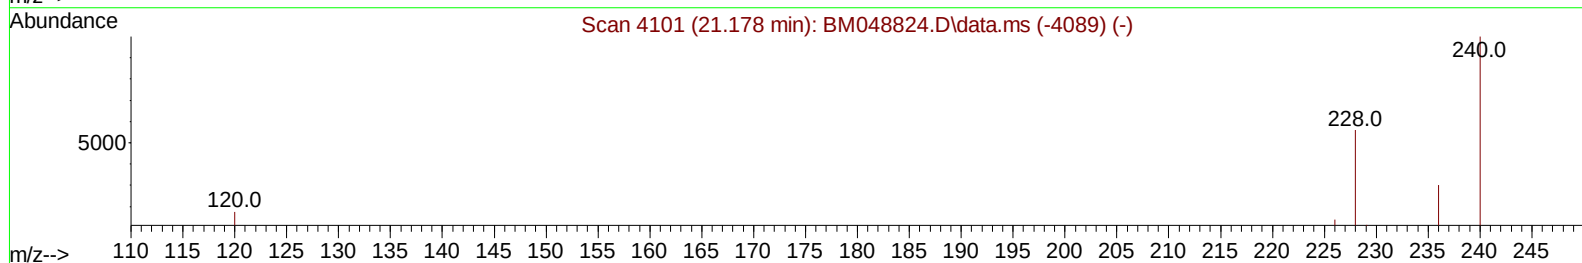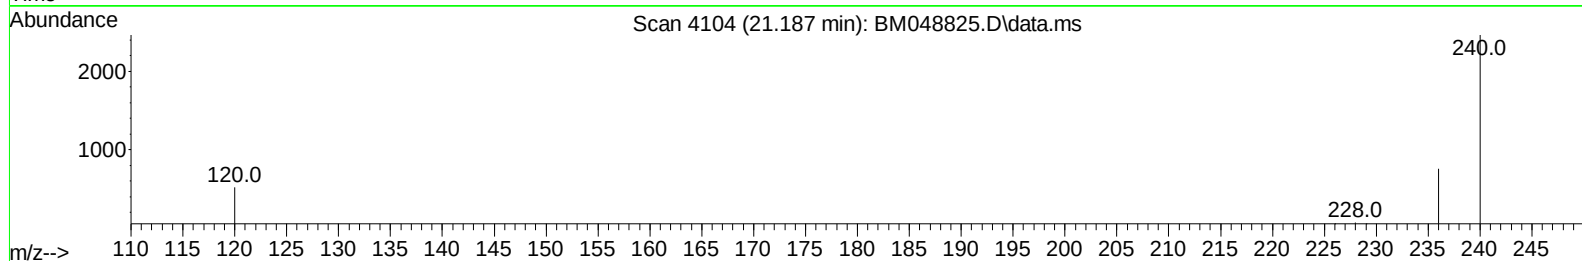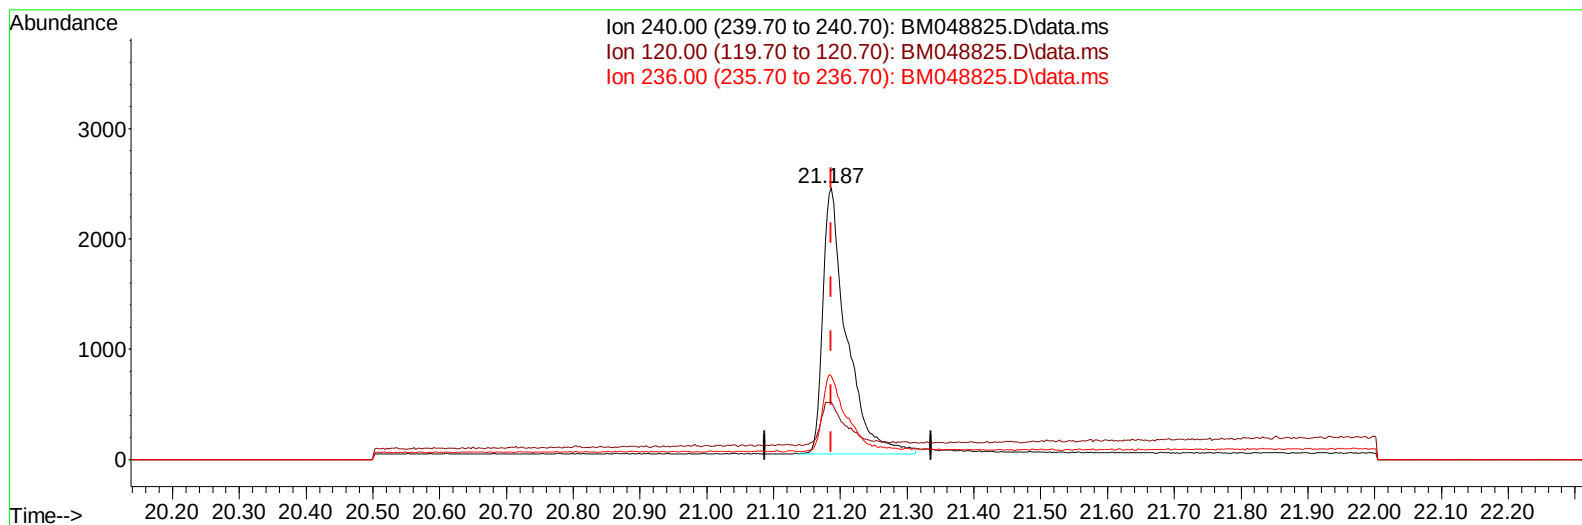

TIC: BM048825.D\data.ms

(17) Chrysene-d12




21.187min (+ 0.000) 0.40 ng/ul m

response 5896

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	21.20
236.00	32.10	30.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120424\
Data File : BM048825.D
Acq On : 04 Dec 2024 09:40
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 14:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

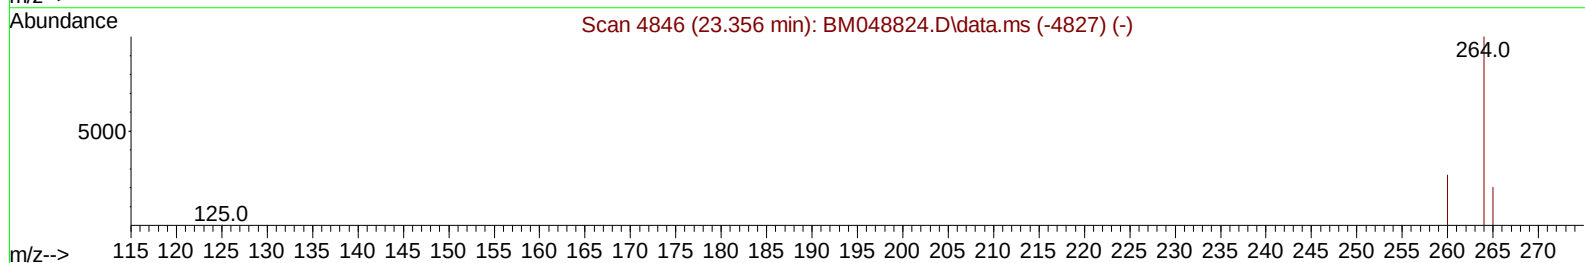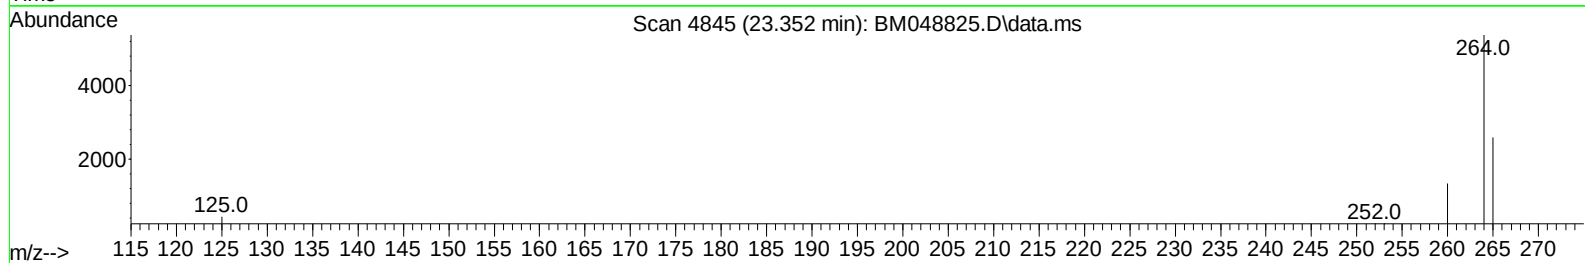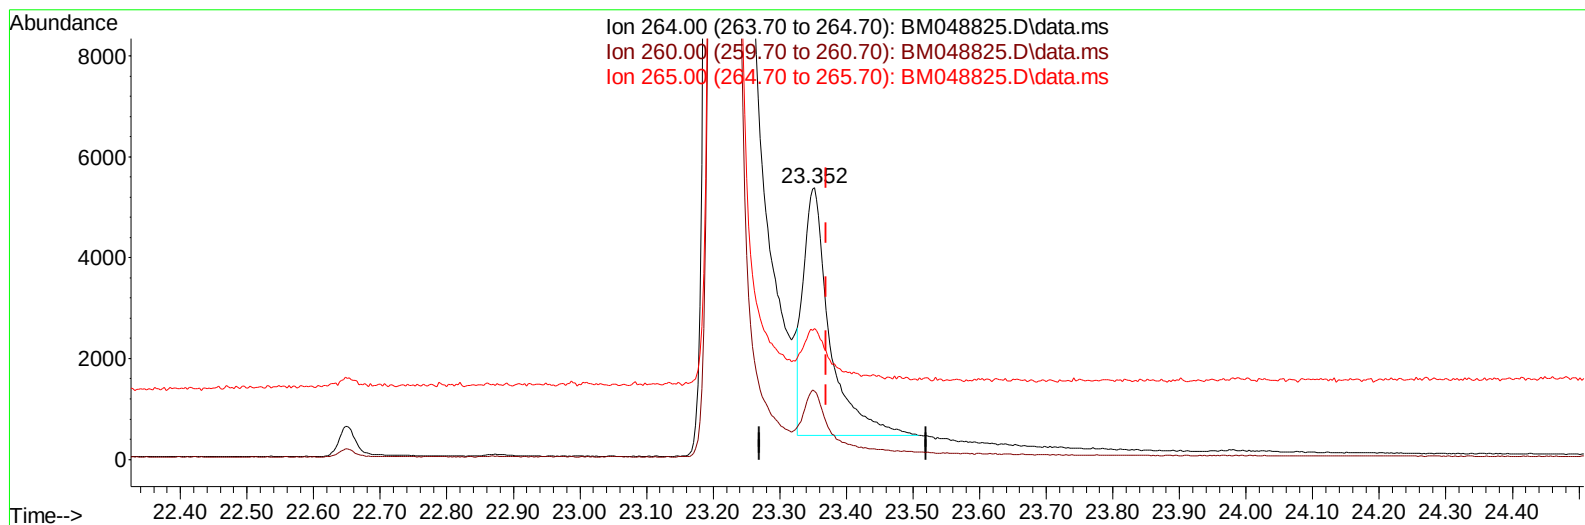

TIC: BM048825.D\data.ms

(23) Perylene-d12 (I)




23.352min (-0.017) 0.40 ng/u1

response 13629

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.20
265.00	78.50	48.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120424\
Data File : BM048825.D
Acq On : 04 Dec 2024 09:40
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 14:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

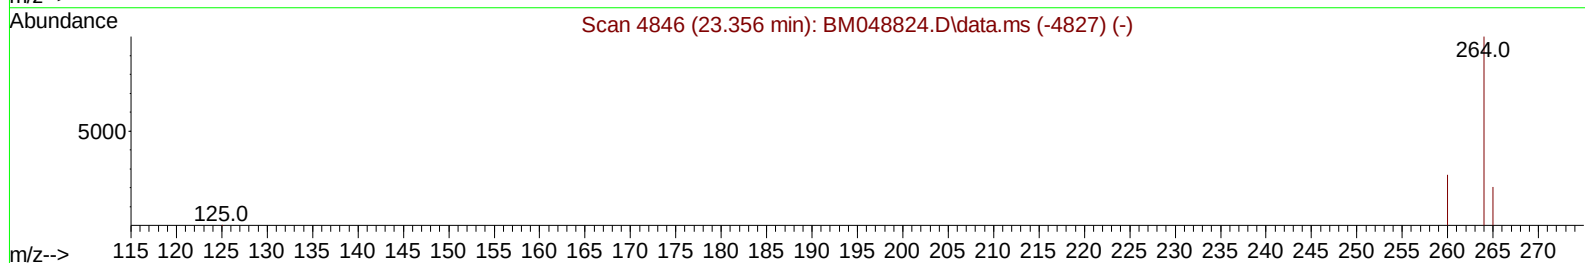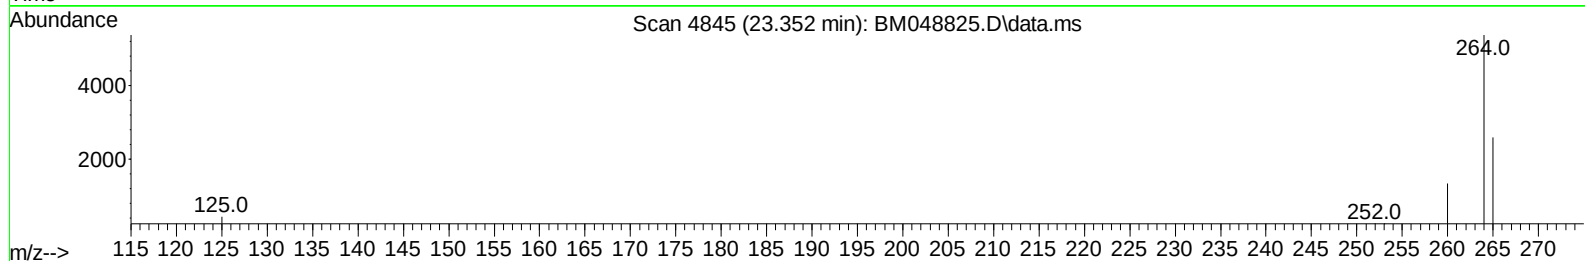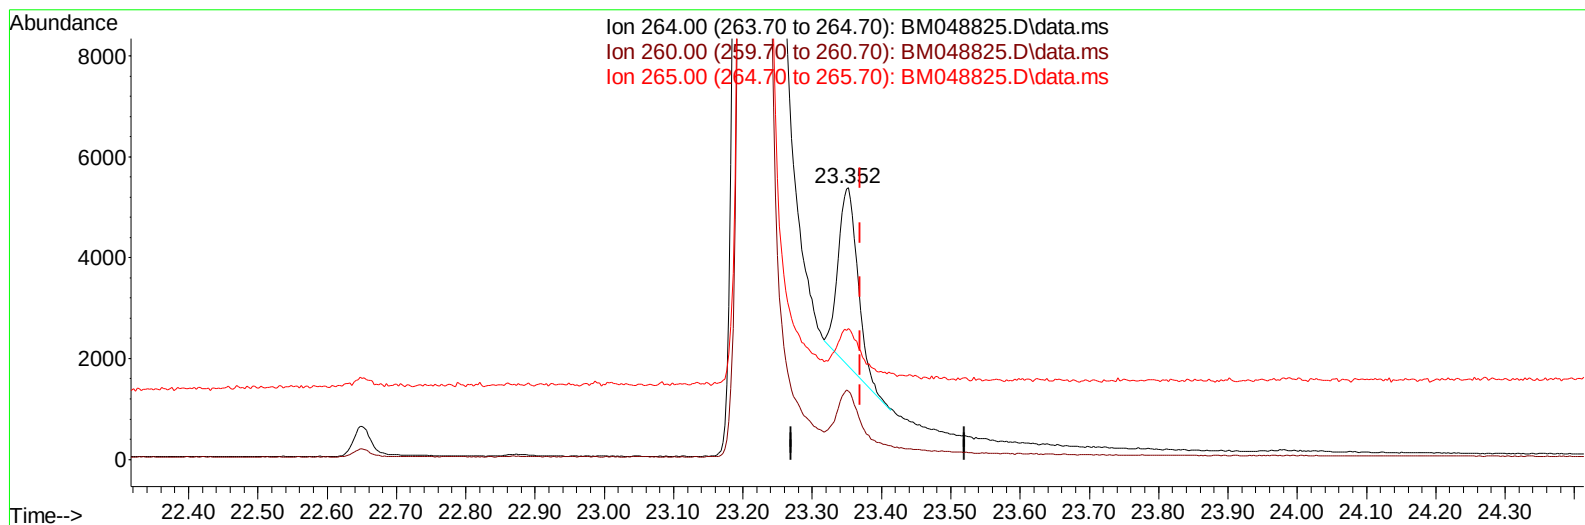

TIC: BM048825.D\data.ms

(23) Perylene-d12 (I)

23.352min (-0.017) 0.40 ng/ul m

response 6792

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.20
265.00	78.50	48.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120424\
 Data File : BM048825.D
 Acq On : 04 Dec 2024 09:40
 Operator : RC/JU
 Sample : PB165200BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 14:18:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 03 00:22:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.598	152	4291	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.365	136	11616	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.234	164	5964	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.977	188	11336m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.187	240	5896m	0.400	ng/ul	0.00
23) Perylene-d12	23.352	264	6792m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.168	96	28747	5.245	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.970	152	4942	0.353	ng/ul	0.00
18) Fluoranthene-d10	19.016	212	7788	0.428	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120424\
Data File : BM048825.D
Acq On : 04 Dec 2024 09:40
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 14:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

