

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM120517\
 Data File : BM013189.D
 Acq On : 05 Dec 2017 13:42
 Operator : SJ/JU
 Sample : I6647-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0286

Quant Time: Dec 05 16:23:34 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 05 16:20:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	244726	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1151713	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	737864	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	1730155	20.00	ng/ul	0.00
75) Chrysene-d12	21.28	240	1745806	20.00	ng/ul	0.00
83) Perylene-d12	23.51	264	1481933	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	23475	4.75	ng/uL	0.00
5) Phenol-d5	6.88	99	102599	4.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	292878	24.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	329656	19.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	209211	11.57	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	223215	24.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	237268	24.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	402371	19.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	260	0.01	ng/ul	-0.12
43) Dimethylphthalate-d6	13.76	166	1543382	23.51	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1866510	23.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	48575	4.26	ng/ul	0.00
57) Fluorene-d10	15.34	176	1311664	23.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	208253	19.13	ng/ul	0.00
70) Anthracene-d10	17.19	188	2117289	24.44	ng/ul	0.00
76) Pyrene-d10	19.49	212	2314408	26.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	1839962	24.38	ng/ul	0.00


Target Compounds					Ovalue	
33) 4-Chloro-3-methylphenol	11.78	107	33123	1.623	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM120517\
Data File : BM013189.D
Acq On : 05 Dec 2017 13:42
Operator : SJ/JU
Sample : I6647-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0286

Quant Time: Dec 05 16:23:34 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 05 16:20:21 2017
Response via : Initial Calibration

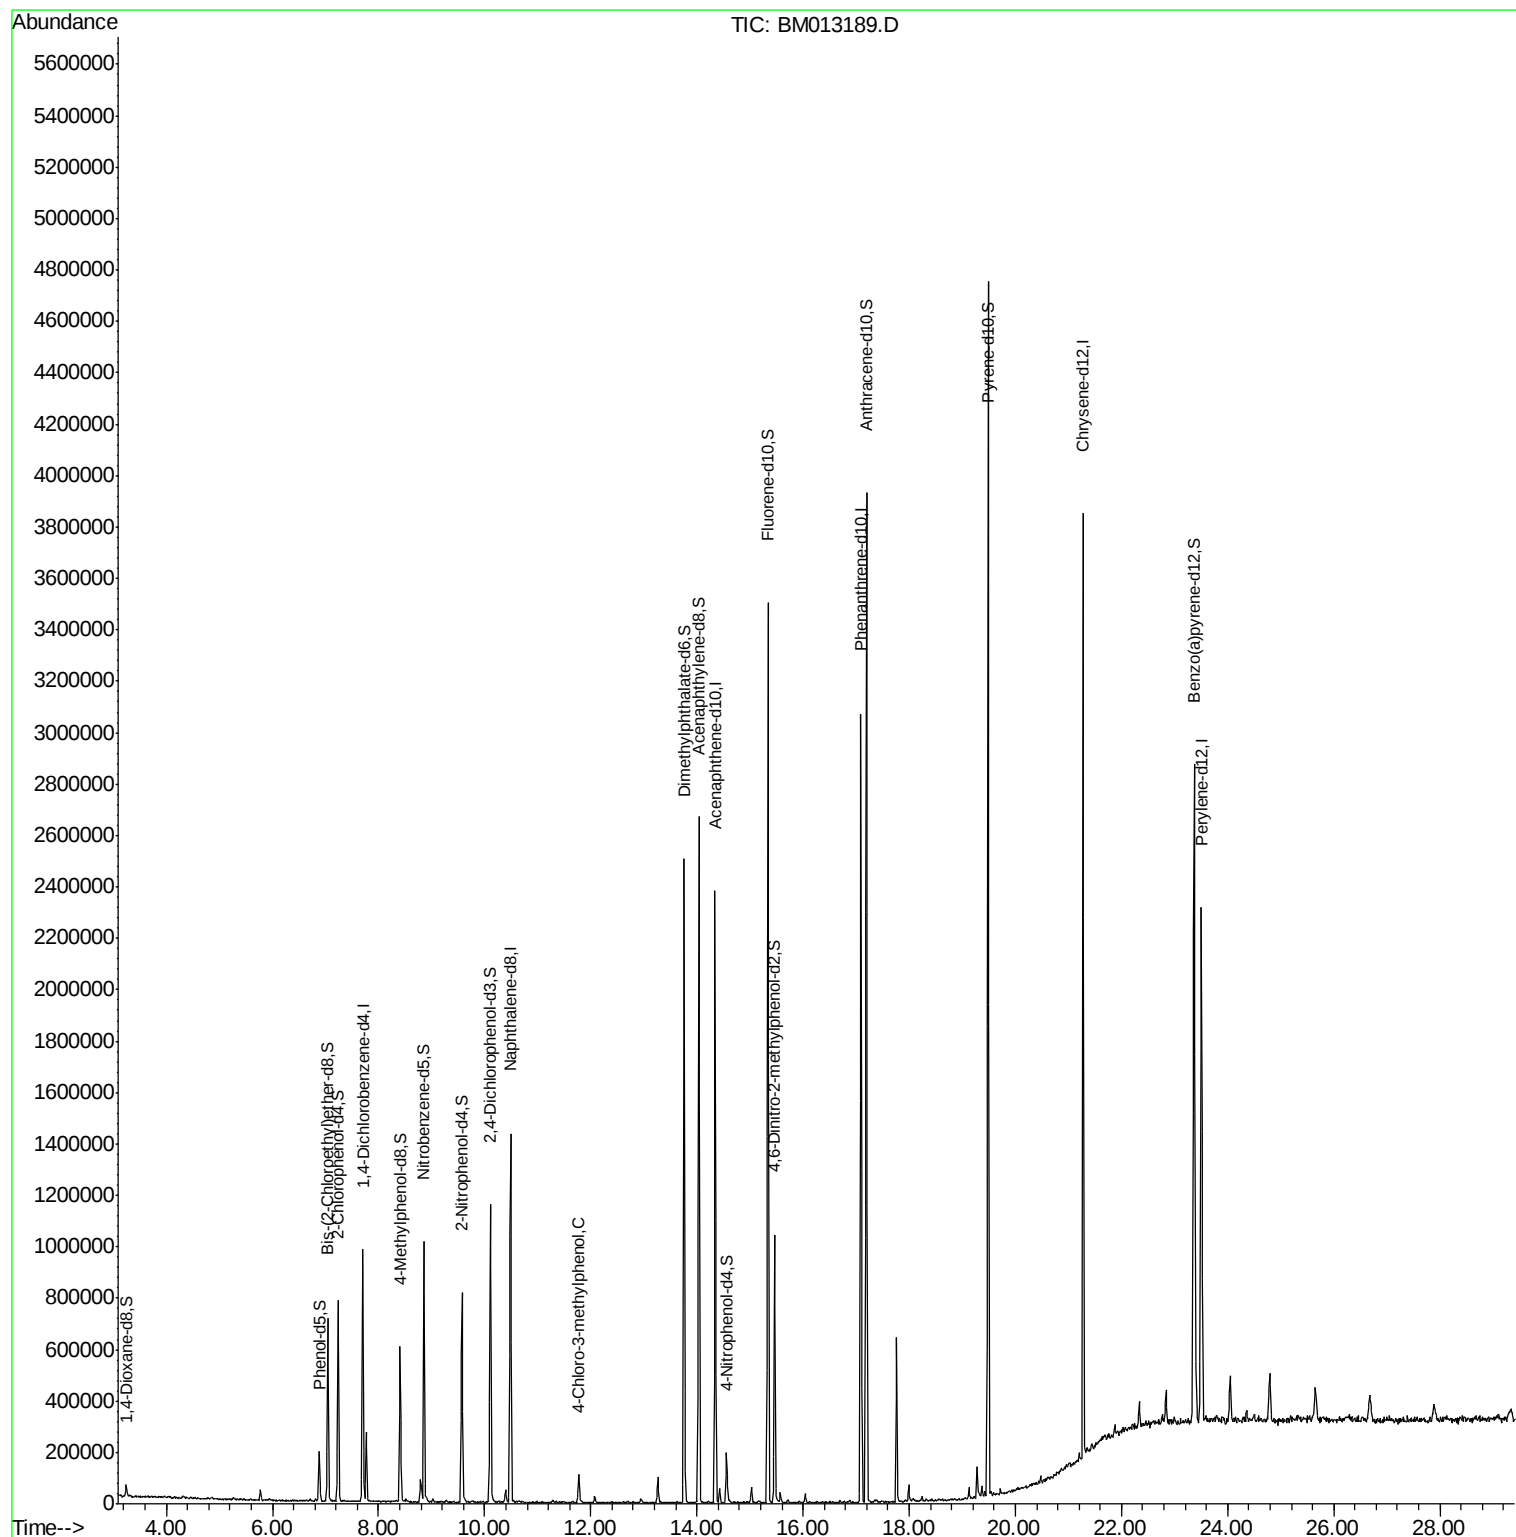

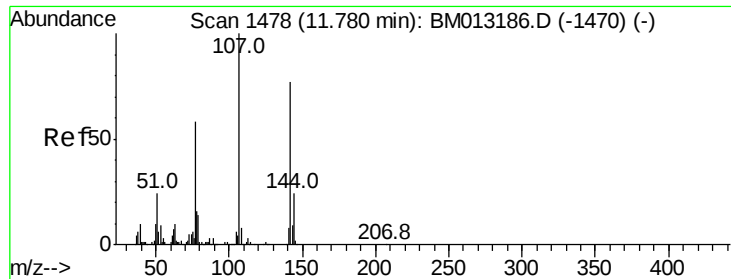

#33
 4-Chloro-3-methylphenol
 Concen: 1.623 ng/ul
 RT: 11.78 min Scan# 1478
 Delta R.T. 0.00 min
 Lab File: BM013189.D
 Acq: 05 Dec 2017 13:42

Instrument :
 BNA_M
 ClientSampleId :
 C0286

Tot Ion	Ratio	Lower	Upper
107	100		
144	26.7	20.4	30.6
142	79.2	60.5	90.7

