

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM120517\
 Data File : BM013194.D
 Acq On : 05 Dec 2017 18:19
 Operator : SJ/JU
 Sample : I6689-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHPP1

Manual Integrations
 APPROVED

Sohil
 12/6/2017 5:15:04 PM

Quant Time: Dec 06 01:49:20 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 06 01:31:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	259854	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	1136375	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	703952	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	1610213	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1445634	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	1125054	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	27948	5.33	ng/uL	0.00
5) Phenol-d5	6.88	99	109452	4.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	313426	24.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	348179	19.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	220311	11.47	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	237402	26.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	260828	27.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	431354	21.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	6498	0.36	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	1711360	27.32	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1941136	25.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	48476m	4.45	ng/ul	0.00
57) Fluorene-d10	15.34	176	1413090	26.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	241429	23.83	ng/ul	0.00
70) Anthracene-d10	17.19	188	2246692	27.86	ng/ul	0.00
76) Pyrene-d10	19.49	212	2319849	32.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	1668810	29.12	ng/ul	-0.01

Target Compounds				Ovalue
44) Dimethylphthalate	13.80	163	88415	1.476 ng/ul 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM120517\
Data File : BM013194.D
Acq On : 05 Dec 2017 18:19
Operator : SJ/JU
Sample : I6689-01
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
JHPP1

Quant Time: Dec 06 01:49:20 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 06 01:31:21 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/6/2017 5:15:04 PM

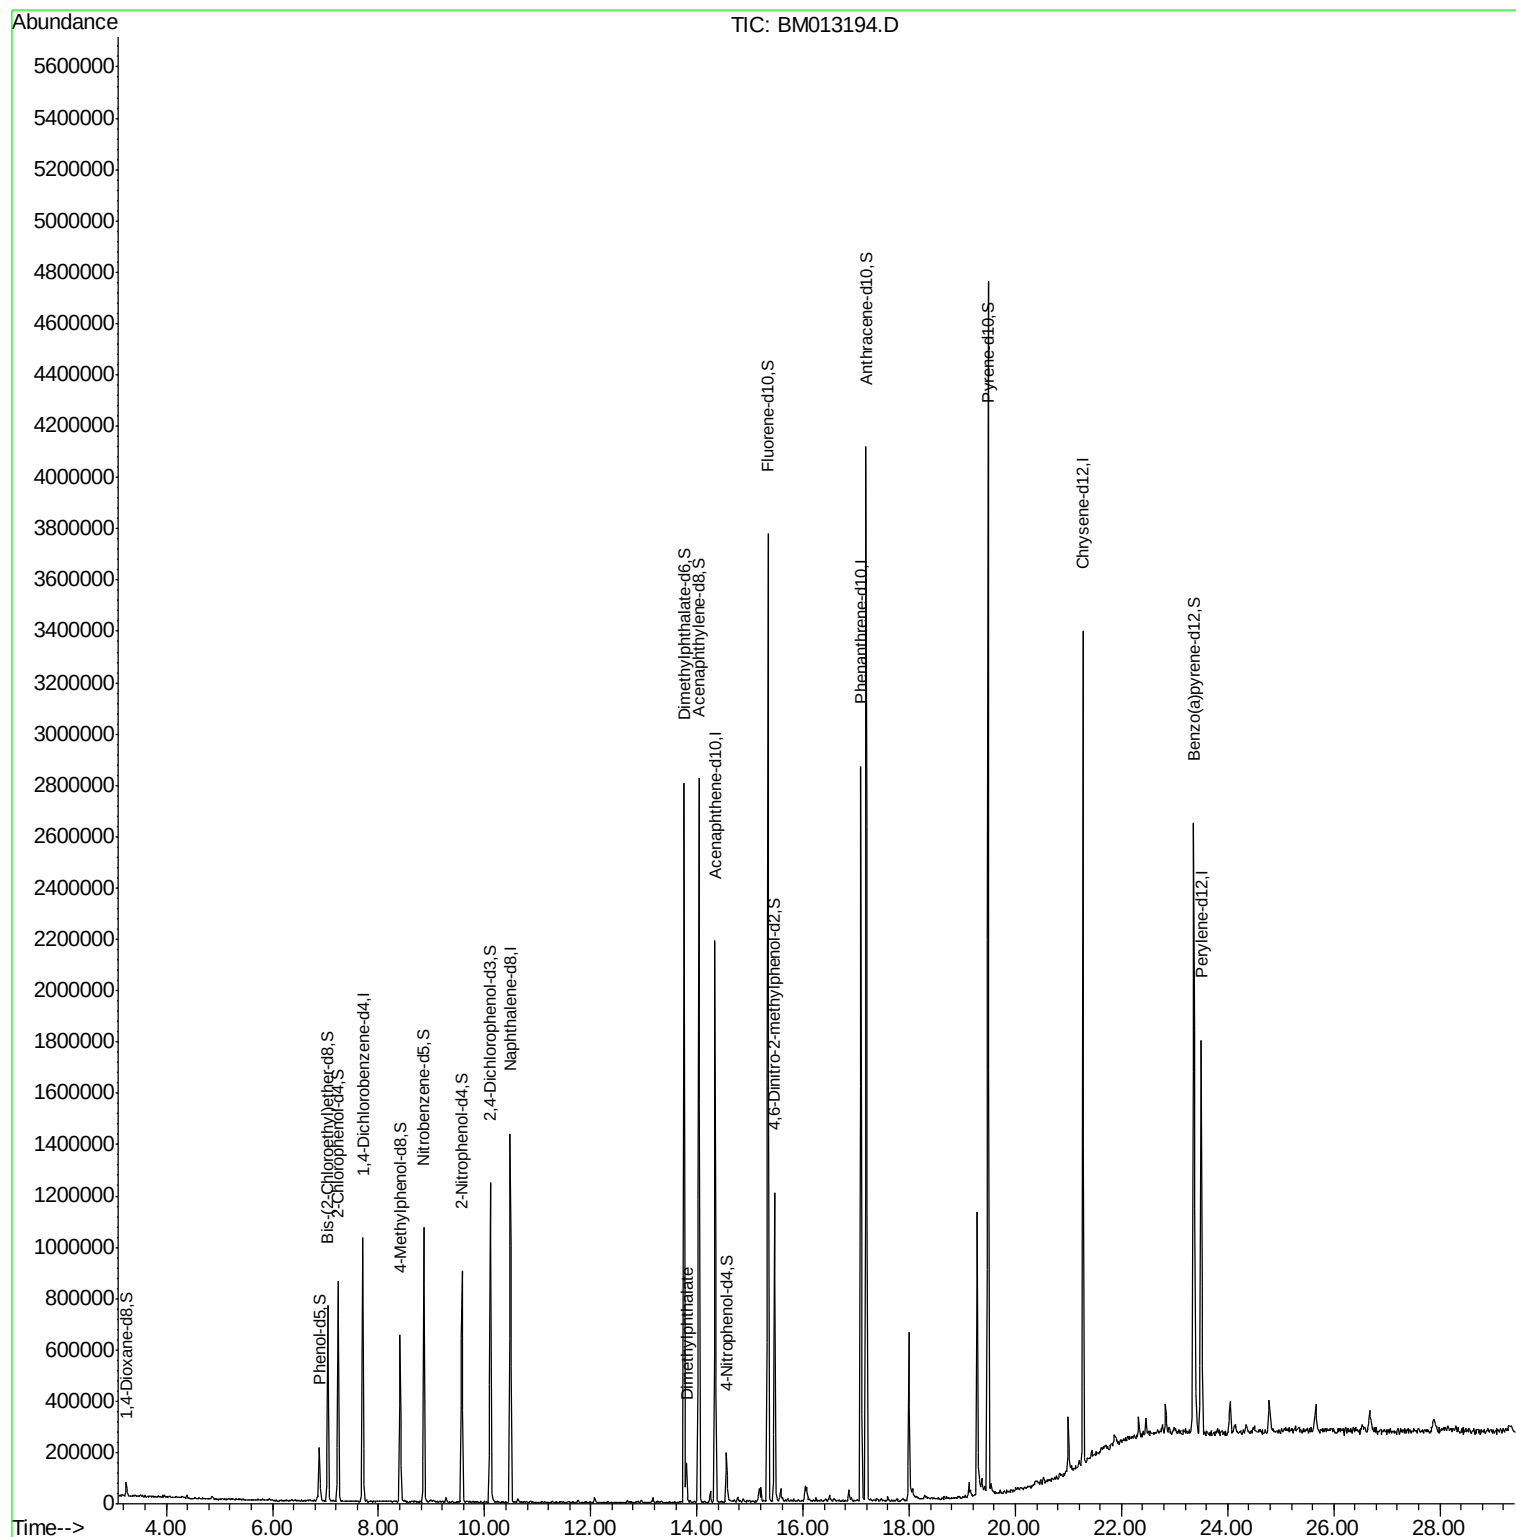

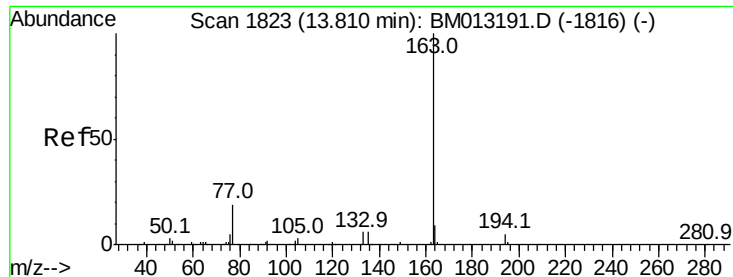

#44
 Dimethylphthalate
 Concen: 1.476 ng/ul
 RT: 13.80 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM013194.D
 Acq: 05 Dec 2017 18:19

Instrument :
 BNA_M
 ClientSampleId :
 JHPP1

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.8	3.5	5.3
164	8.7	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 12/6/2017 5:15:04 PM

