

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048893.D
 Acq On : 07 Dec 2024 12:48
 Operator : RC/JU
 Sample : PB165452BL
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK452

Quant Time: Dec 08 21:46:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	5226	0.400	ng/ul	0.00
4) Naphthalene-d8	10.354	136	14047	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.225	164	7234	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.070	188	1029091	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.17
23) Perylene-d12	23.343	264	12766	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	35088	5.256	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.959	152	5180	0.306	ng/ul	0.00
18) Fluoranthene-d10	19.007	212	8756	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.224	166	1911	0.081	ng/ul#	15
26) Benzo(a)pyrene	23.206	252	3145	0.086	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048893.D
Acq On : 07 Dec 2024 12:48
Operator : RC/JU
Sample : PB165452BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK452

Quant Time: Dec 08 21:46:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

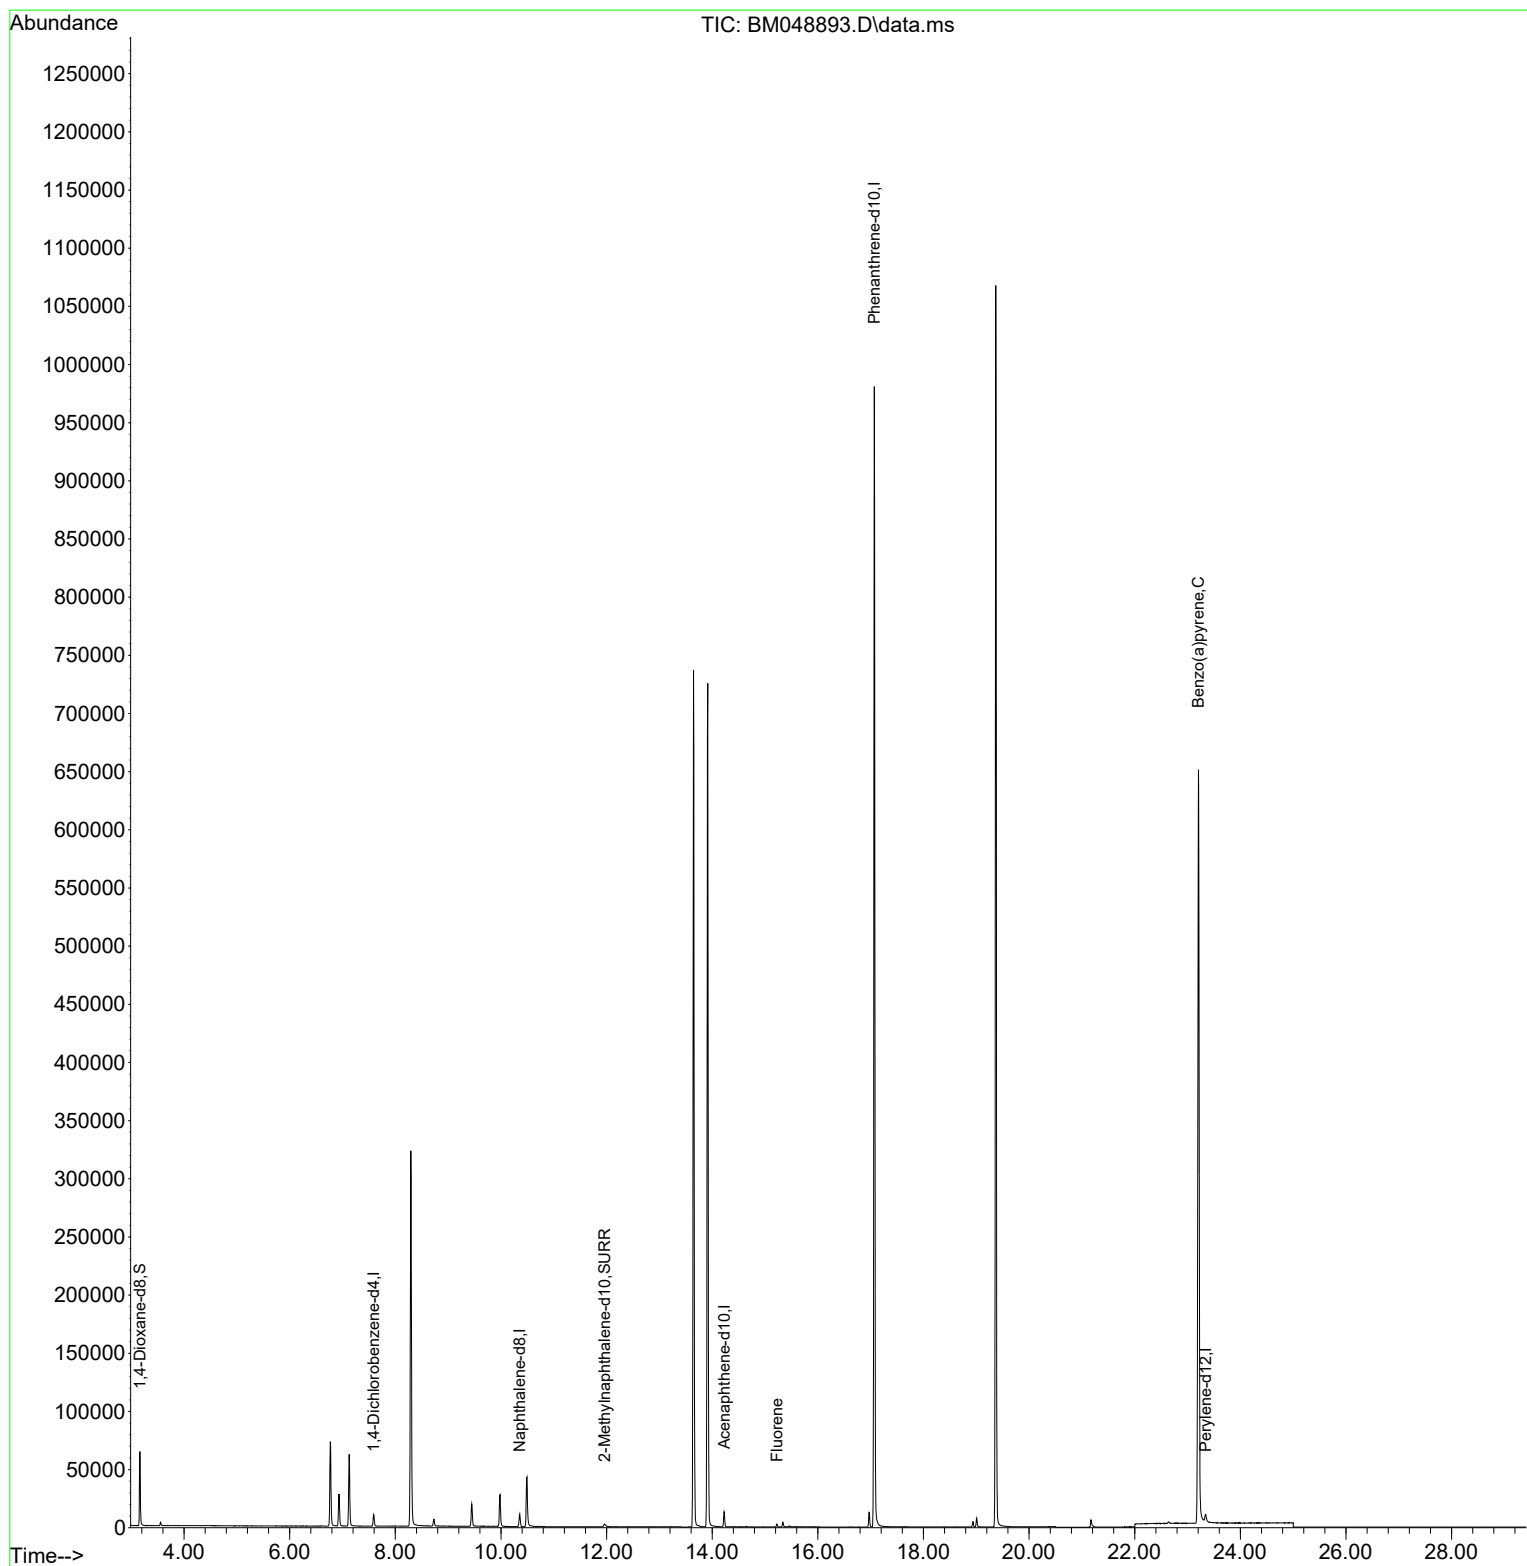

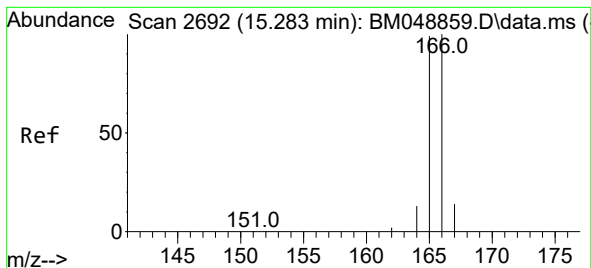

#12

Fluorene

Concen: 0.081 ng/ul

RT: 15.224 min Scan# 2

Delta R.T. -0.063 min

Lab File: BM048893.D

Acq: 07 Dec 2024 12:48

Instrument :

BNA_M

ClientSampleId :

SBLK452





Tgt Ion:166 Resp: 1911

Ion Ratio Lower Upper

166 100

165 8.7 79.8 119.6#

167 34.9 12.2 18.2#

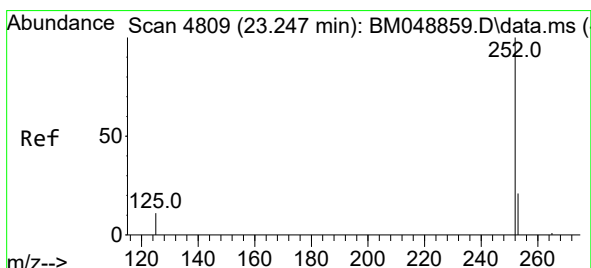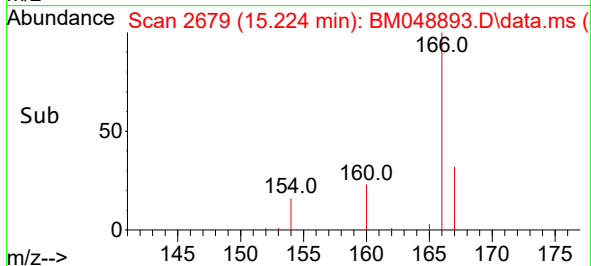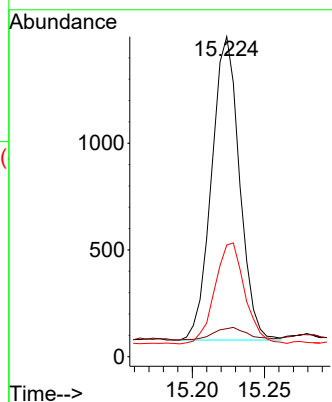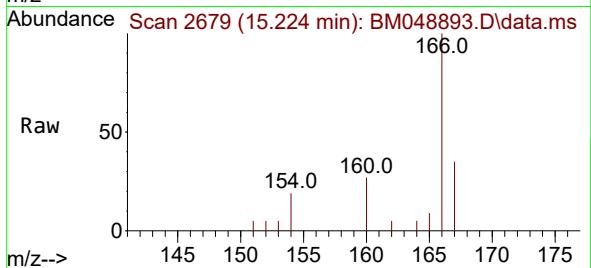

#26

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.206 min Scan# 4795

Delta R.T. -0.047 min

Lab File: BM048893.D

Acq: 07 Dec 2024 12:48

Tgt Ion:252 Resp: 3145

Ion Ratio Lower Upper

252 100

253 39.5 22.5 33.7#

125 39.5 20.6 30.8#

