

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048894.D
 Acq On : 07 Dec 2024 13:24
 Operator : RC/JU
 Sample : P5114-04
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1PK0

Quant Time: Dec 08 21:47:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	5582	0.400	ng/ul	0.00
4) Naphthalene-d8	10.354	136	15515	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.225	164	8125	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.070	188	1460425	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.17
23) Perylene-d12	23.338	264	15415	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	32597	4.572	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.954	152	6452	0.346	ng/ul	0.00
18) Fluoranthene-d10	19.007	212	12795	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
26) Benzo(a)pyrene	23.206	252	4811	0.108	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048894.D
Acq On : 07 Dec 2024 13:24
Operator : RC/JU
Sample : P5114-04
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1PK0


Quant Time: Dec 08 21:47:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

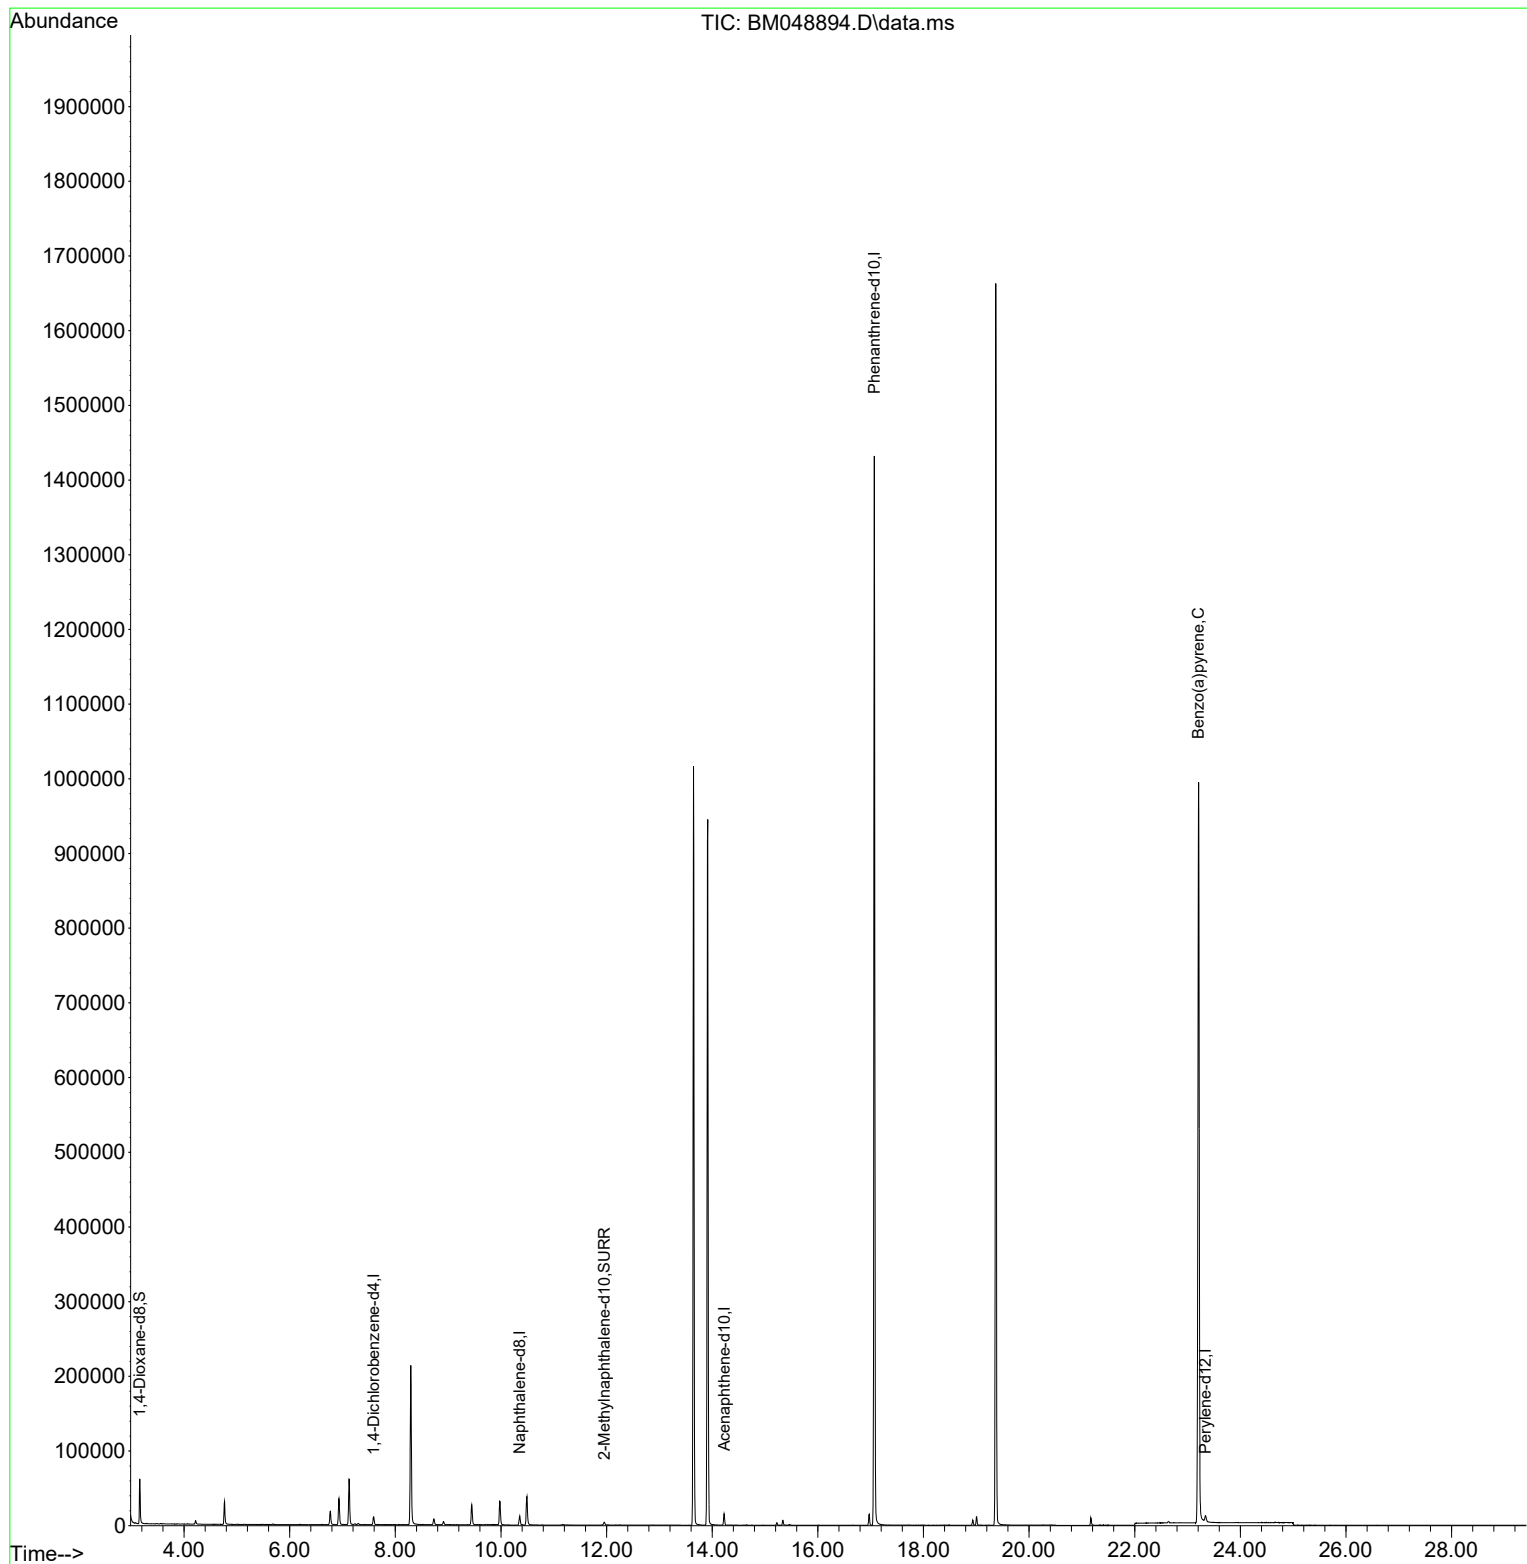

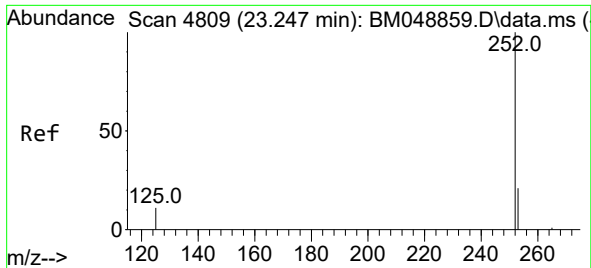

#26
Benzo(a)pyrene
Concen: 0.108 ng/ul
RT: 23.206 min Scan# 41
Delta R.T. -0.047 min
Lab File: BM048894.D
Acq: 07 Dec 2024 13:24

Instrument :
BNA_M
ClientSampleId :
E1PK0

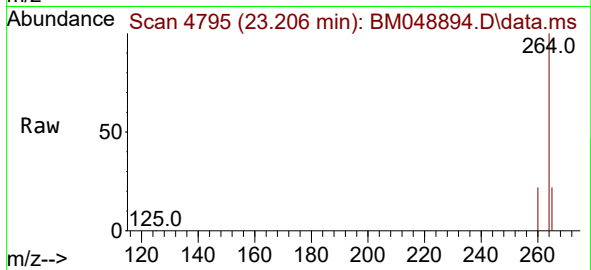

Tgt Ion:252 Resp: 4811
Ion Ratio Lower Upper
252 100
253 36.3 22.5 33.7#
125 33.1 20.6 30.8#

