

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048897.D
 Acq On : 07 Dec 2024 15:11
 Operator : RC/JU
 Sample : P5107-18
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHJ97

Quant Time: Dec 08 21:47:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	5141	0.400	ng/ul	0.00
4) Naphthalene-d8	10.352	136	14501	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.223	164	7675	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.068	188	1431830	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.17
23) Perylene-d12	23.338	264	14029	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	28102	4.279	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.953	152	5688	0.326	ng/ul	-0.01
18) Fluoranthene-d10	19.006	212	12158	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.223	166	2408	0.096	ng/ul#	13
26) Benzo(a)pyrene	23.204	252	4728	0.117	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

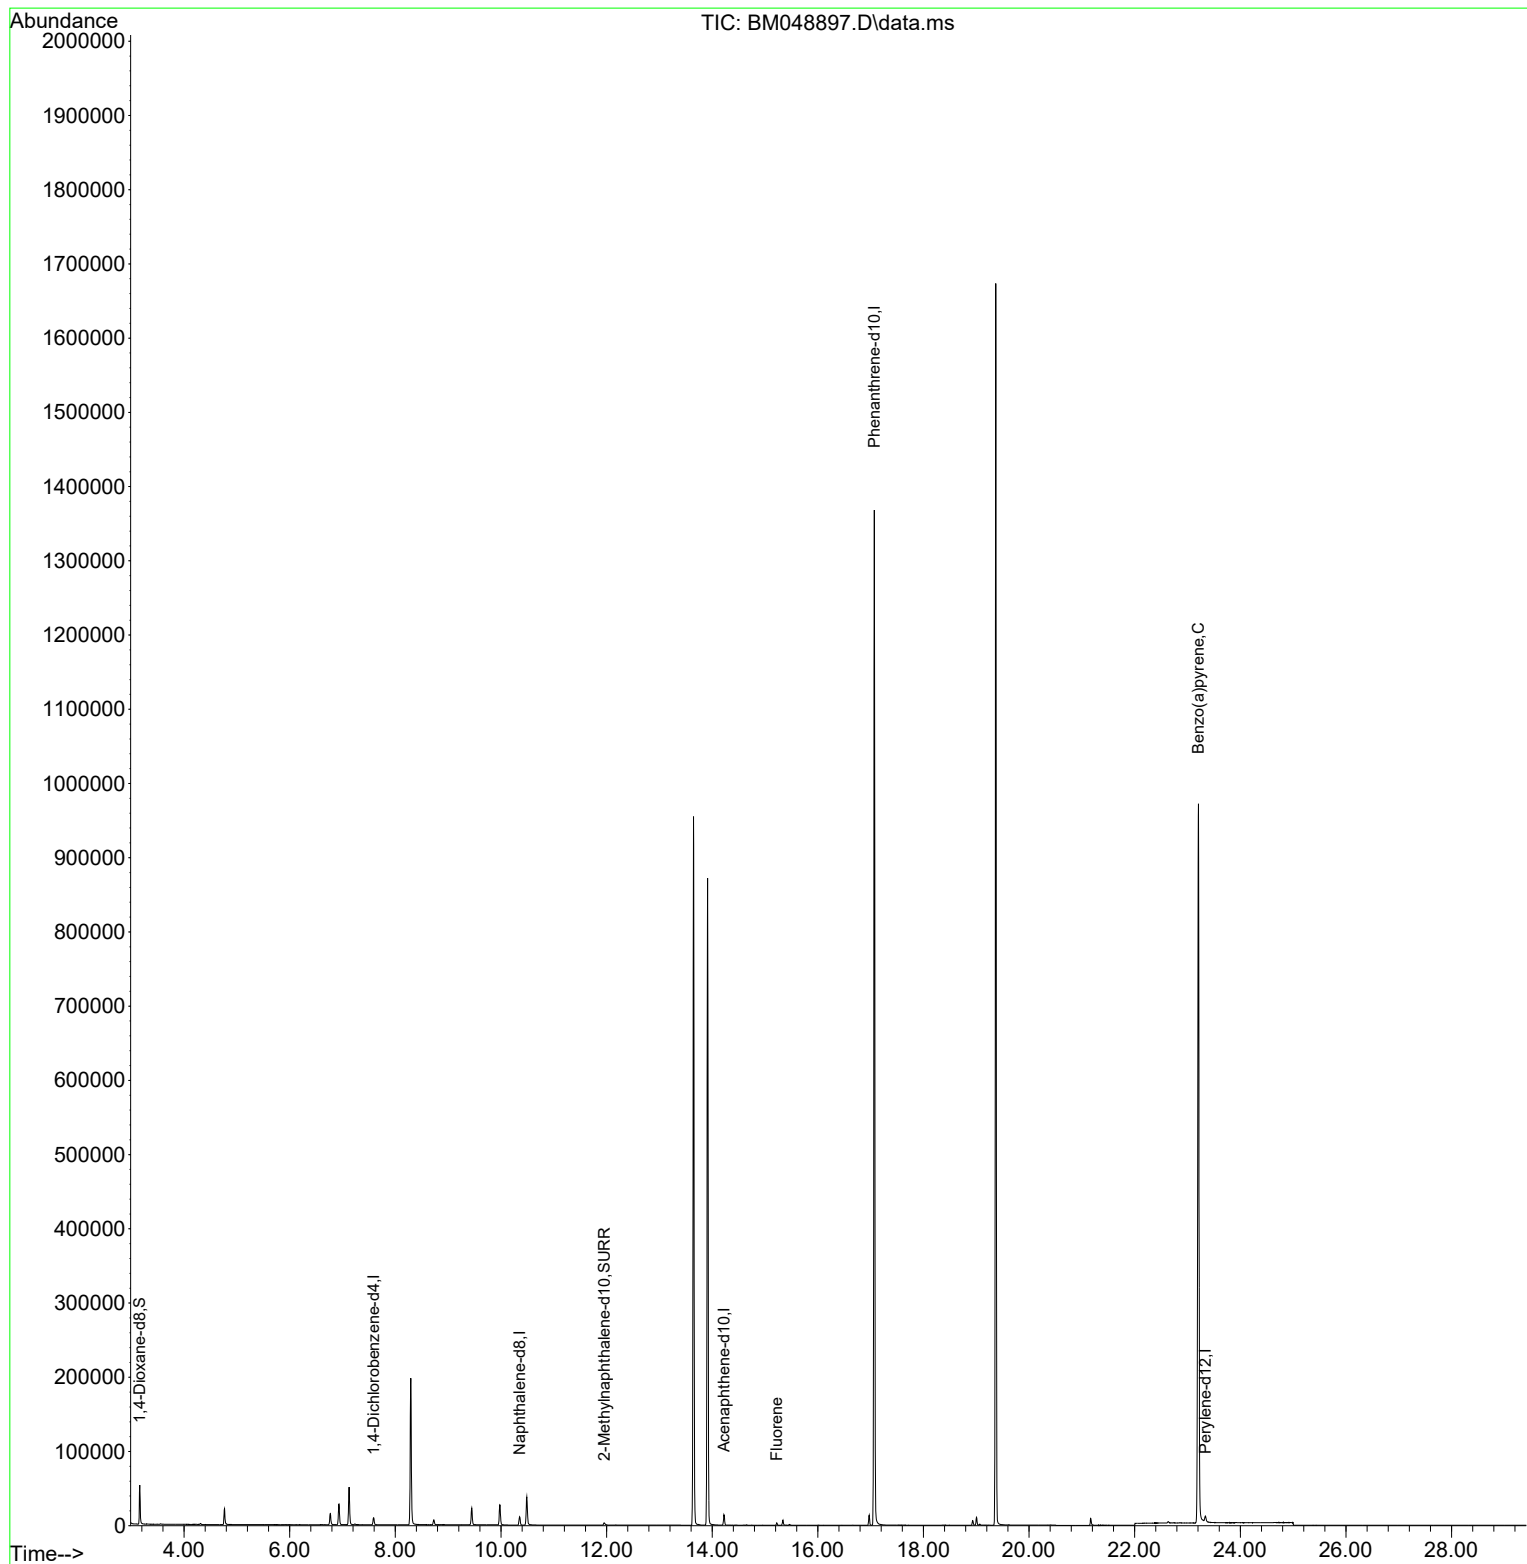

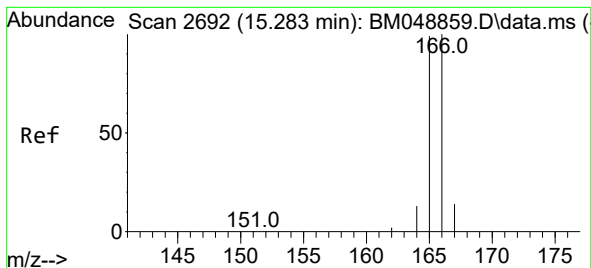

#12

Fluorene

Concen: 0.096 ng/ul

RT: 15.223 min Scan# 2

Delta R.T. -0.065 min

Lab File: BM048897.D

Acq: 07 Dec 2024 15:11

Instrument :

BNA_M

ClientSampleId :

BHJ97





Tgt Ion:166 Resp: 2408

Ion Ratio Lower Upper

166 100

165 7.0 79.8 119.6#

167 34.0 12.2 18.2#

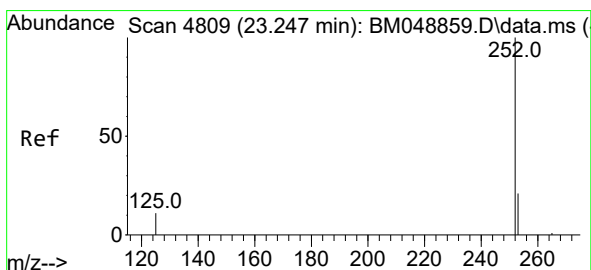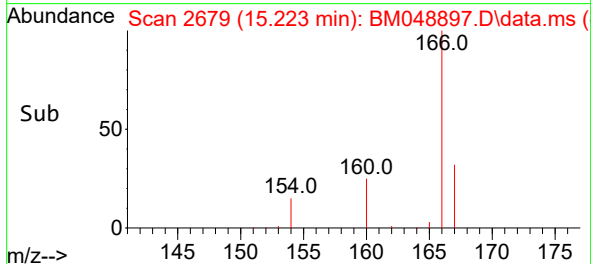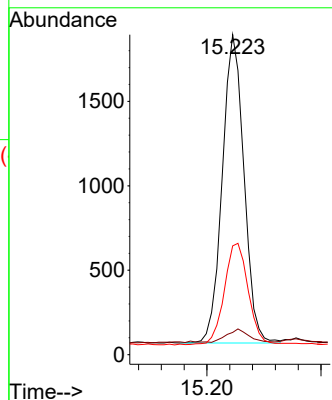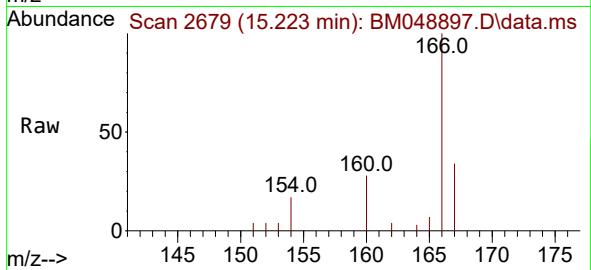

#26

Benzo(a)pyrene

Concen: 0.117 ng/ul

RT: 23.204 min Scan# 4794

Delta R.T. -0.050 min

Lab File: BM048897.D

Acq: 07 Dec 2024 15:11

Tgt Ion:252 Resp: 4728

Ion Ratio Lower Upper

252 100

253 36.0 22.5 33.7#

125 33.0 20.6 30.8#

