

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048899.D
 Acq On : 07 Dec 2024 16:23
 Operator : RC/JU
 Sample : P5114-01
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1PJ6

Quant Time: Dec 08 21:47:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	4576	0.400	ng/ul	0.00
4) Naphthalene-d8	10.352	136	12895	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.223	164	6820	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.068	188	1528085	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.17
23) Perylene-d12	23.338	264	13572	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	24762	4.236	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.952	152	6459	0.416	ng/ul	-0.01
18) Fluoranthene-d10	19.005	212	13599	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.222	166	2658	0.119	ng/ul#	14
26) Benzo(a)pyrene	23.203	252	5564	0.142	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048899.D
Acq On : 07 Dec 2024 16:23
Operator : RC/JU
Sample : P5114-01
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1PJ6

Quant Time: Dec 08 21:47:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

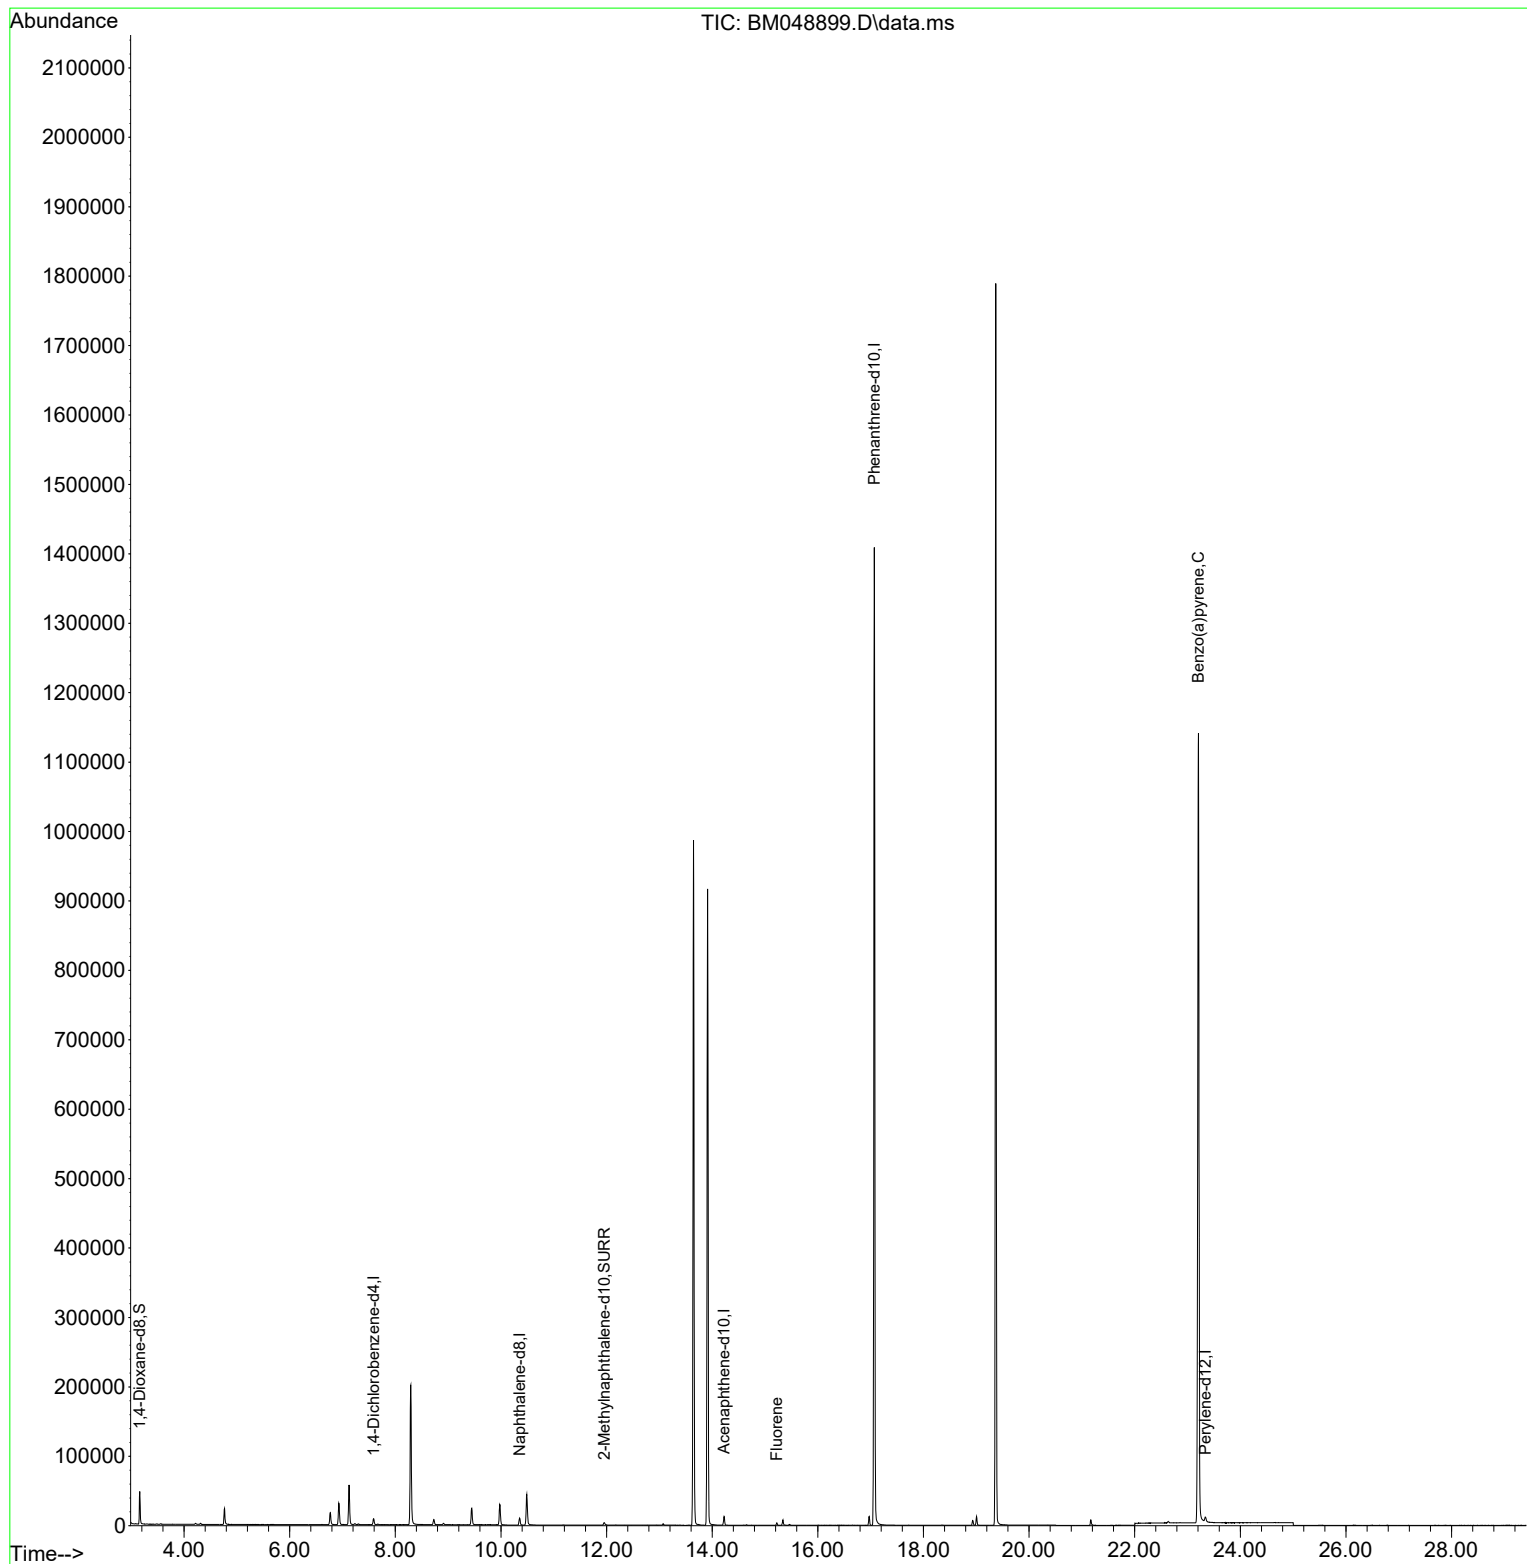

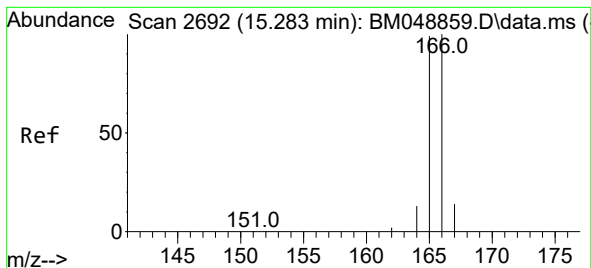

#12

Fluorene

Concen: 0.119 ng/ul

RT: 15.222 min Scan# 2

Delta R.T. -0.065 min

Lab File: BM048899.D

Acq: 07 Dec 2024 16:23

Instrument :

BNA_M

ClientSampleId :

E1PJ6





Tgt Ion:166 Resp: 2658

Ion Ratio Lower Upper

166 100

165 7.3 79.8 119.6#

167 34.7 12.2 18.2#

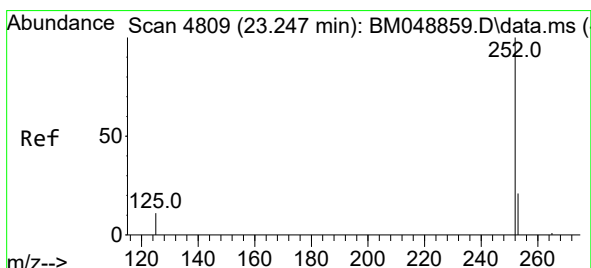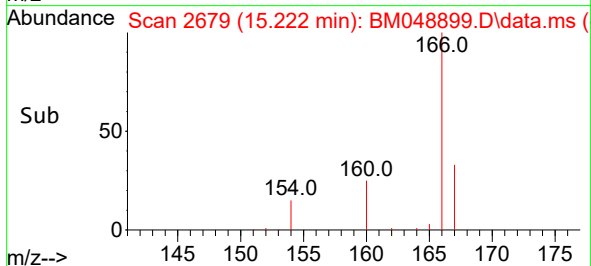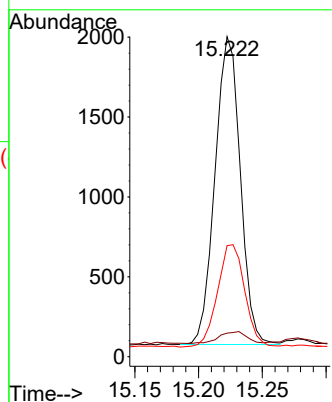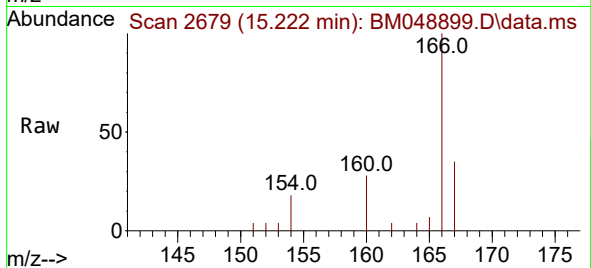

#26

Benzo(a)pyrene

Concen: 0.142 ng/ul

RT: 23.203 min Scan# 4794

Delta R.T. -0.050 min

Lab File: BM048899.D

Acq: 07 Dec 2024 16:23

Tgt Ion:252 Resp: 5564

Ion Ratio Lower Upper

252 100

253 36.3 22.5 33.7#

125 32.9 20.6 30.8#

