

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048900.D
 Acq On : 07 Dec 2024 16:58
 Operator : RC/JU
 Sample : P5114-02
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1PJ7

Quant Time: Dec 08 21:47:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.586	152	6482	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.354	136	18626	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.225	164	9859	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.070	188	1868106	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.17
23) Perylene-d12	23.338	264	16731	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	35044	4.232	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.954	152	7819	0.349	ng/ul	0.00
18) Fluoranthene-d10	19.007	212	16178	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.224	166	3348	0.104	ng/ul#	13
26) Benzo(a)pyrene	23.203	252	6039	0.125	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048900.D
Acq On : 07 Dec 2024 16:58
Operator : RC/JU
Sample : P5114-02
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1PJ7

Quant Time: Dec 08 21:47:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

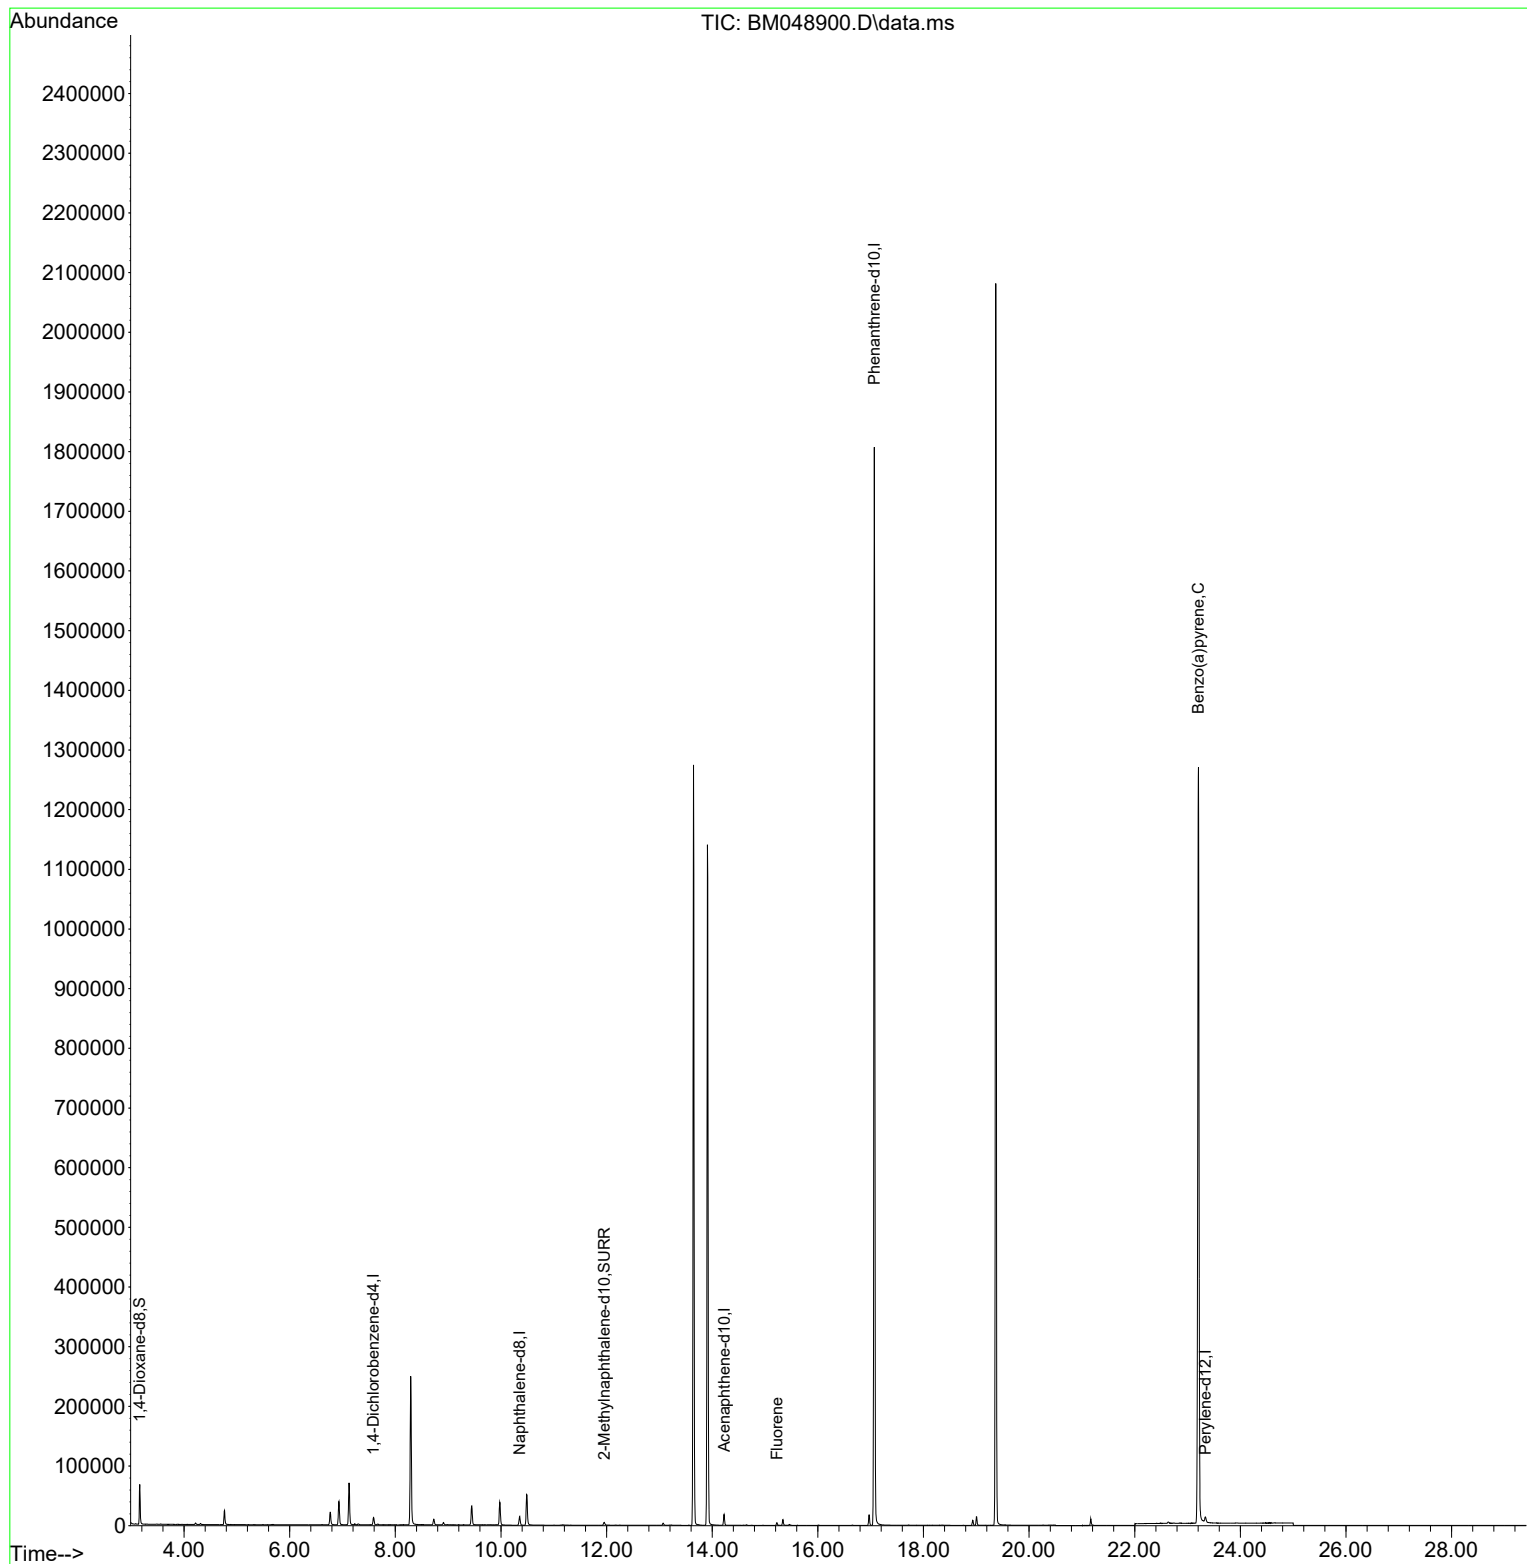

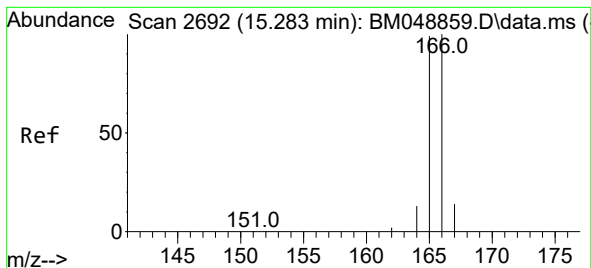

#12

Fluorene

Concen: 0.104 ng/ul

RT: 15.224 min Scan# 2

Delta R.T. -0.063 min

Lab File: BM048900.D

Acq: 07 Dec 2024 16:58

Instrument :

BNA_M

ClientSampleId :

E1PJ7





Tgt Ion:166 Resp: 3348

Ion Ratio Lower Upper

166 100

165 6.5 79.8 119.6#

167 33.5 12.2 18.2#

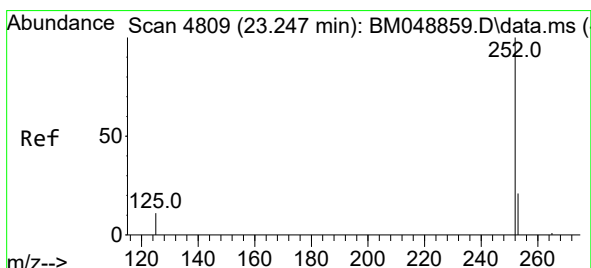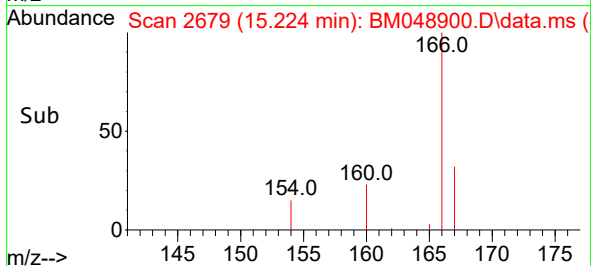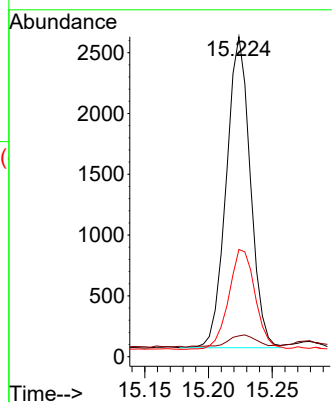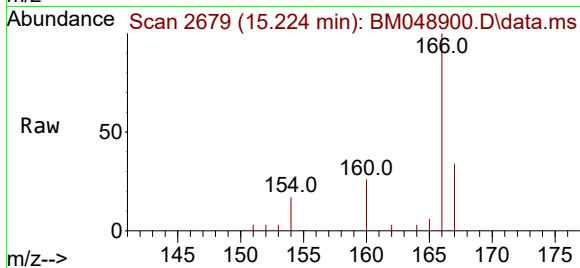

#26

Benzo(a)pyrene

Concen: 0.125 ng/ul

RT: 23.203 min Scan# 4794

Delta R.T. -0.050 min

Lab File: BM048900.D

Acq: 07 Dec 2024 16:58

Tgt Ion:252 Resp: 6039

Ion Ratio Lower Upper

252 100

253 34.9 22.5 33.7#

125 31.6 20.6 30.8#

