

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048901.D
 Acq On : 07 Dec 2024 17:34
 Operator : RC/JU
 Sample : P5114-03
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1PJ8

Quant Time: Dec 08 21:48:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	7552	0.400	ng/ul	0.00
4) Naphthalene-d8	10.352	136	22545	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.223	164	11958	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.068	188	2076128	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.17
23) Perylene-d12	23.338	264	18058	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	36781	3.813	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.953	152	8705	0.321	ng/ul	-0.01
18) Fluoranthene-d10	19.005	212	18024	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
26) Benzo(a)pyrene	23.206	252	6925	0.133	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048901.D
Acq On : 07 Dec 2024 17:34
Operator : RC/JU
Sample : P5114-03
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1PJ8


Quant Time: Dec 08 21:48:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

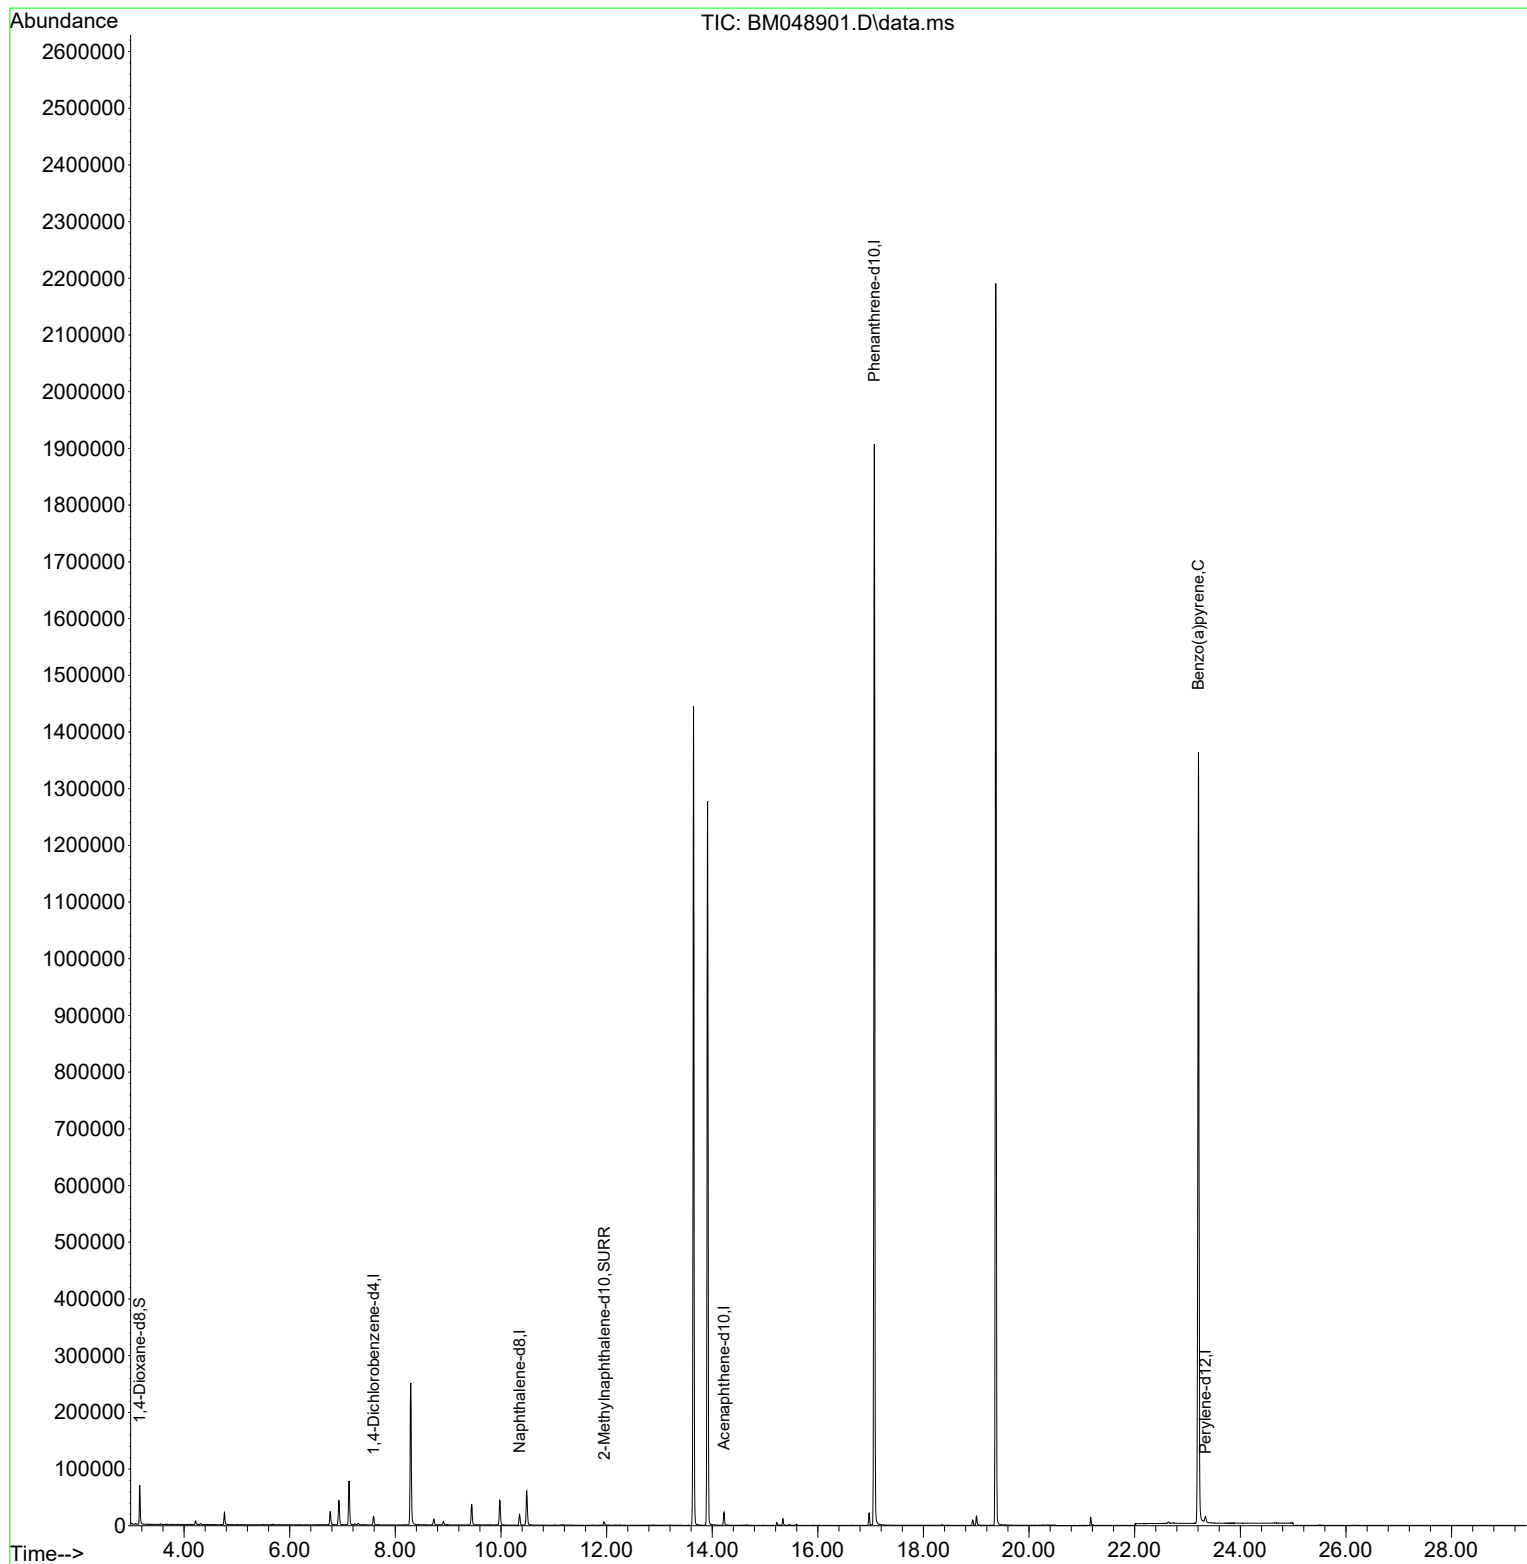

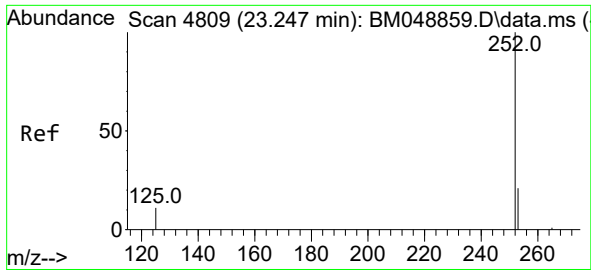

#26
Benzo(a)pyrene
Concen: 0.133 ng/ul
RT: 23.206 min Scan# 41
Delta R.T. -0.047 min
Lab File: BM048901.D
Acq: 07 Dec 2024 17:34

Instrument :
BNA_M
ClientSampleId :
E1PJ8

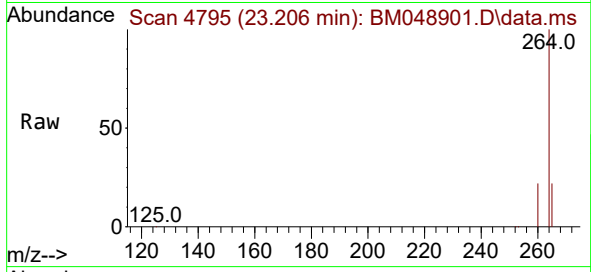

Tgt Ion:252 Resp: 6925
Ion Ratio Lower Upper
252 100
253 34.3 22.5 33.7#
125 30.4 20.6 30.8

