




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048833.D
Acq On : 05 Dec 2024 14:22
Operator : RC/JU
Sample : PB165389BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Dec 05 14:50:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

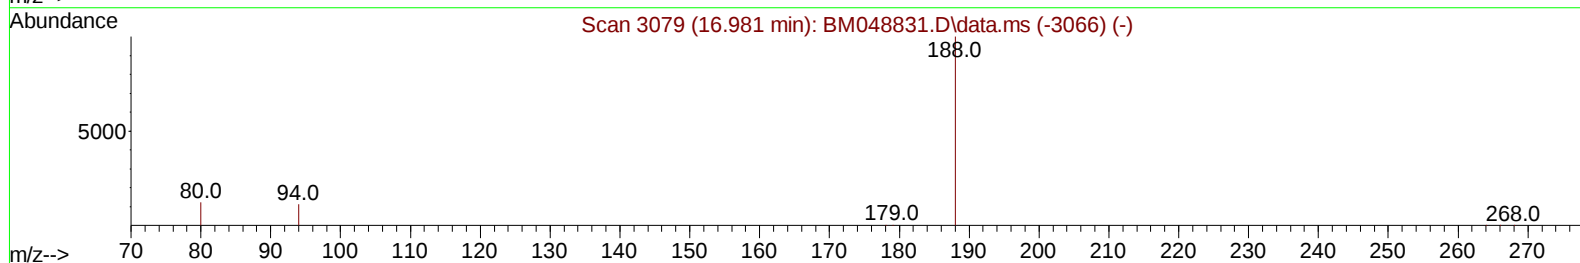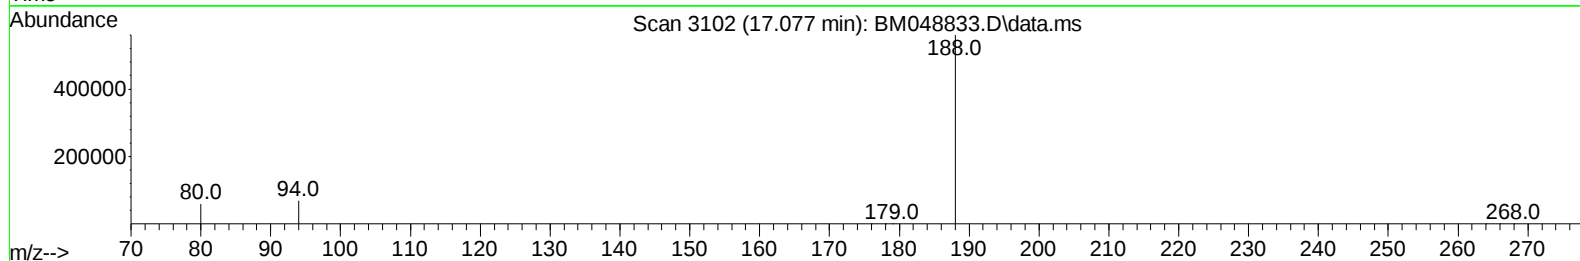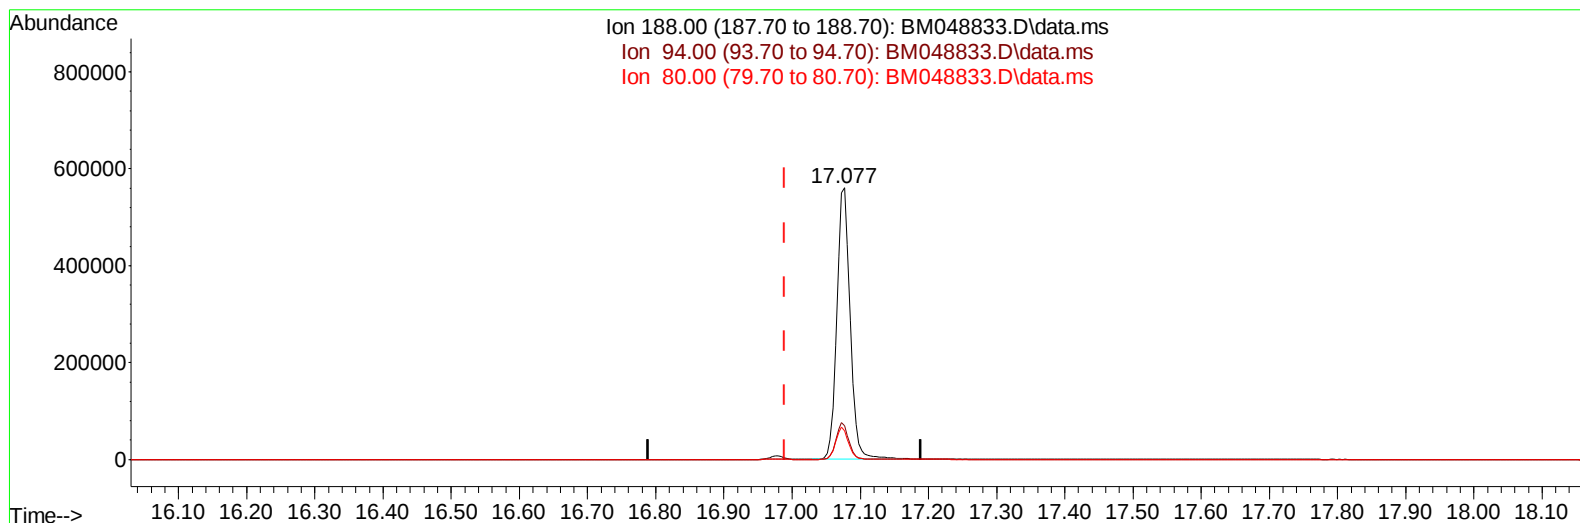

TIC: BM048833.D\data.ms

(13) Phenanthrene-d10 (I)

17.077min (+ 0.088) 0.40 ng/u1

response 761298

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.38
80.00	12.50	10.53
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048833.D
Acq On : 05 Dec 2024 14:22
Operator : RC/JU
Sample : PB165389BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Dec 05 14:50:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

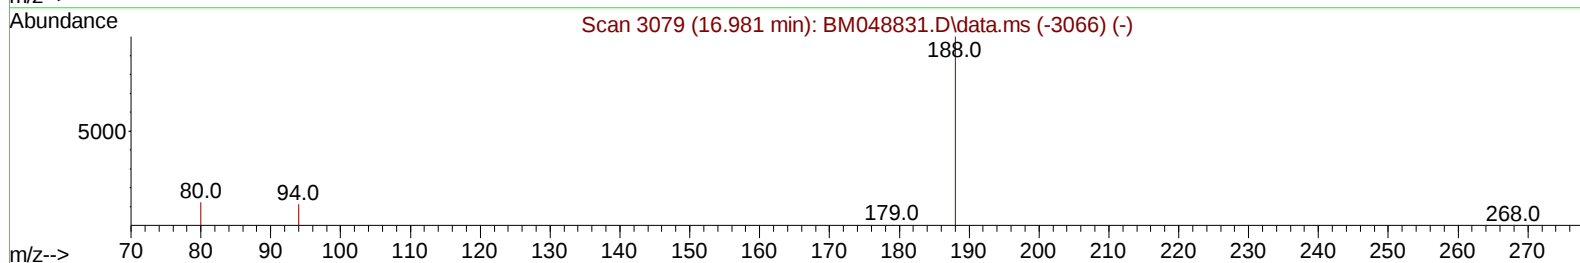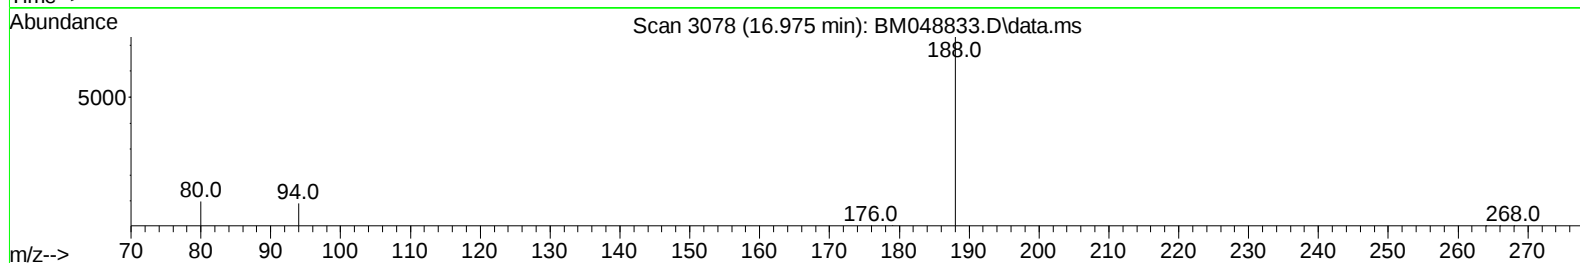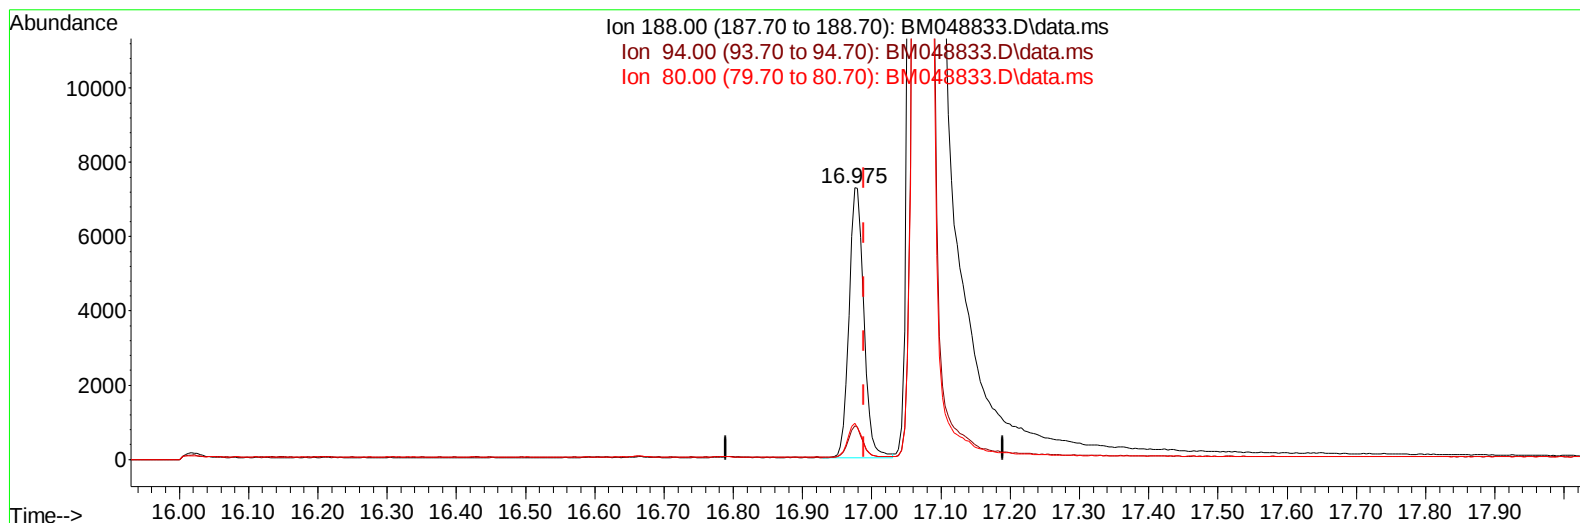

TIC: BM048833.D\data.ms

(13) Phenanthrene-d10 (I)

16.975min (-0.014) 0.40 ng/u1 m

response 10749

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.31
80.00	12.50	13.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048833.D
Acq On : 05 Dec 2024 14:22
Operator : RC/JU
Sample : PB165389BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Dec 05 14:50:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

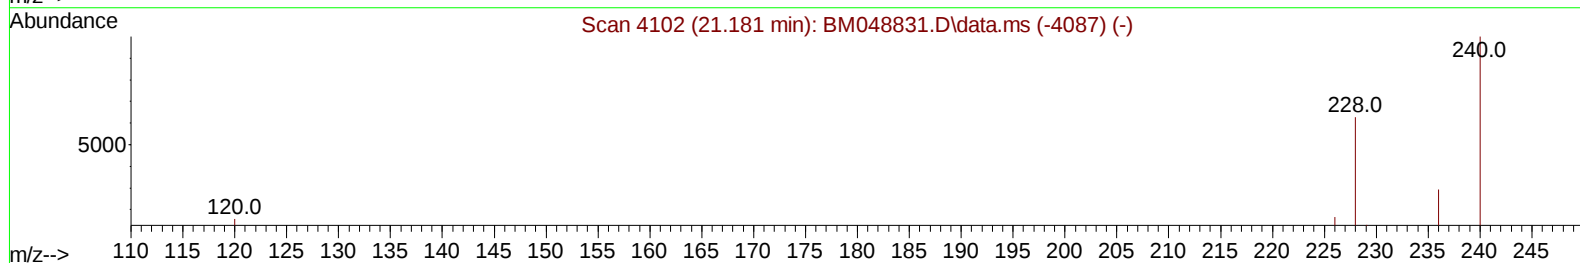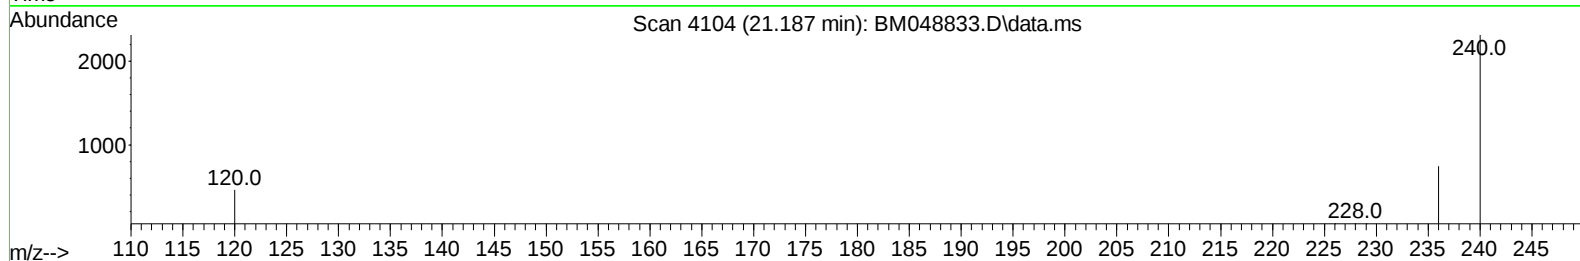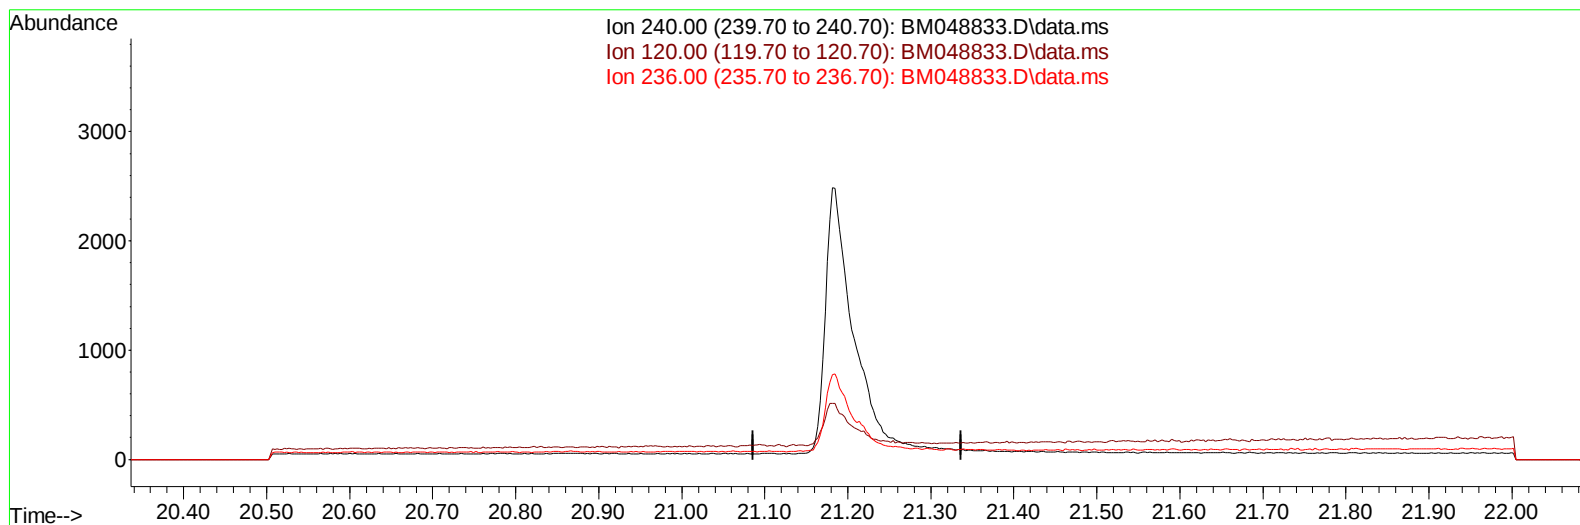

TIC: BM048833.D\data.ms

(17) Chrysene-d12

21.186min (-21.186) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048833.D
Acq On : 05 Dec 2024 14:22
Operator : RC/JU
Sample : PB165389BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Dec 05 14:50:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

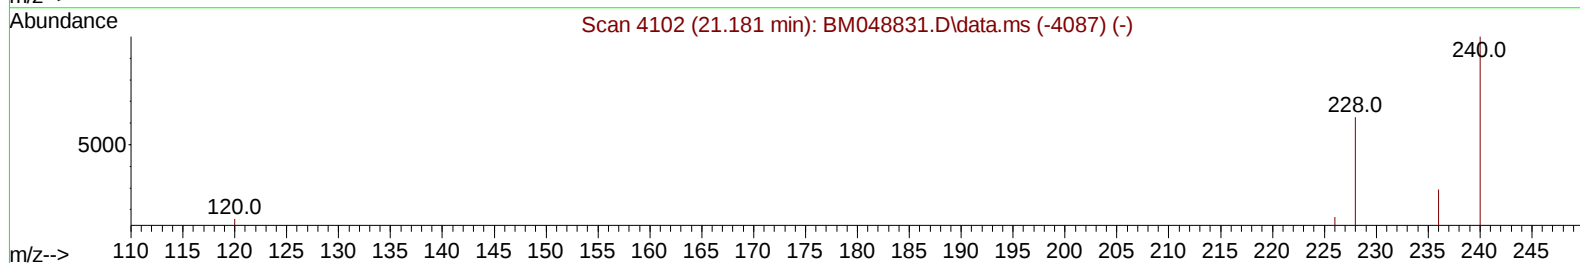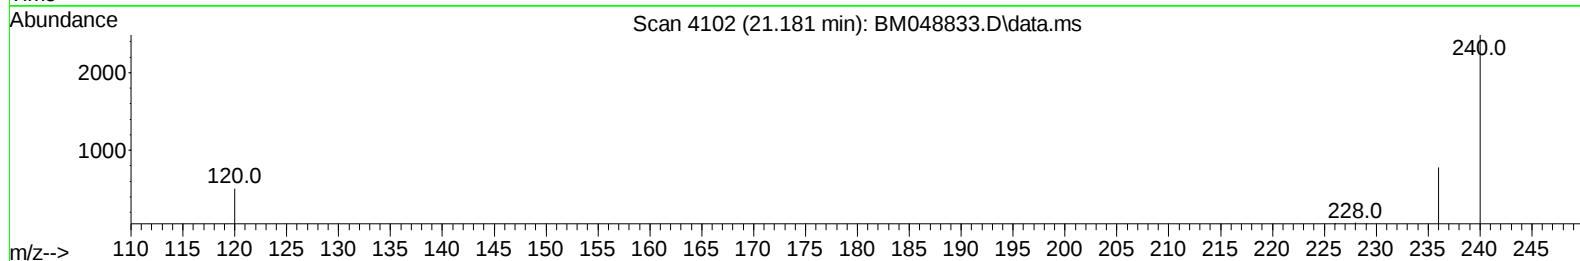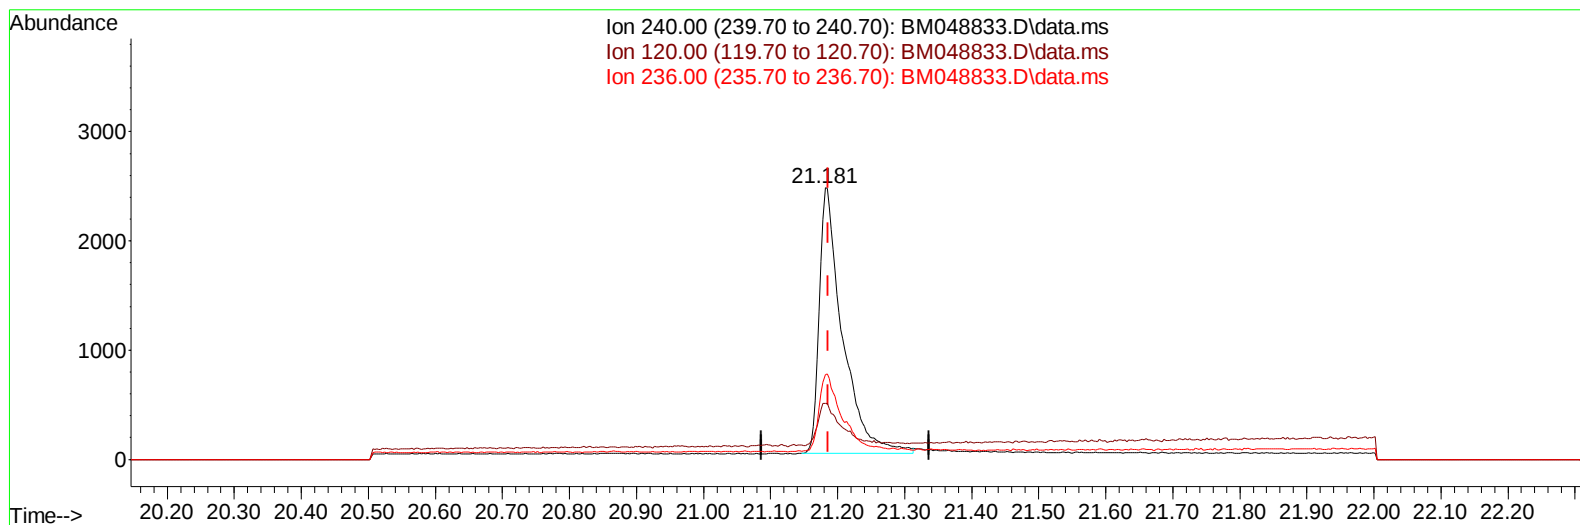

TIC: BM048833.D\data.ms

(17) Chrysene-d12

21.181min (-0.005) 0.40 ng/ul m

response 5825

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	20.52
236.00	32.10	31.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048833.D
Acq On : 05 Dec 2024 14:22
Operator : RC/JU
Sample : PB165389BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Dec 05 14:50:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

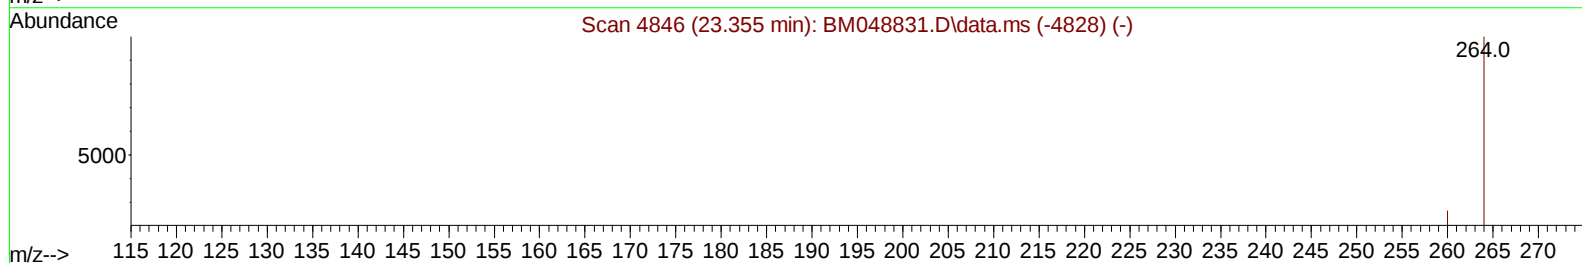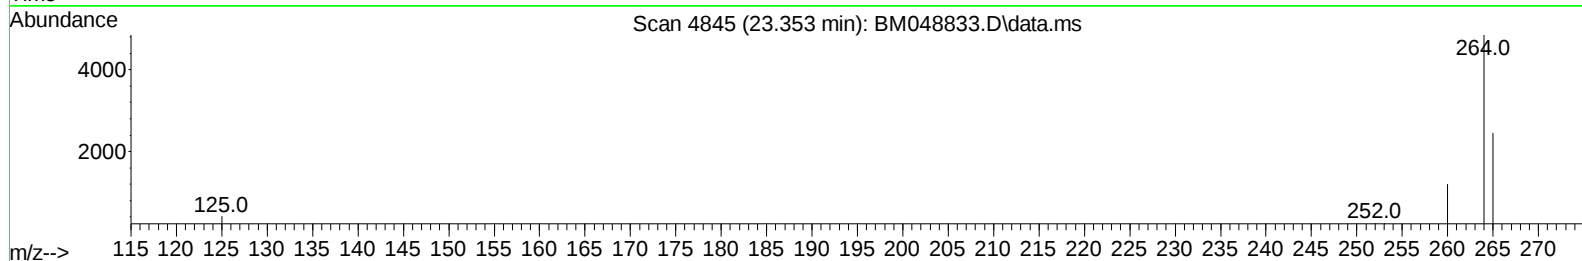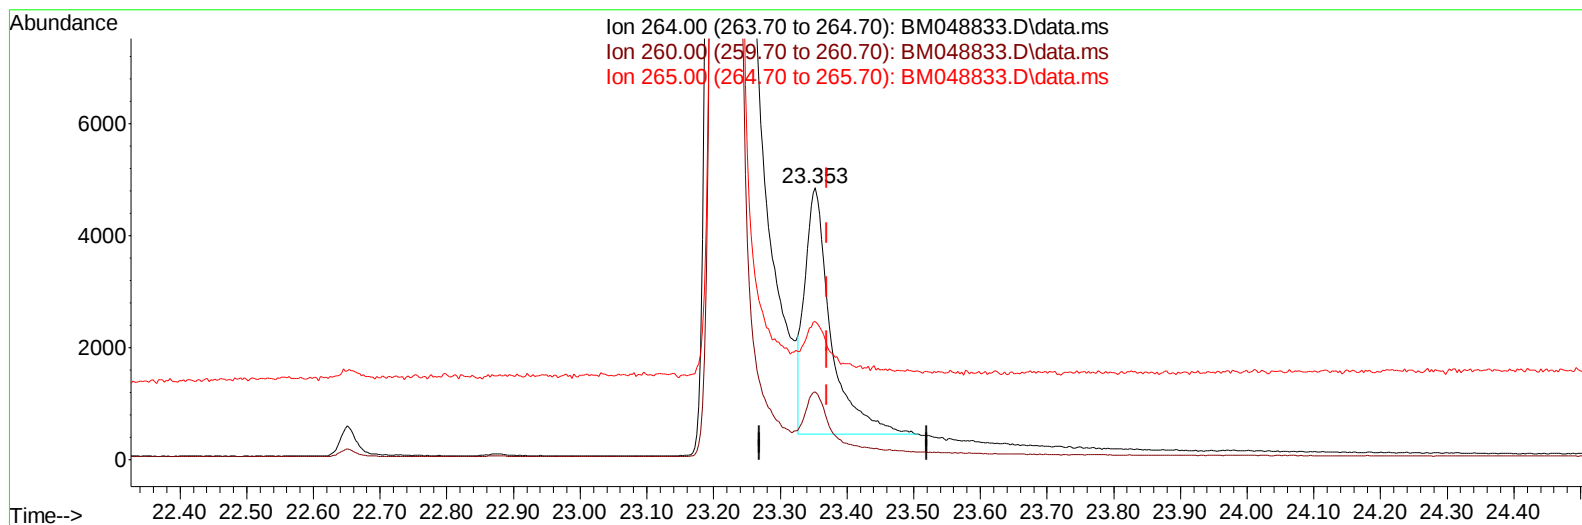

TIC: BM048833.D\data.ms

(23) Perylene-d12 (I)

23.353min (-0.017) 0.40 ng/u1

response 11977

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	24.91
265.00	78.50	50.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048833.D
Acq On : 05 Dec 2024 14:22
Operator : RC/JU
Sample : PB165389BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Dec 05 14:50:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

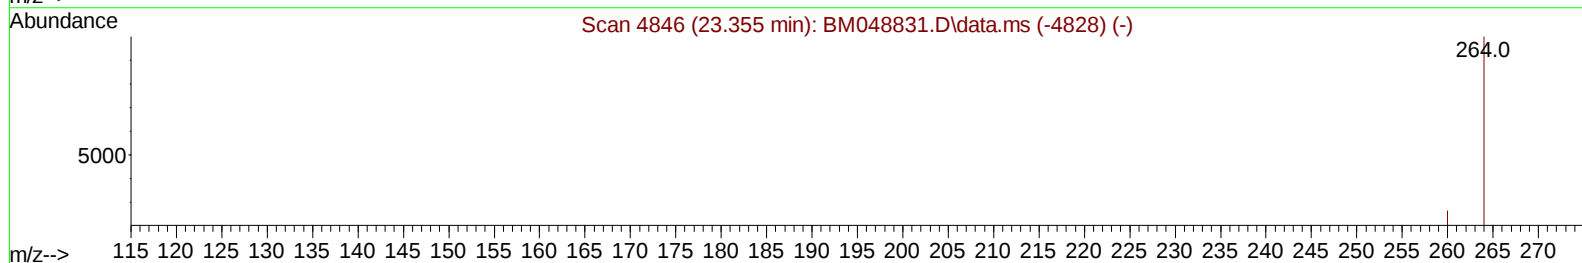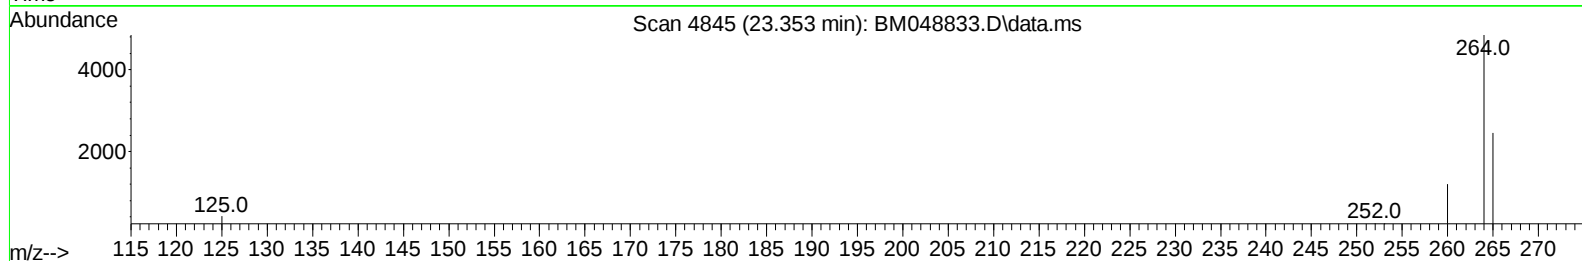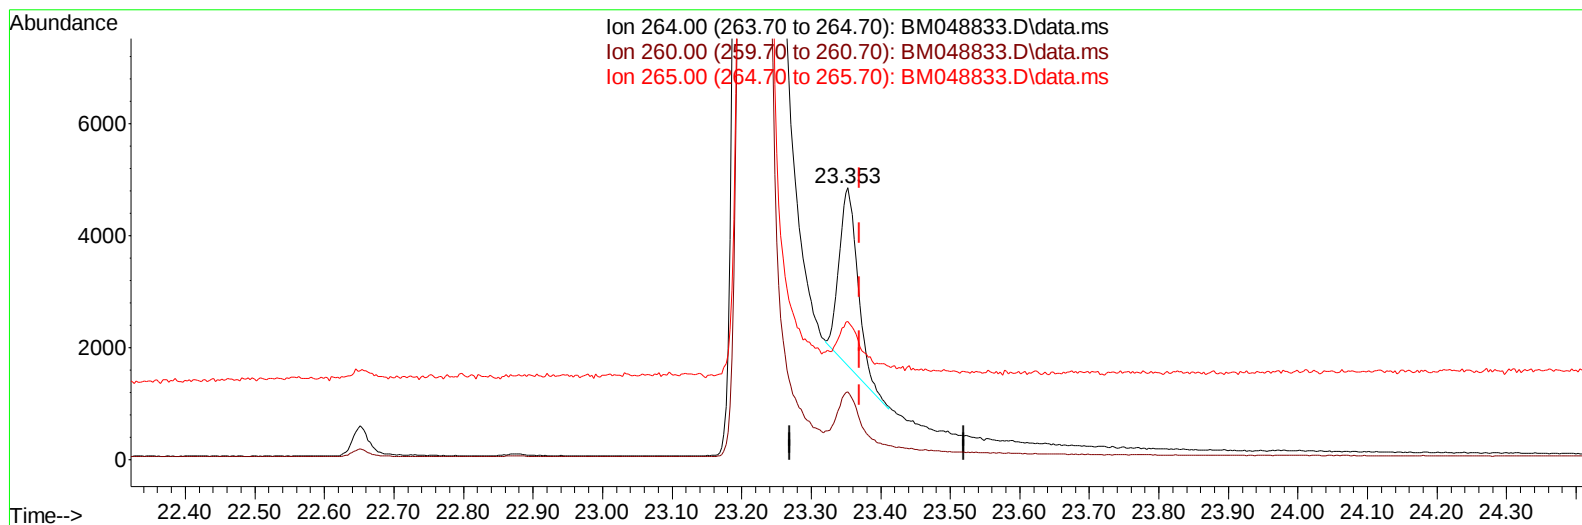

TIC: BM048833.D\data.ms

(23) Perylene-d12 (I)

23.353min (-0.017) 0.40 ng/ul m

response 5828

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	24.91
265.00	78.50	50.75#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048833.D
 Acq On : 05 Dec 2024 14:22
 Operator : RC/JU
 Sample : PB165389BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK389

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 05 14:50:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 03 00:22:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.598	152	4046	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.363	136	11003	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.233	164	5644	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.975	188	10749m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.181	240	5825m	0.400	ng/ul	0.00
23) Perylene-d12	23.353	264	5828m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.168	96	24591	4.758	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.969	152	3578	0.270	ng/ul	0.00
18) Fluoranthene-d10	19.015	212	5810	0.323	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048833.D
Acq On : 05 Dec 2024 14:22
Operator : RC/JU
Sample : PB165389BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Dec 05 14:50:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 00:22:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

