




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048848.D
Acq On : 06 Dec 2024 00:02
Operator : RC/JU
Sample : PB165401BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Manual IntegrationsAPPROVED

Quant Time: Dec 06 01:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

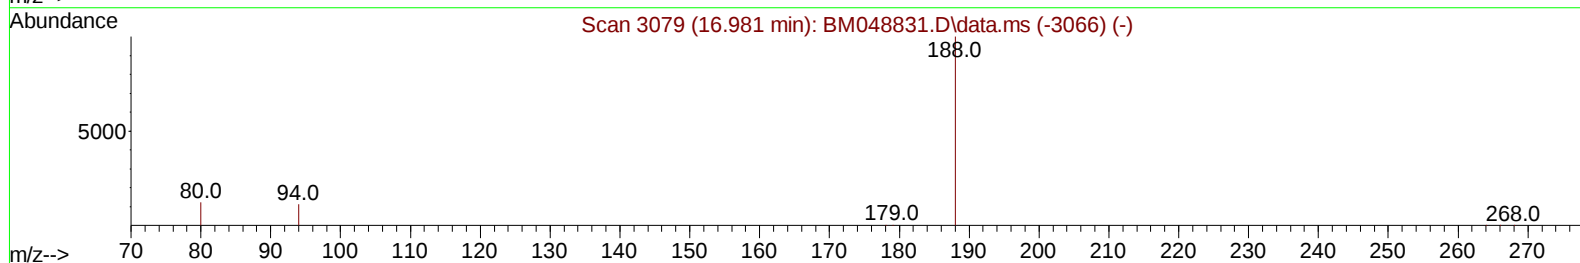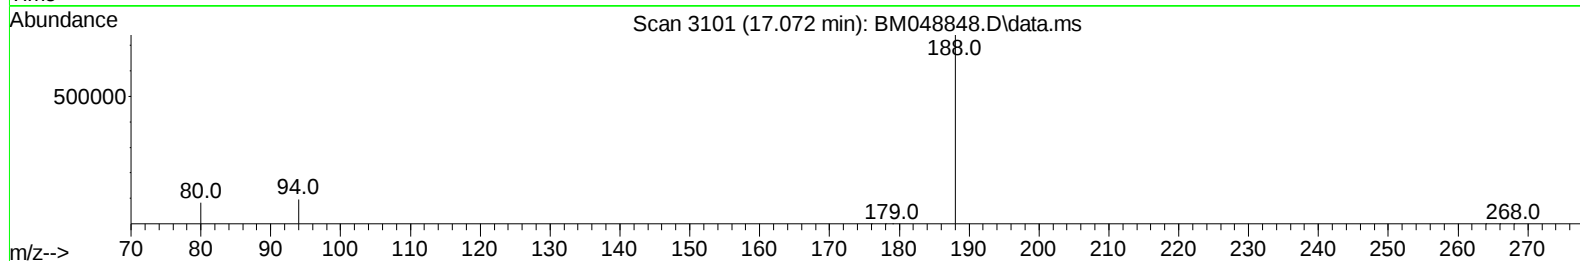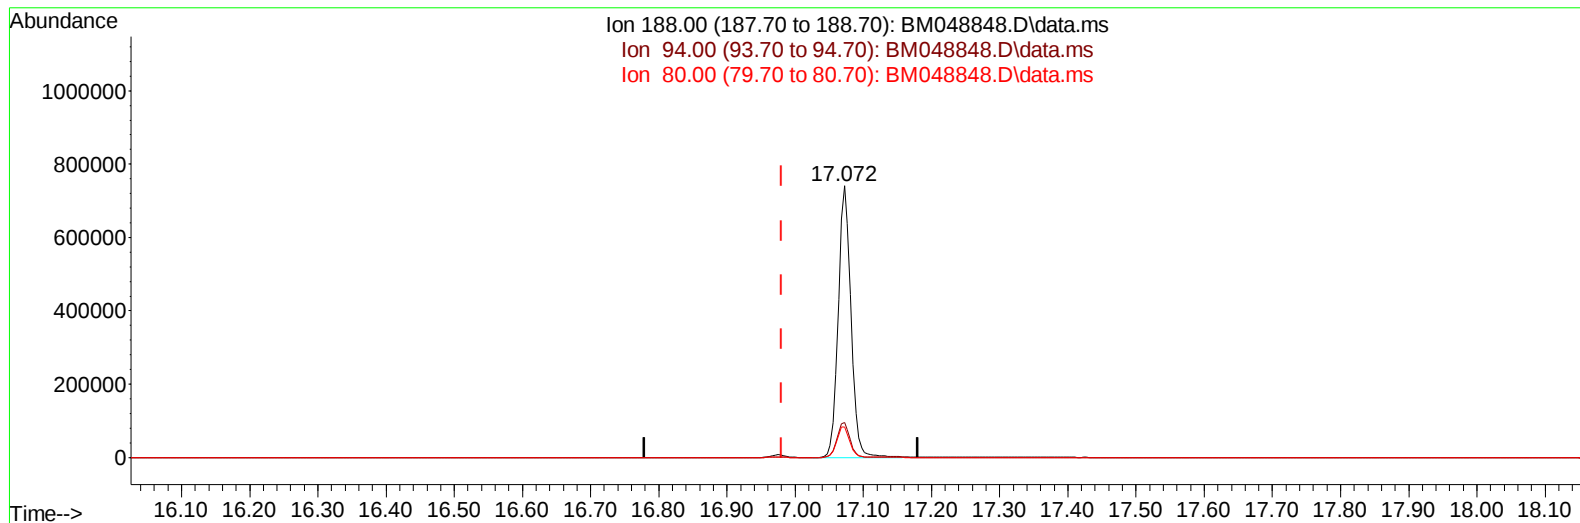

TIC: BM048848.D\data.ms

(13) Phenanthrene-d10 (I)

17.072min (+ 0.093) 0.40 ng/u1

response 961516

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.98
80.00	12.50	11.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048848.D
Acq On : 06 Dec 2024 00:02
Operator : RC/JU
Sample : PB165401BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Manual IntegrationsAPPROVED

Quant Time: Dec 06 01:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

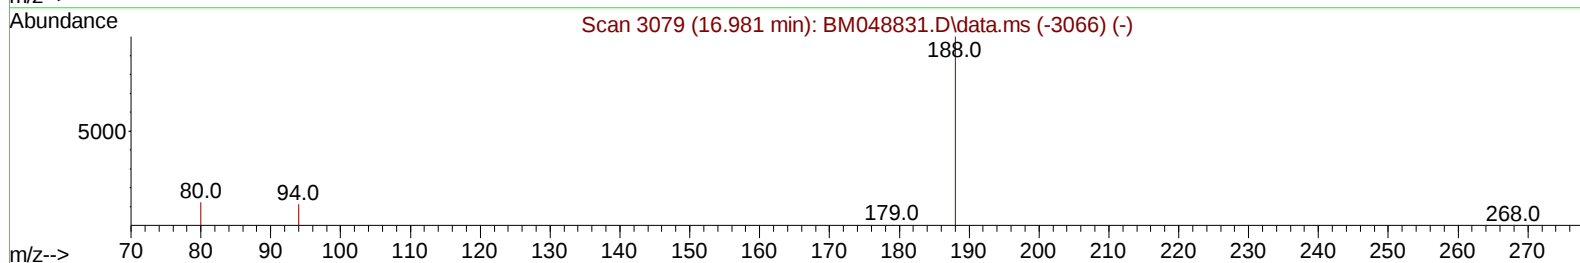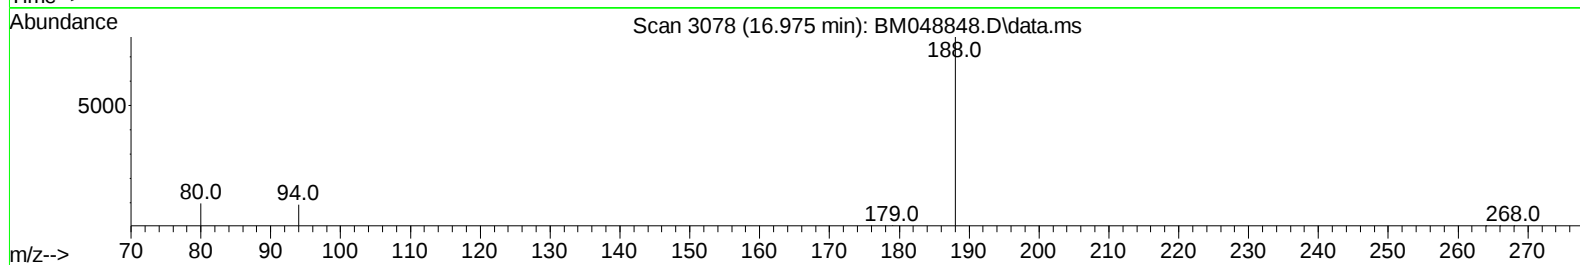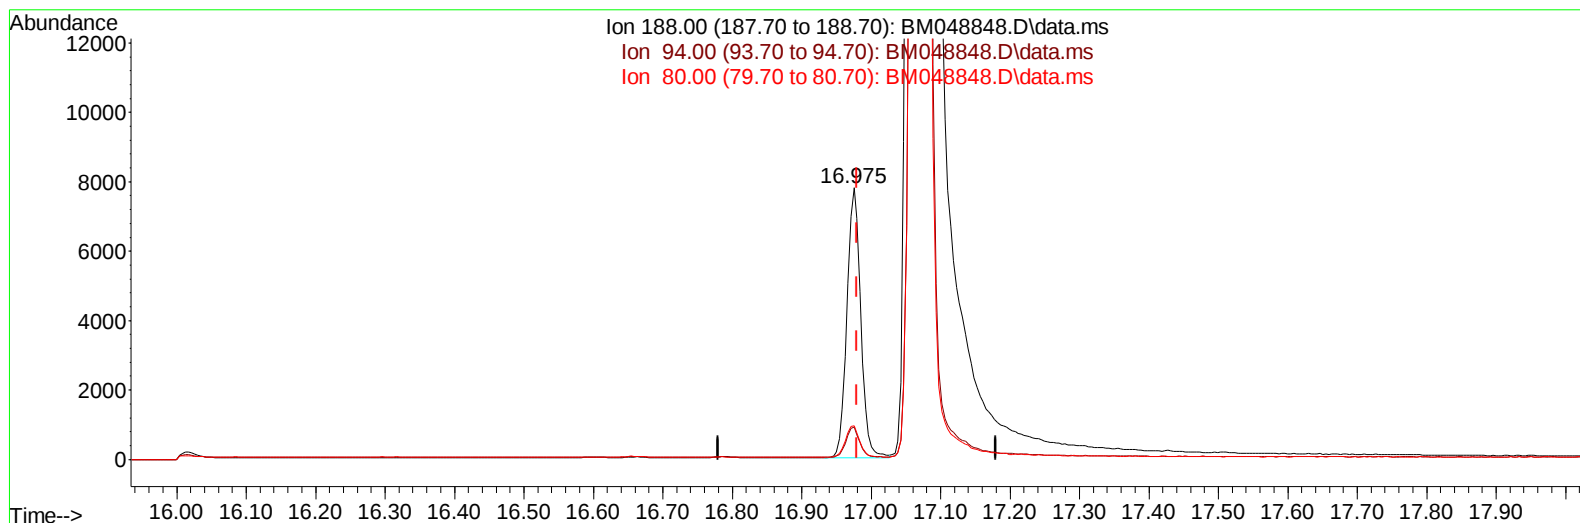

TIC: BM048848.D\data.ms

(13) Phenanthrene-d10 (I)

16.975min (-0.004) 0.40 ng/ul m

response 10723

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	11.82
80.00	12.50	12.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048848.D
Acq On : 06 Dec 2024 00:02
Operator : RC/JU
Sample : PB165401BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Manual IntegrationsAPPROVED

Quant Time: Dec 06 01:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

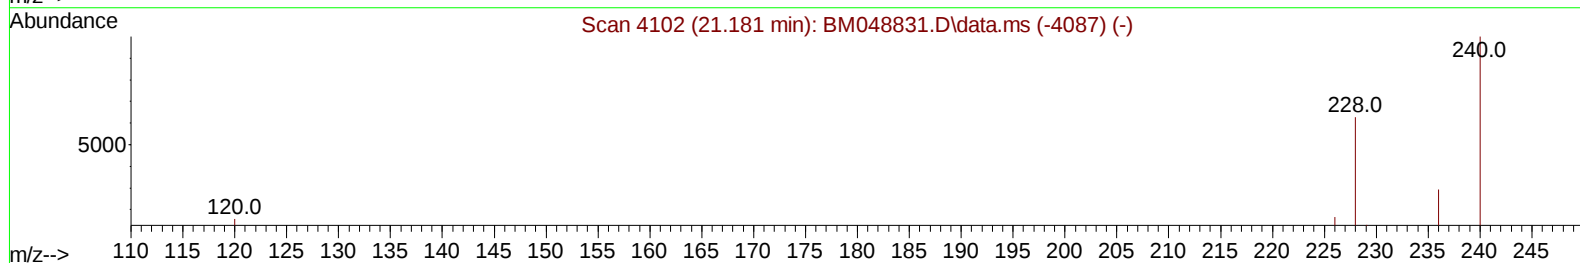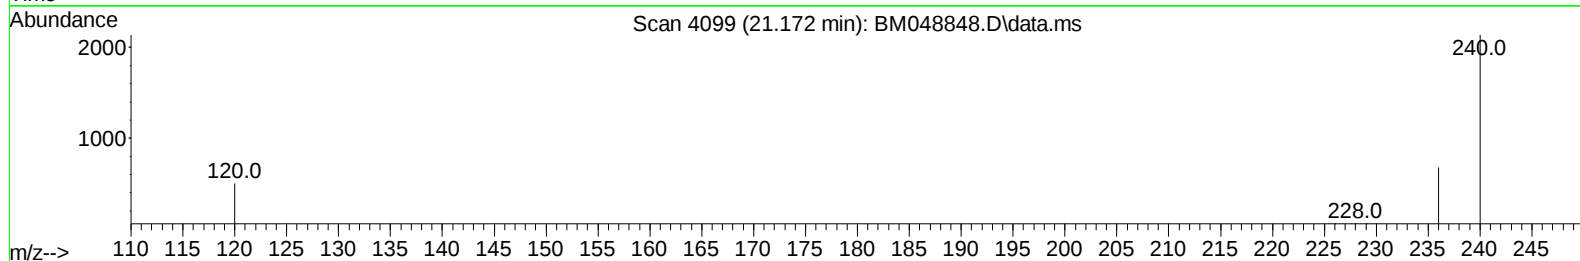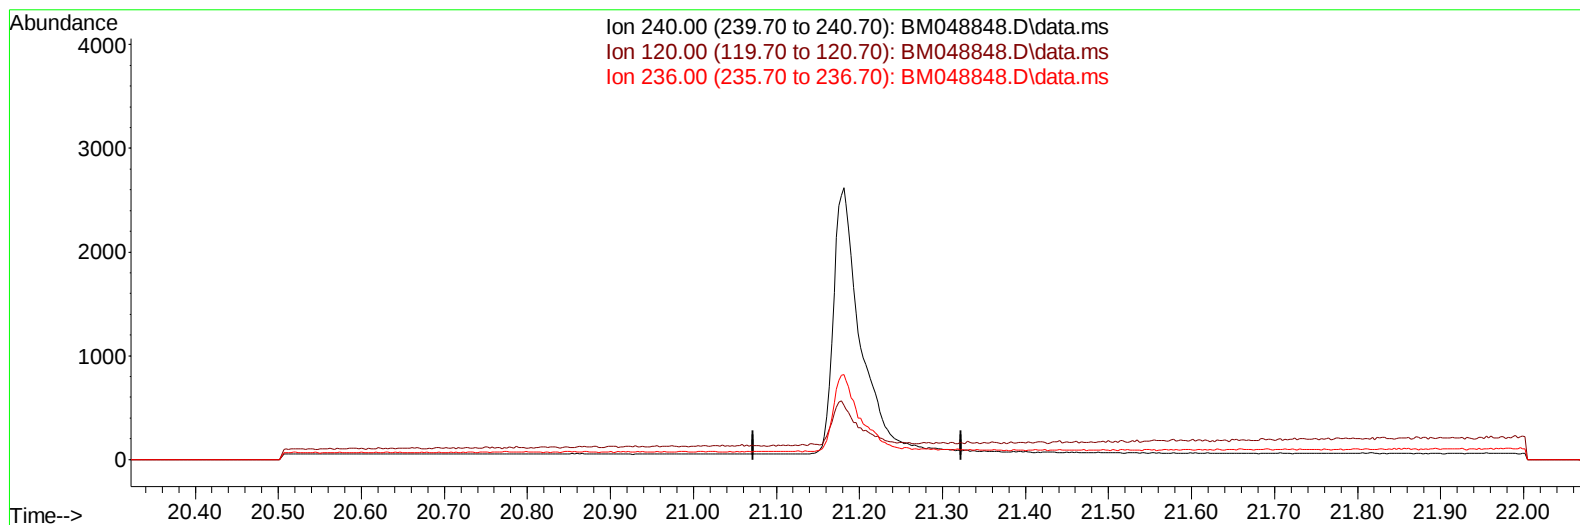

TIC: BM048848.D\data.ms

(17) Chrysene-d12

21.173min (-21.173) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048848.D
Acq On : 06 Dec 2024 00:02
Operator : RC/JU
Sample : PB165401BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Manual IntegrationsAPPROVED

Quant Time: Dec 06 01:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

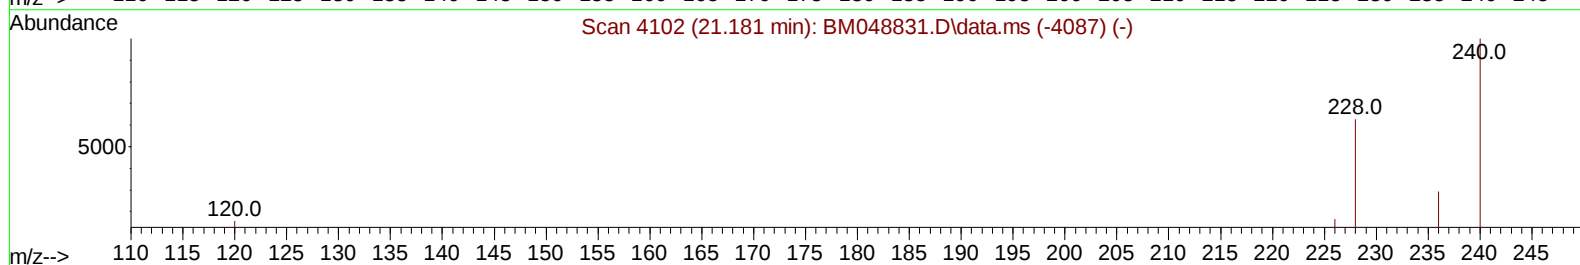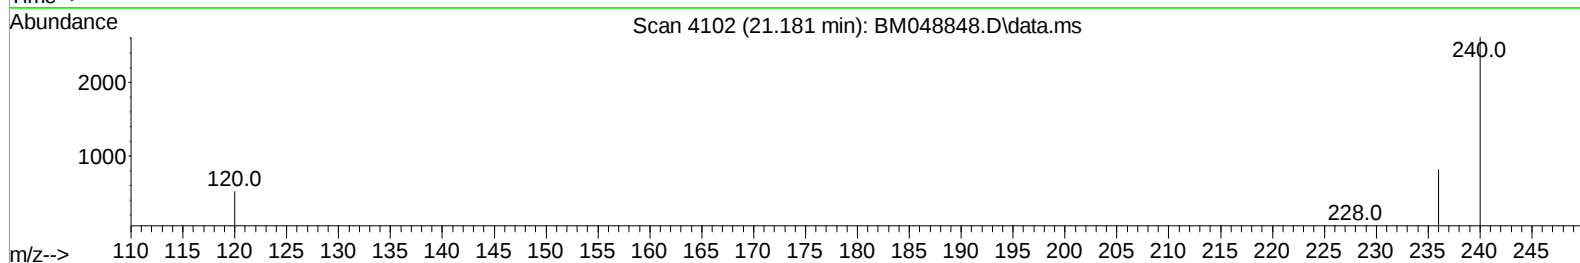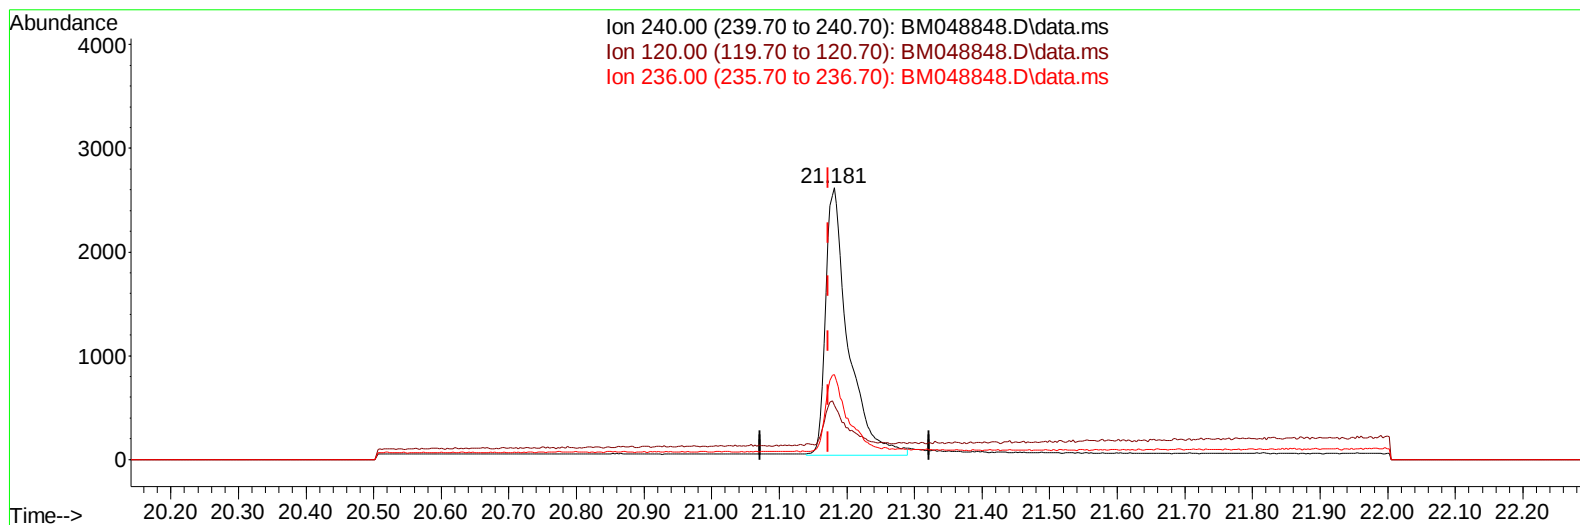

TIC: BM048848.D\data.ms

(17) Chrysene-d12

21.181min (+ 0.009) 0.40 ng/ul m

response 5925

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	20.02
236.00	32.10	31.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048848.D
Acq On : 06 Dec 2024 00:02
Operator : RC/JU
Sample : PB165401BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Manual IntegrationsAPPROVED

Quant Time: Dec 06 01:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

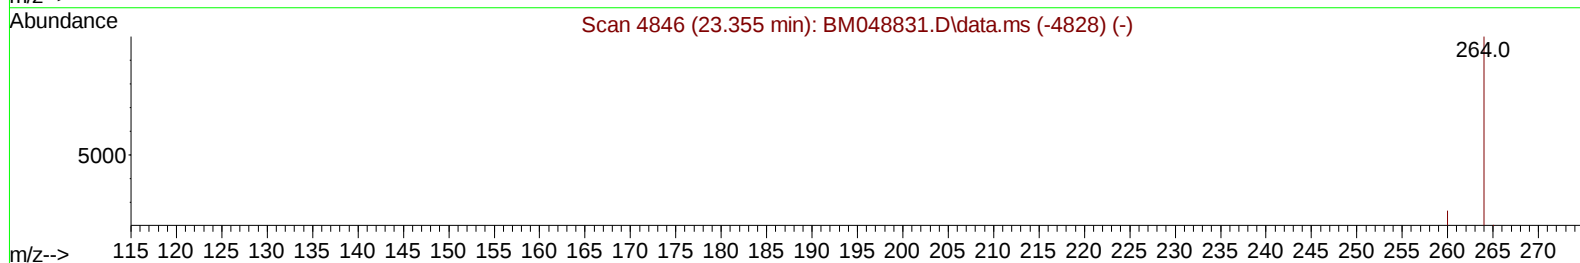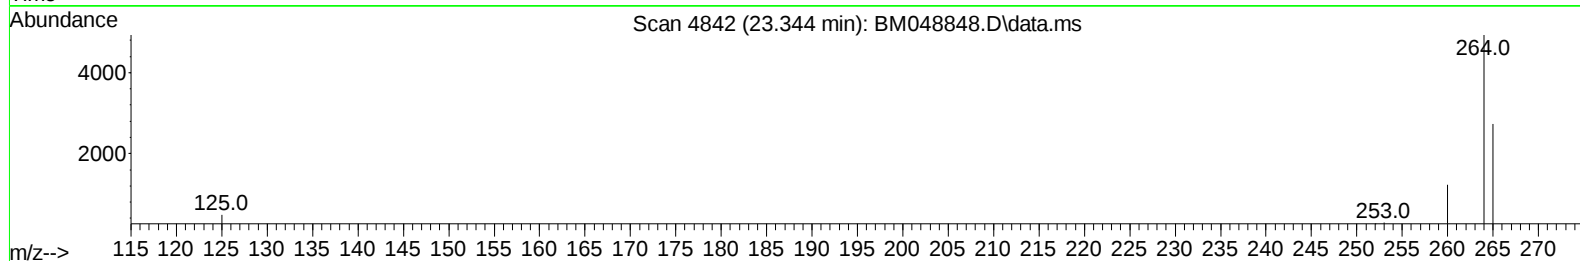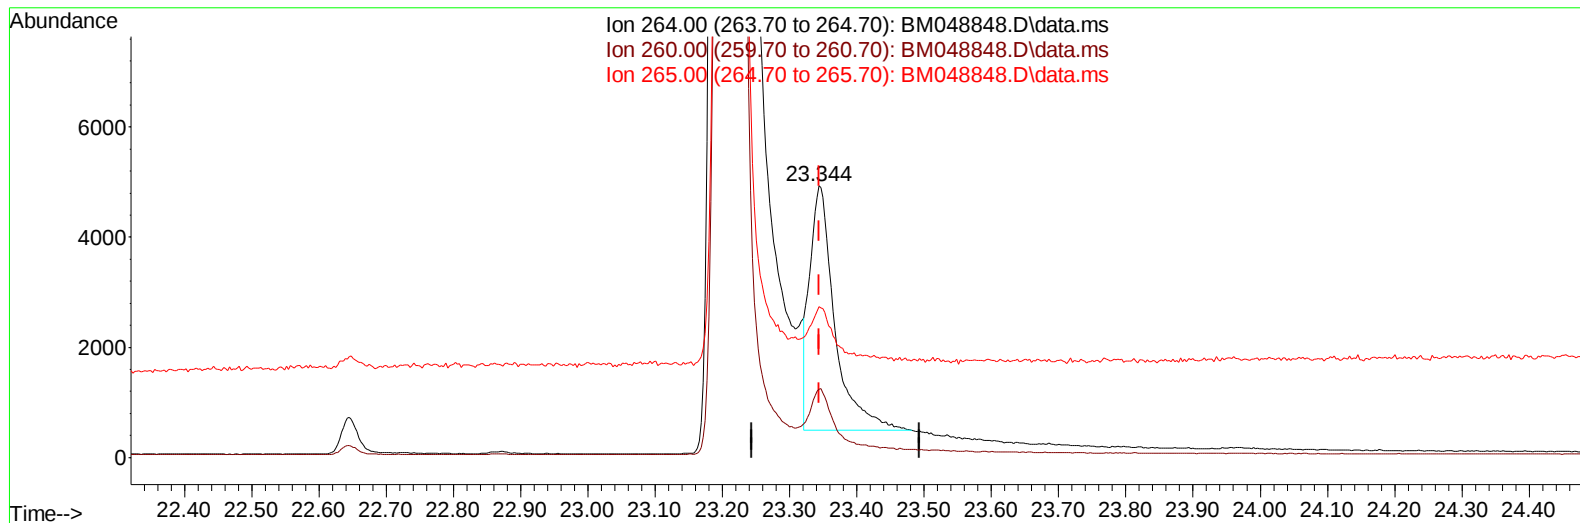

TIC: BM048848.D\data.ms

(23) Perylene-d12 (I)

23.344min (-0.000) 0.40 ng/u1

response 11636

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.07
265.00	78.50	55.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048848.D
Acq On : 06 Dec 2024 00:02
Operator : RC/JU
Sample : PB165401BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Manual IntegrationsAPPROVED

Quant Time: Dec 06 01:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

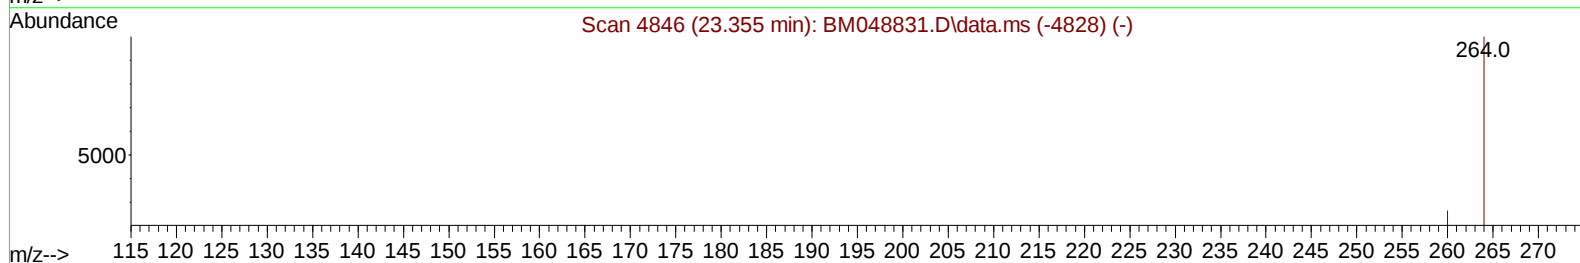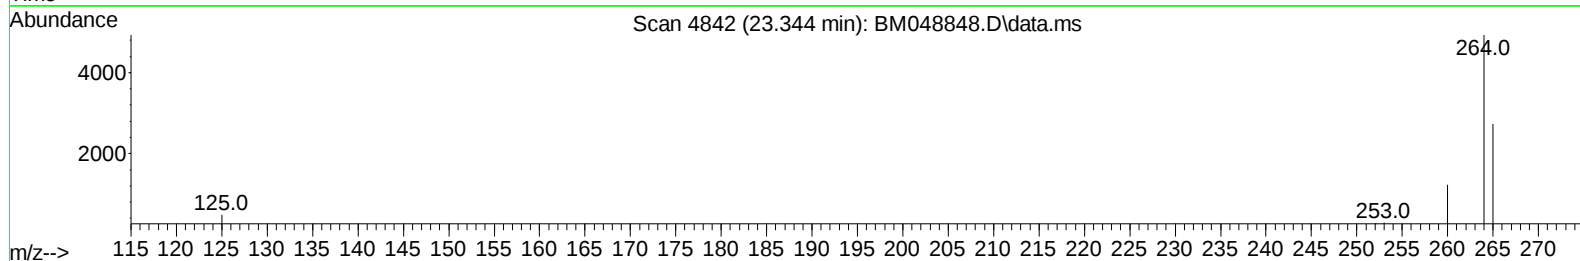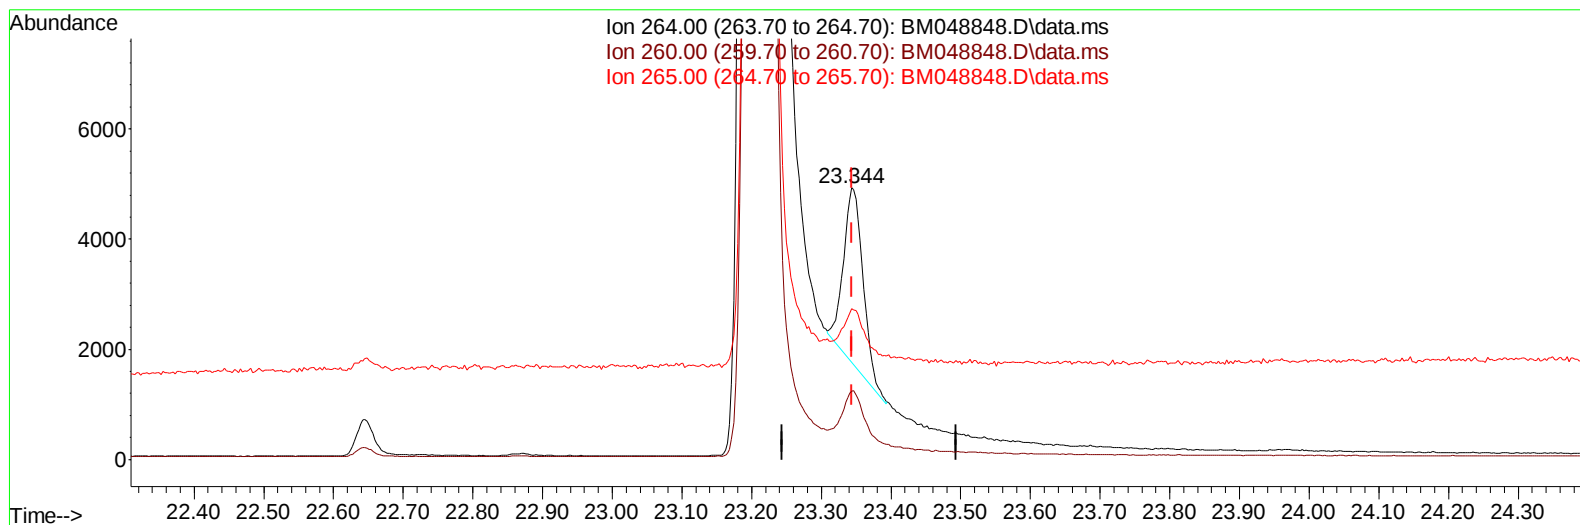

TIC: BM048848.D\data.ms

(23) Perylene-d12 (I)

23.344min (-0.000) 0.40 ng/ul m

response 6107

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.07
265.00	78.50	55.50#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048848.D
 Acq On : 06 Dec 2024 00:02
 Operator : RC/JU
 Sample : PB165401BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK401

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 01:36:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	3833	0.400	ng/ul	0.00
4) Naphthalene-d8	10.358	136	10400	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.228	164	5533	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	10723m	0.400	ng/ul	0.00
17) Chrysene-d12	21.181	240	5925m	0.400	ng/ul	0.00
23) Perylene-d12	23.344	264	6107m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.168	96	28247	5.769	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.969	152	4425	0.354	ng/ul	0.00
18) Fluoranthene-d10	19.010	212	7493	0.410	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048848.D
Acq On : 06 Dec 2024 00:02
Operator : RC/JU
Sample : PB165401BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Manual IntegrationsAPPROVED

Quant Time: Dec 06 01:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

