




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048852.D
Acq On : 06 Dec 2024 02:25
Operator : RC/JU
Sample : P5104-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ69

Manual IntegrationsAPPROVED

Quant Time: Dec 06 03:04:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

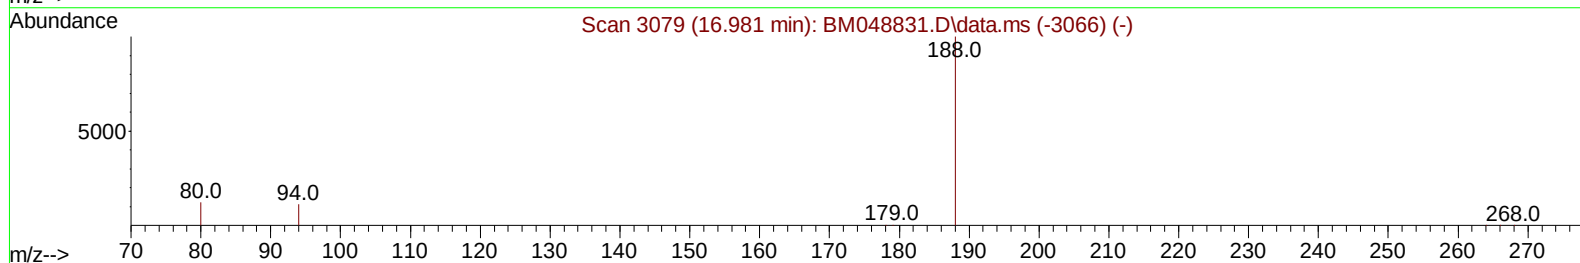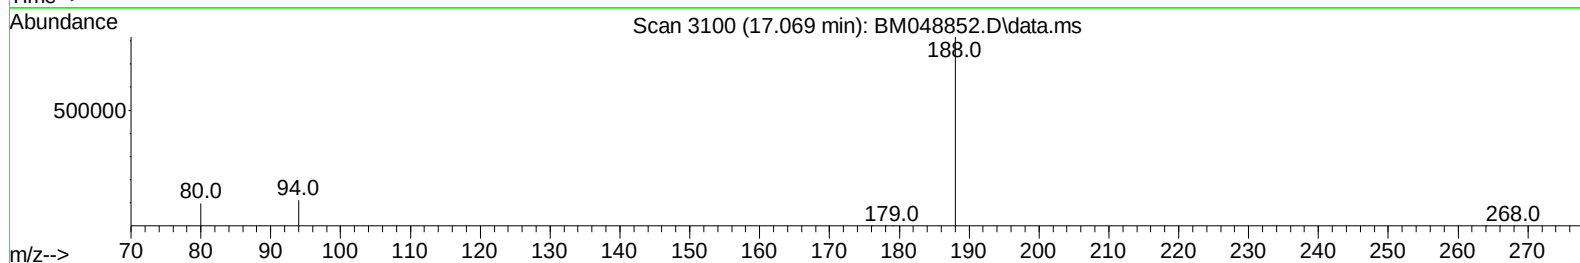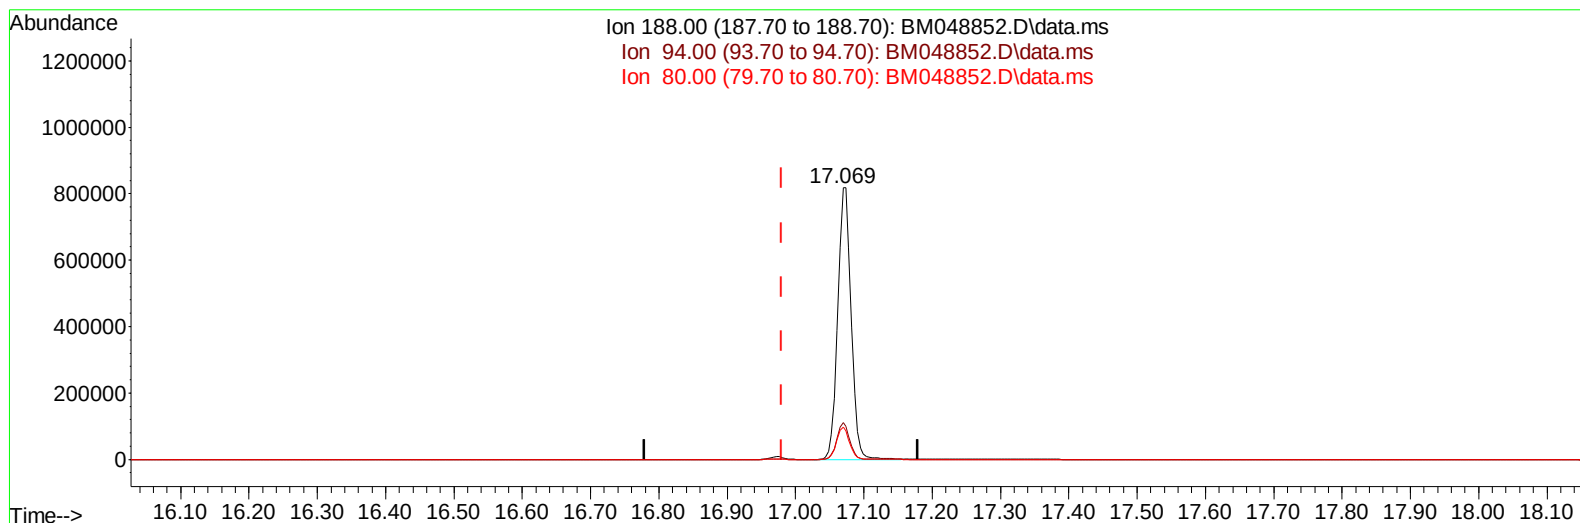

TIC: BM048852.D\data.ms

(13) Phenanthrene-d10 (I)

17.069min (+ 0.090) 0.40 ng/u1

response 1106542

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	13.68
80.00	12.50	11.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048852.D
Acq On : 06 Dec 2024 02:25
Operator : RC/JU
Sample : P5104-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ69

Manual IntegrationsAPPROVED

Quant Time: Dec 06 03:04:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

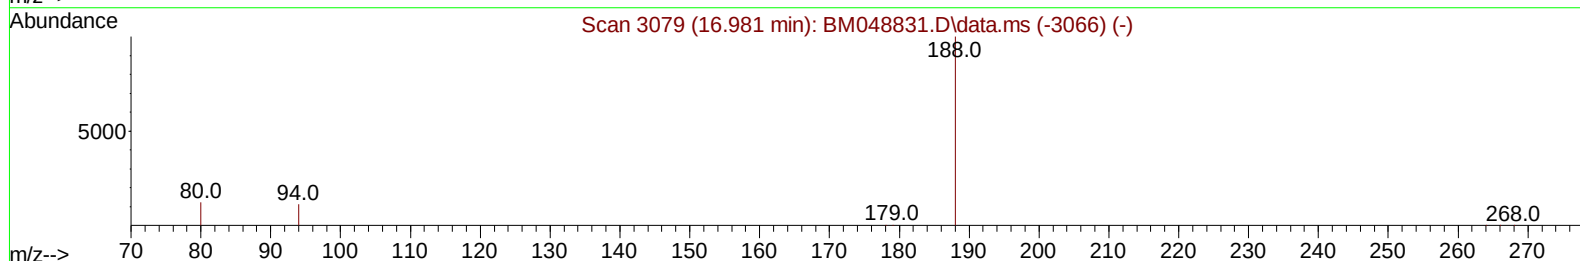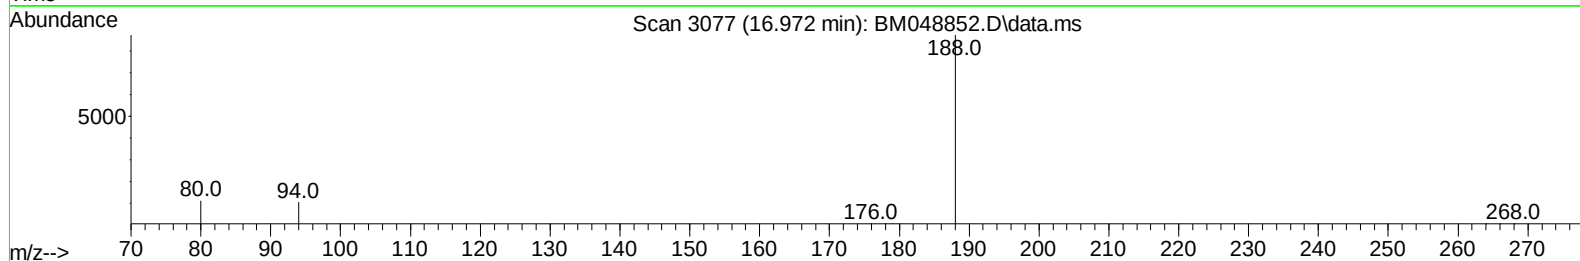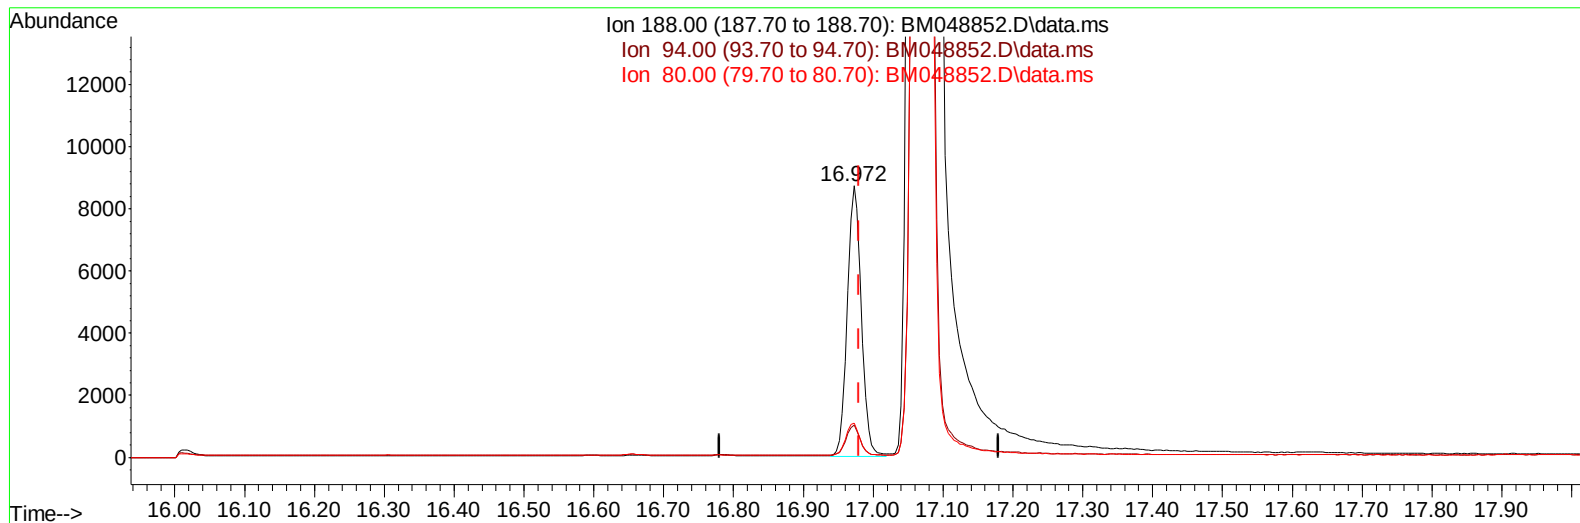

TIC: BM048852.D\data.ms

(13) Phenanthrene-d10 (I)

16.972min (-0.007) 0.40 ng/ul m

response 12118

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.01
80.00	12.50	12.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048852.D
Acq On : 06 Dec 2024 02:25
Operator : RC/JU
Sample : P5104-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ69

Manual IntegrationsAPPROVED

Quant Time: Dec 06 03:04:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

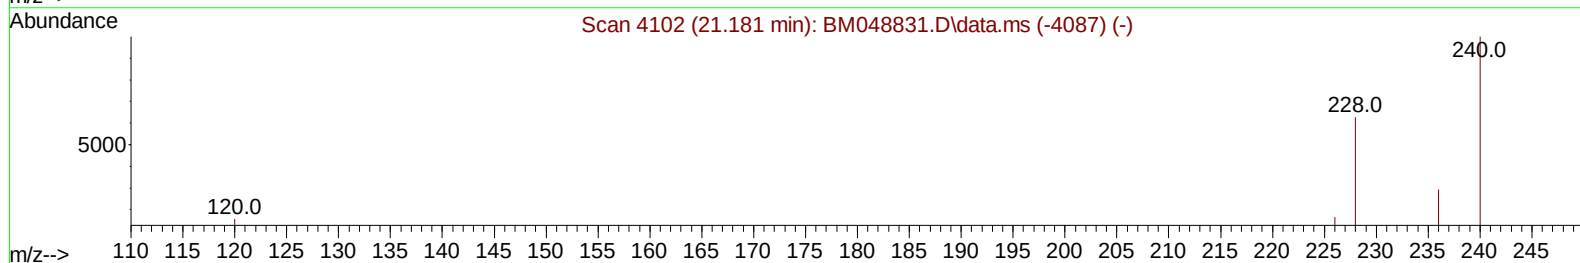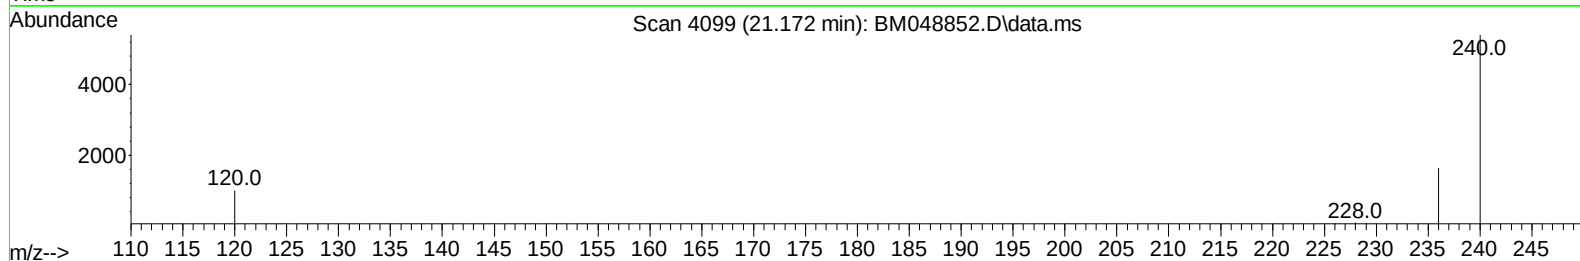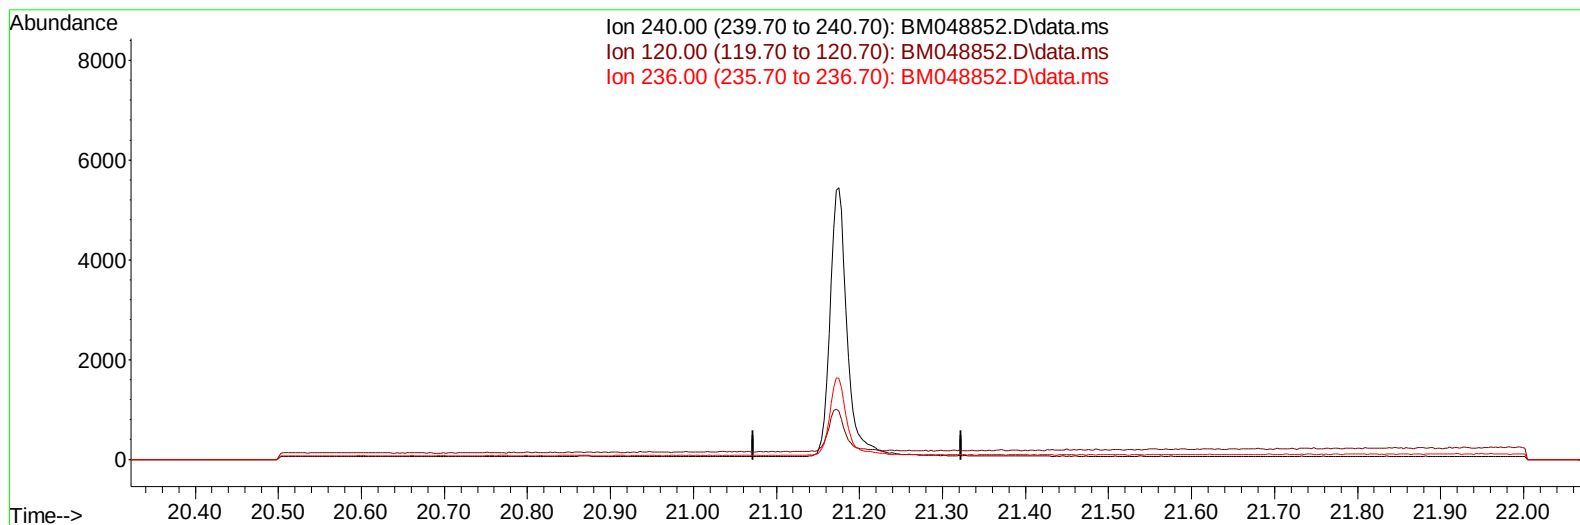

TIC: BM048852.D\data.ms

(17) Chrysene-d12

21.173min (-21.173) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048852.D
Acq On : 06 Dec 2024 02:25
Operator : RC/JU
Sample : P5104-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ69

Manual IntegrationsAPPROVED

Quant Time: Dec 06 03:04:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

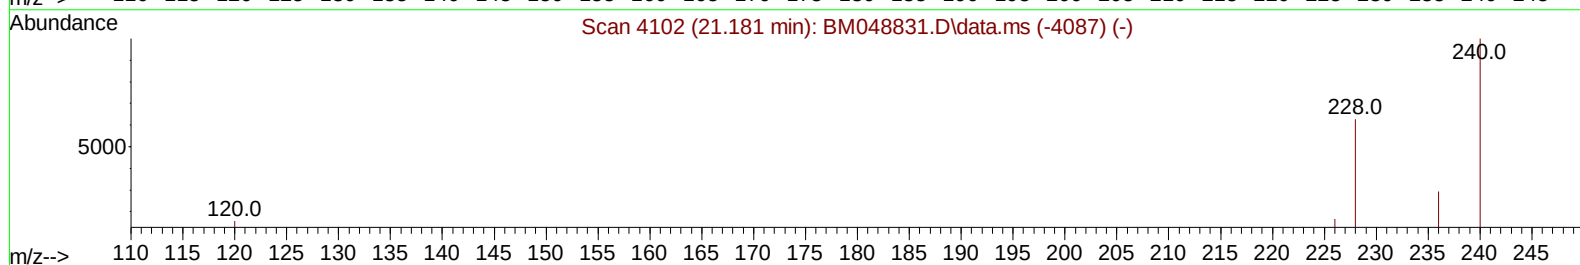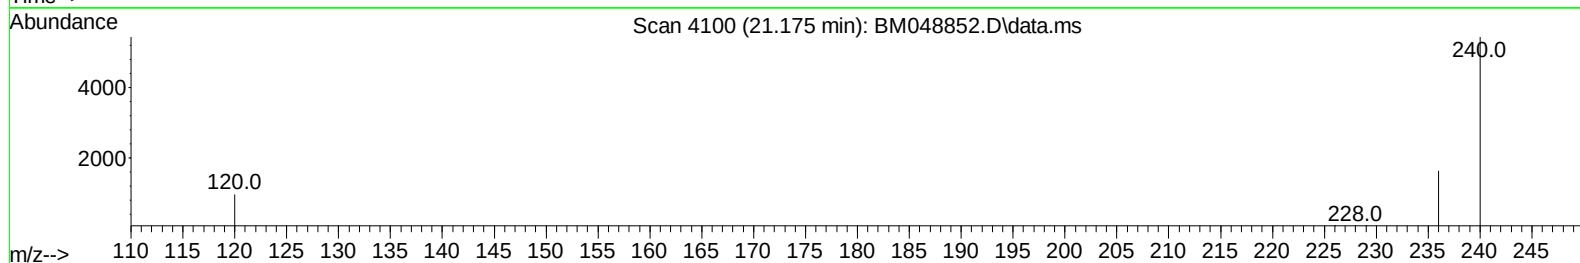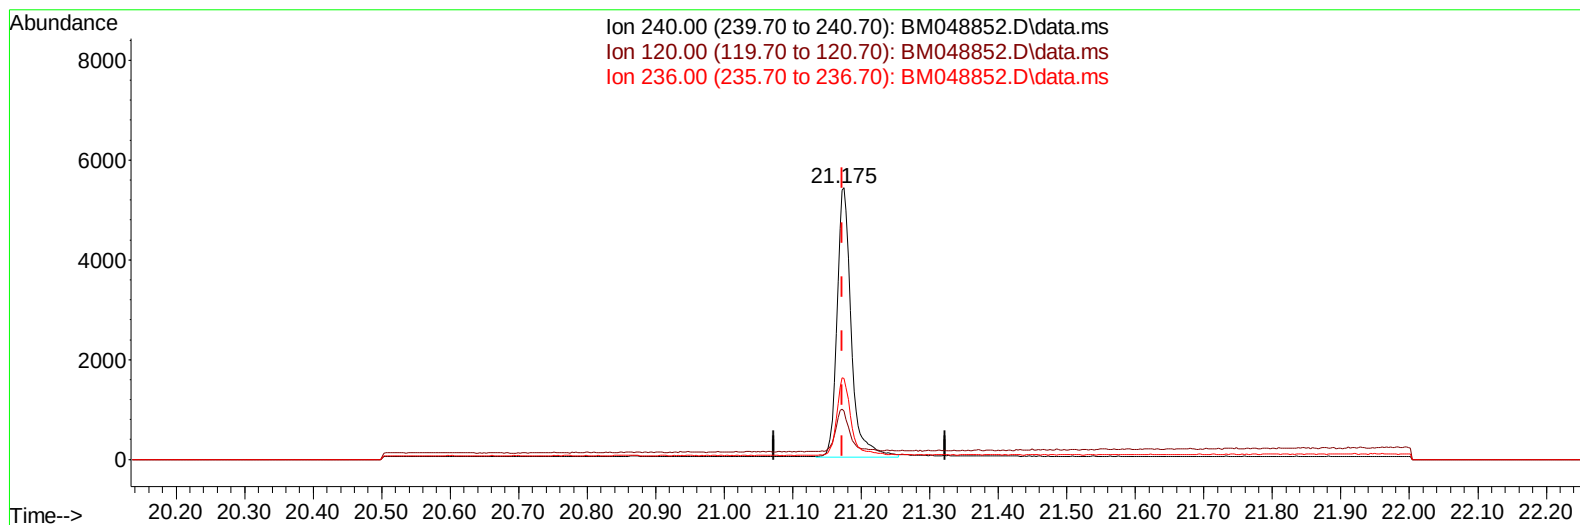

TIC: BM048852.D\data.ms

(17) Chrysene-d12

21.175min (+ 0.002) 0.40 ng/ul m

response 7789

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	17.75
236.00	32.10	29.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048852.D
Acq On : 06 Dec 2024 02:25
Operator : RC/JU
Sample : P5104-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ69

Manual IntegrationsAPPROVED

Quant Time: Dec 06 03:04:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

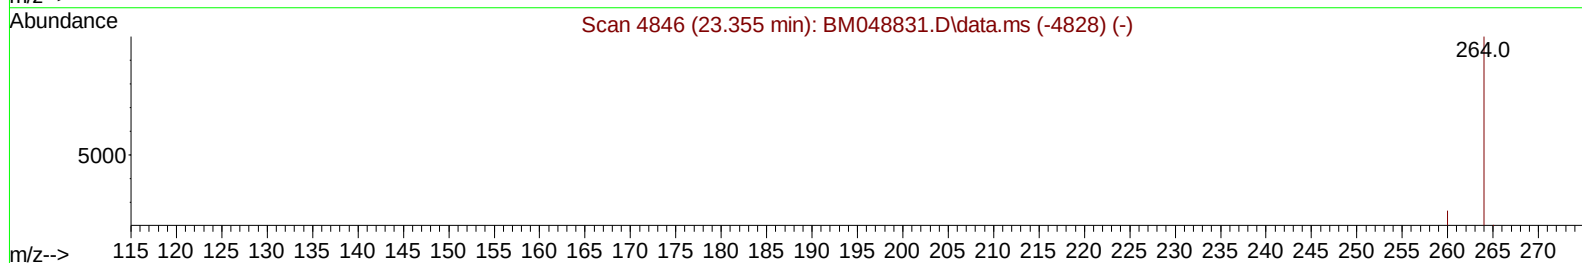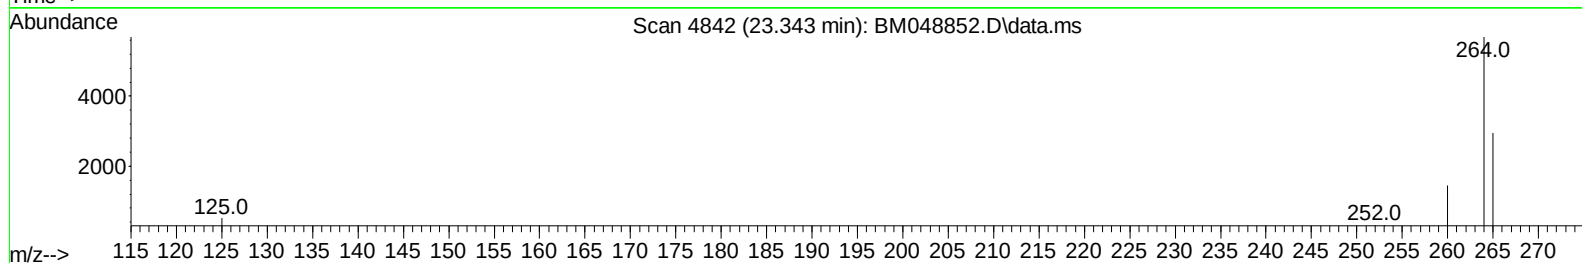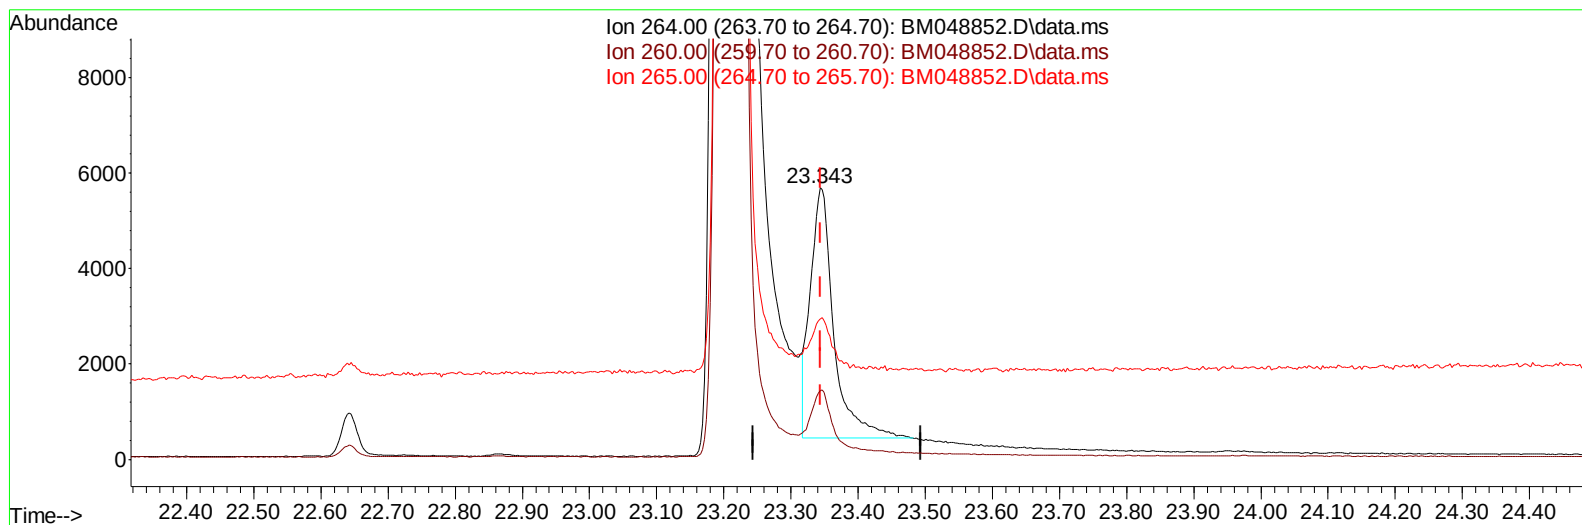

TIC: BM048852.D\data.ms

(23) Perylene-d12 (I)

23.343min (-0.000) 0.40 ng/u1

response 12782

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.43
265.00	78.50	51.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048852.D
Acq On : 06 Dec 2024 02:25
Operator : RC/JU
Sample : P5104-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ69

Manual IntegrationsAPPROVED

Quant Time: Dec 06 03:04:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

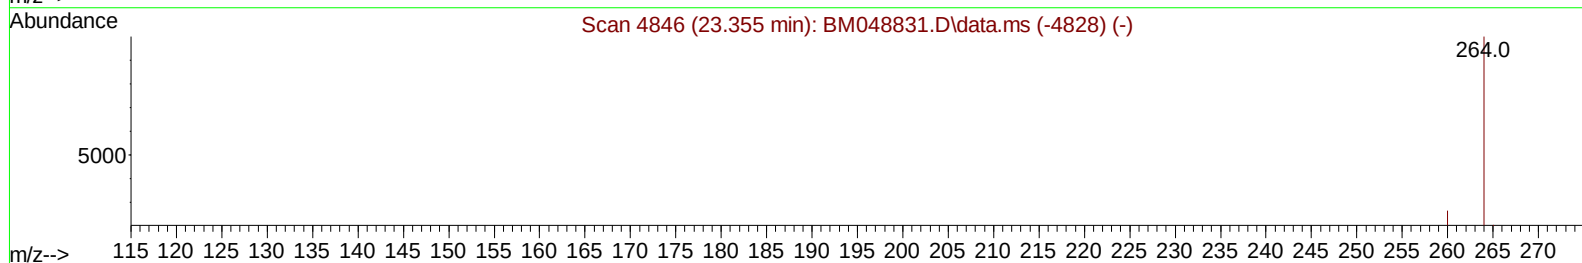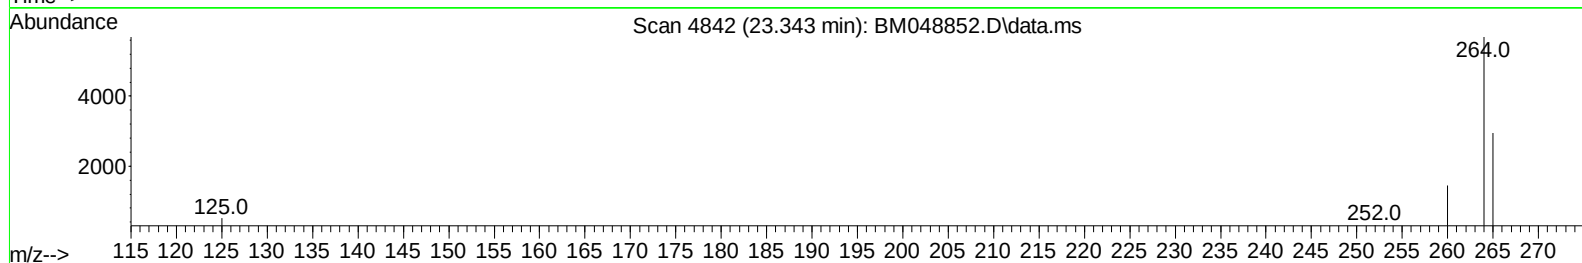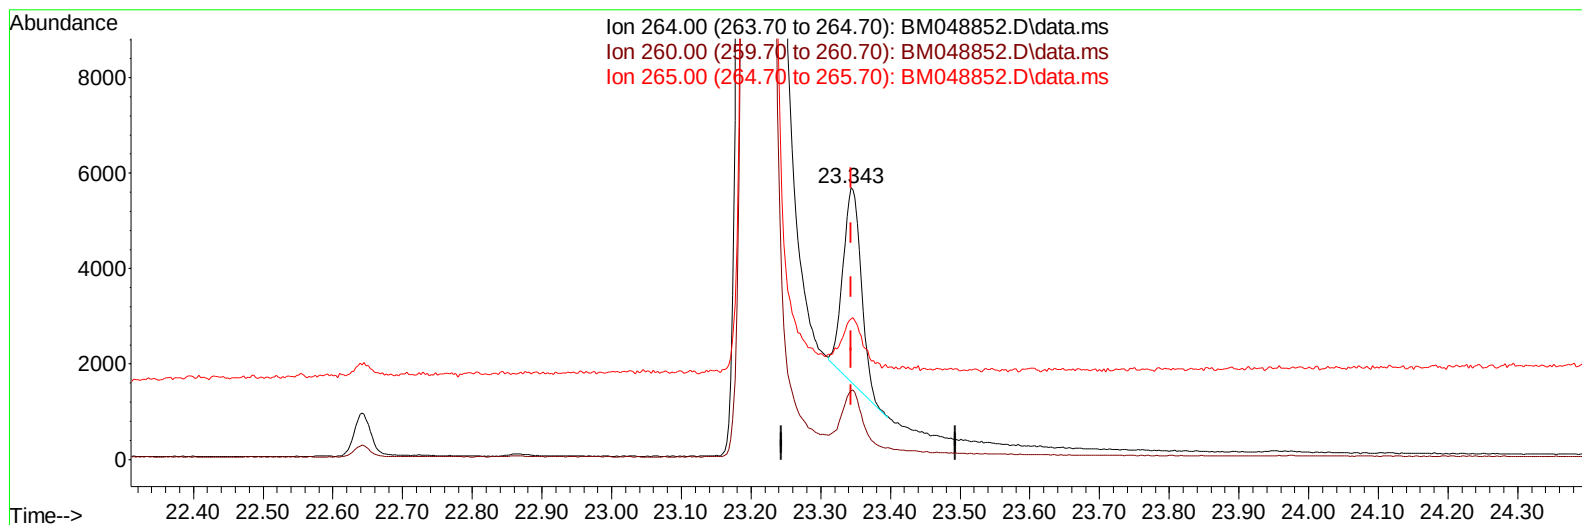

TIC: BM048852.D\data.ms

(23) Perylene-d12 (I)

23.343min (-0.000) 0.40 ng/ul m

response 7352

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.43
265.00	78.50	51.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048852.D
 Acq On : 06 Dec 2024 02:25
 Operator : RC/JU
 Sample : P5104-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHJ69

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 03:04:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.594	152		3968	0.400	ng/ul	0.00
4) Naphthalene-d8	10.359	136		11213	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.224	164		6126	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.972	188		12118m	0.400	ng/ul	0.00
17) Chrysene-d12	21.175	240		7789m	0.400	ng/ul	0.00
23) Perylene-d12	23.343	264		7352m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.168	96		21826	4.306	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.959	152		4392	0.325	ng/ul	0.00
18) Fluoranthene-d10	19.007	212		9167	0.381	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.202	88		261	0.044	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048852.D
Acq On : 06 Dec 2024 02:25
Operator : RC/JU
Sample : P5104-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ69

Manual IntegrationsAPPROVED

Quant Time: Dec 06 03:04:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

