




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048861.D
Acq On : 06 Dec 2024 10:56
Operator : RC/JU
Sample : PB165412BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Manual IntegrationsAPPROVED

Quant Time: Dec 06 12:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

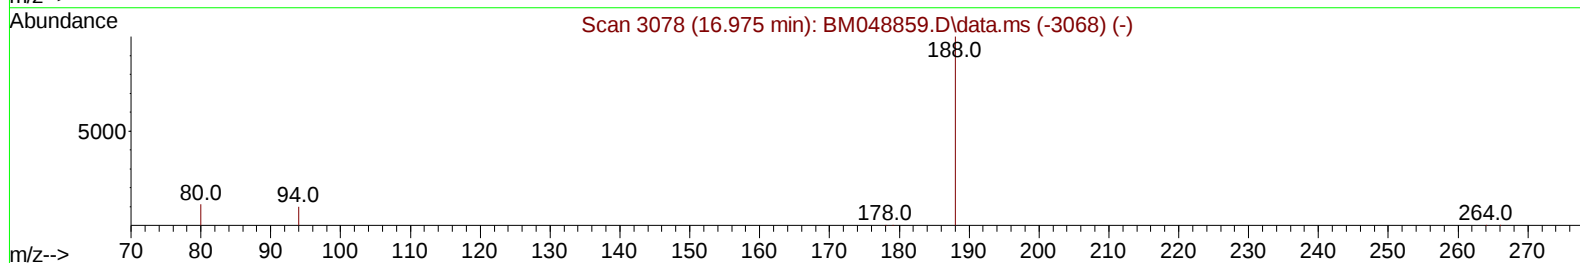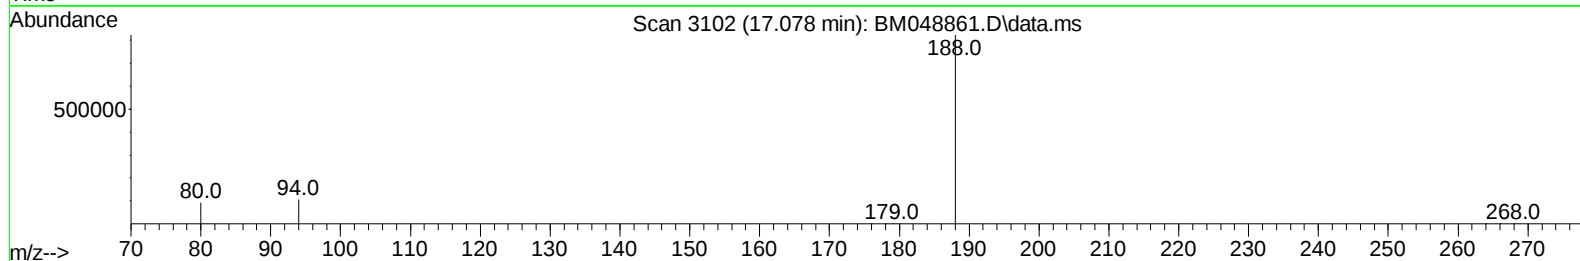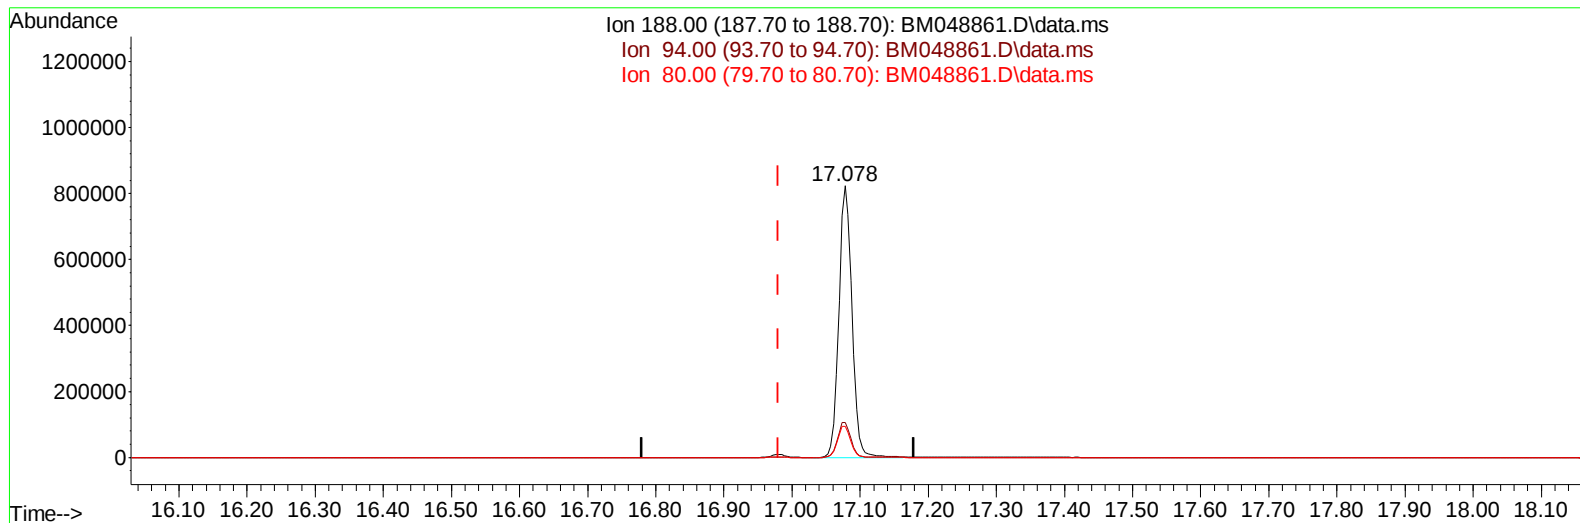

TIC: BM048861.D\data.ms

(13) Phenanthrene-d10 (I)

17.078min (+ 0.098) 0.40 ng/u1

response 1095950

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.81
80.00	12.50	11.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048861.D
Acq On : 06 Dec 2024 10:56
Operator : RC/JU
Sample : PB165412BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Manual IntegrationsAPPROVED

Quant Time: Dec 06 12:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

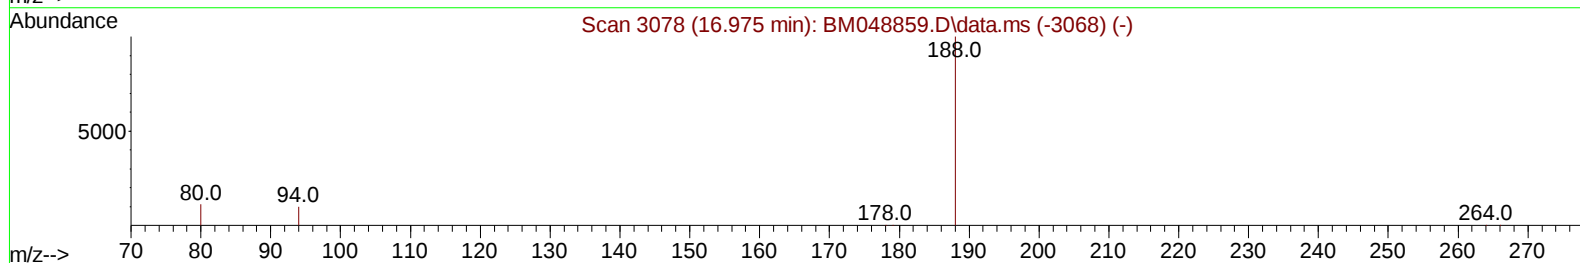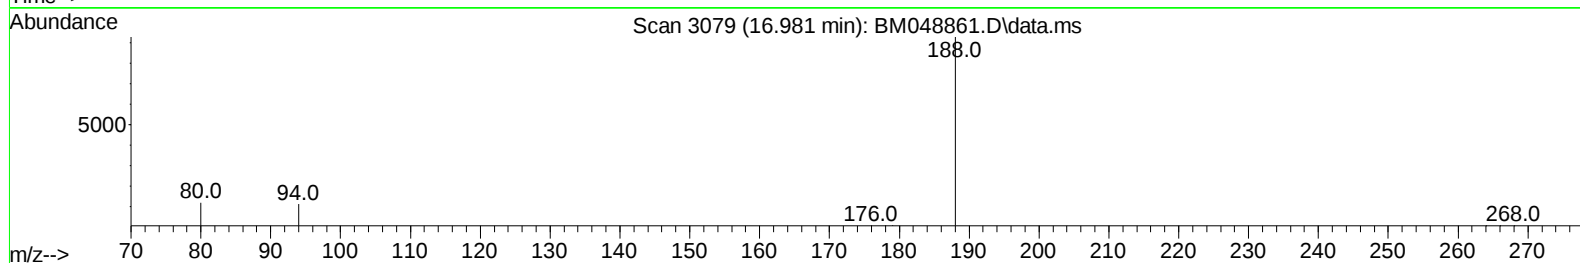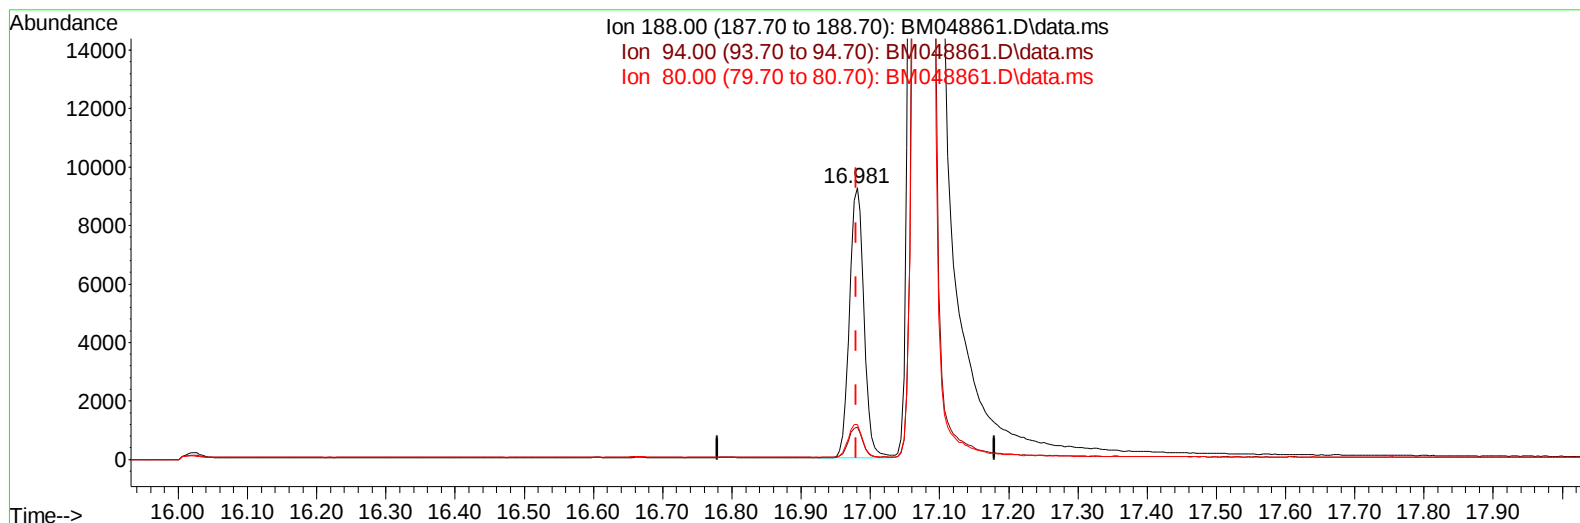

TIC: BM048861.D\data.ms

(13) Phenanthrene-d10 (I)

16.981min (+ 0.001) 0.40 ng/ul m

response 13350

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	11.95
80.00	12.50	12.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048861.D
Acq On : 06 Dec 2024 10:56
Operator : RC/JU
Sample : PB165412BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Manual IntegrationsAPPROVED

Quant Time: Dec 06 12:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

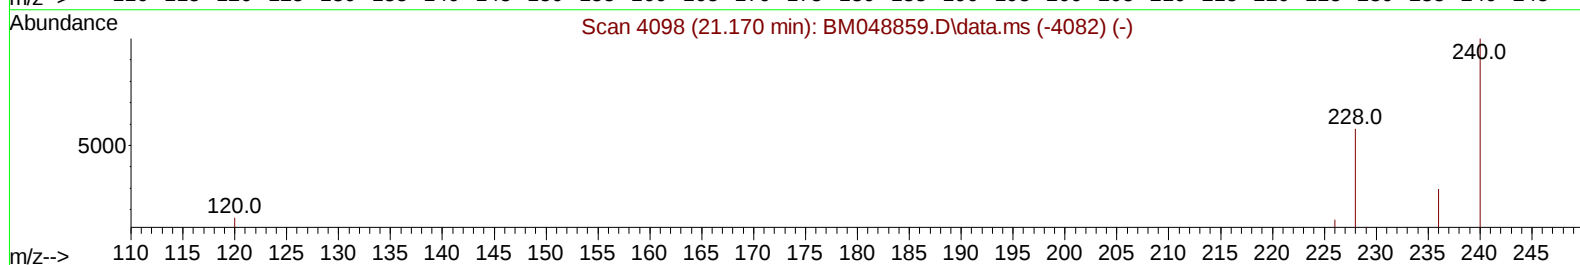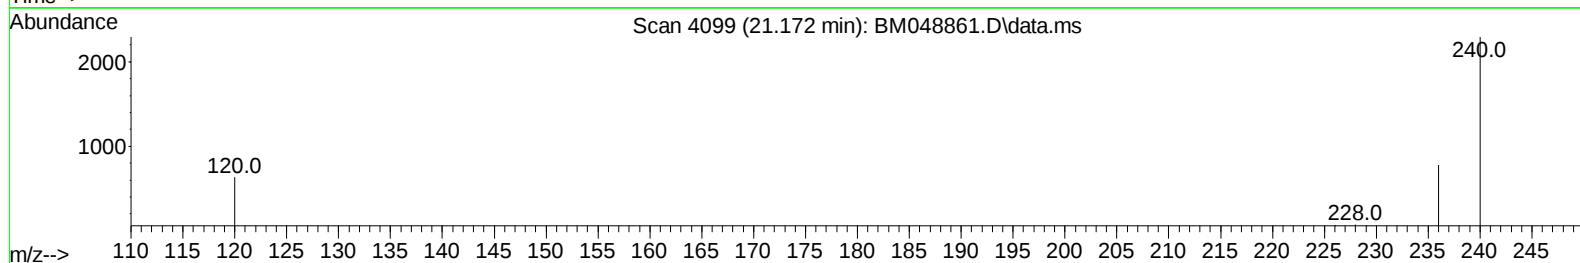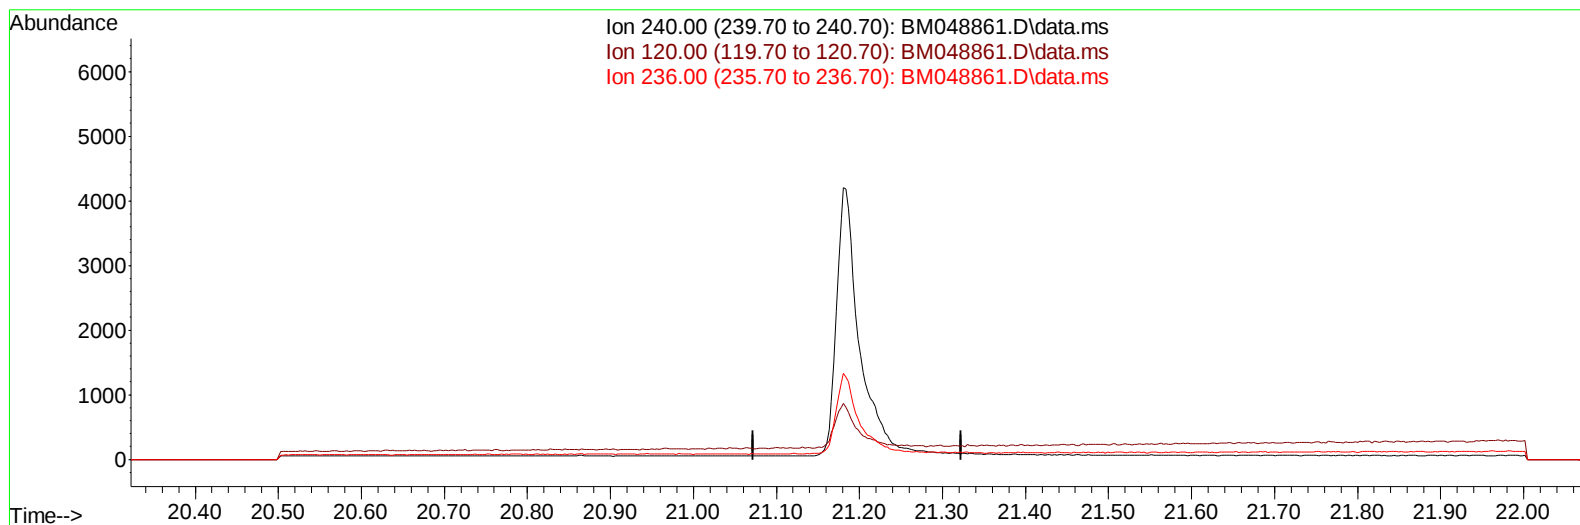

TIC: BM048861.D\data.ms

(17) Chrysene-d12

21.173min (-21.173) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048861.D
Acq On : 06 Dec 2024 10:56
Operator : RC/JU
Sample : PB165412BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Manual IntegrationsAPPROVED

Quant Time: Dec 06 12:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

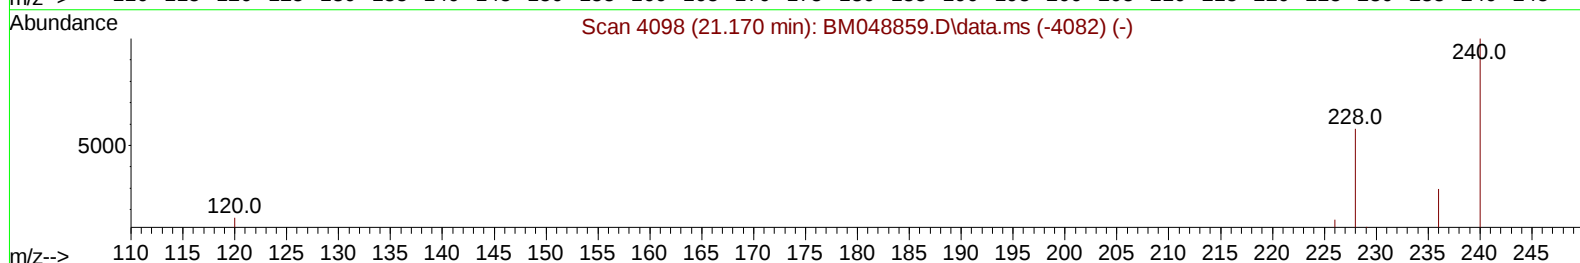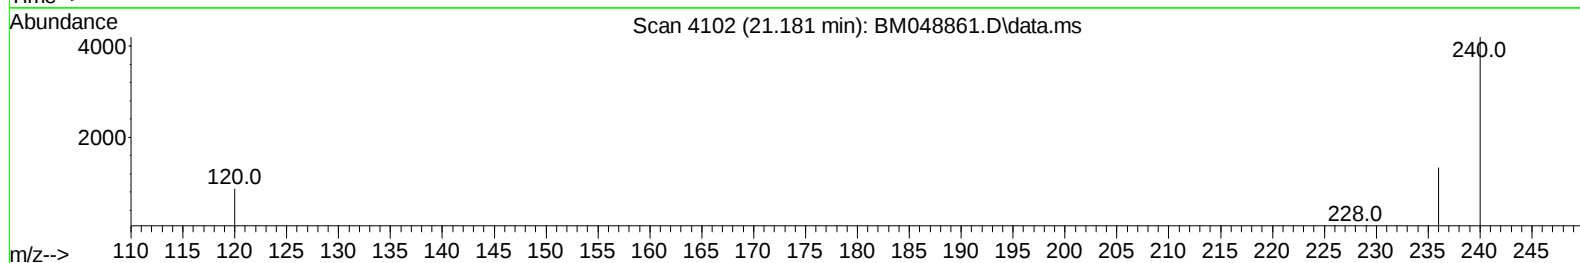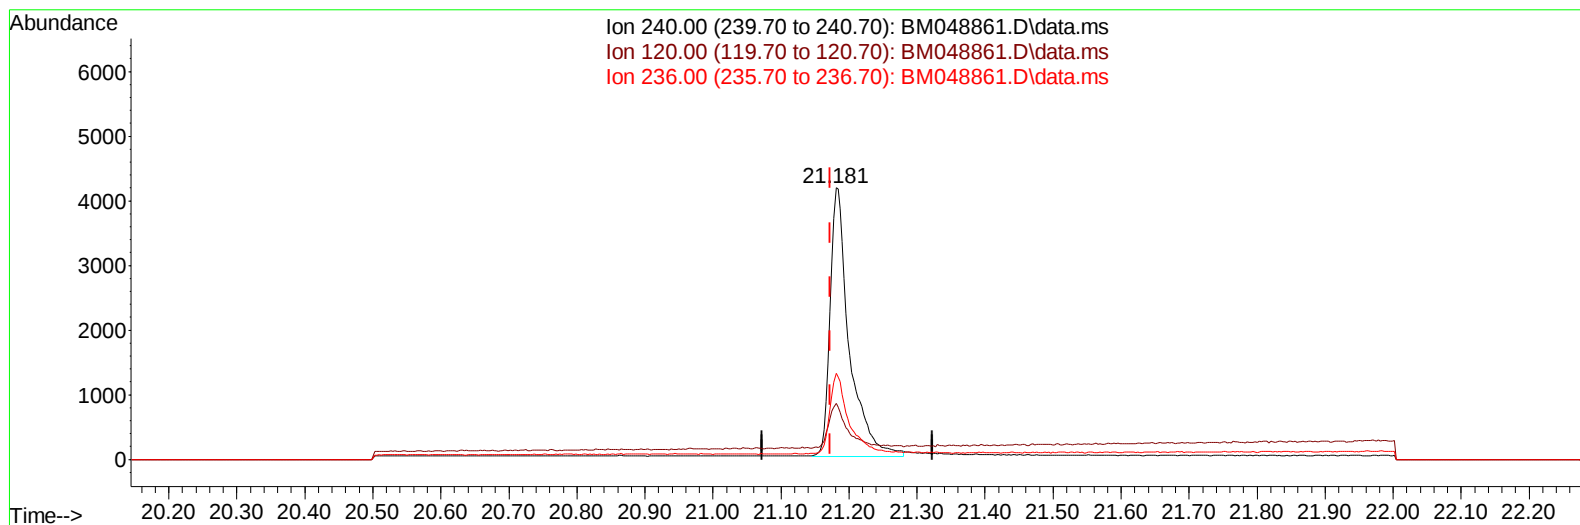

TIC: BM048861.D\data.ms

(17) Chrysene-d12

21.181min (+ 0.008) 0.40 ng/ul m

response 8082

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	20.62
236.00	32.10	31.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048861.D
Acq On : 06 Dec 2024 10:56
Operator : RC/JU
Sample : PB165412BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 12:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

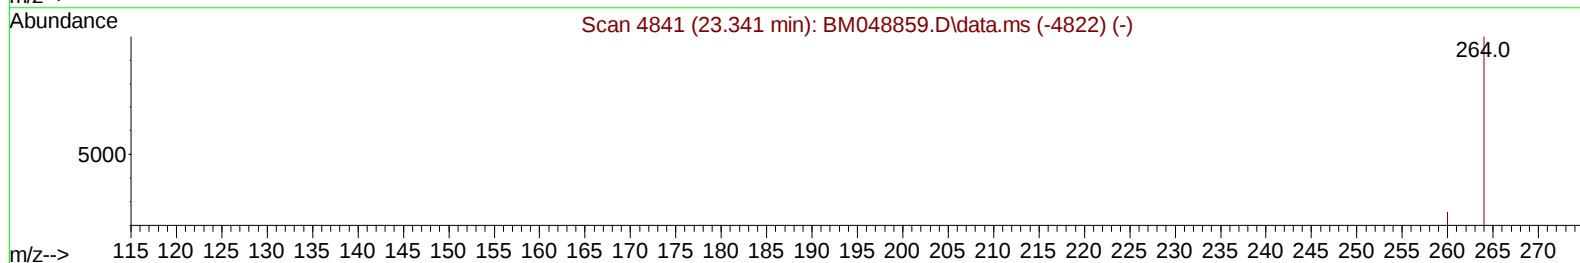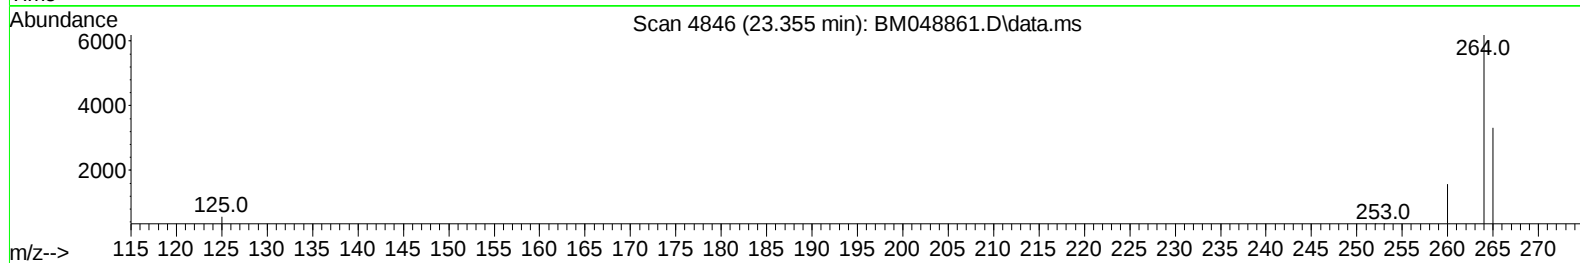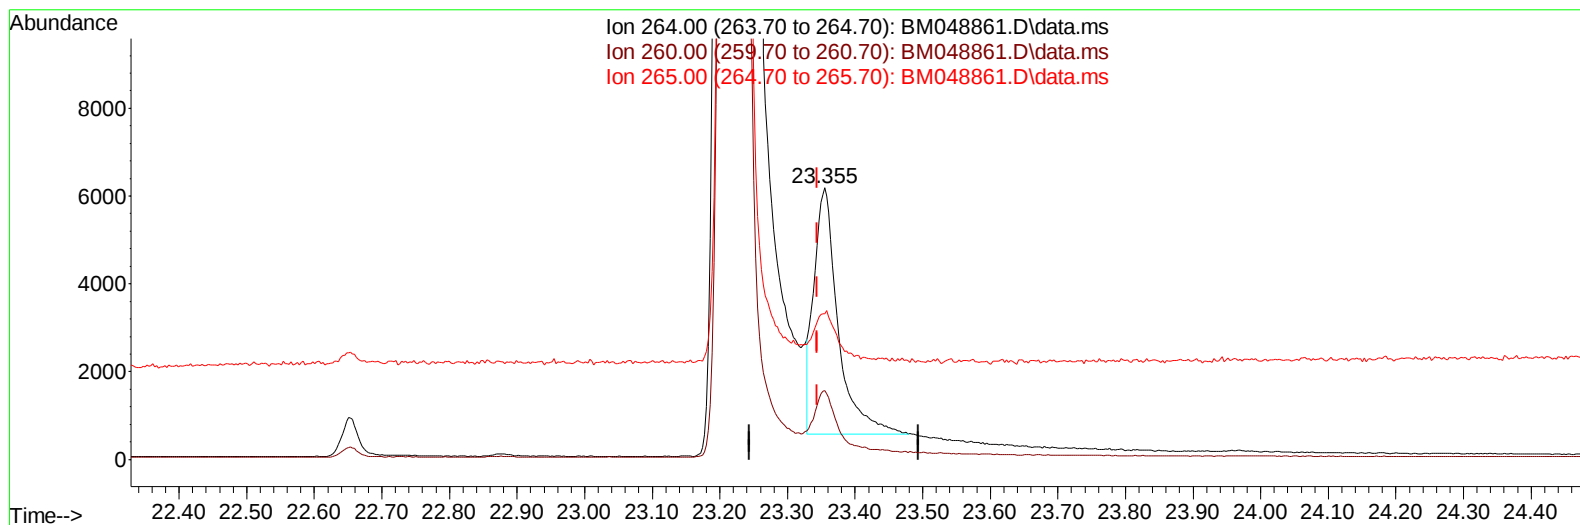

TIC: BM048861.D\data.ms

(23) Perylene-d12 (I)

23.355min (+ 0.011) 0.40 ng/ul

response 13955

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.43
265.00	78.50	53.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048861.D
Acq On : 06 Dec 2024 10:56
Operator : RC/JU
Sample : PB165412BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 12:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

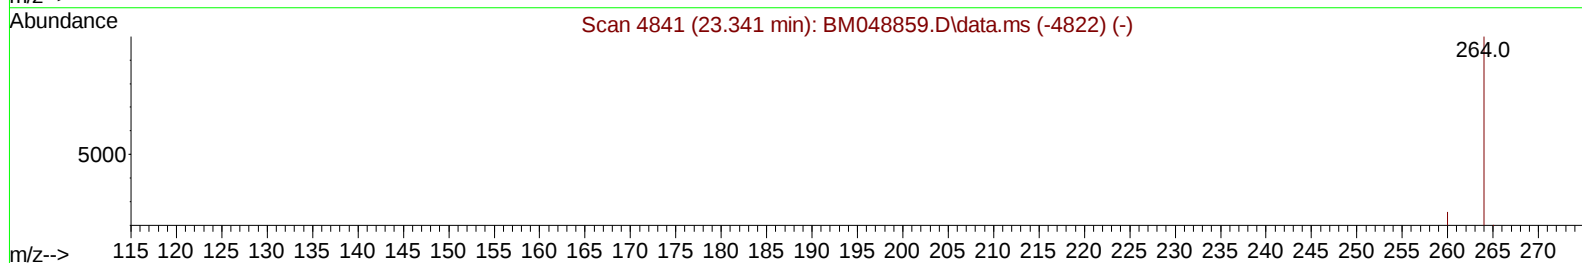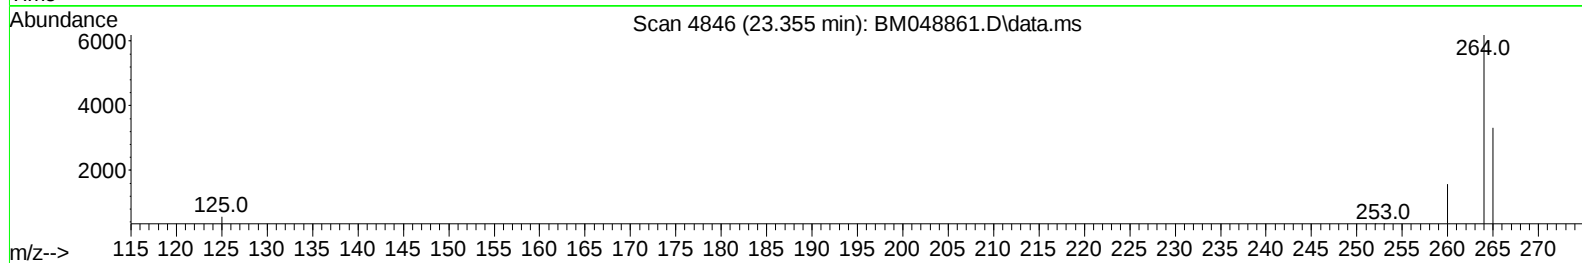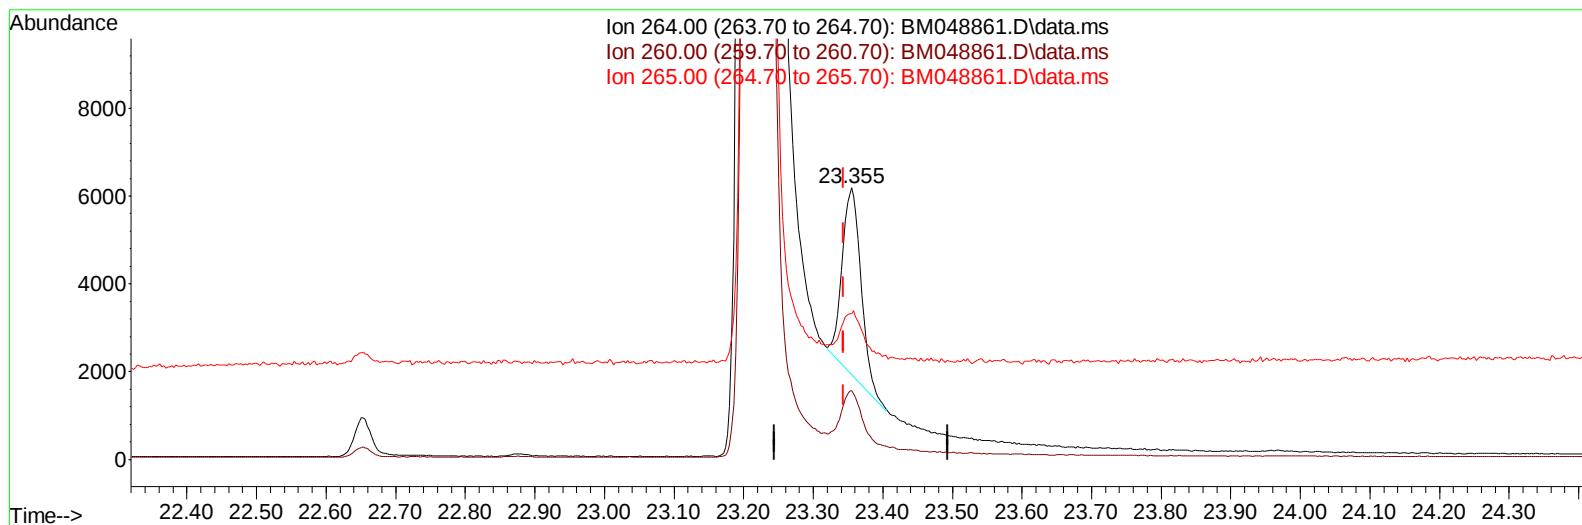

TIC: BM048861.D\data.ms

(23) Perylene-d12 (I)

23.355min (+ 0.011) 0.40 ng/ul m

response 7897

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.43
265.00	78.50	53.63#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048861.D
 Acq On : 06 Dec 2024 10:56
 Operator : RC/JU
 Sample : PB165412BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK412

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 12:25:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	5113	0.400	ng/ul	0.00
4) Naphthalene-d8	10.365	136	13580	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.234	164	6857	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.981	188	13350m	0.400	ng/ul	0.00
17) Chrysene-d12	21.181	240	8082m	0.400	ng/ul	0.00
23) Perylene-d12	23.355	264	7897m	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.168	96	38732	5.930	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.965	152	5549	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.016	212	9099	0.365	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048861.D
Acq On : 06 Dec 2024 10:56
Operator : RC/JU
Sample : PB165412BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Manual IntegrationsAPPROVED

Quant Time: Dec 06 12:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

