




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048873.D
Acq On : 06 Dec 2024 18:43
Operator : RC/JU
Sample : PB165418BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:53:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

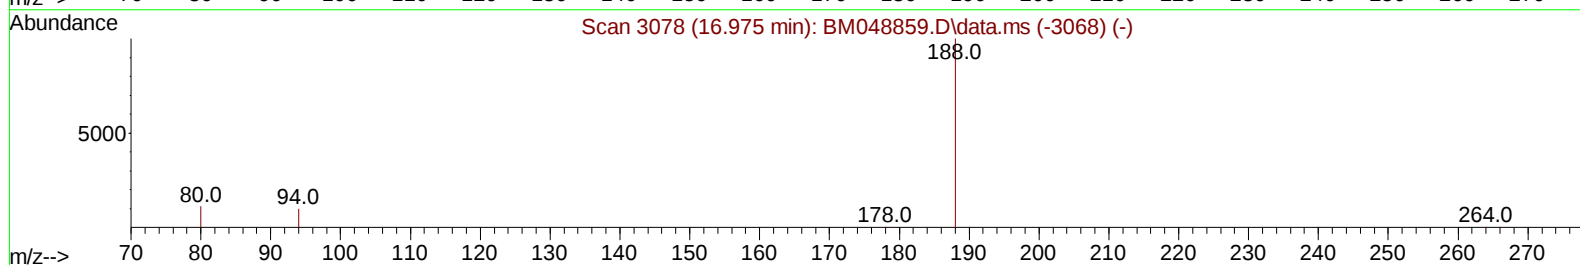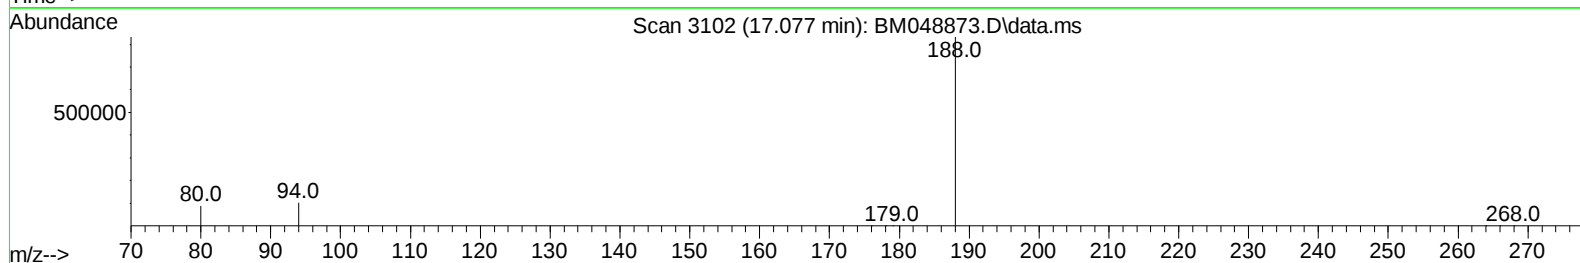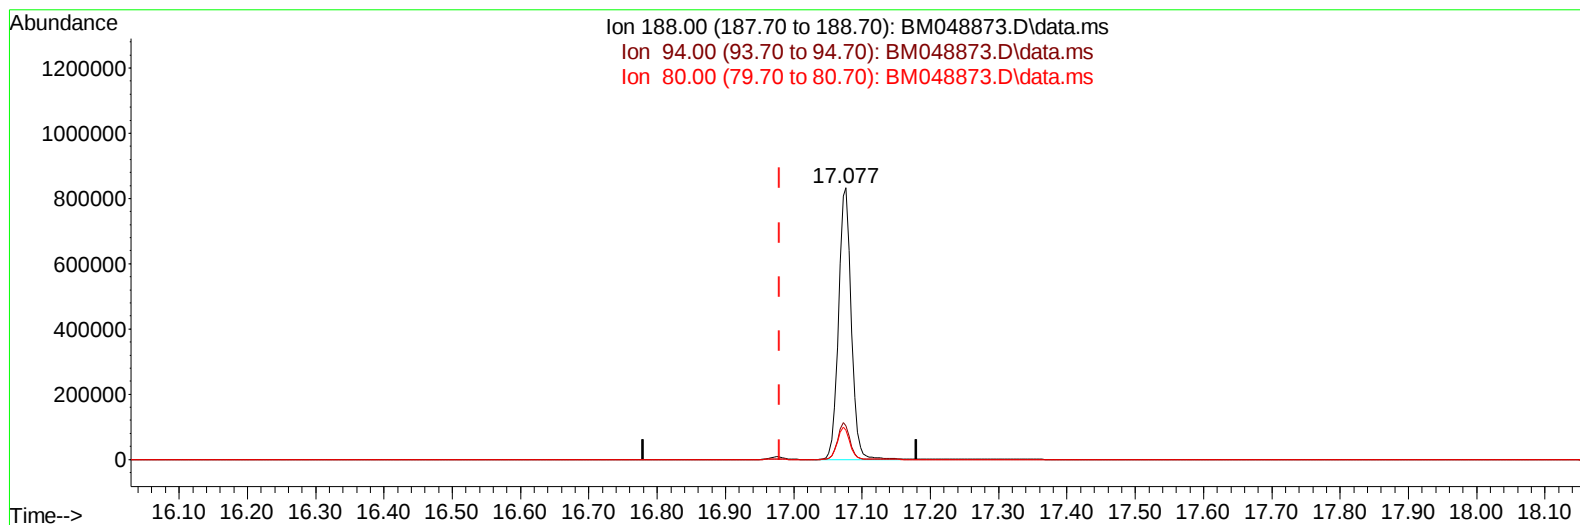

TIC: BM048873.D\data.ms

(13) Phenanthrene-d10 (I)

17.077min (+ 0.097) 0.40 ng/u1

response 1074662

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.32
80.00	12.50	10.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048873.D
Acq On : 06 Dec 2024 18:43
Operator : RC/JU
Sample : PB165418BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:53:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

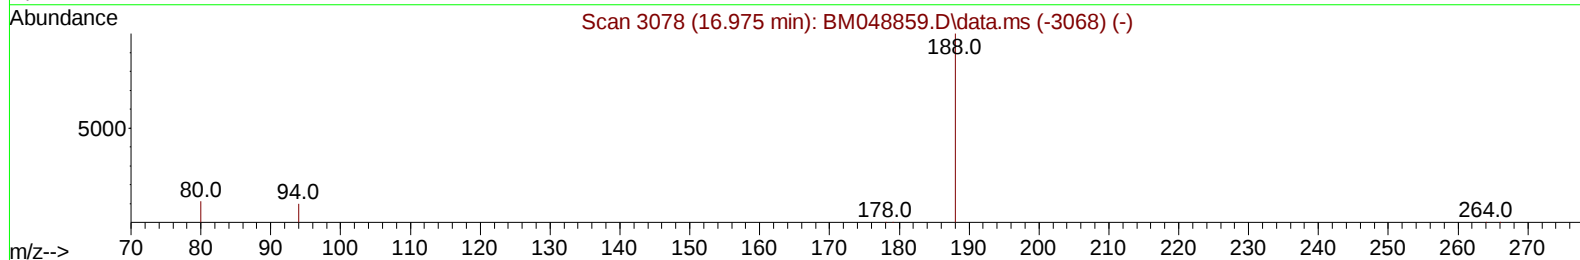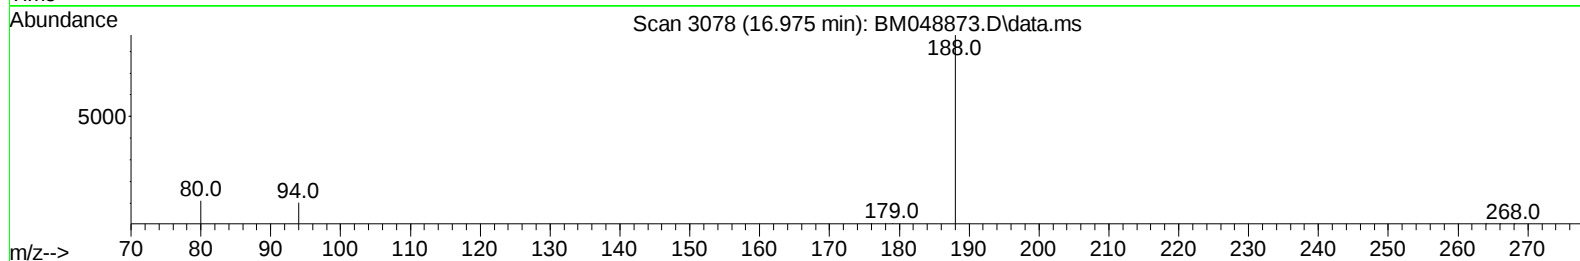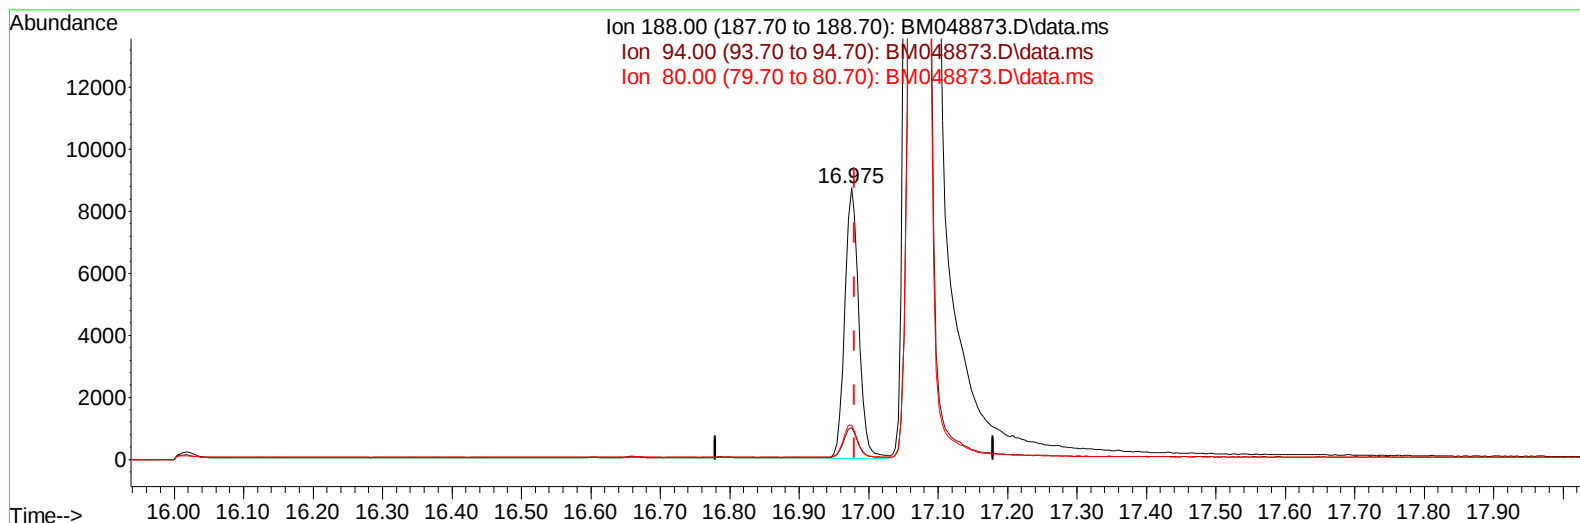

TIC: BM048873.D\data.ms

(13) Phenanthrene-d10 (I)

16.975min (-0.004) 0.40 ng/ul m

response 12167

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	11.61
80.00	12.50	12.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048873.D
Acq On : 06 Dec 2024 18:43
Operator : RC/JU
Sample : PB165418BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:53:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

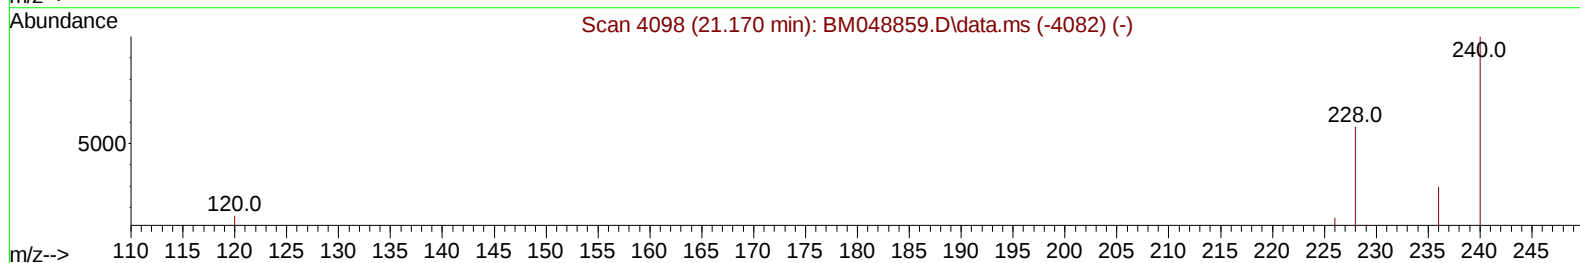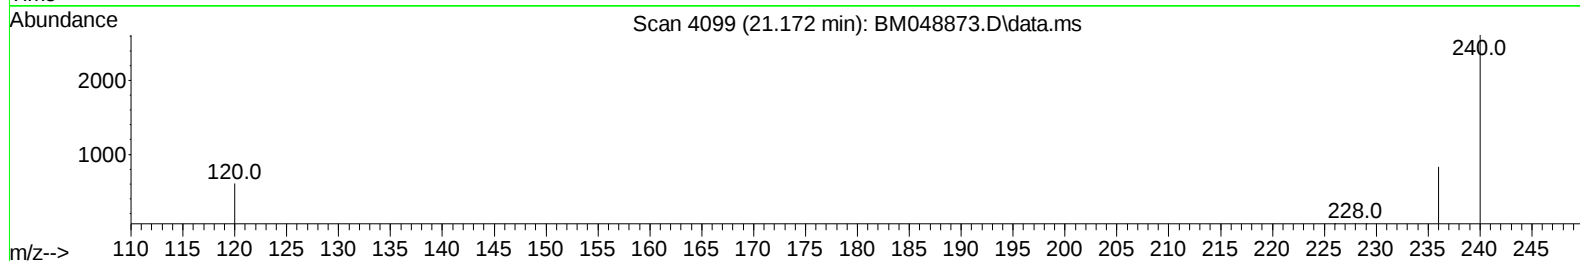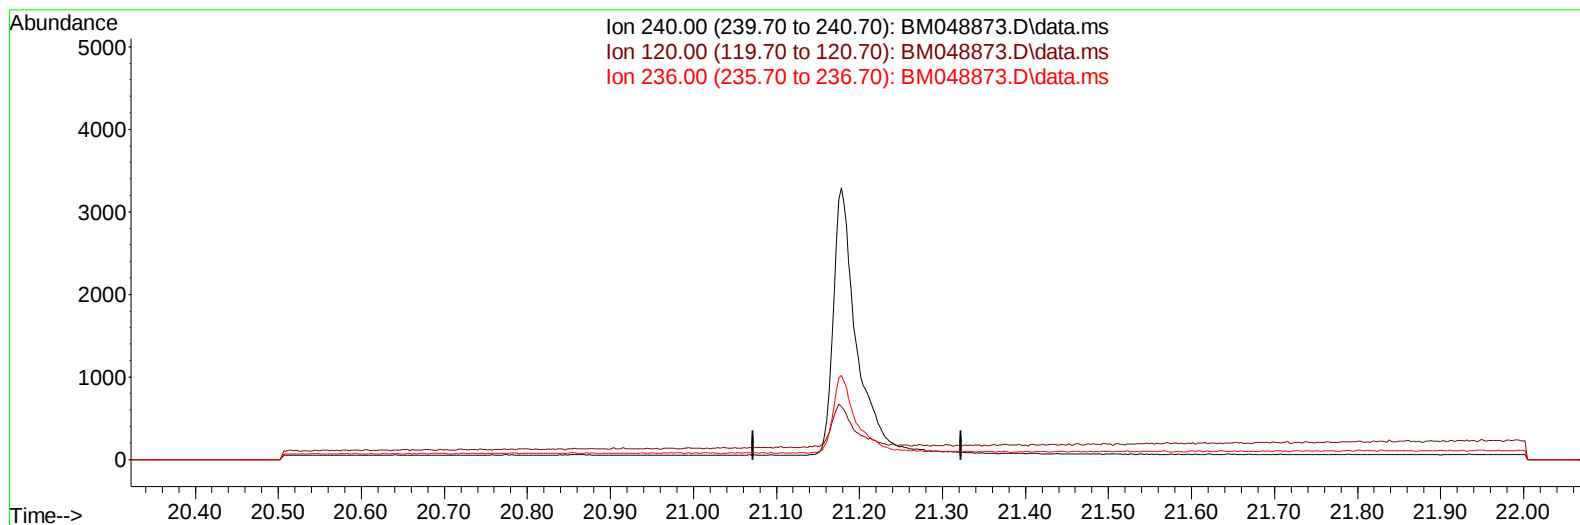

TIC: BM048873.D\data.ms

(17) Chrysene-d12

21.173min (-21.173) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048873.D
Acq On : 06 Dec 2024 18:43
Operator : RC/JU
Sample : PB165418BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:53:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

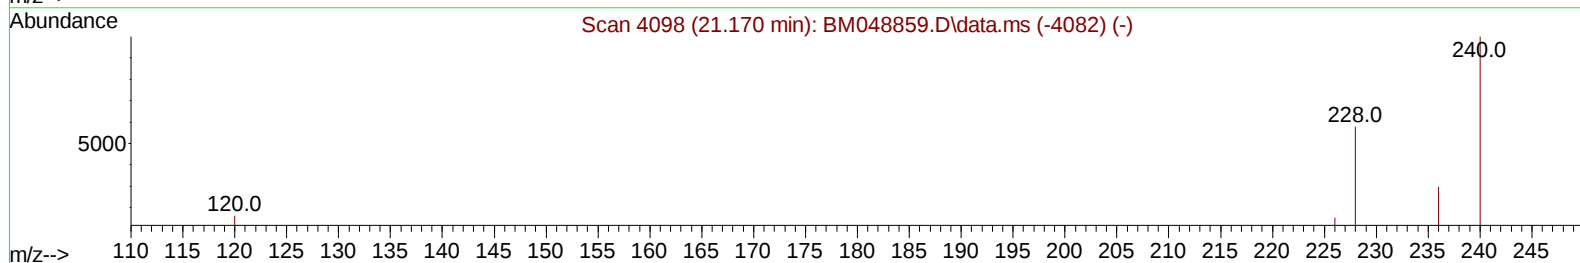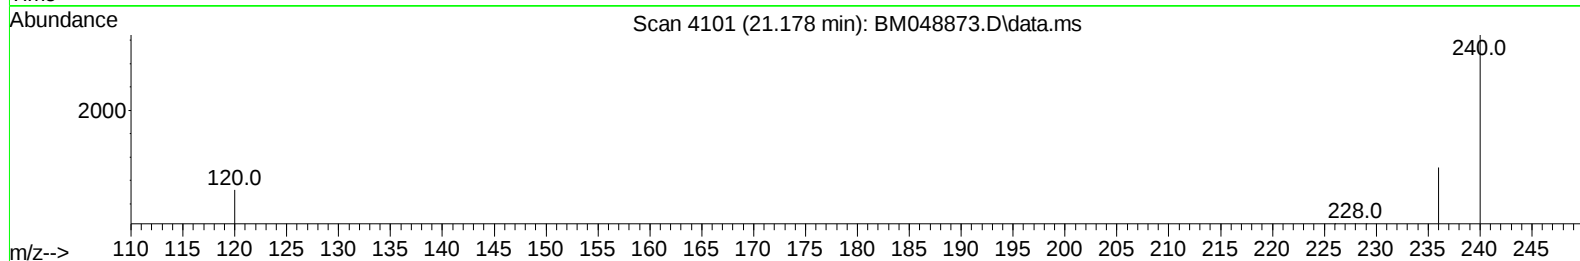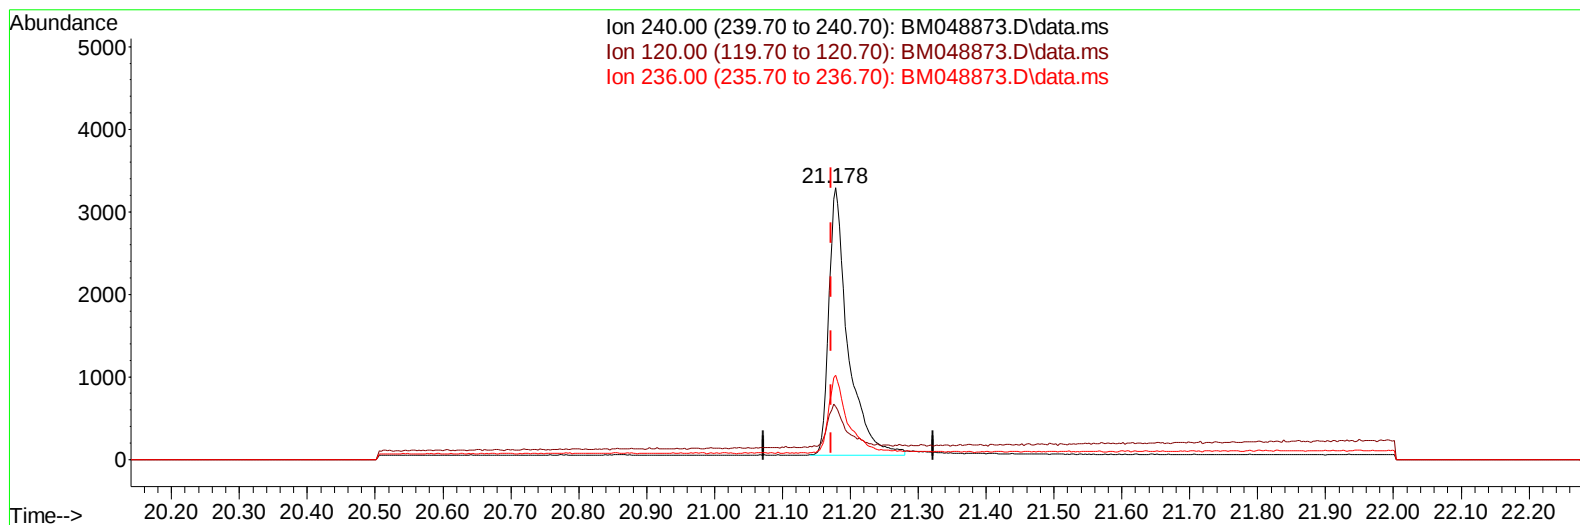

TIC: BM048873.D\data.ms

(17) Chrysene-d12

21.178min (+ 0.006) 0.40 ng/ul m

response 6335

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	19.39
236.00	32.10	31.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048873.D
Acq On : 06 Dec 2024 18:43
Operator : RC/JU
Sample : PB165418BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 21:53:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

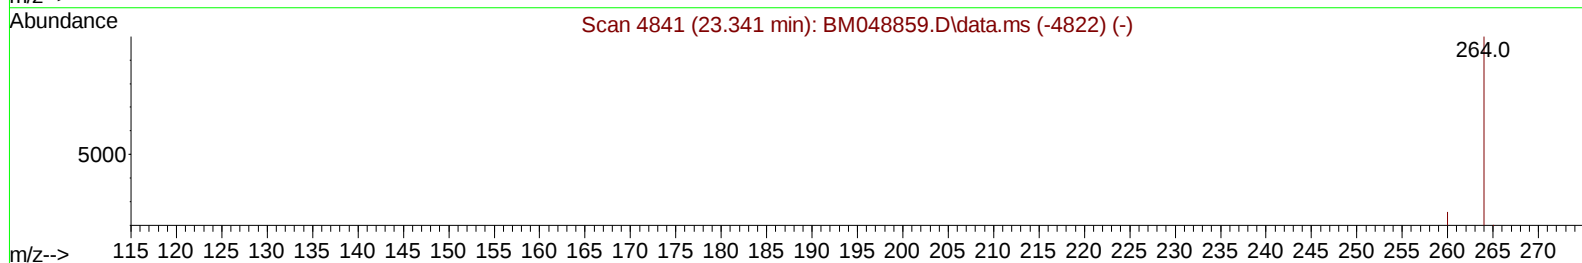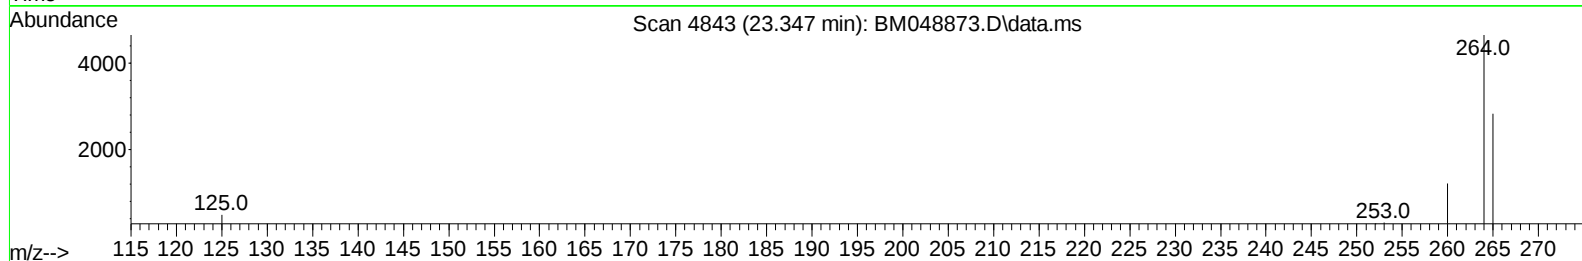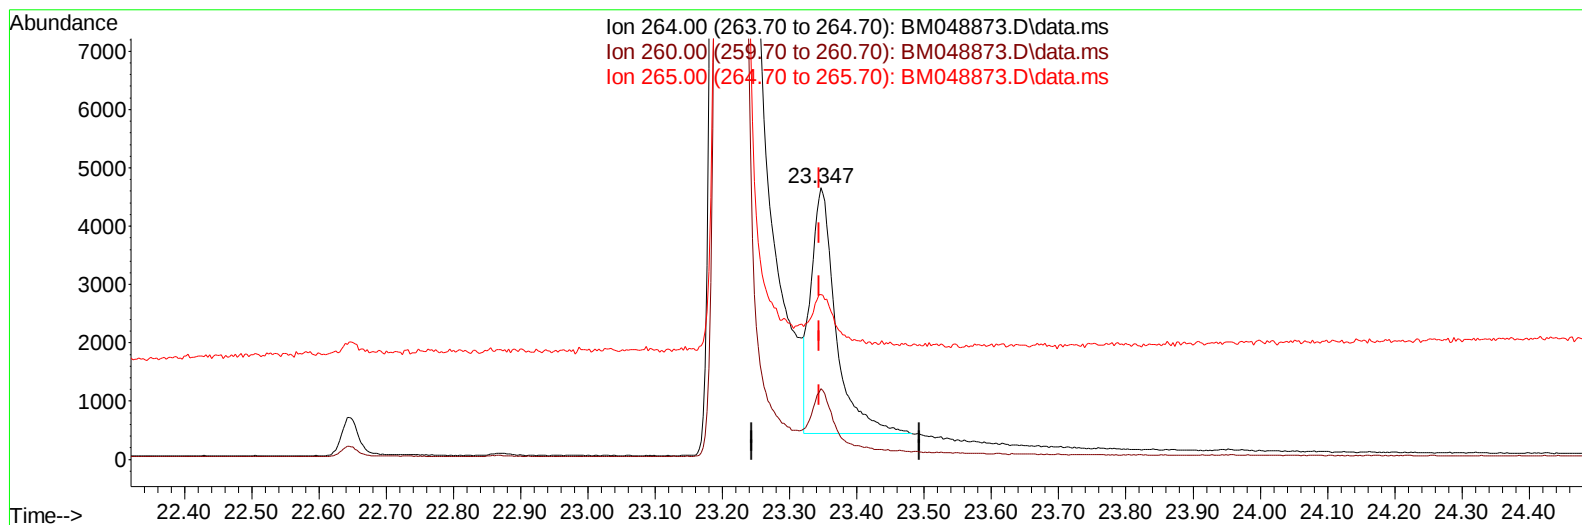

TIC: BM048873.D\data.ms

(23) Perylene-d12 (I)

23.347min (+ 0.003) 0.40 ng/u1

response 10949

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	26.07
265.00	78.50	60.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048873.D
Acq On : 06 Dec 2024 18:43
Operator : RC/JU
Sample : PB165418BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 21:53:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

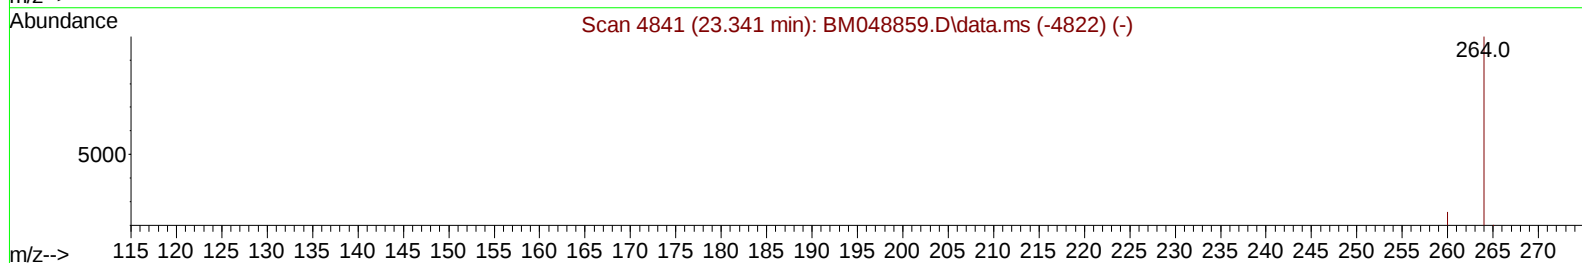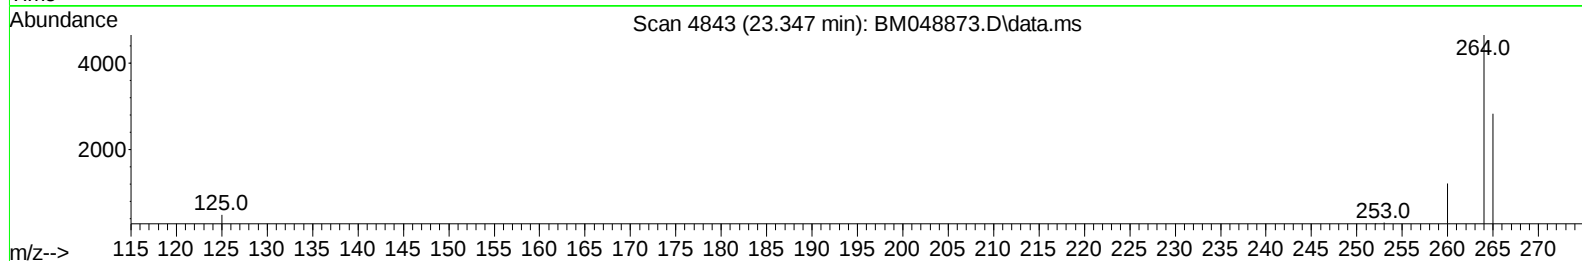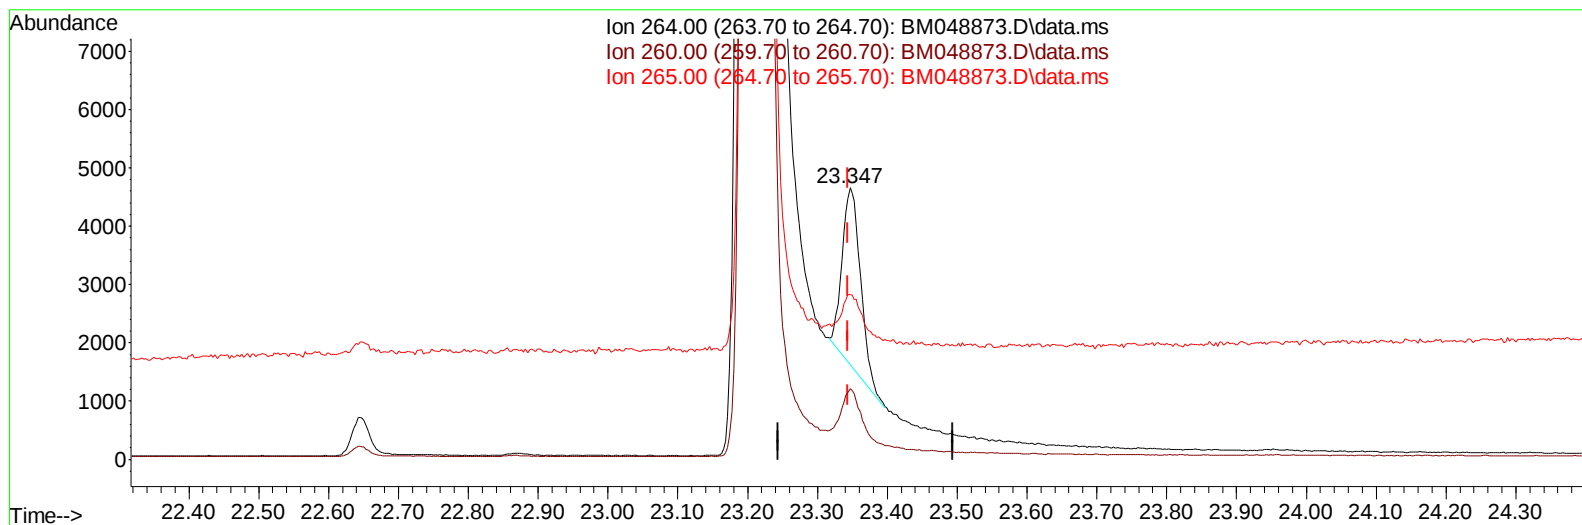

TIC: BM048873.D\data.ms

(23) Perylene-d12 (I)

23.347min (+ 0.003) 0.40 ng/ul m

response 5517

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	26.07
265.00	78.50	60.76#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048873.D
 Acq On : 06 Dec 2024 18:43
 Operator : RC/JU
 Sample : PB165418BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK418

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 21:53:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	4004	0.400	ng/ul	0.00
4) Naphthalene-d8	10.358	136	11507	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.228	164	6210	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	12167m	0.400	ng/ul	0.00
17) Chrysene-d12	21.178	240	6335m	0.400	ng/ul	0.00
23) Perylene-d12	23.347	264	5517m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	29519	5.771	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.963	152	5021	0.363	ng/ul	0.00
18) Fluoranthene-d10	19.010	212	8219	0.420	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048873.D
Acq On : 06 Dec 2024 18:43
Operator : RC/JU
Sample : PB165418BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:53:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

