




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048874.D
Acq On : 06 Dec 2024 19:19
Operator : RC/JU
Sample : PB165445BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

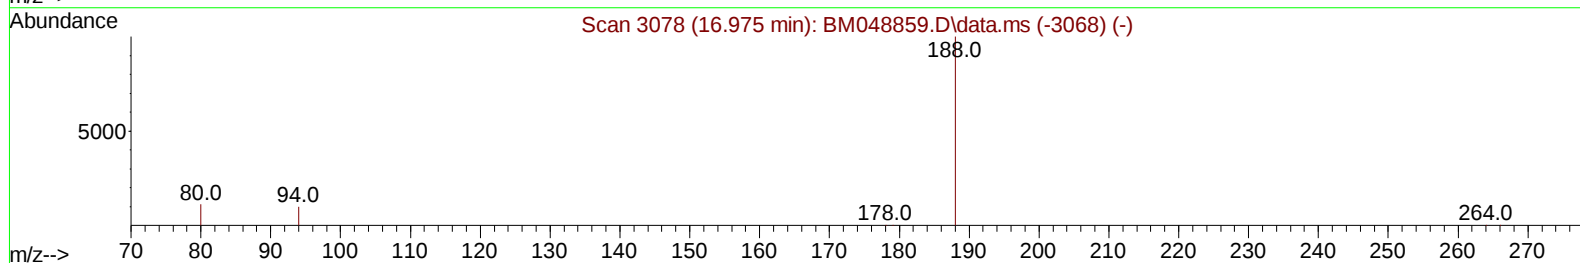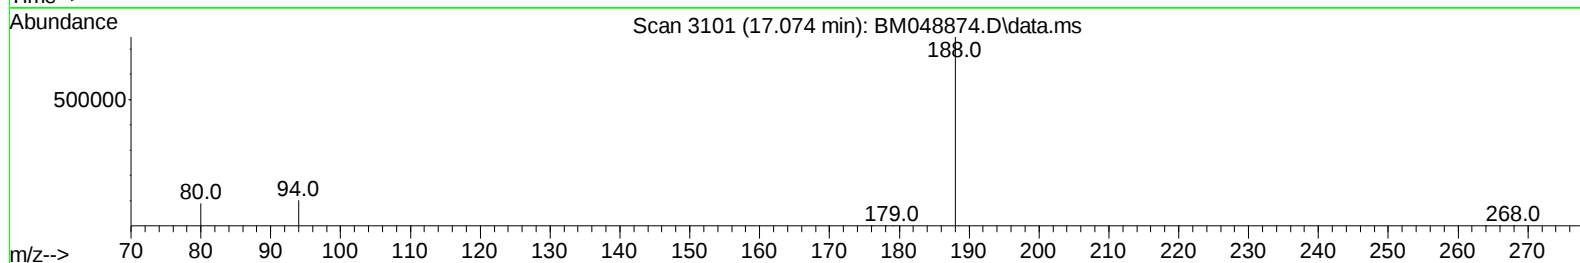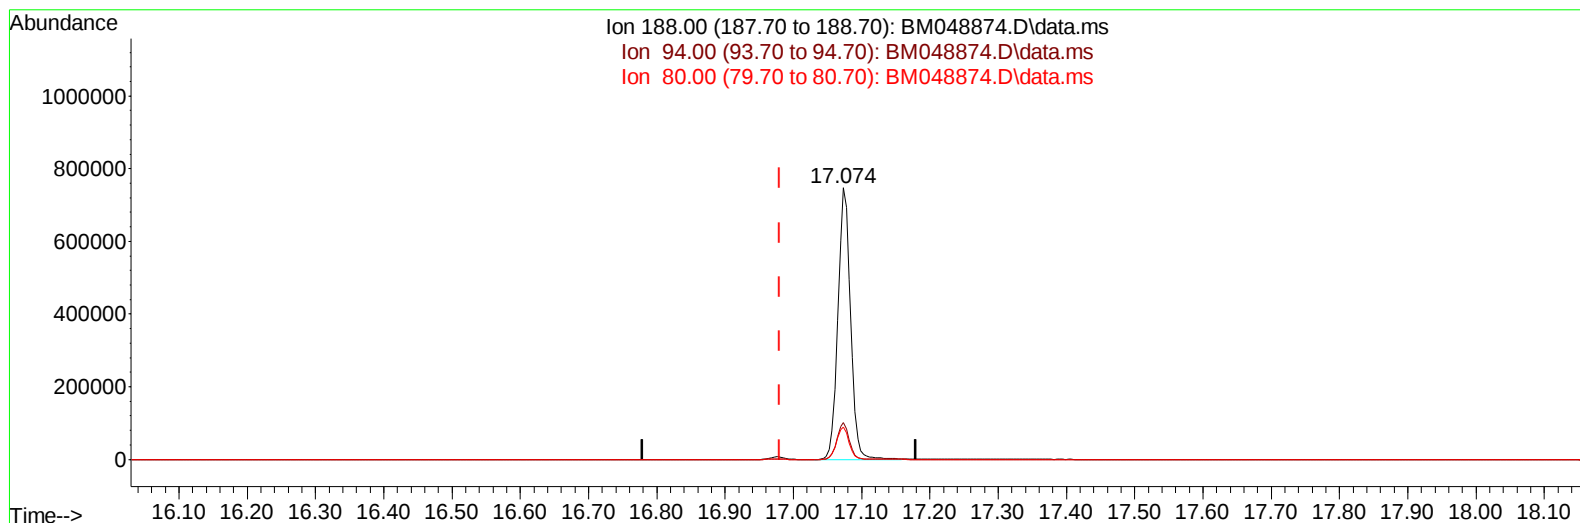

TIC: BM048874.D\data.ms

(13) Phenanthrene-d10 (I)

17.074min (+ 0.094) 0.40 ng/u1

response 959991

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	13.53
80.00	12.50	11.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048874.D
Acq On : 06 Dec 2024 19:19
Operator : RC/JU
Sample : PB165445BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

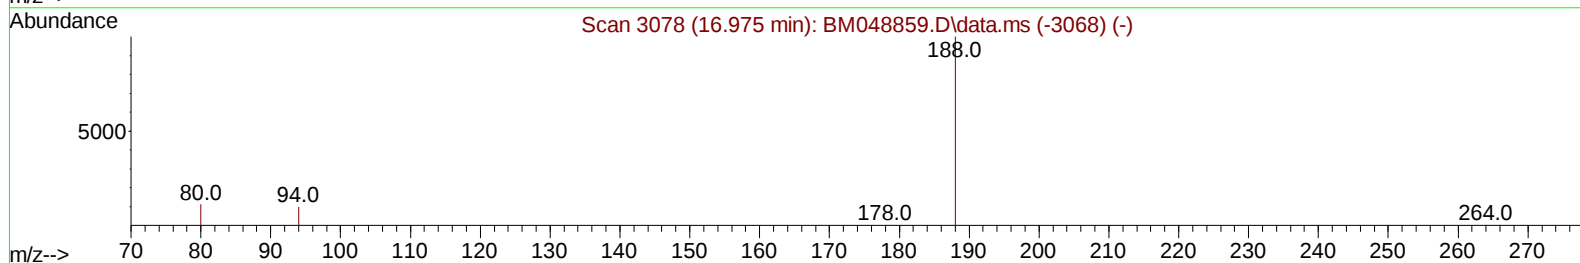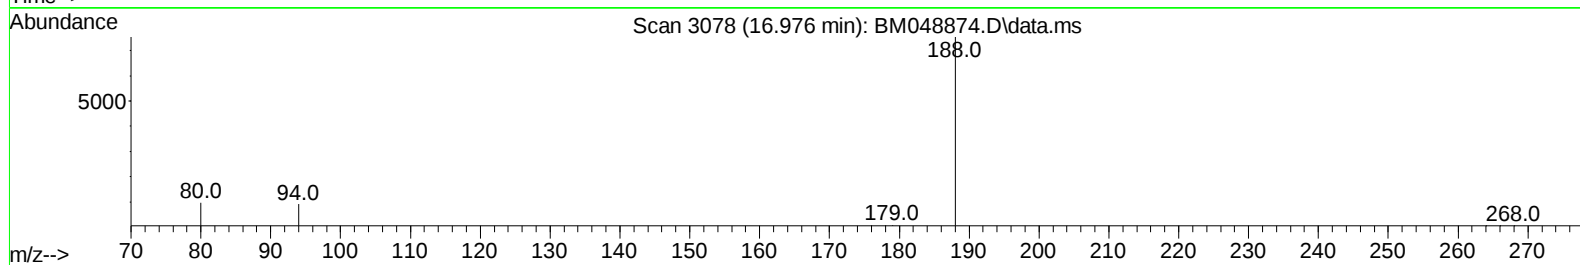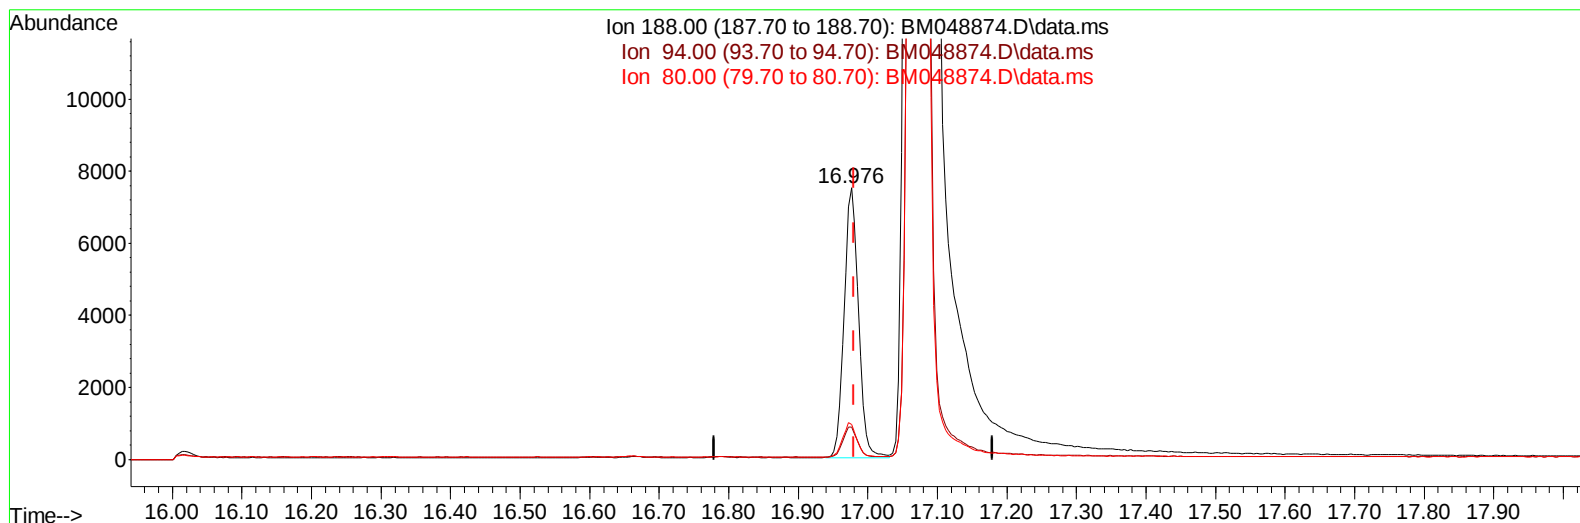

TIC: BM048874.D\data.ms

(13) Phenanthrene-d10 (I)

16.976min (-0.003) 0.40 ng/u1 m

response 10778

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	12.02
80.00	12.50	12.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048874.D
Acq On : 06 Dec 2024 19:19
Operator : RC/JU
Sample : PB165445BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

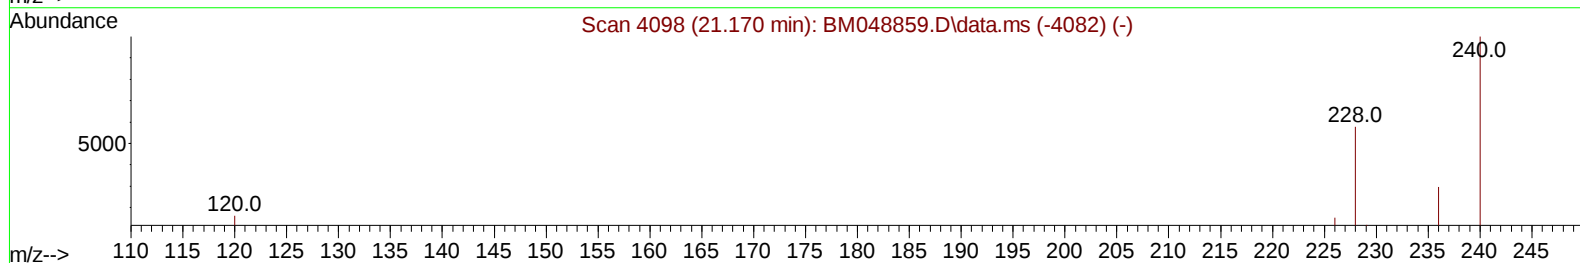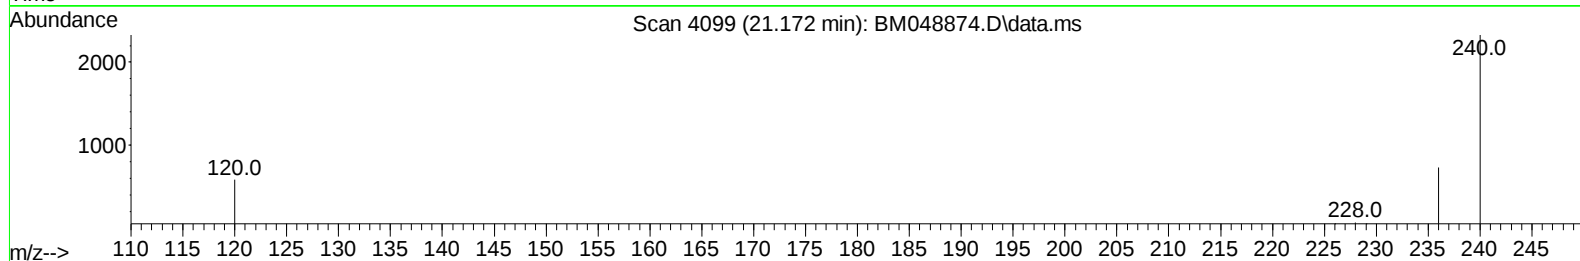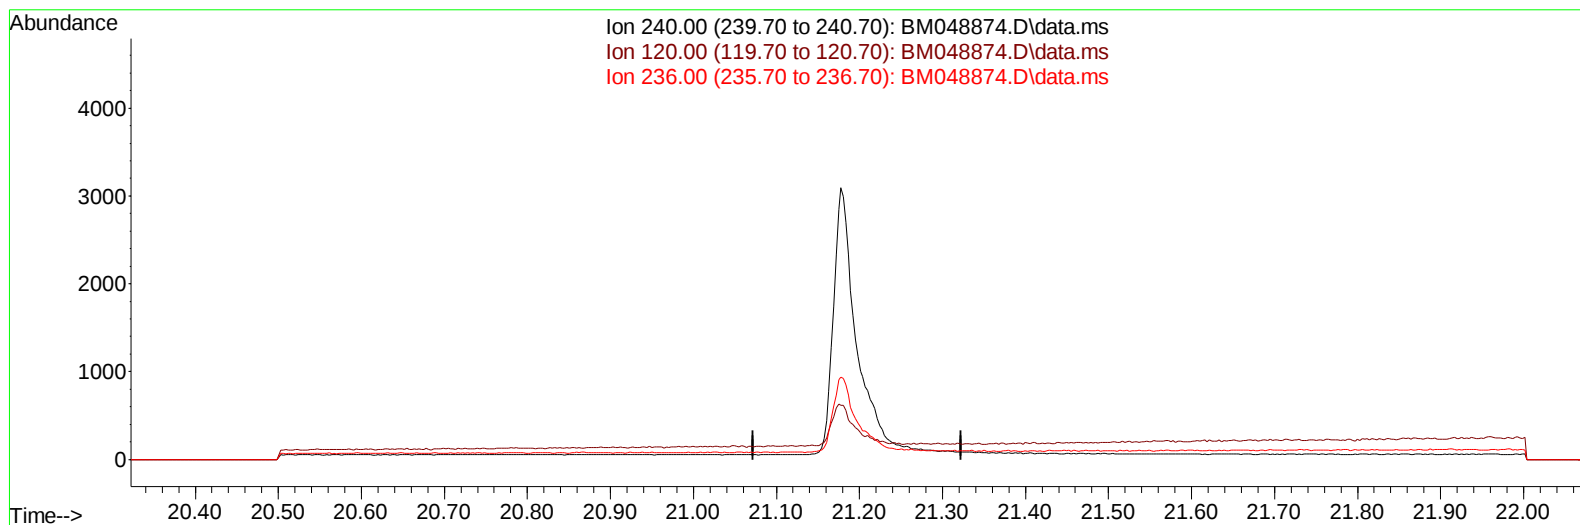

TIC: BM048874.D\data.ms

(17) Chrysene-d12

21.173min (-21.173) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048874.D
Acq On : 06 Dec 2024 19:19
Operator : RC/JU
Sample : PB165445BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

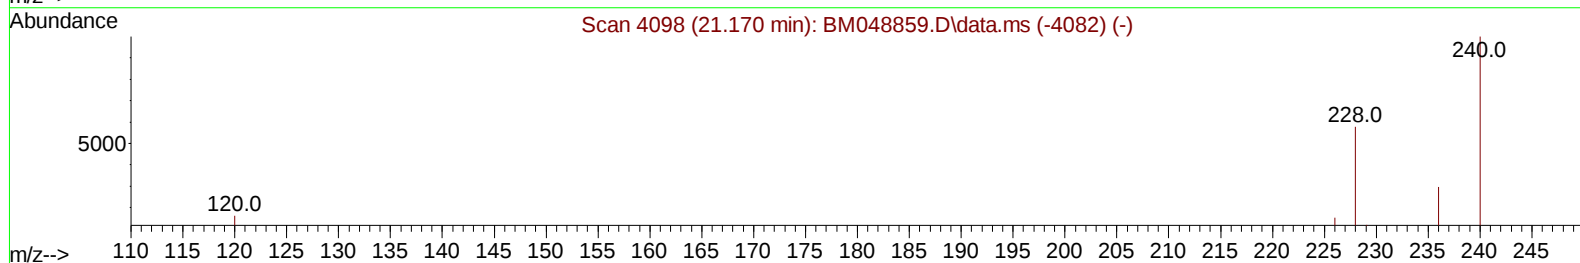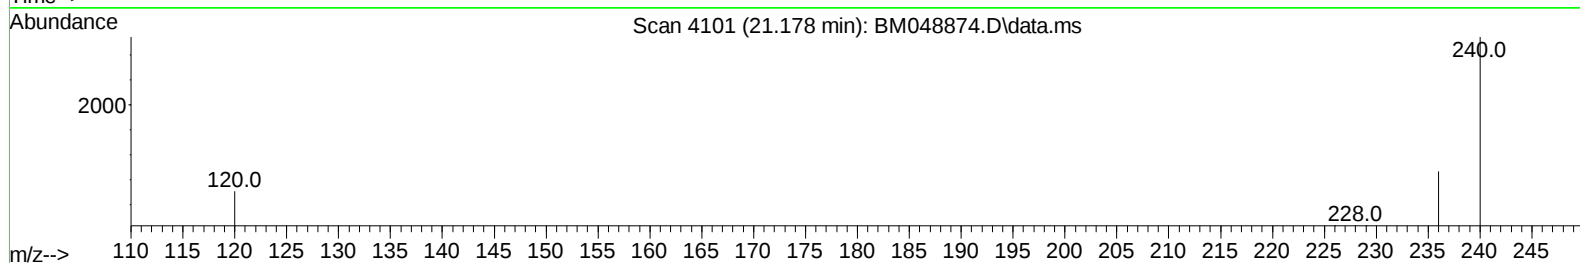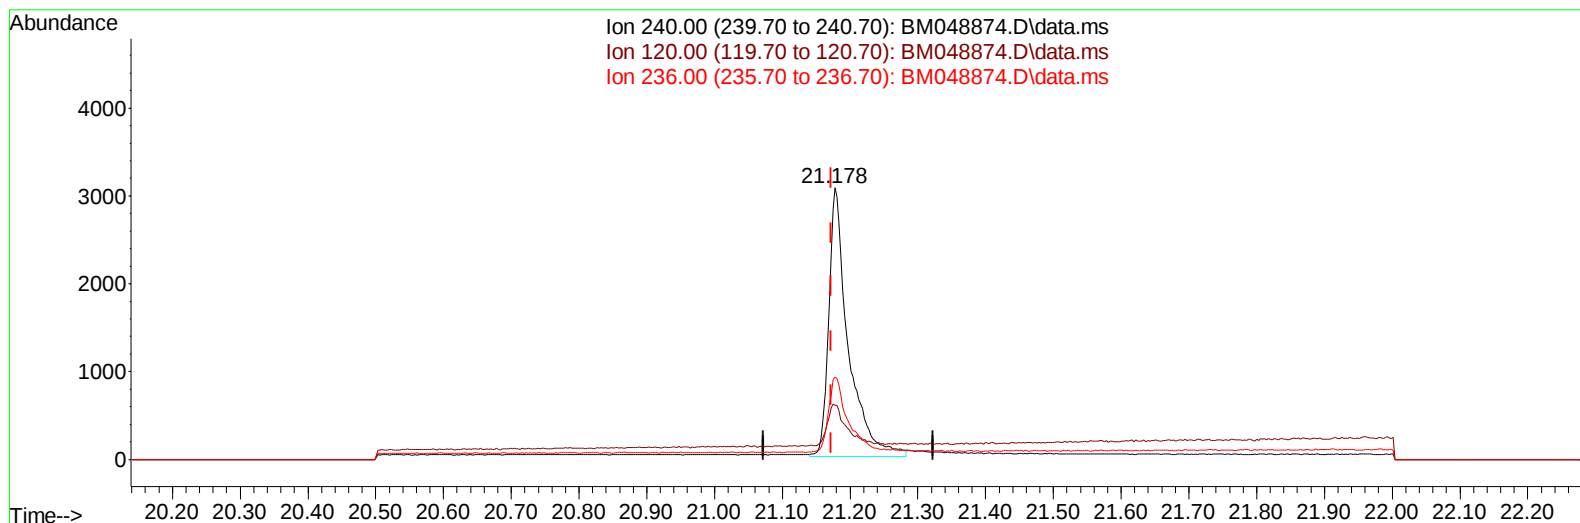

TIC: BM048874.D\data.ms

(17) Chrysene-d12

21.178min (+ 0.005) 0.40 ng/ul m

response 6144

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	19.83
236.00	32.10	30.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048874.D
Acq On : 06 Dec 2024 19:19
Operator : RC/JU
Sample : PB165445BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 21:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

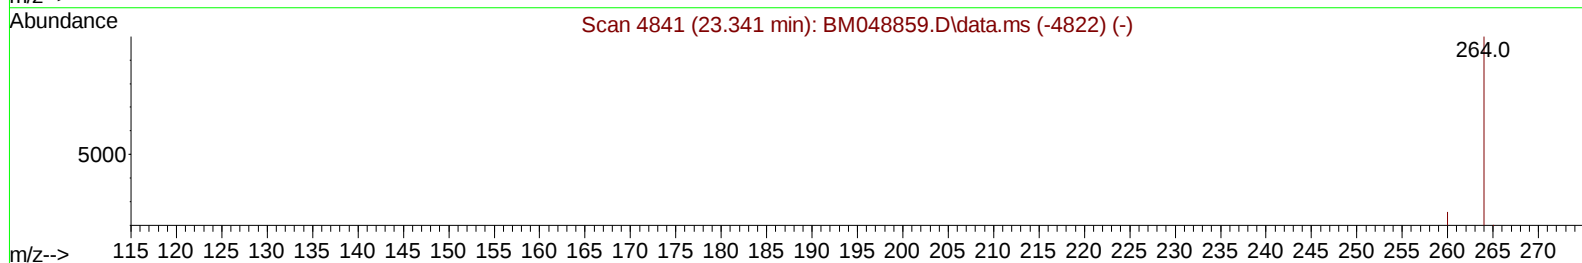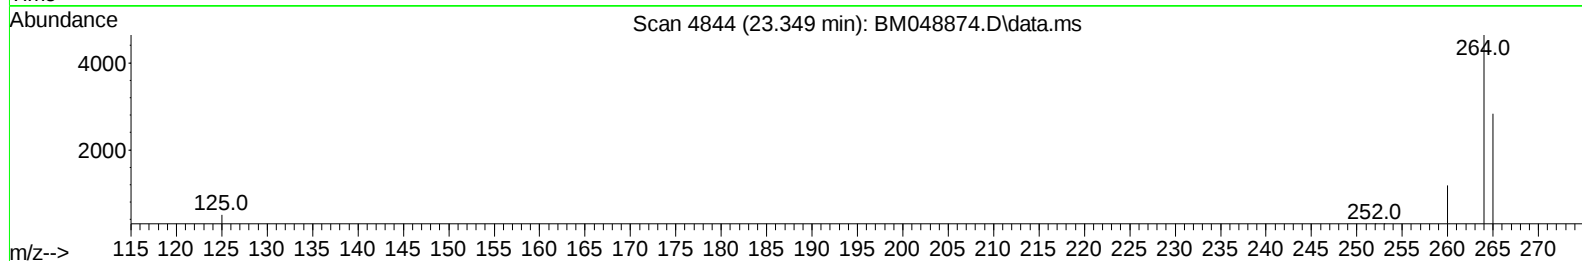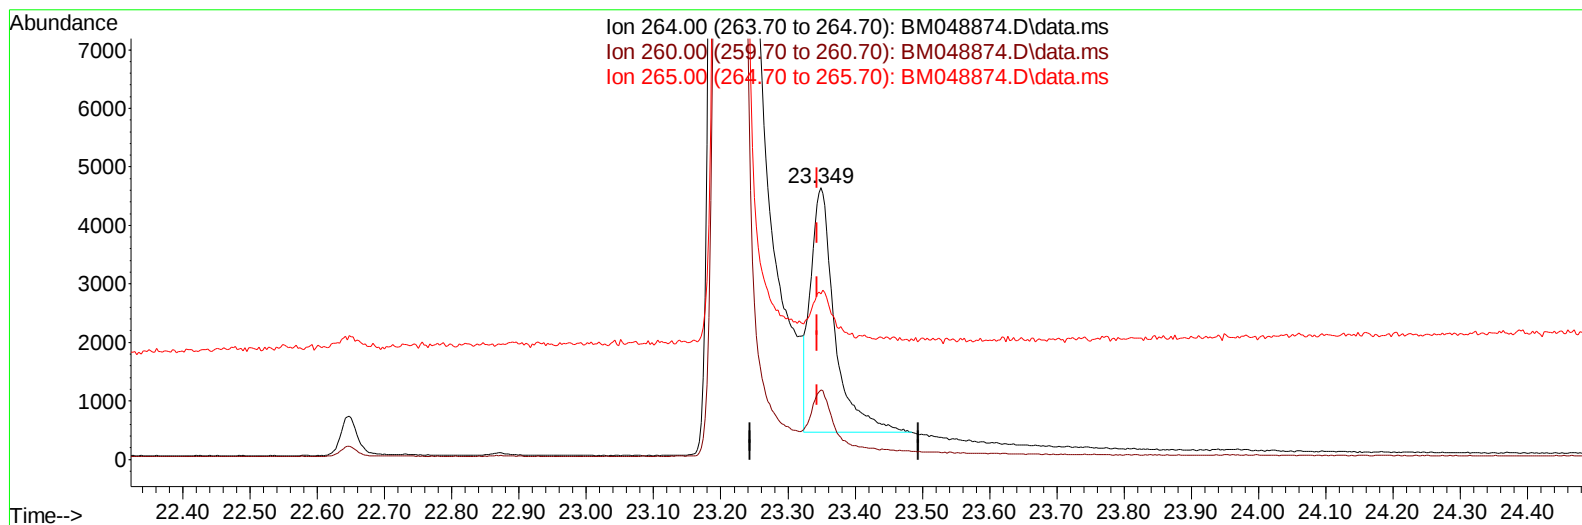

TIC: BM048874.D\data.ms

(23) Perylene-d12 (I)

23.349min (+ 0.005) 0.40 ng/u1

response 10601

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.60
265.00	78.50	60.99#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048874.D
Acq On : 06 Dec 2024 19:19
Operator : RC/JU
Sample : PB165445BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

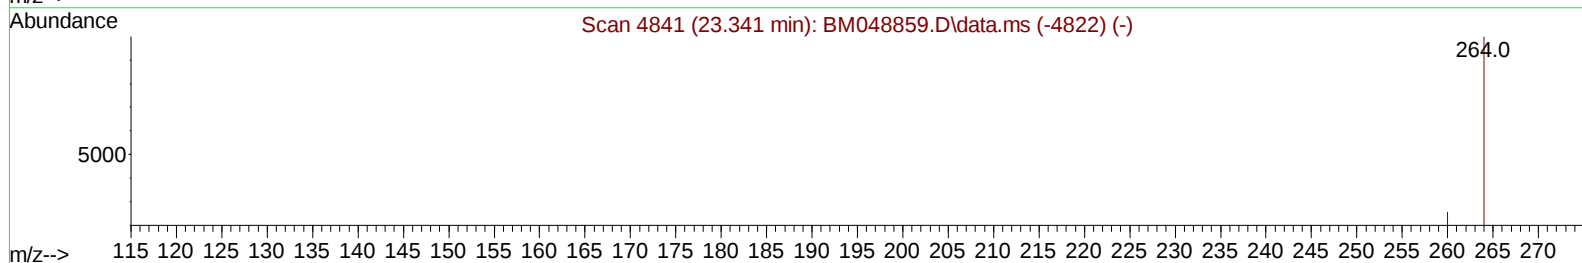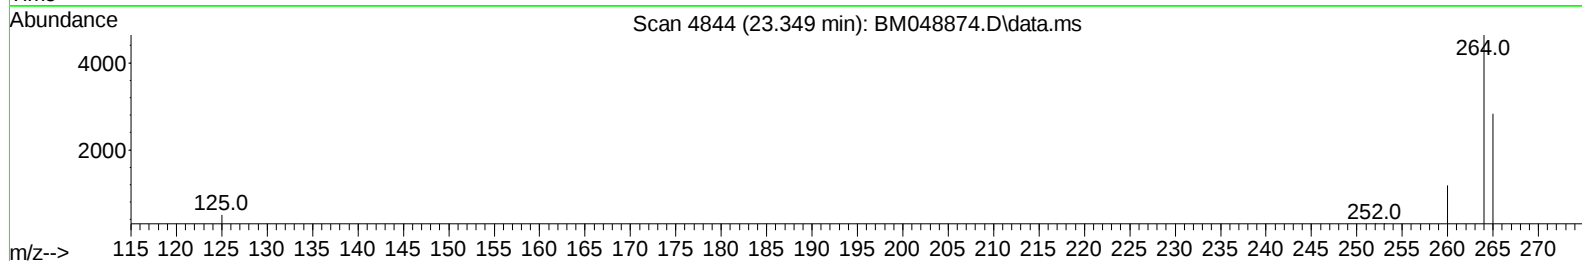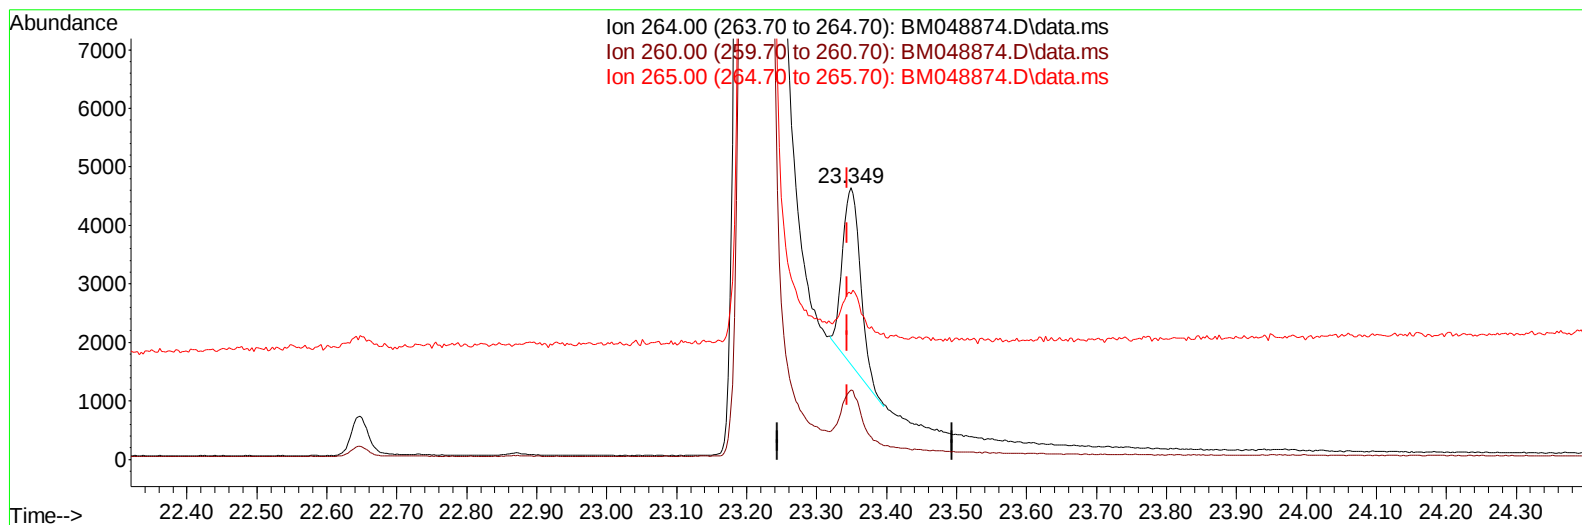

TIC: BM048874.D\data.ms

(23) Perylene-d12 (I)

23.349min (+ 0.005) 0.40 ng/ul m

response 5312

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.60
265.00	78.50	60.99#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048874.D
 Acq On : 06 Dec 2024 19:19
 Operator : RC/JU
 Sample : PB165445BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK445

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 21:57:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	3974	0.400	ng/ul	0.00
4) Naphthalene-d8	10.359	136	10929	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.229	164	5674	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.976	188	10778m	0.400	ng/ul	0.00
17) Chrysene-d12	21.178	240	6144m	0.400	ng/ul	0.00
23) Perylene-d12	23.349	264	5312m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	30584	6.025	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.965	152	4734	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.011	212	7448	0.393	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048874.D
Acq On : 06 Dec 2024 19:19
Operator : RC/JU
Sample : PB165445BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Dec 06 21:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024

