




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

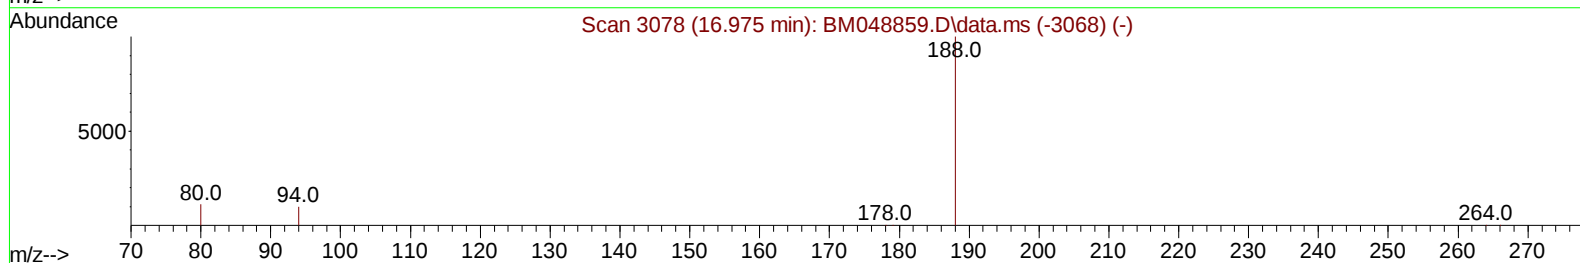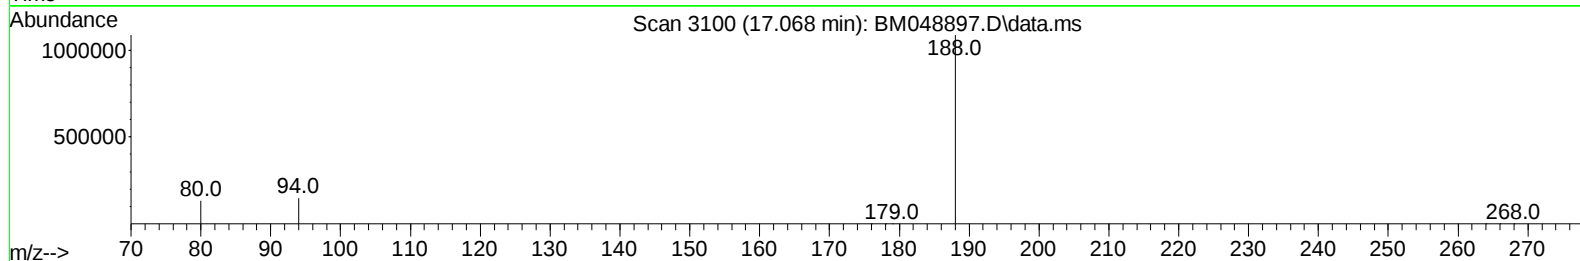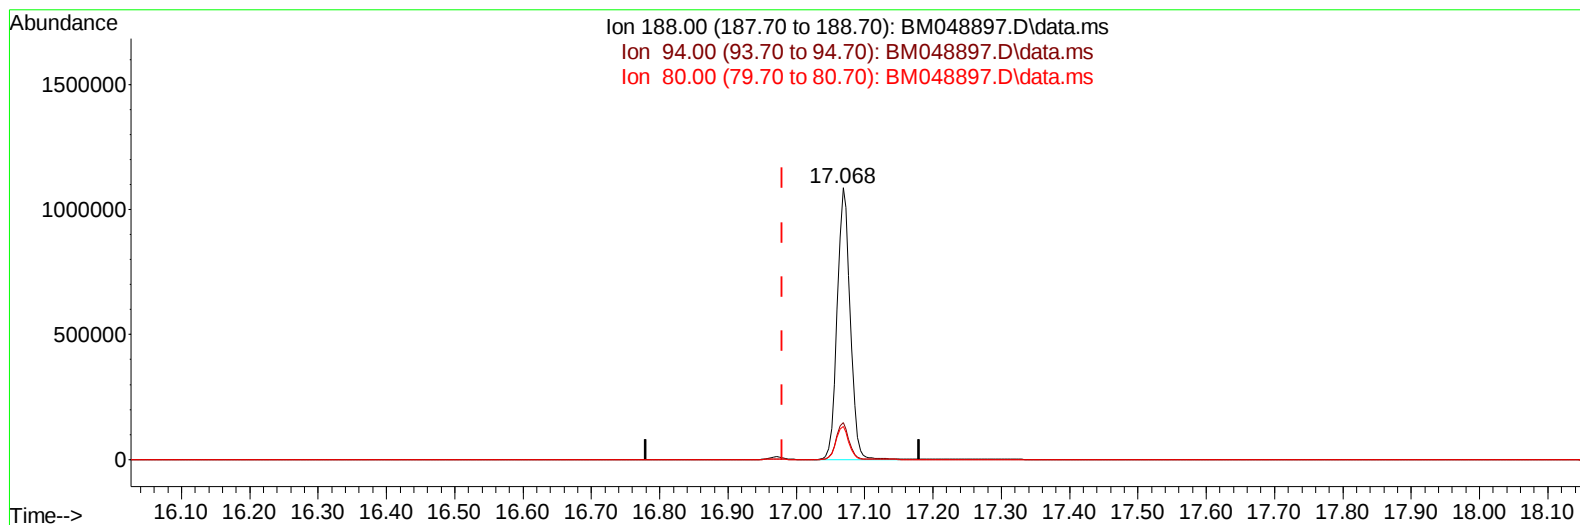

TIC: BM048897.D\data.ms

(13) Phenanthrene-d10 (I)

17.068min (+ 0.089) 0.40 ng/u1

response 1431830

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	13.58
80.00	12.50	12.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

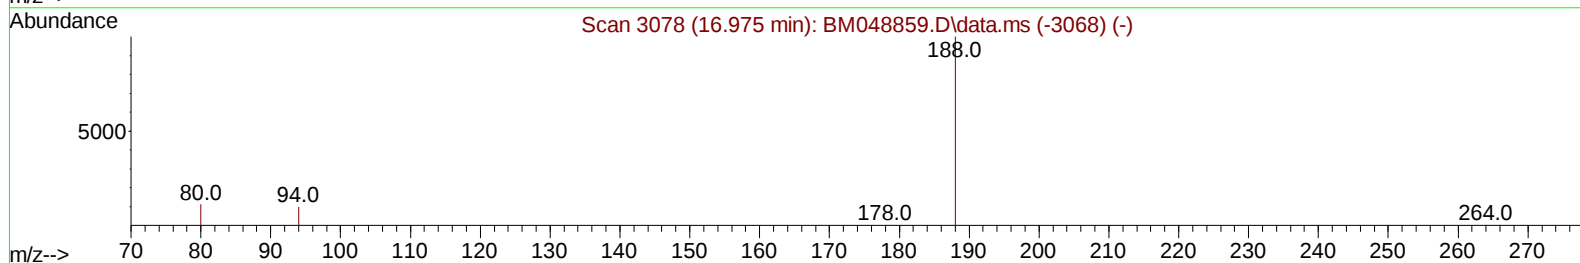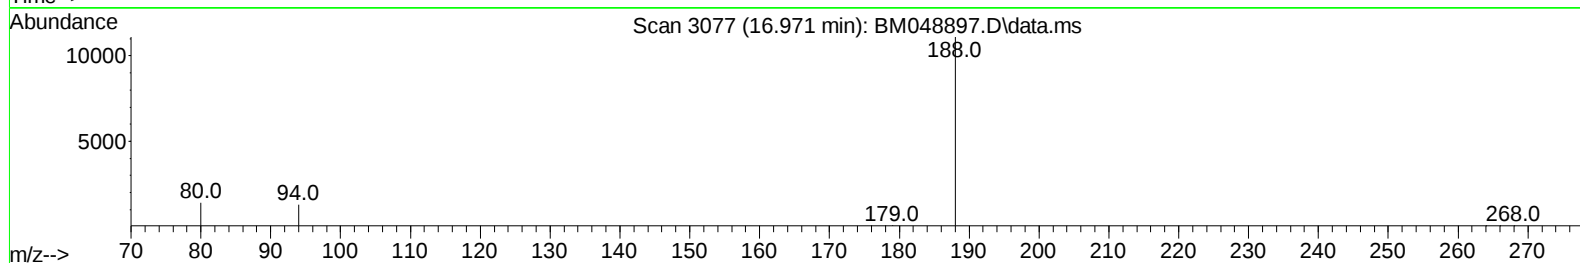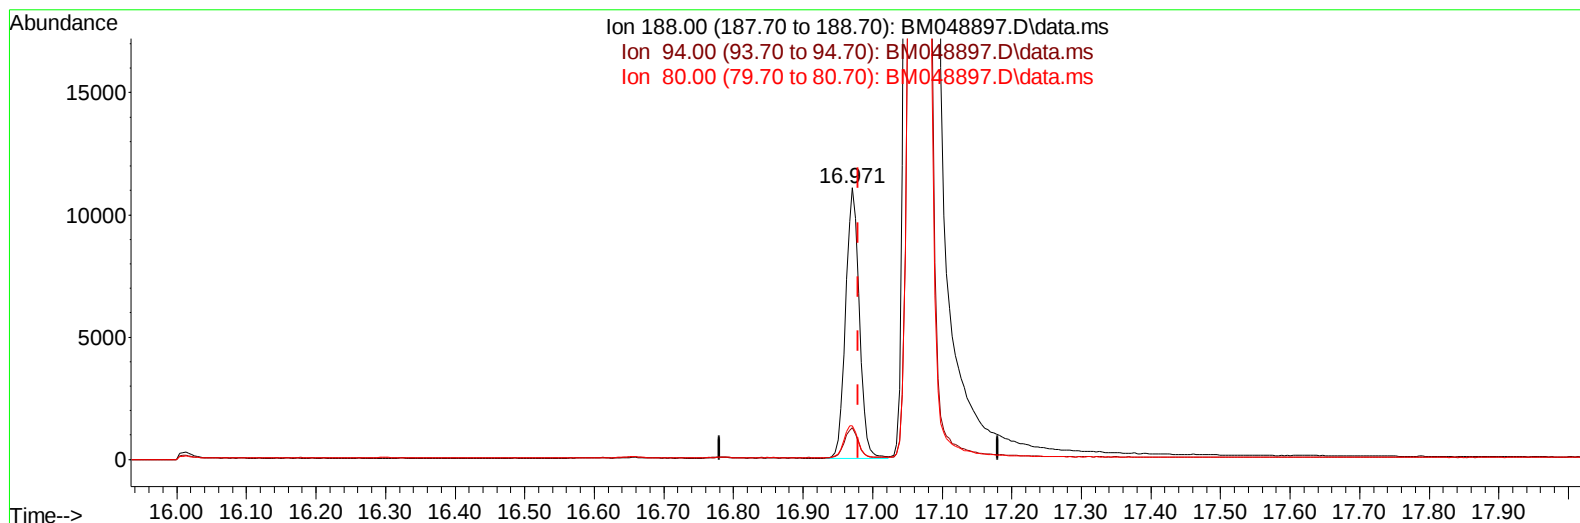

TIC: BM048897.D\data.ms

(13) Phenanthrene-d10 (I)

16.971min (-0.008) 0.40 ng/ul m

response 15131

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	11.61
80.00	12.50	12.52
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

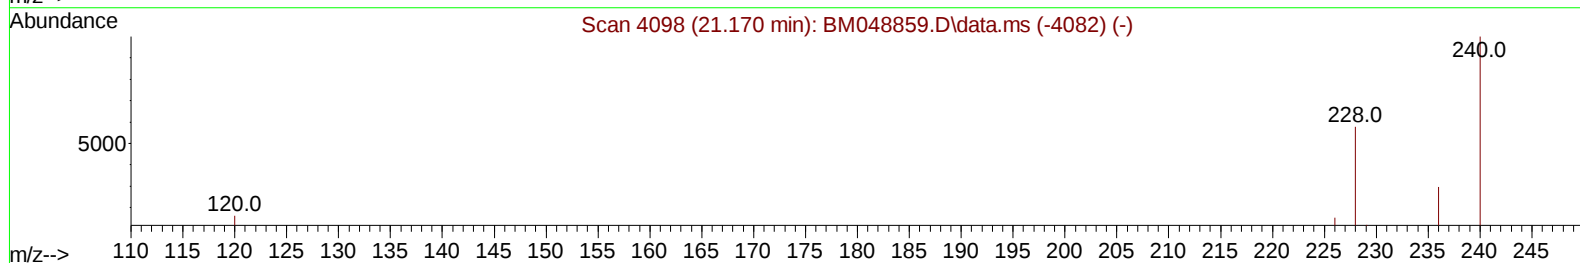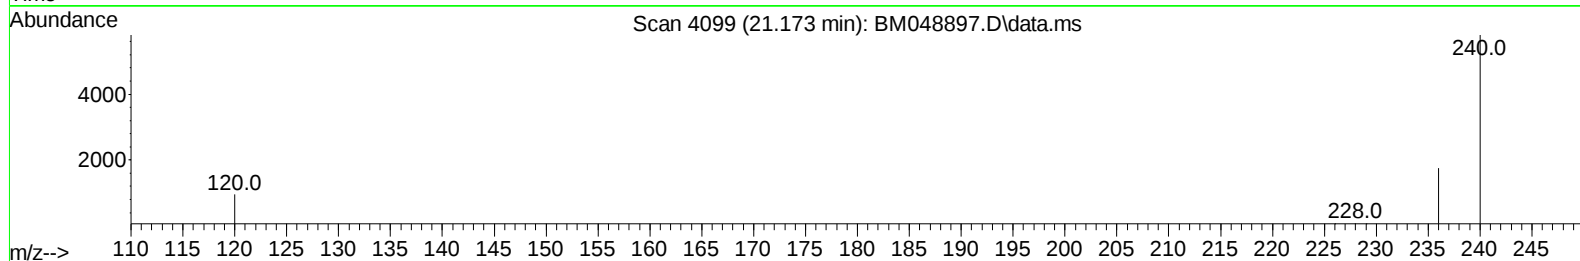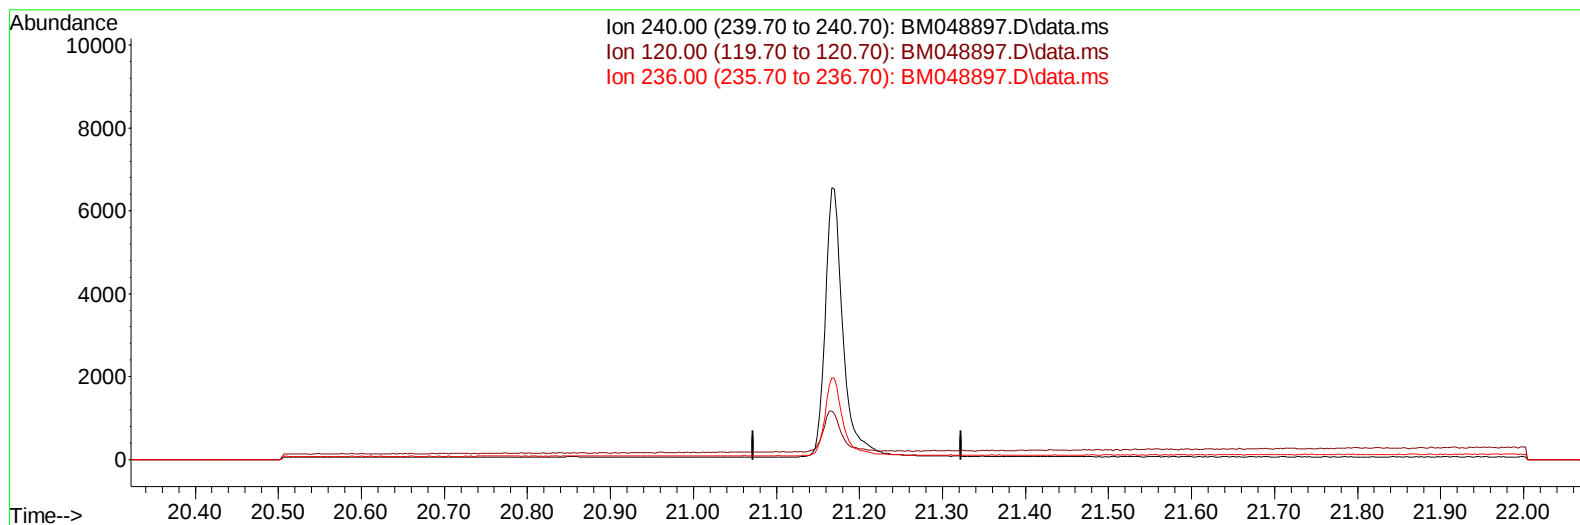

TIC: BM048897.D\data.ms

(17) Chrysene-d12

21.173min (-21.173) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

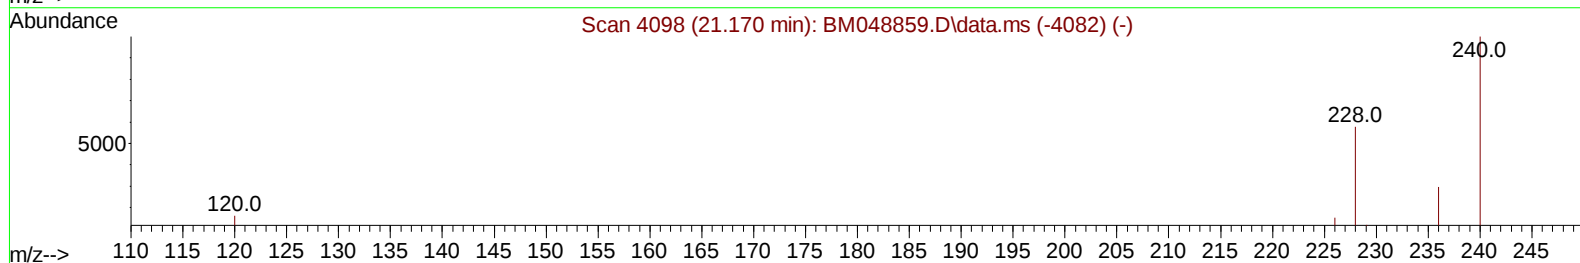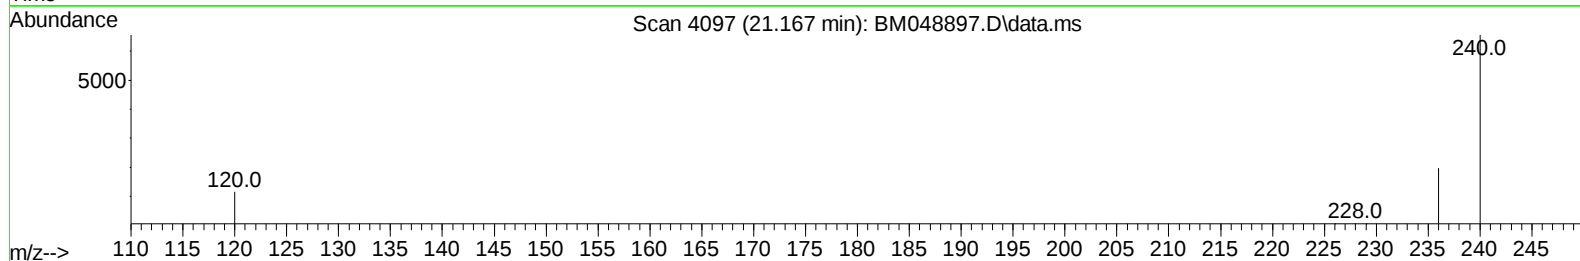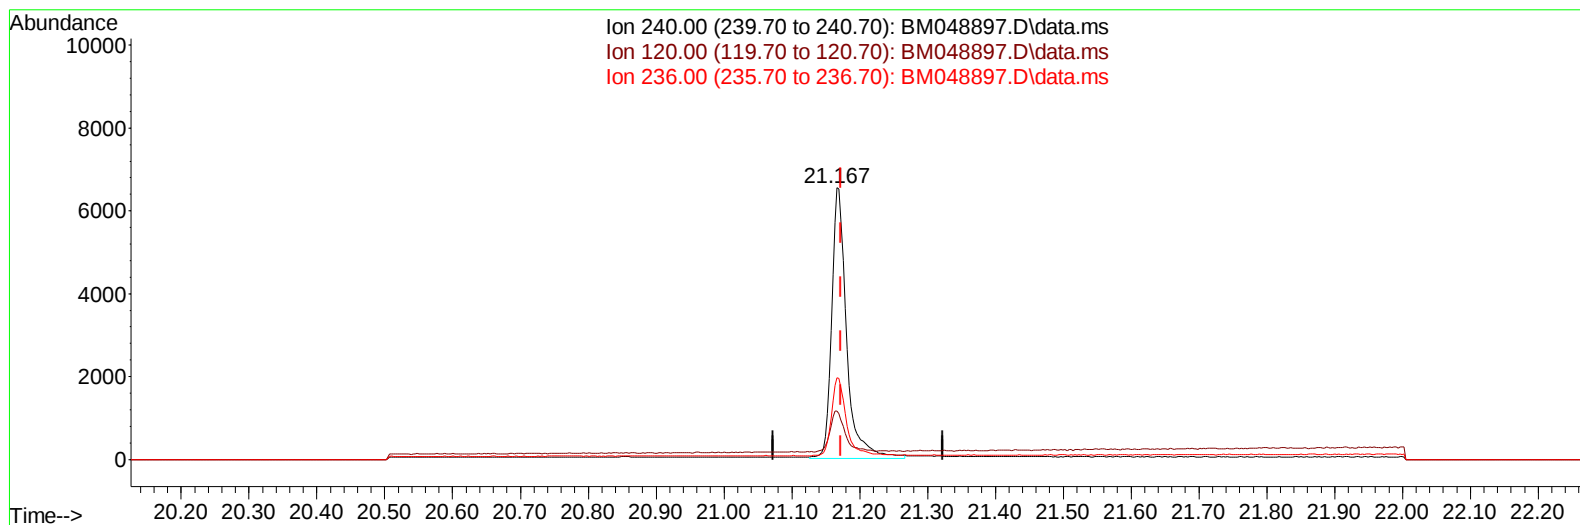

TIC: BM048897.D\data.ms

(17) Chrysene-d12

21.167min (-0.006) 0.40 ng/u1 m

response 9944

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	17.82
236.00	32.10	30.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

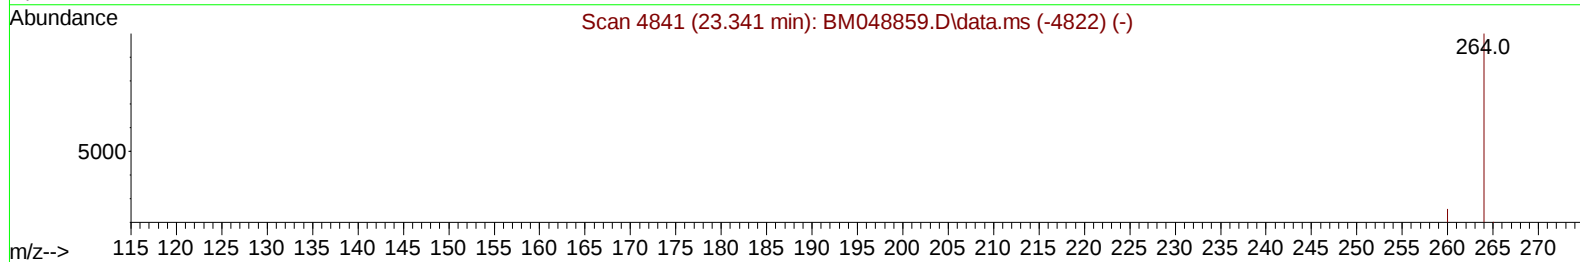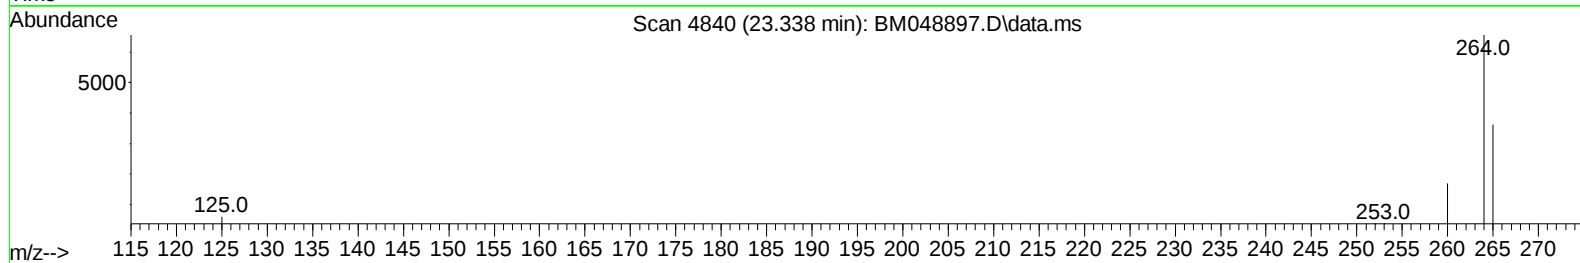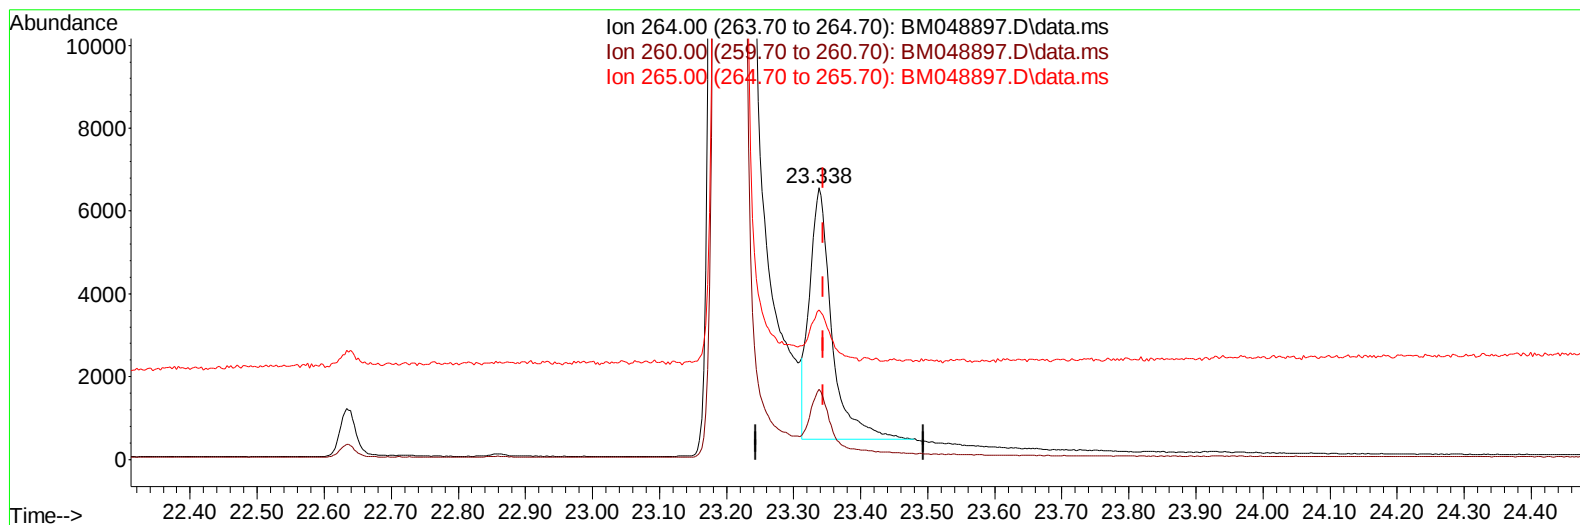

TIC: BM048897.D\data.ms

(23) Perylene-d12 (I)

23.338min (-0.006) 0.40 ng/u1

response 14029

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.91
265.00	78.50	55.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

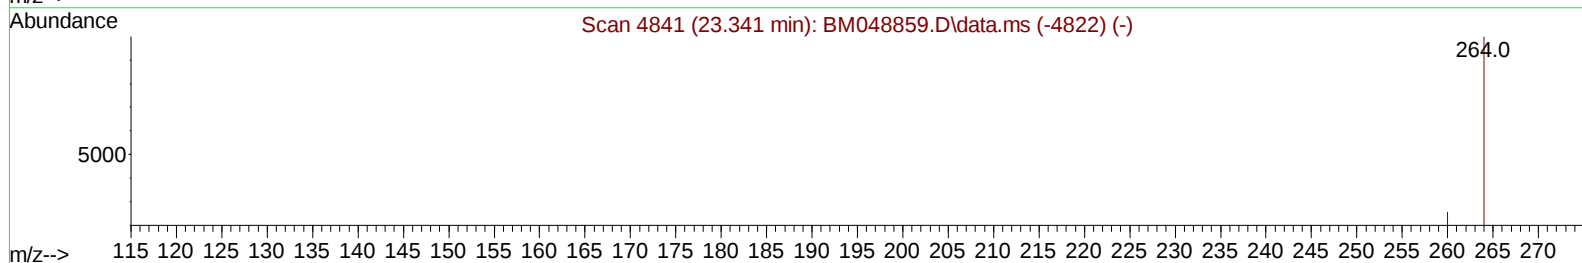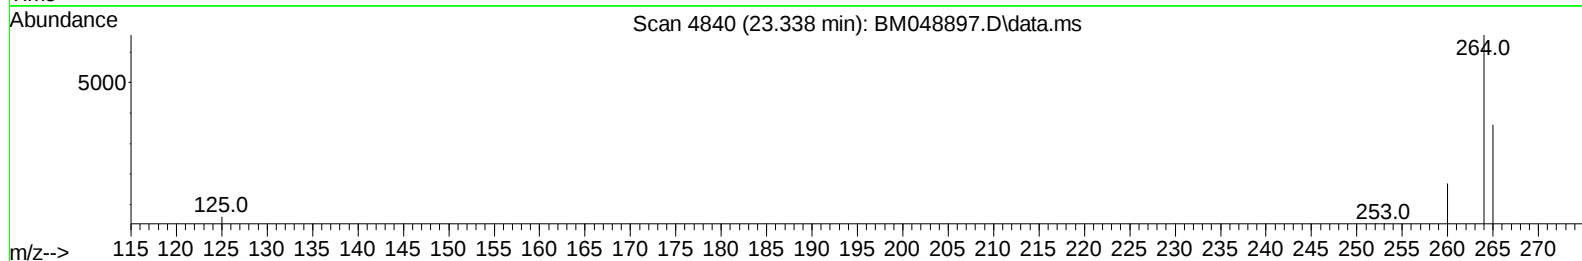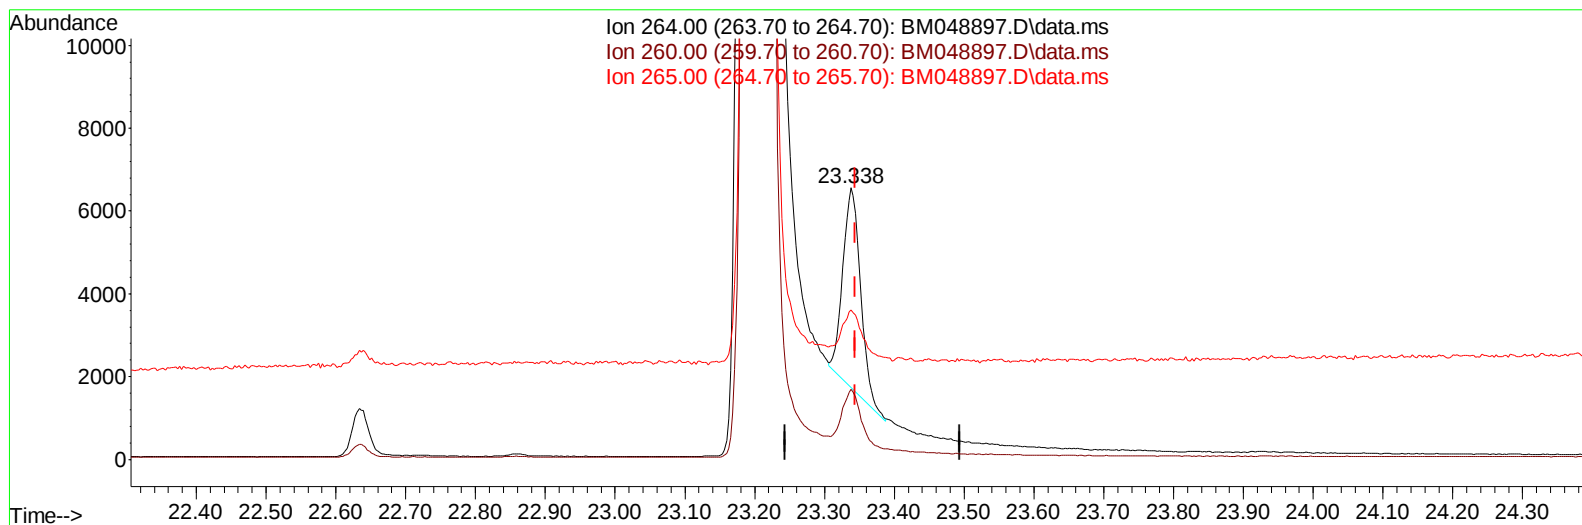

TIC: BM048897.D\data.ms

(23) Perylene-d12 (I)

23.338min (-0.006) 0.40 ng/ul m

response 8375

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.91
265.00	78.50	55.12#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048897.D
 Acq On : 07 Dec 2024 15:11
 Operator : RC/JU
 Sample : P5107-18
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHJ97

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/10/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 08 21:47:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	5141	0.400	ng/ul	0.00
4) Naphthalene-d8	10.352	136	14501	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.223	164	7675	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.971	188	15131m	0.400	ng/ul	0.00
17) Chrysene-d12	21.167	240	9944m	0.400	ng/ul	0.00
23) Perylene-d12	23.338	264	8375m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	28102	4.279	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.953	152	5688	0.326	ng/ul	-0.01
18) Fluoranthene-d10	19.006	212	12158	0.396	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048897.D
Acq On : 07 Dec 2024 15:11
Operator : RC/JU
Sample : P5107-18
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ97

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

