




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048898.D
Acq On : 07 Dec 2024 15:47
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ98

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

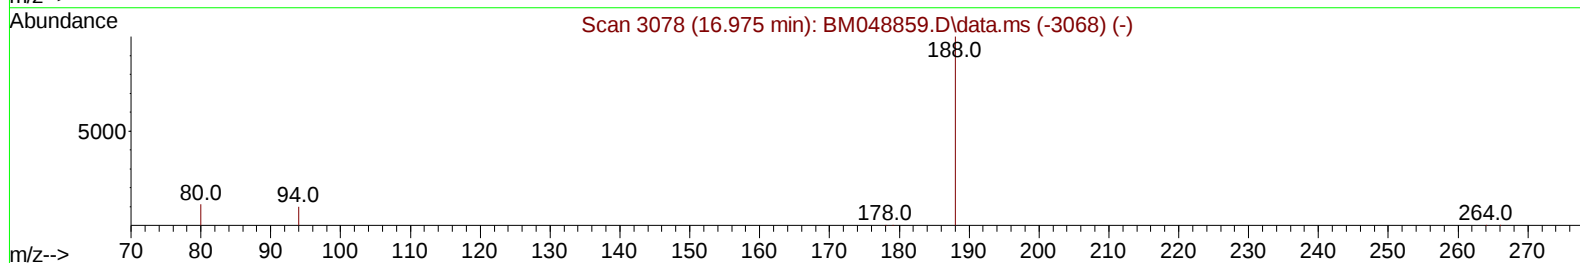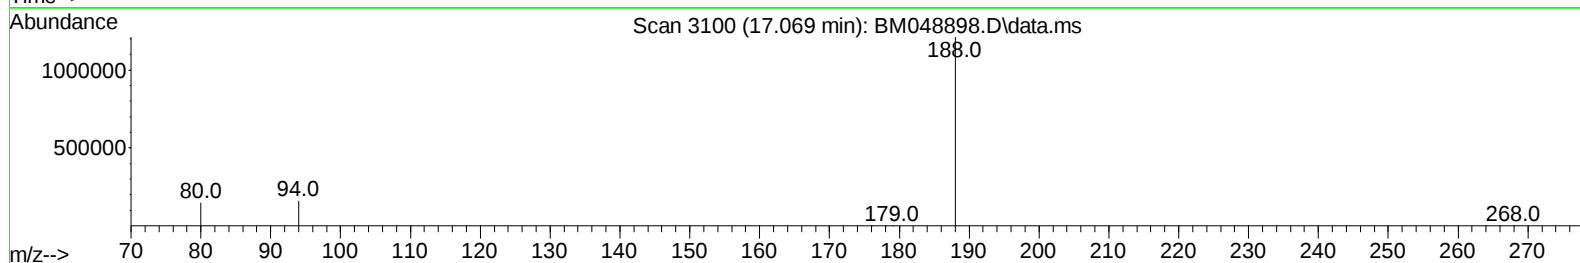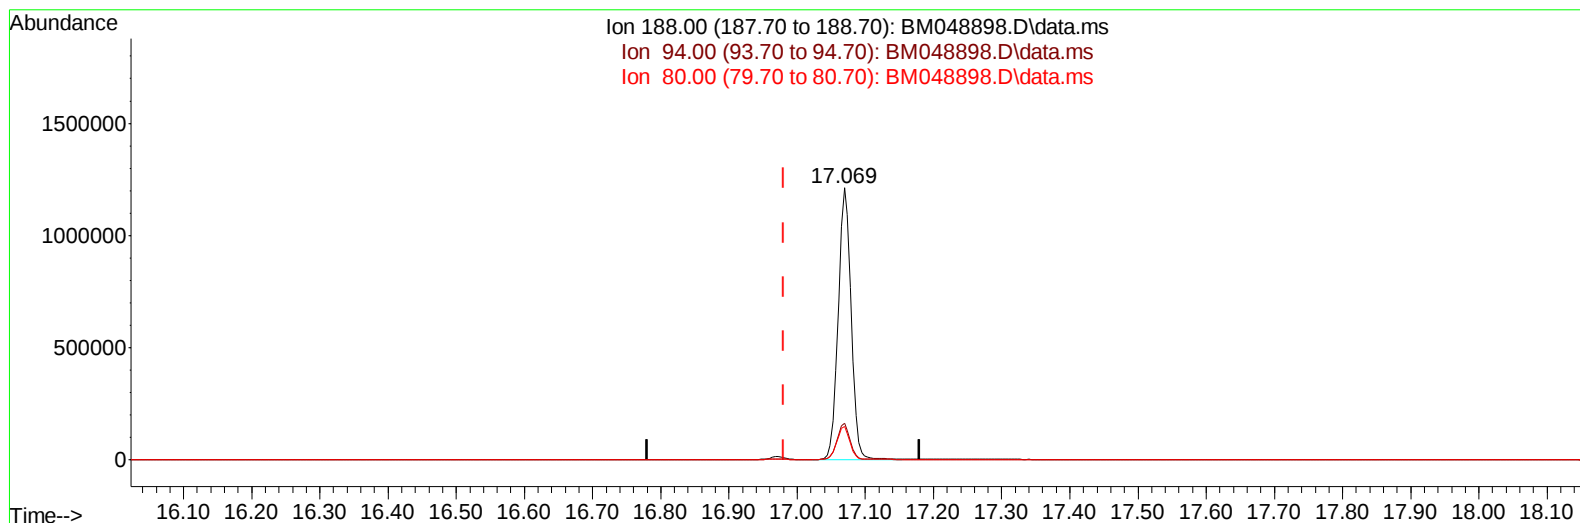

TIC: BM048898.D\data.ms

(13) Phenanthrene-d10 (I)

17.069min (+ 0.090) 0.40 ng/u1

response 1590586

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	13.37
80.00	12.50	12.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048898.D
Acq On : 07 Dec 2024 15:47
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ98

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

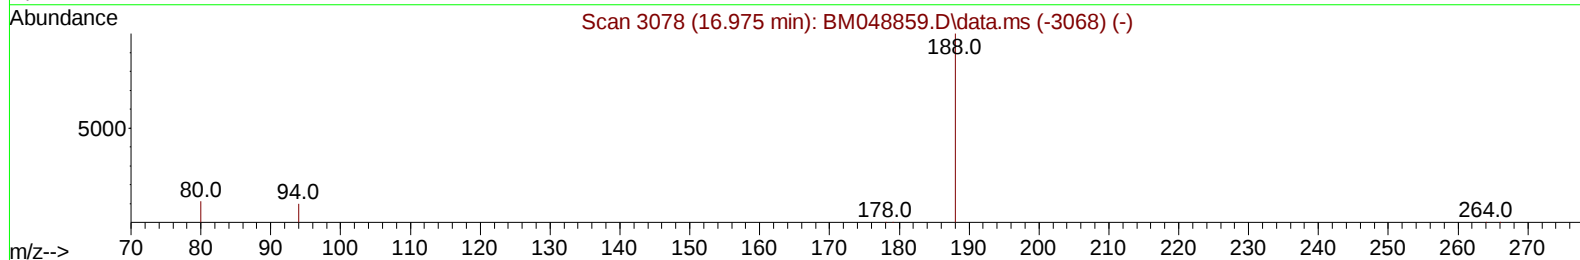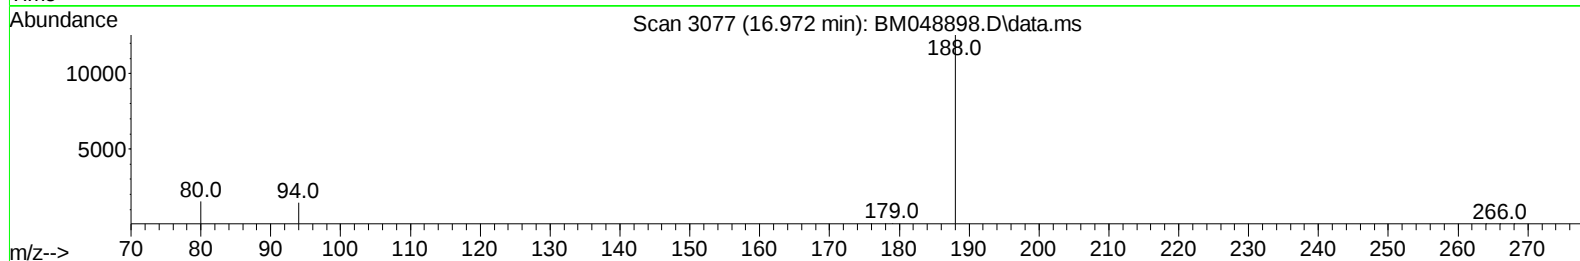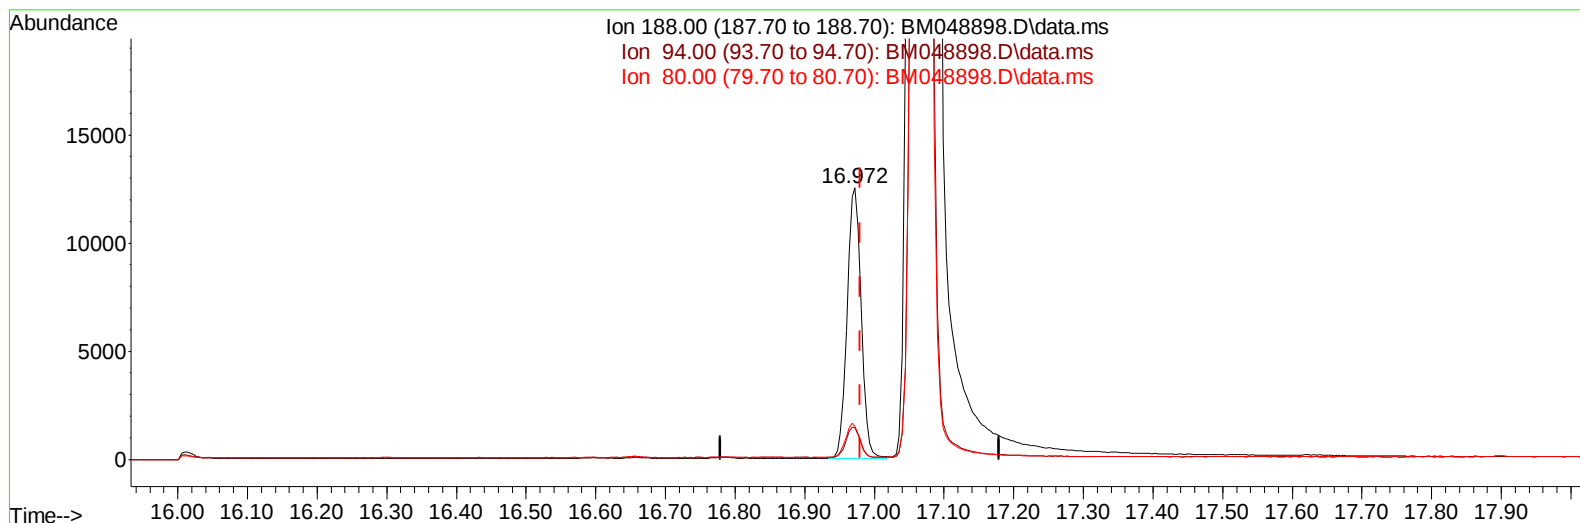

TIC: BM048898.D\data.ms

(13) Phenanthrene-d10 (I)

16.972min (-0.007) 0.40 ng/ul m

response 17464

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.20	11.60
80.00	12.50	12.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048898.D
Acq On : 07 Dec 2024 15:47
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ98

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

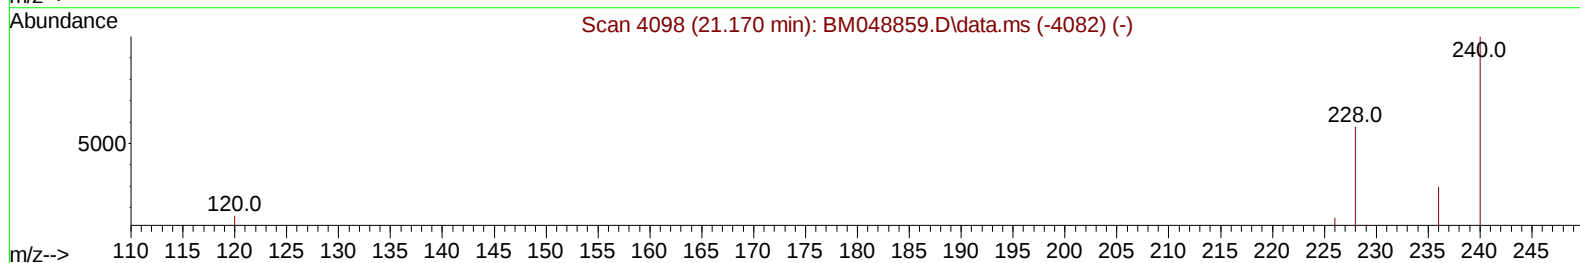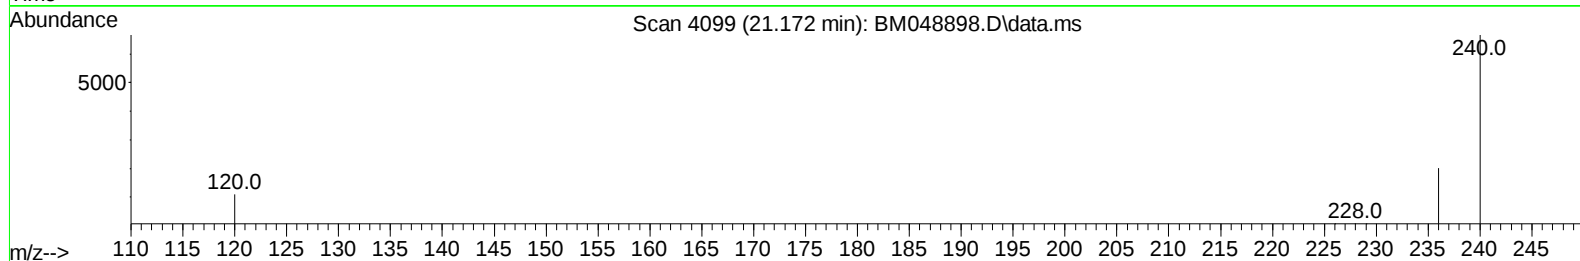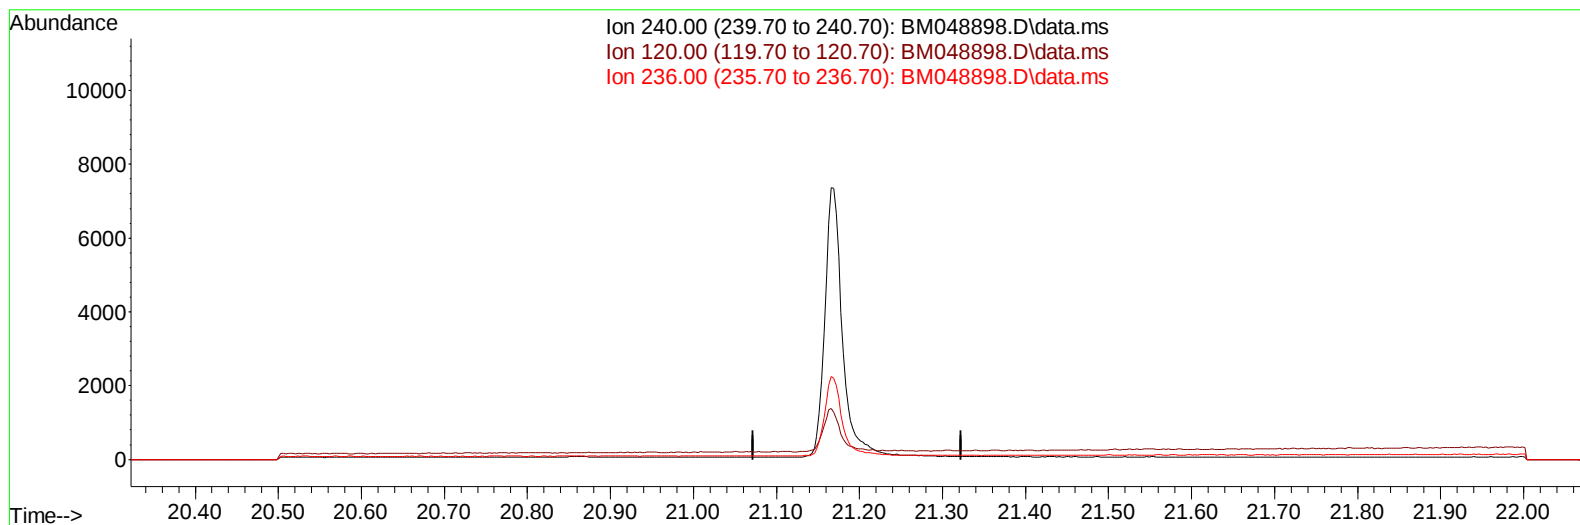

TIC: BM048898.D\data.ms

(17) Chrysene-d12

21.173min (-21.173) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	32.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048898.D
Acq On : 07 Dec 2024 15:47
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ98

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

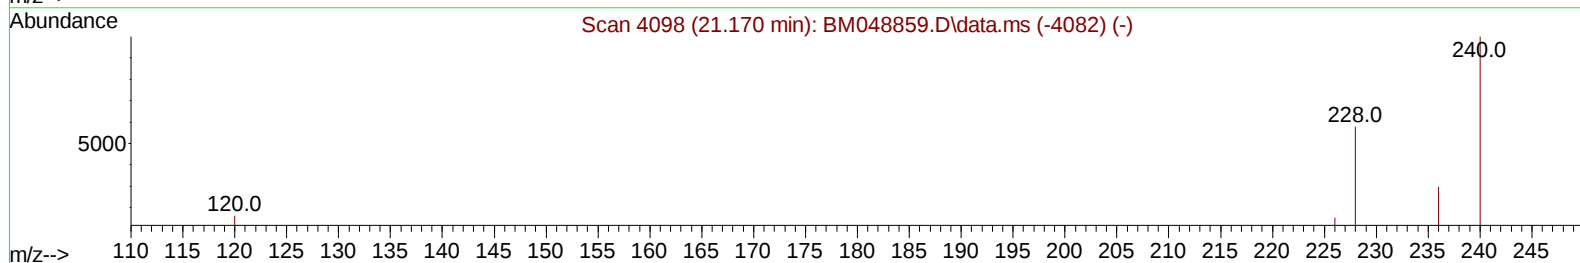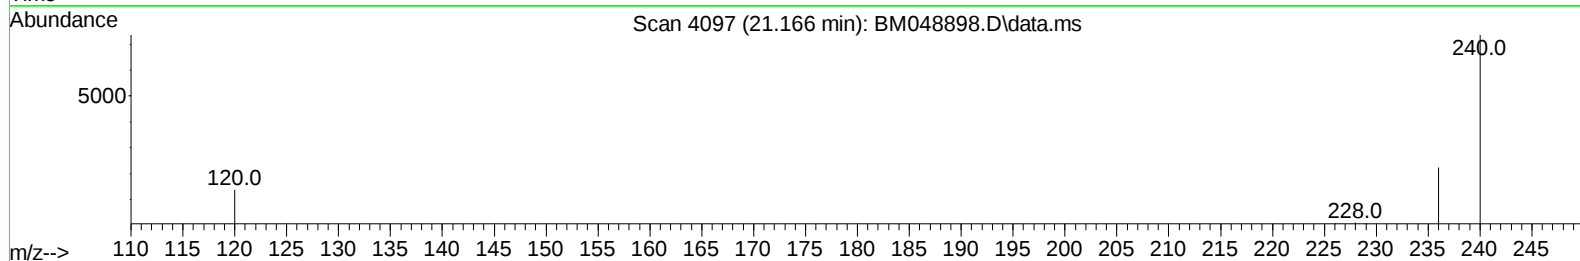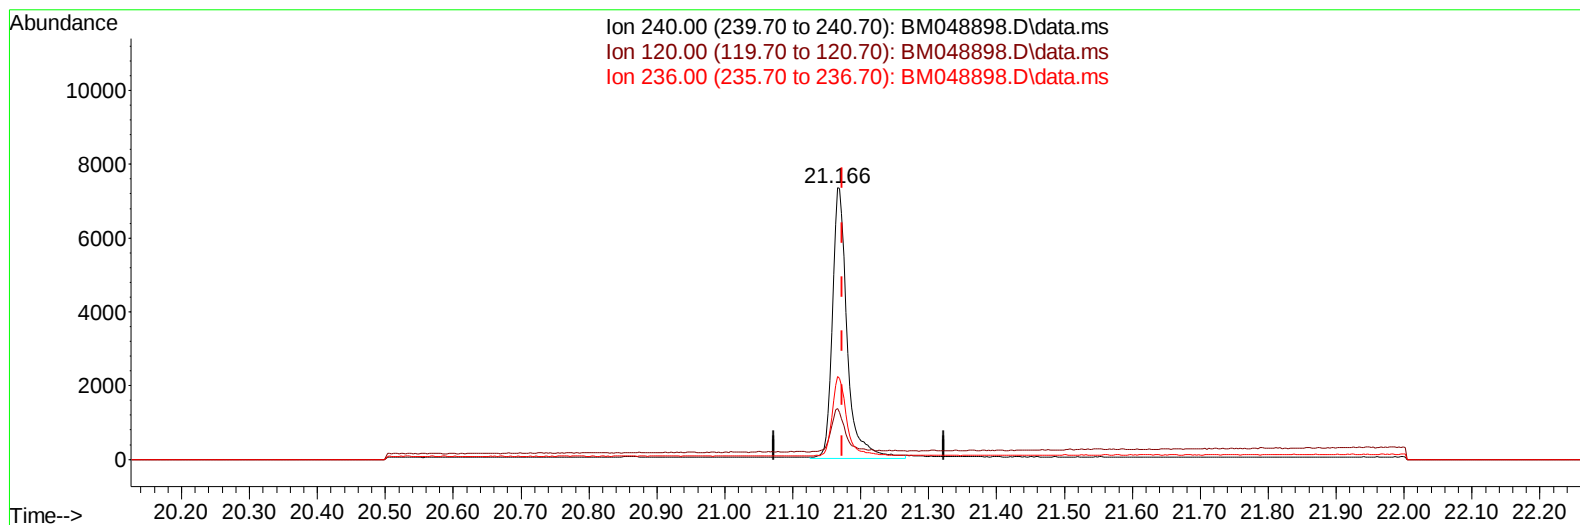

TIC: BM048898.D\data.ms

(17) Chrysene-d12

21.166min (-0.006) 0.40 ng/u1 m

response 11133

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	18.67
236.00	32.10	30.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048898.D
Acq On : 07 Dec 2024 15:47
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ98

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

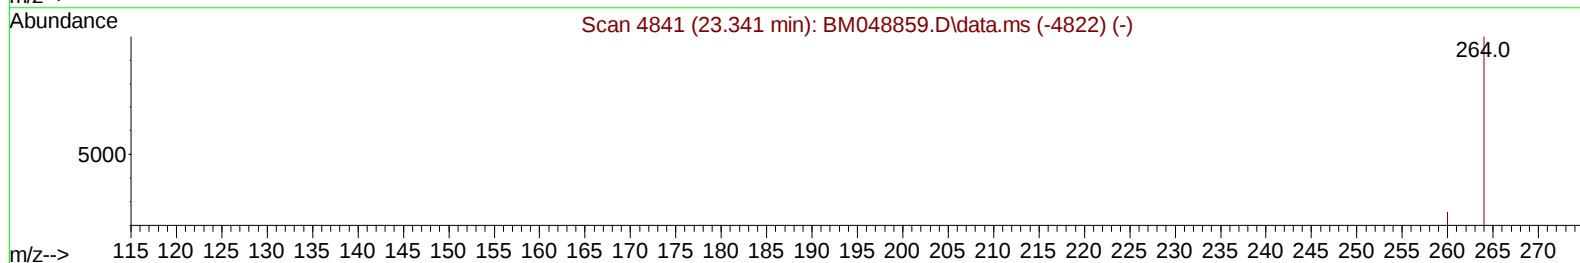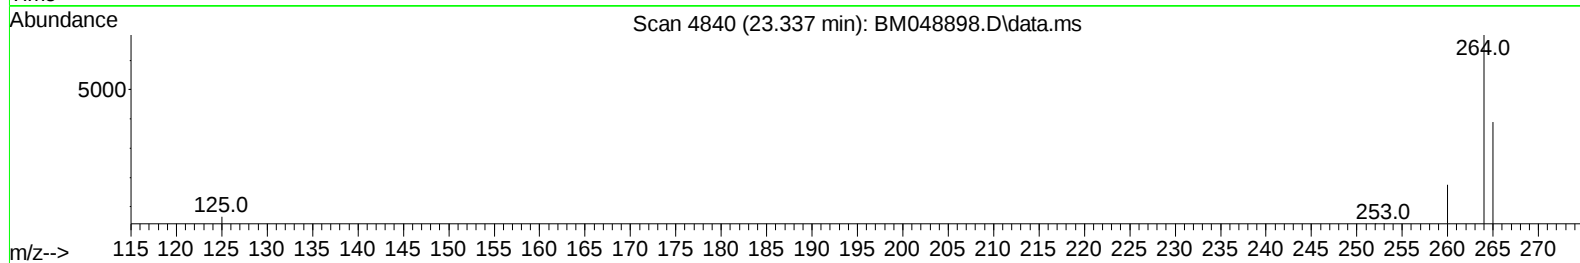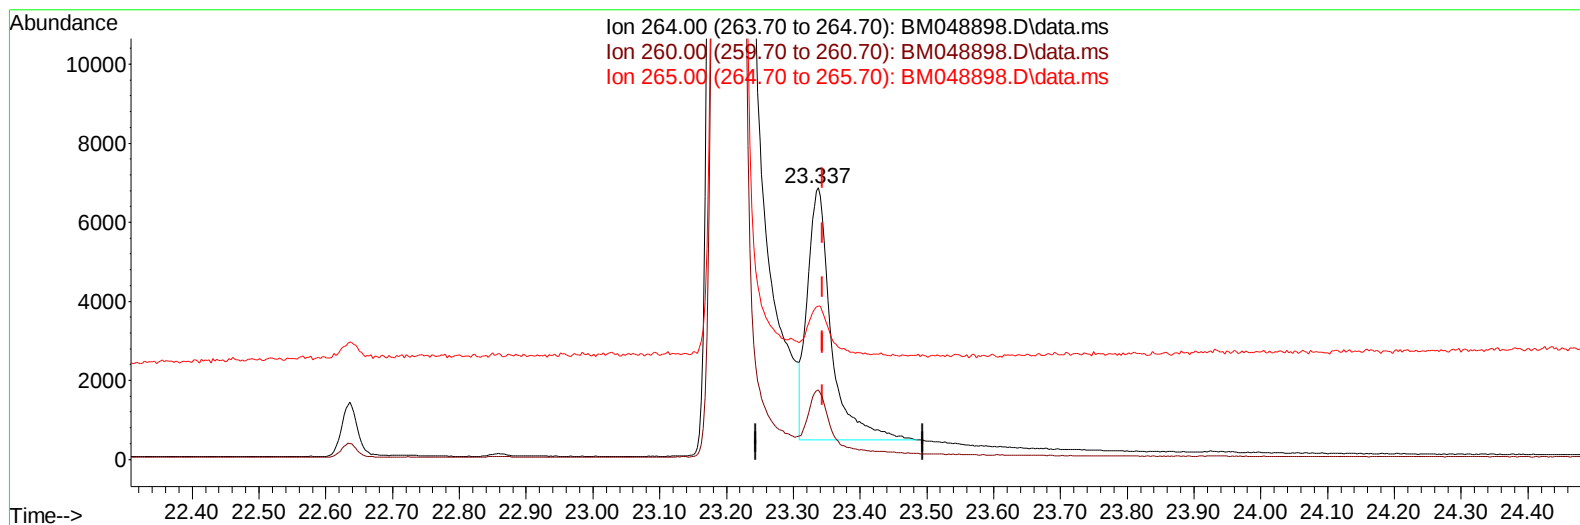

TIC: BM048898.D\data.ms

(23) Perylene-d12 (I)

23.337min (-0.006) 0.40 ng/u1

response 15985

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.52
265.00	78.50	56.59#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048898.D
Acq On : 07 Dec 2024 15:47
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ98

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

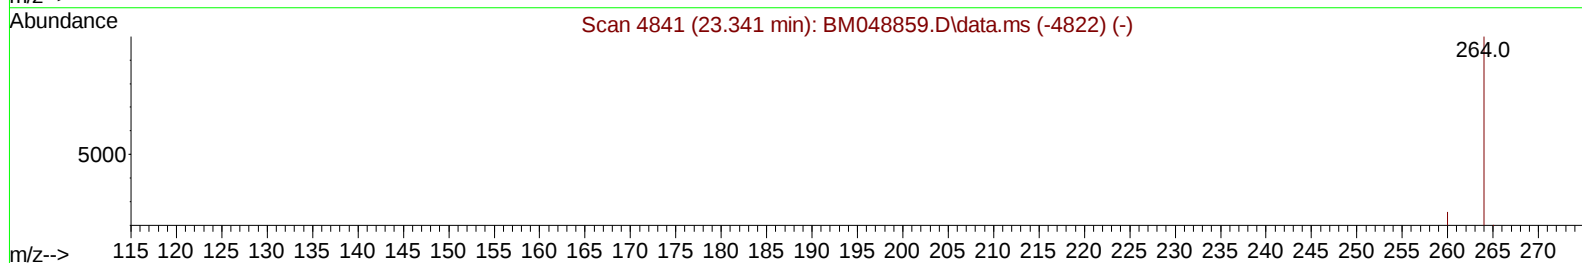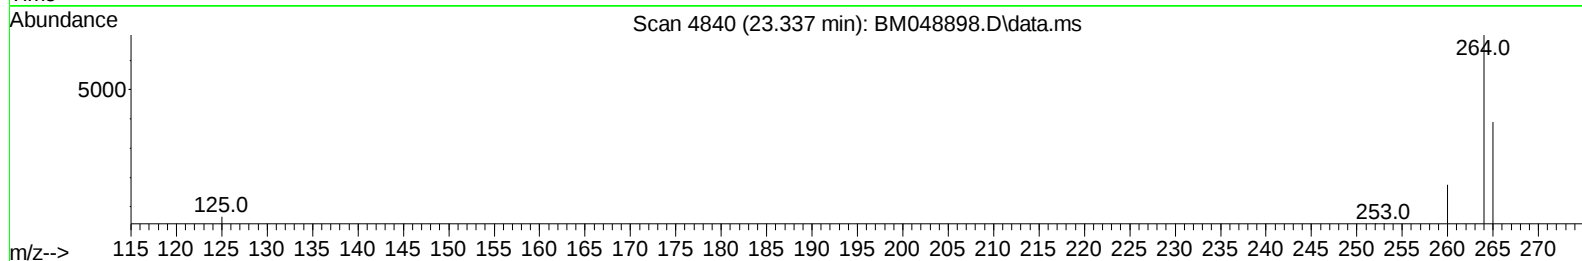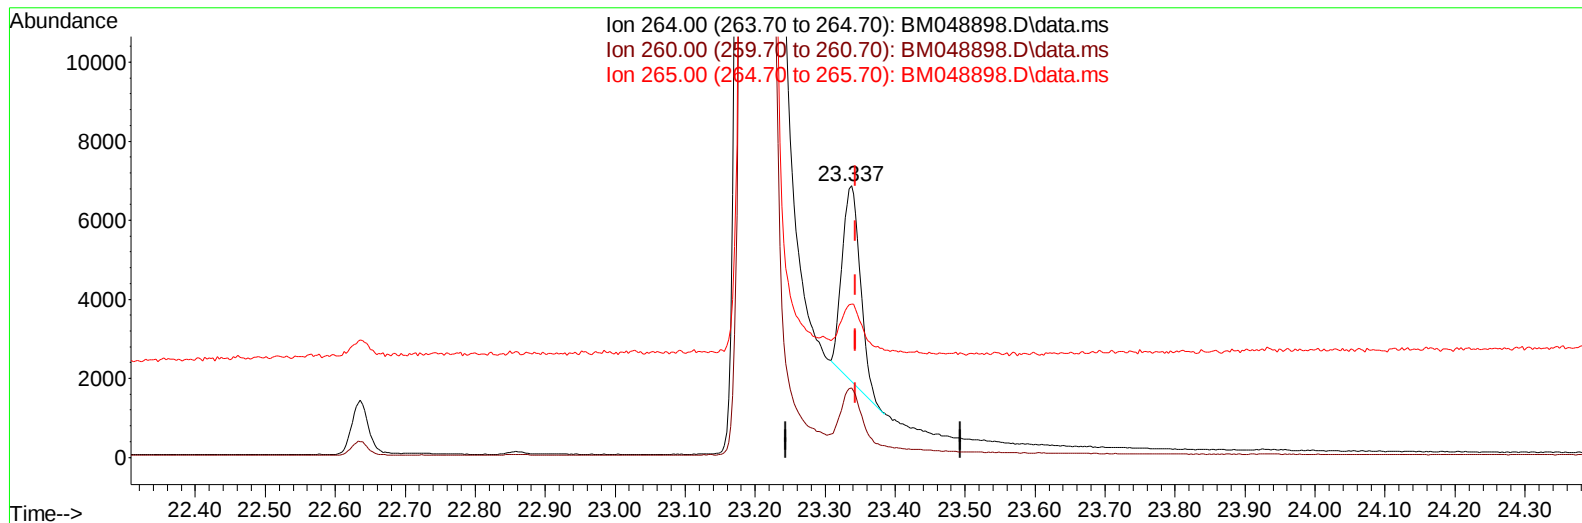

TIC: BM048898.D\data.ms

(23) Perylene-d12 (I)

23.337min (-0.006) 0.40 ng/ul m

response 8868

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.70	25.52
265.00	78.50	56.59#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048898.D
 Acq On : 07 Dec 2024 15:47
 Operator : RC/JU
 Sample : P5107-19
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHJ98

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/10/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 08 21:47:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	5590	0.400	ng/ul	0.00
4) Naphthalene-d8	10.353	136	15760	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.224	164	8197	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.972	188	17464m	0.400	ng/ul	0.00
17) Chrysene-d12	21.166	240	11133m	0.400	ng/ul	0.00
23) Perylene-d12	23.337	264	8868m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	33364	4.672	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.954	152	6504	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.007	212	15601	0.454	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048898.D
Acq On : 07 Dec 2024 15:47
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHJ98

Manual IntegrationsAPPROVED

Quant Time: Dec 08 21:47:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :mohammad ahmed 12/10/2024

