

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048864.D
 Acq On : 06 Dec 2024 12:45
 Operator : RC/JU
 Sample : P5104-19
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHJ76

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 12:33:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	5164	0.400	ng/ul	0.00
4) Naphthalene-d8	10.363	136	14730	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.232	164	7776	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.979	188	15824m	0.400	ng/ul	0.00
17) Chrysene-d12	21.178	240	9661m	0.400	ng/ul	0.00
23) Perylene-d12	23.347	264	7788m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	26911	4.080	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.963	152	5383	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.015	212	12965	0.435	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.197	88	604	0.077	ng/ul#	71

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048864.D
Acq On : 06 Dec 2024 12:45
Operator : RC/JU
Sample : P5104-19
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BHJ76

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024


Quant Time: Dec 06 12:33:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

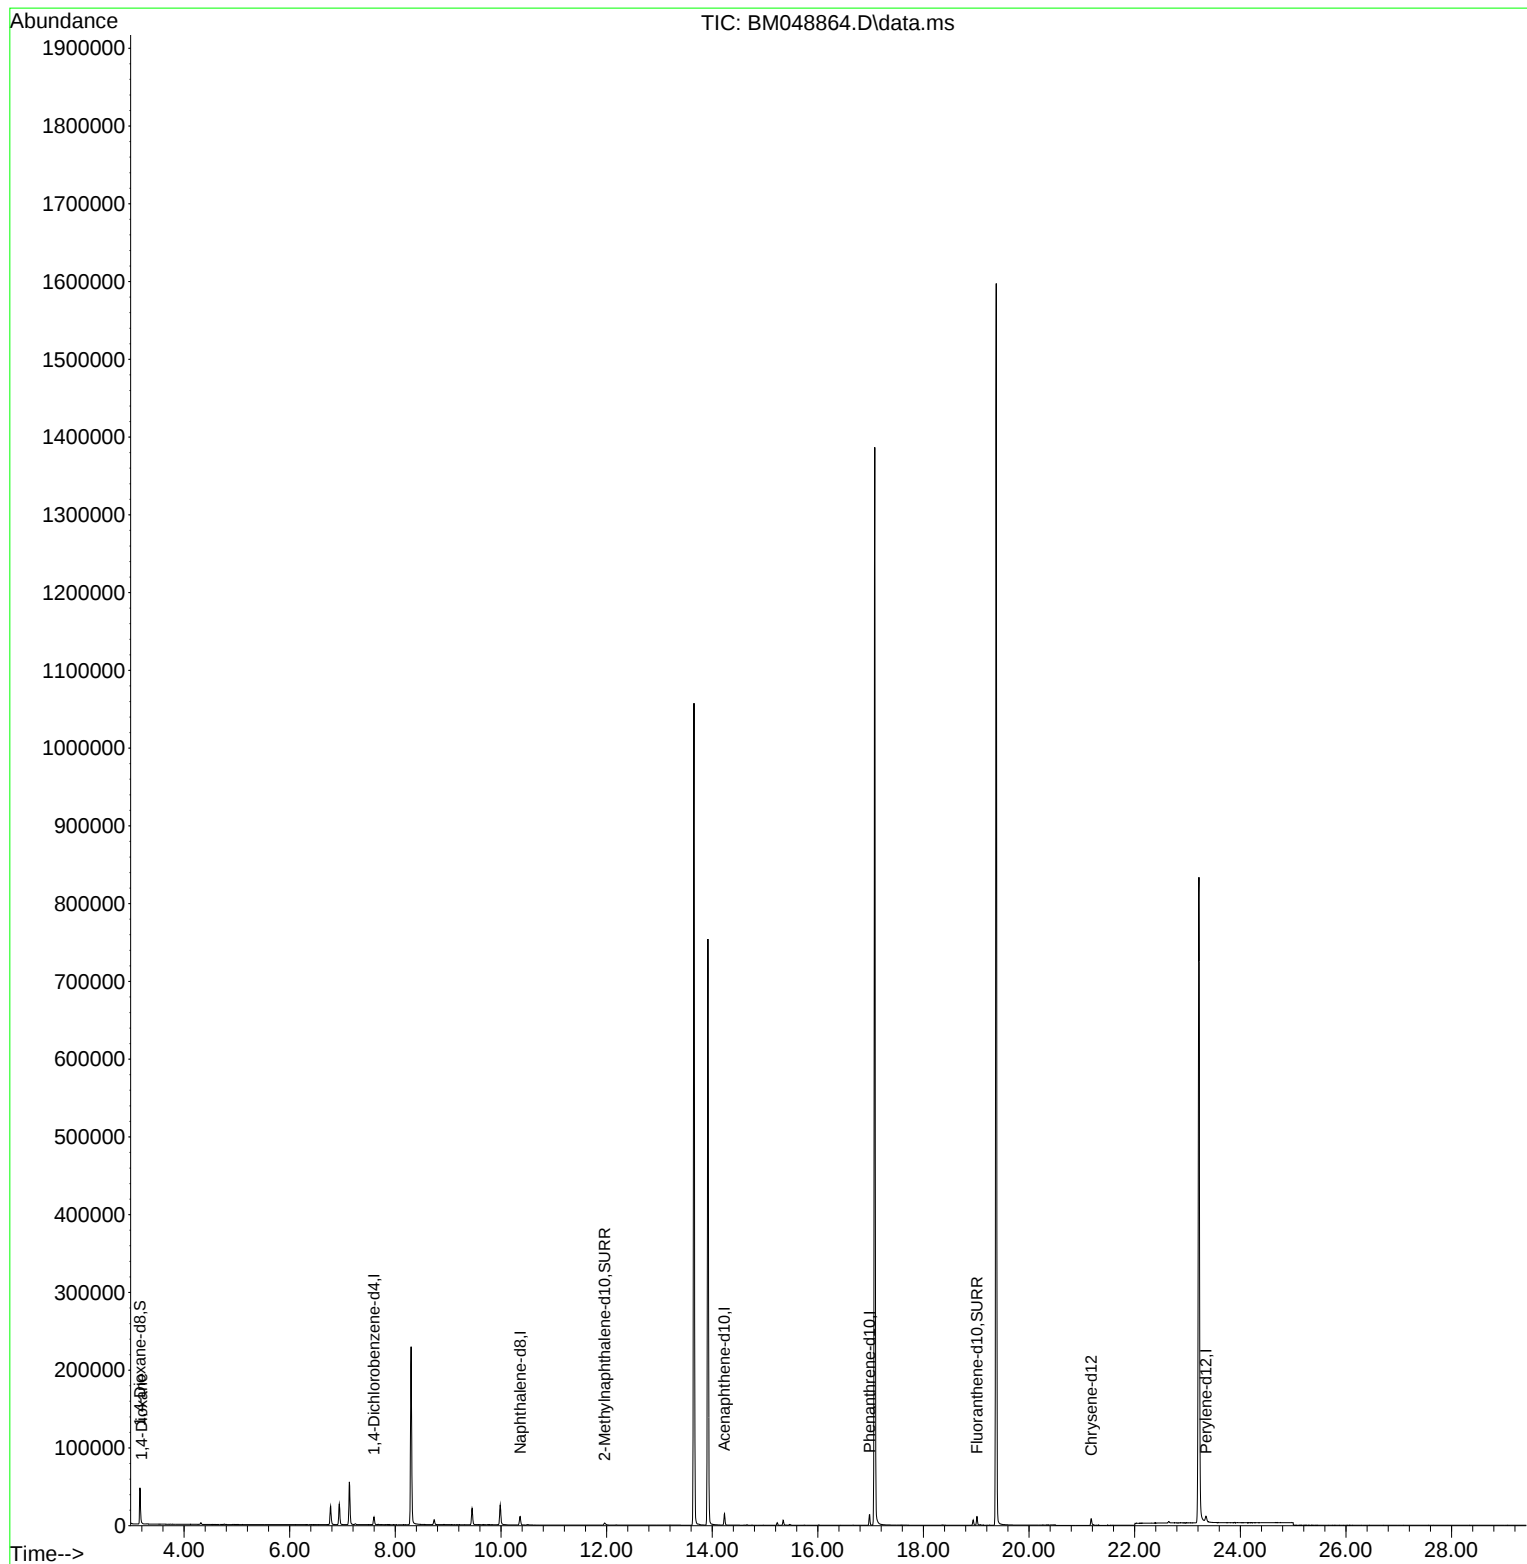

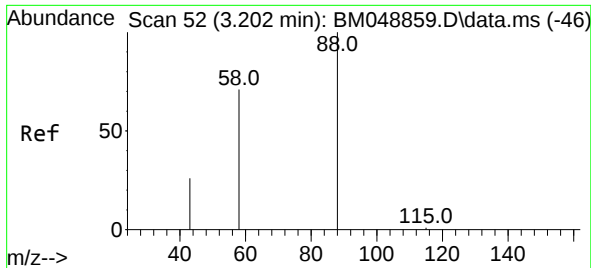

#2
 1,4-Dioxane
 Concen: 0.077 ng/ul
 RT: 3.197 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM048864.D
 Acq: 06 Dec 2024 12:45

Instrument :
 BNA_M
 ClientSampleId :
 BHJ76

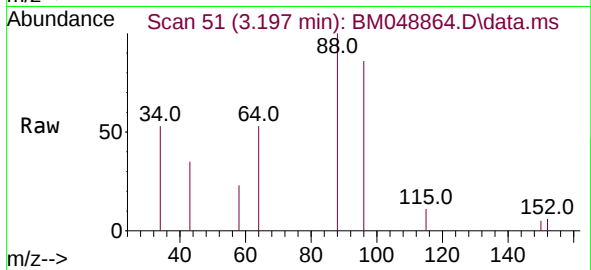

Tgt Ion: 88 Resp: 604

Ion	Ratio	Lower	Upper
88	100		
43	34.7	20.6	30.8
58	23.3	37.6	56.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

