

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
 Data File : BM048868.D
 Acq On : 06 Dec 2024 15:09
 Operator : RC/JU
 Sample : P5107-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHJ81

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

Quant Time: Dec 06 15:21:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 00:05:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	4872	0.400	ng/ul	0.00
4) Naphthalene-d8	10.359	136	13783	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.229	164	7030	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.976	188	14574m	0.400	ng/ul	0.00
17) Chrysene-d12	21.175	240	10151m	0.400	ng/ul	0.00
23) Perylene-d12	23.349	264	9694m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	26644	4.281	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.959	152	5012	0.302	ng/ul	0.00
18) Fluoranthene-d10	19.011	212	11905	0.380	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.197	88	374	0.051	ng/ul#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120524\
Data File : BM048868.D
Acq On : 06 Dec 2024 15:09
Operator : RC/JU
Sample : P5107-04
Misc :
ALS Vial : 40 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BHJ81

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/10/2024


Quant Time: Dec 06 15:21:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 00:05:00 2024
Response via : Initial Calibration

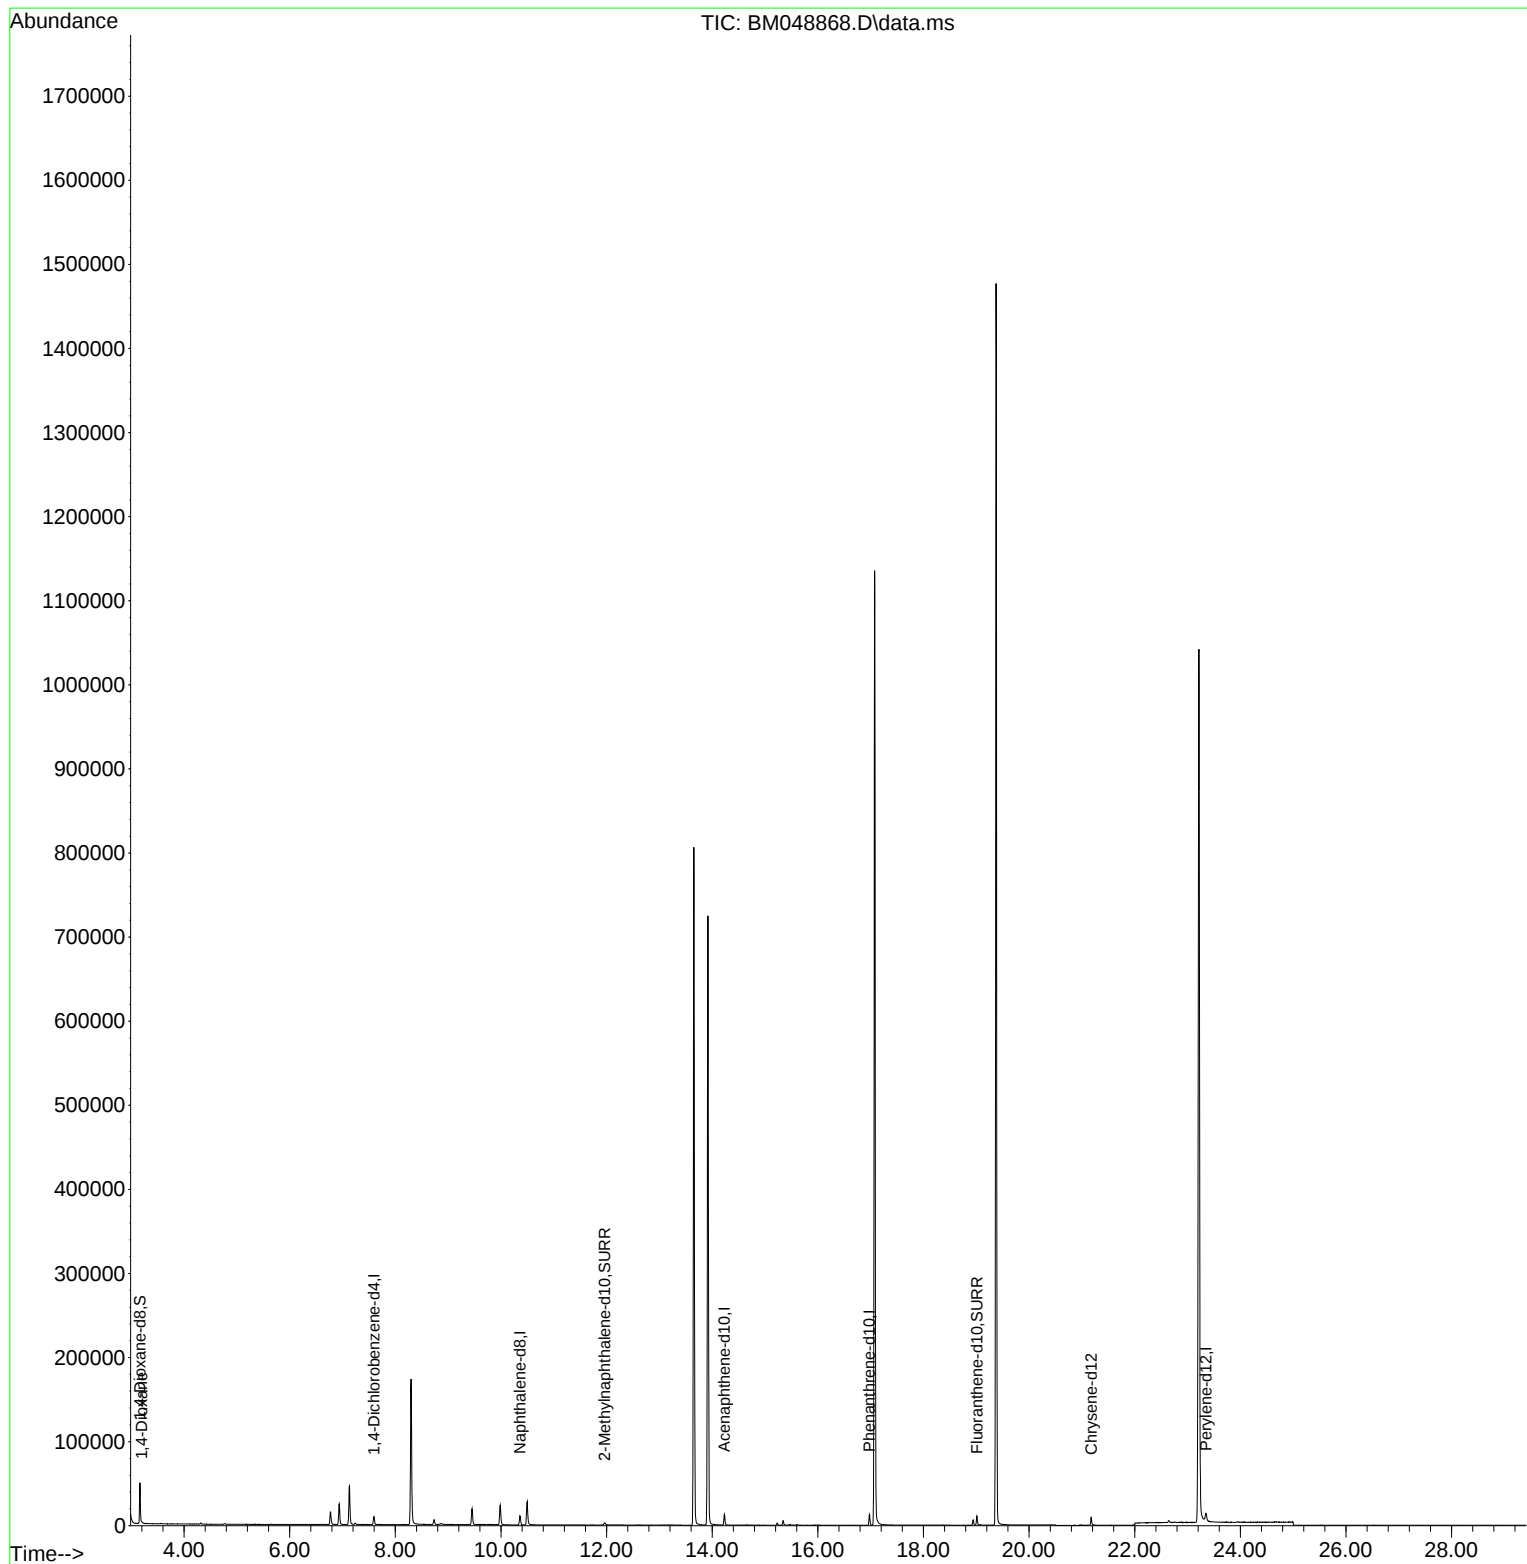

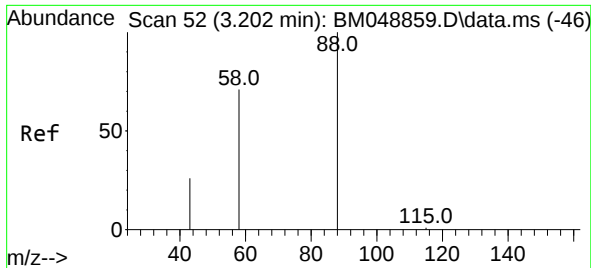

#2
 1,4-Dioxane
 Concen: 0.051 ng/ul
 RT: 3.197 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM048868.D
 Acq: 06 Dec 2024 15:09

Instrument :
 BNA_M
 ClientSampleId :
 BHJ81

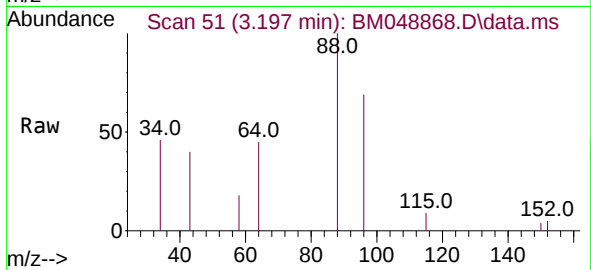

Tgt Ion: 88 Resp: 374

Ion	Ratio	Lower	Upper
88	100		
43	39.7	20.6	30.8
58	17.8	37.6	56.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/10/2024

