

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
 Data File : BM003389.D
 Acq On : 06 Dec 2015 15:09
 Operator : UM/IZ
 Sample : G4664-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5E81

Quant Time: Dec 07 04:23:02 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 07 04:19:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	75827	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	343678	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	207438	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	457131	20.00	ng/ul	0.00
78) Chrysene-d12	21.32	240	408723	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	364579	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	2552	1.67	ng/uL	0.00
5) Phenol-d5	6.89	99	48347	7.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	113300	33.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	141759	28.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	92120	18.14	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	80232	34.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	86214	35.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	153930	31.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	3408	0.62	ng/ul	0.00
44) Dimethylphthalate-d6	13.78	166	562929	36.10	ng/ul	0.00
47) Acenaphthylene-d8	14.07	160	667528	34.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.57	143	13337	4.77	ng/ul	0.00
58) Fluorene-d10	15.37	176	489193	36.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	65548	28.03	ng/ul	0.00
71) Anthracene-d10	17.22	188	740309	36.45	ng/ul	0.00
79) Pyrene-d10	19.52	212	766560	38.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	612284	34.81	ng/ul	0.00


Target Compounds					Qvalue
46) 2,6-Dinitrotoluene	13.79	165	3212	1.09 ng/ul#	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
Data File : BM003389.D
Acq On : 06 Dec 2015 15:09
Operator : UM/IZ
Sample : G4664-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E81

Quant Time: Dec 07 04:23:02 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 07 04:19:45 2015
Response via : Initial Calibration

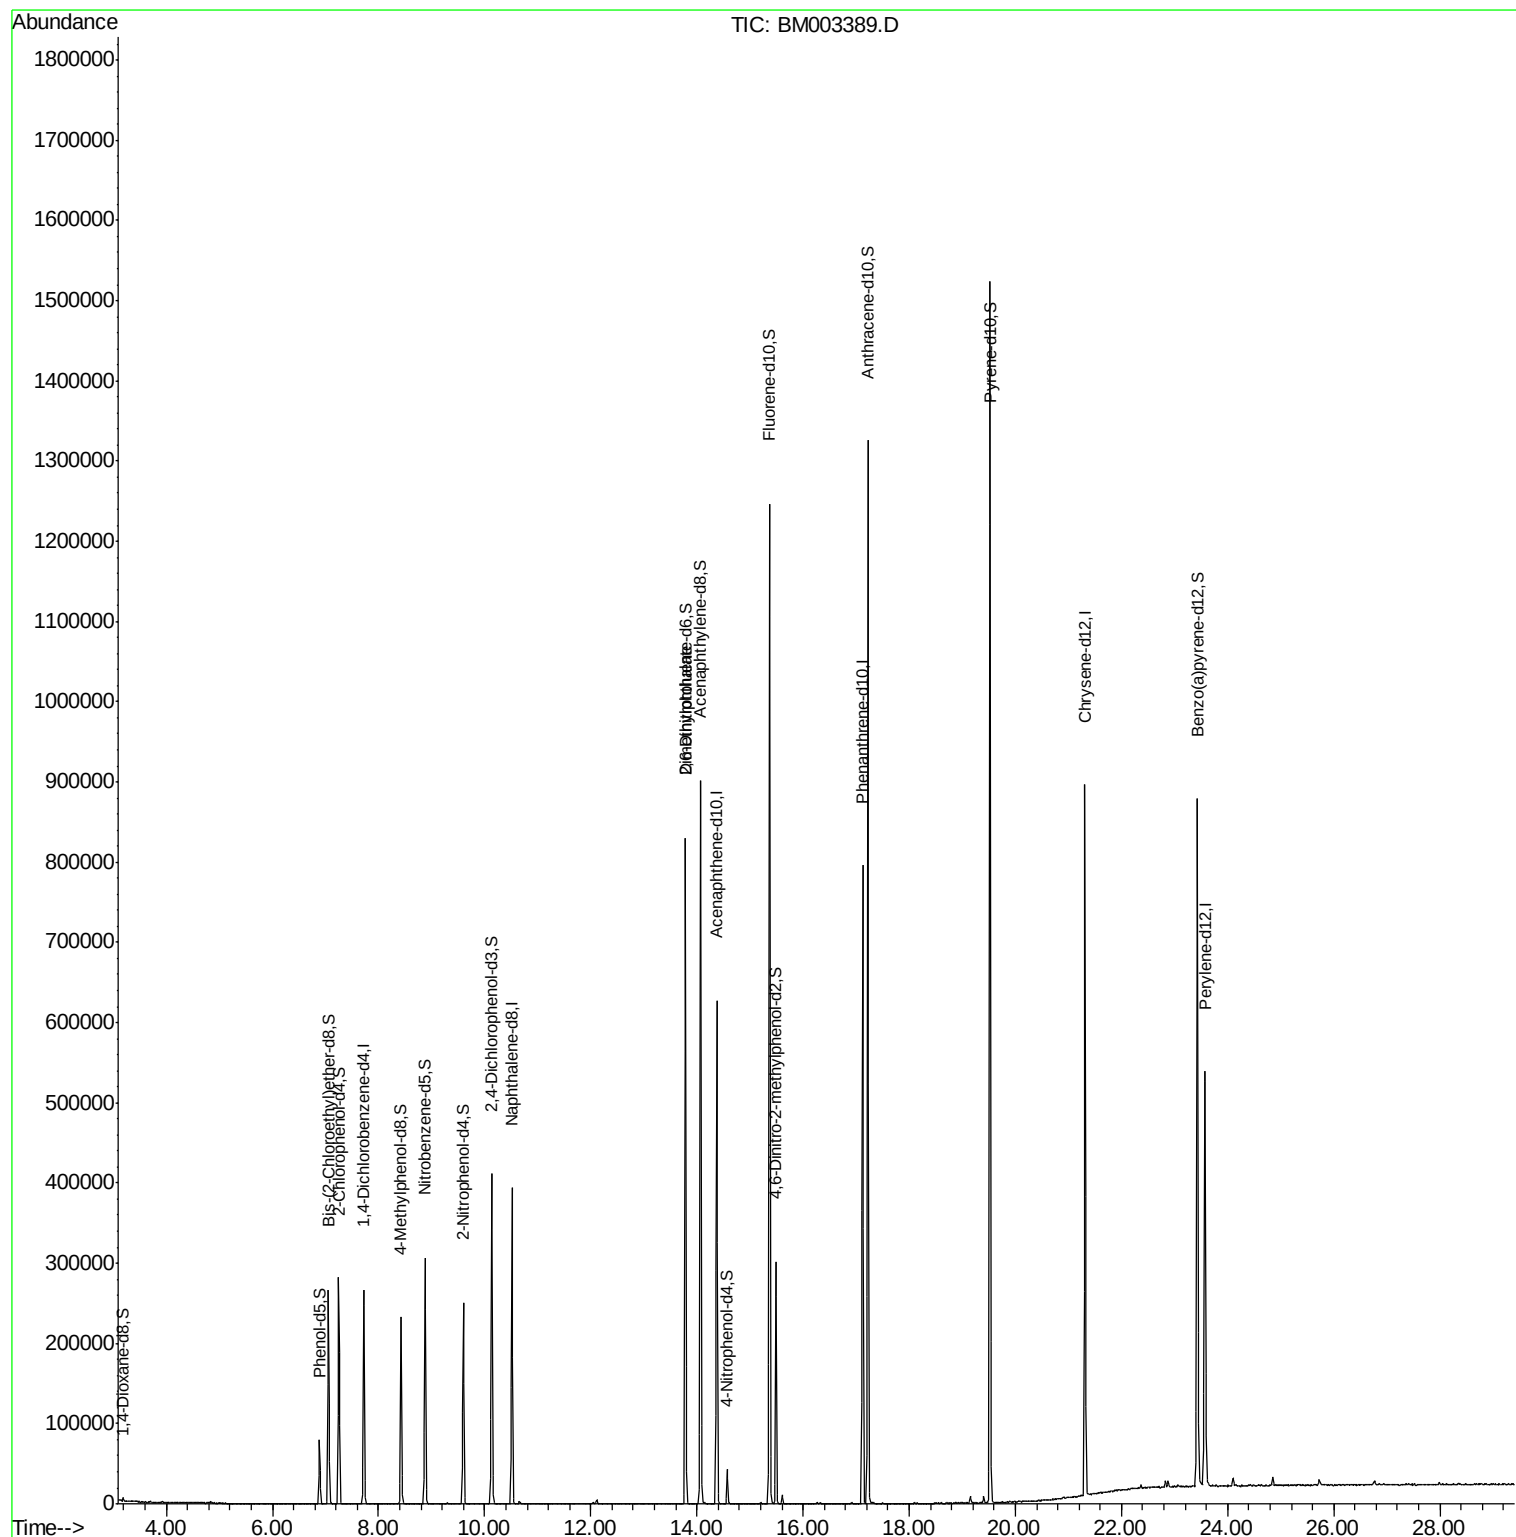

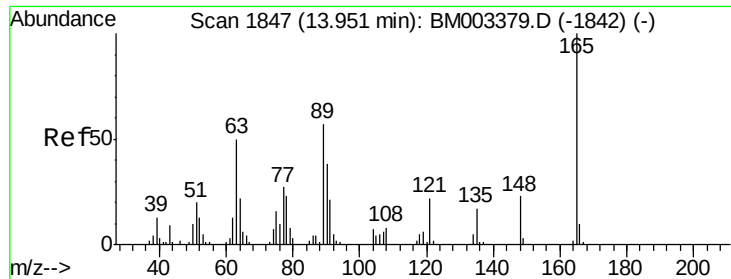

#46

2,6-Dinitrotoluene

Concen: 1.09 ng/ul

RT: 13.79 min Scan# 1819

Delta R.T. -0.16 min

Lab File: BM003389.D


Acq: 06 Dec 2015 15:09

Instrument :

BNA_M

ClientSampleId :

E5E81

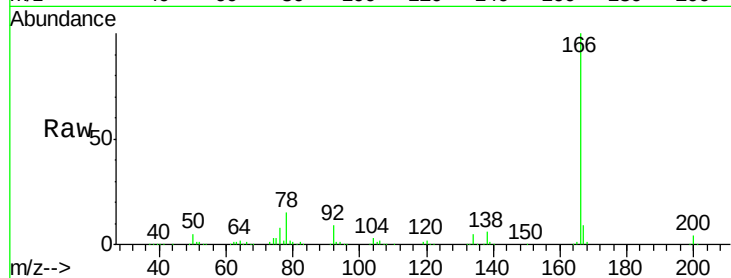

Tgt Ion:	165	Resp:	3212
Ion Ratio	Lower	Upper	
165	100		
89	0.0	42.0	63.0#
121	49.9	16.6	24.8#

