

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120615\
 Data File : BM003386.D
 Acq On : 06 Dec 2015 13:21
 Operator : UM/IZ
 Sample : G4664-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5E79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	13	17	21	rVB	2242	3182	0.17%	0.019%
2	6.886	641	646	654	rBB	54378	80365	4.31%	0.472%
3	7.057	669	675	685	rBB	239963	365009	19.60%	2.145%
4	7.251	702	708	717	rBB	233413	365782	19.64%	2.149%
5	7.722	782	788	795	rBB	266590	419121	22.50%	2.463%
6	8.422	902	907	918	rBB	175295	273499	14.68%	1.607%
7	8.880	978	985	993	rBB	277568	432746	23.24%	2.543%
8	9.304	1053	1057	1060	rBB	1662	2161	0.12%	0.013%
9	9.598	1101	1107	1115	rBB	226778	350523	18.82%	2.060%
10	10.133	1192	1198	1207	rBV	346688	559533	30.04%	3.288%
11	10.516	1256	1263	1271	rBB	405749	668228	35.88%	3.927%
12	10.651	1282	1286	1292	rBB	10599	16104	0.86%	0.095%
13	12.110	1530	1534	1538	rBB	4715	6459	0.35%	0.038%
14	13.780	1812	1818	1828	rBV	751069	1017488	54.63%	5.979%
15	14.062	1860	1866	1877	rBV	849212	1248912	67.06%	7.339%
16	14.374	1912	1919	1927	rBB2	642877	964932	51.81%	5.670%
17	14.568	1948	1952	1961	rBB	24926	35783	1.92%	0.210%
18	15.368	2082	2088	2096	rBV	1168568	1638387	87.97%	9.627%
19	15.486	2103	2108	2117	rBV	252955	323032	17.34%	1.898%
20	15.609	2124	2129	2133	rVB2	9231	11259	0.60%	0.066%
21	16.909	2347	2350	2354	rBV2	1915	2495	0.13%	0.015%
22	17.121	2380	2386	2396	rBV	823623	1138477	61.13%	6.690%
23	17.221	2396	2403	2420	rVV	1196098	1705962	91.60%	10.024%
24	19.150	2727	2731	2737	rBV	8725	11717	0.63%	0.069%
25	19.409	2771	2775	2782	rBV	7332	10534	0.57%	0.062%
26	19.521	2788	2794	2805	rBV2	1403841	1862473	100.00%	10.944%
27	19.756	2829	2834	2838	rBV	2923	3265	0.18%	0.019%
28	20.844	3015	3019	3021	rBV4	1453	2076	0.11%	0.012%
29	21.321	3094	3100	3109	rBV	872596	1114223	59.82%	6.547%
30	23.432	3451	3459	3472	rBV	767779	1412639	75.85%	8.301%
31	23.574	3476	3483	3496	rVB	516636	971852	52.18%	5.711%


Sum of corrected areas: 17018218

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120615\
Data File : BM003386.D
Acq On : 06 Dec 2015 13:21
Operator : UM/IZ
Sample : G4664-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E79

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

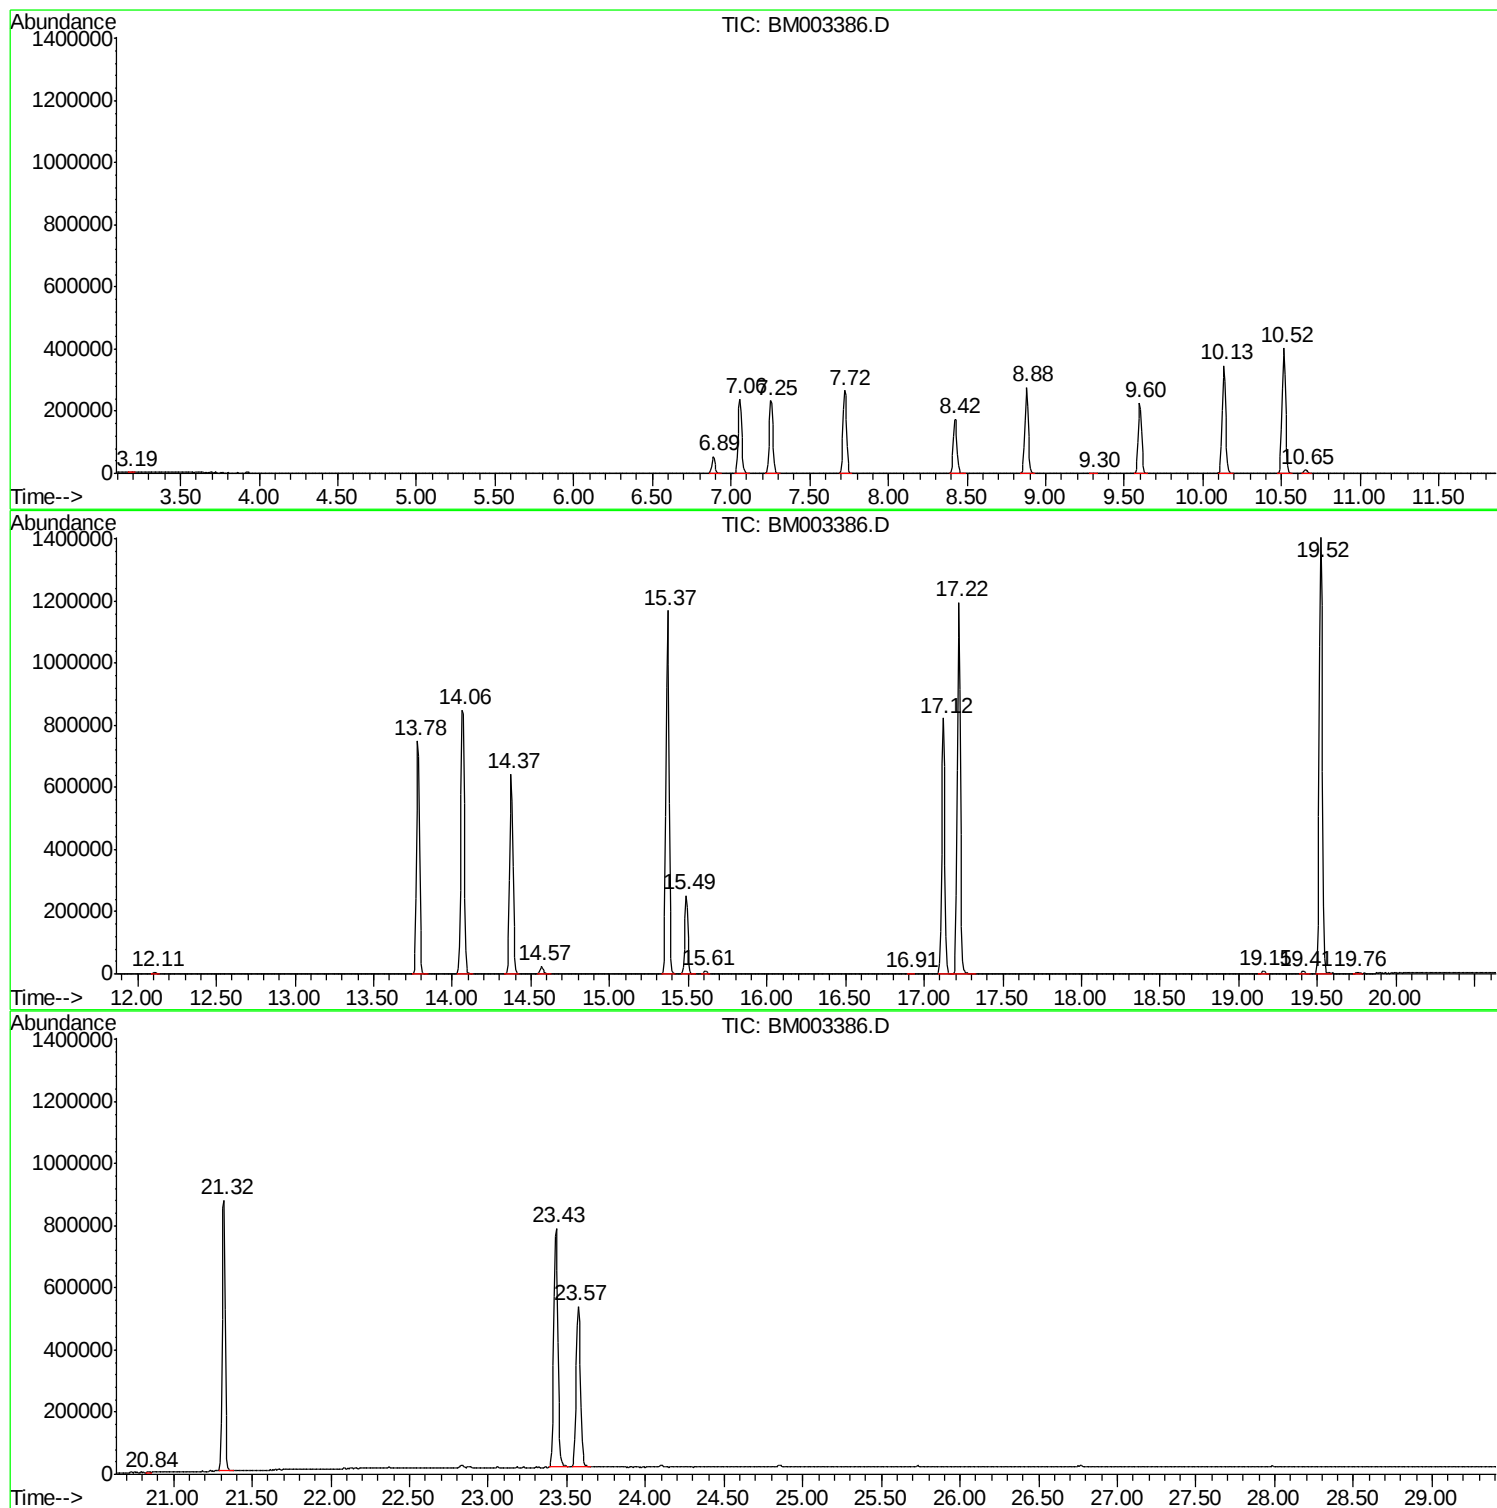

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
Data File : BM003386.D
Acq On : 06 Dec 2015 13:21
Operator : UM/IZ
Sample : G4664-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E79

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
Data File : BM003386.D
Acq On : 06 Dec 2015 13:21
Operator : UM/IZ
Sample : G4664-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E79

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc