

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120615\
 Data File : BM003387.D
 Acq On : 06 Dec 2015 13:57
 Operator : UM/IZ
 Sample : PB87108BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK08

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	13	17	23	rVB	18617	24583	1.51%	0.136%
2	3.740	109	111	115	rBV	2171	2327	0.14%	0.013%
3	6.887	640	646	654	rBV	323189	482410	29.56%	2.675%
4	7.057	669	675	686	rBB	261429	393518	24.11%	2.182%
5	7.251	702	708	718	rVB	319989	508509	31.16%	2.820%
6	7.722	782	788	796	rBB	264727	412493	25.28%	2.287%
7	8.428	901	908	919	rBB	412344	650202	39.84%	3.605%
8	8.881	978	985	994	rBB	285574	446147	27.34%	2.474%
9	9.598	1101	1107	1114	rBV	234737	364977	22.37%	2.024%
10	10.133	1191	1198	1209	rBB	402477	643091	39.41%	3.566%
11	10.516	1256	1263	1271	rBB	389262	641648	39.32%	3.558%
12	10.651	1279	1286	1296	rBV	408228	672786	41.23%	3.731%
13	12.110	1530	1534	1538	rBB	4255	6328	0.39%	0.035%
14	13.780	1812	1818	1827	rBV	722462	990949	60.72%	5.495%
15	14.068	1860	1867	1876	rBV	799200	1192951	73.10%	6.615%
16	14.374	1912	1919	1927	rBB2	572983	864628	52.98%	4.794%
17	14.568	1946	1952	1968	rBV	259025	353664	21.67%	1.961%
18	15.368	2082	2088	2095	rBV	1072697	1524130	93.40%	8.451%
19	15.486	2102	2108	2117	rBV	243291	303297	18.59%	1.682%
20	15.610	2125	2129	2135	rVB	9259	11826	0.72%	0.066%
21	16.909	2347	2350	2355	rVB	1512	1961	0.12%	0.011%
22	17.121	2380	2386	2392	rBV	682104	937878	57.47%	5.201%
23	17.221	2396	2403	2415	rBV	1102325	1535079	94.07%	8.512%
24	19.150	2727	2731	2737	rBV	7190	9982	0.61%	0.055%
25	19.409	2770	2775	2780	rBV	6006	7502	0.46%	0.042%
26	19.521	2788	2794	2804	rBV	1240690	1631907	100.00%	9.049%
27	20.127	2892	2897	2898	rBV2	1030	1688	0.10%	0.009%
28	21.321	3094	3100	3106	rBV	757445	950622	58.25%	5.271%
29	23.433	3451	3459	3474	rBV	856032	1538676	94.29%	8.532%
30	23.574	3476	3483	3499	rVB	479808	912157	55.90%	5.058%
31	24.856	3698	3701	3707	rVB5	9446	16323	1.00%	0.091%


Sum of corrected areas: 18034239

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120615\
Data File : BM003387.D
Acq On : 06 Dec 2015 13:57
Operator : UM/IZ
Sample : PB87108BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK08

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

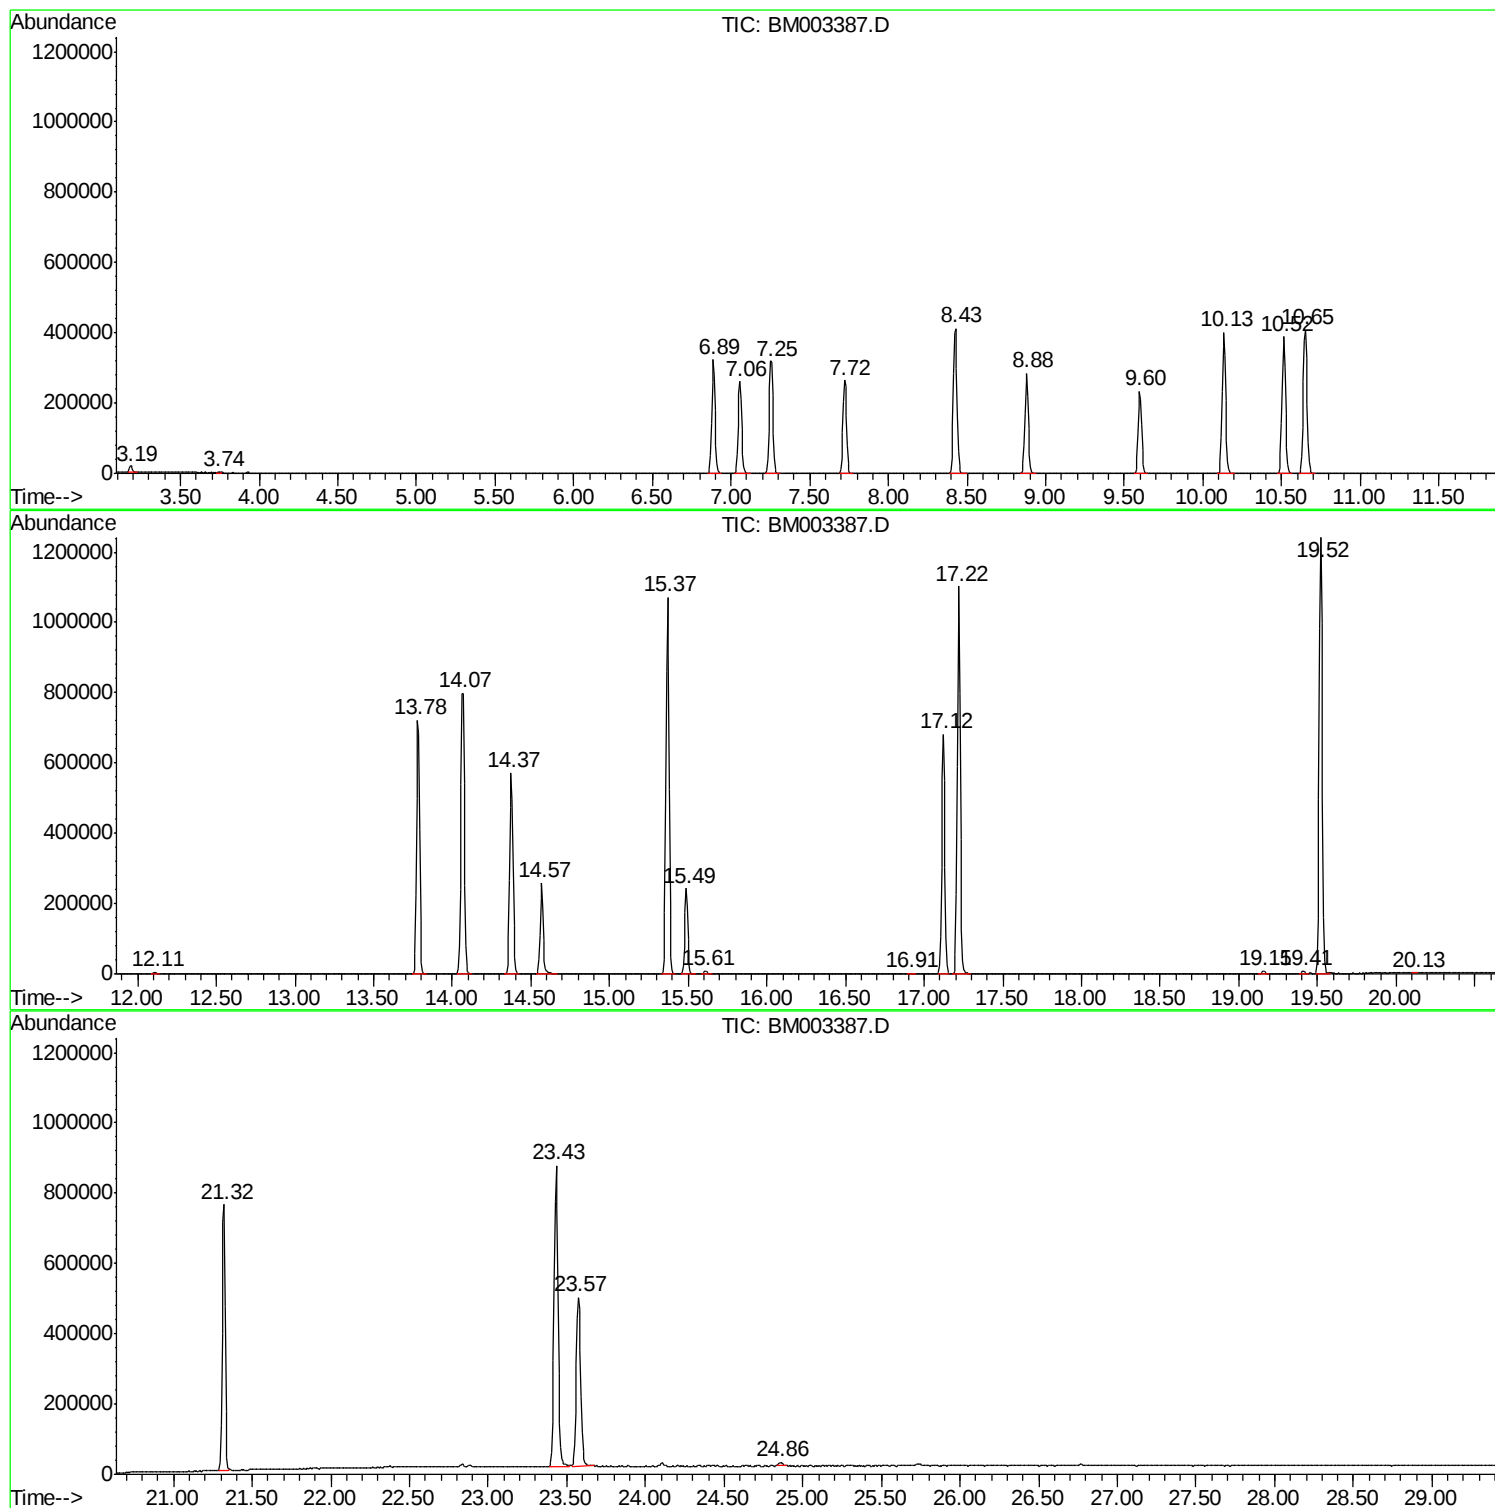

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
Data File : BM003387.D
Acq On : 06 Dec 2015 13:57
Operator : UM/IZ
Sample : PB87108BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK08

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
Data File : BM003387.D
Acq On : 06 Dec 2015 13:57
Operator : UM/IZ
Sample : PB87108BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK08

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc